

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072220\
 Data File : PS011314.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2020 14:02
 Operator : DD\AJ
 Sample : PB130341BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB130341BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 17:24:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.231	6.916	493.1E6	313.5E6	508.223	556.859
Target Compounds							
1) T	Dalapon	2.997	2.577	26315196	25789442	21.868	33.594 #
2) T	3,5-DICHL...	0.000	6.096	0	23187917	N.D.	27.610
7) T	MCPA	7.779	7.379	33480489	13989808	7.851	4.854 #
10) T	Pentachlo...	8.711	8.432	10461527	9953882	<MDL	1.428 #
12) T	2,4,5-T	9.506	9.182	20371349	9856512	4.037	3.250
14) T	DINOSEB	0.000	10.035	0	10805160	N.D.	5.038
15) T	Picloram	11.037	11.007	181.5E6	177.2E6	28.761	40.520 #
16) T	DCPA	11.477	10.943	5783628	9005811	<MDL	2.381 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072220\
Data File : PS011314.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2020 14:02
Operator : DD\AJ
Sample : PB130341BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB130341BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 17:24:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
Quant Title : 8080.M
QLast Update : Mon Jul 13 16:10:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

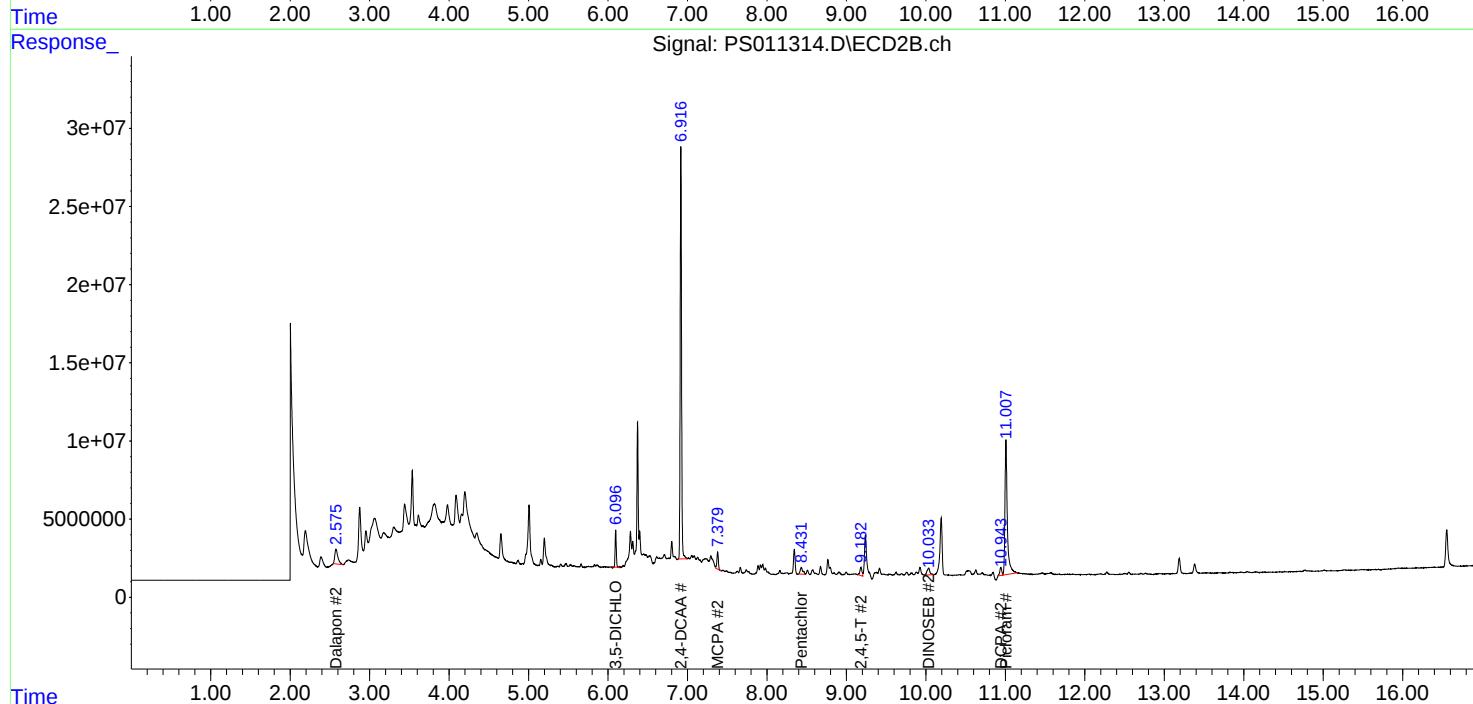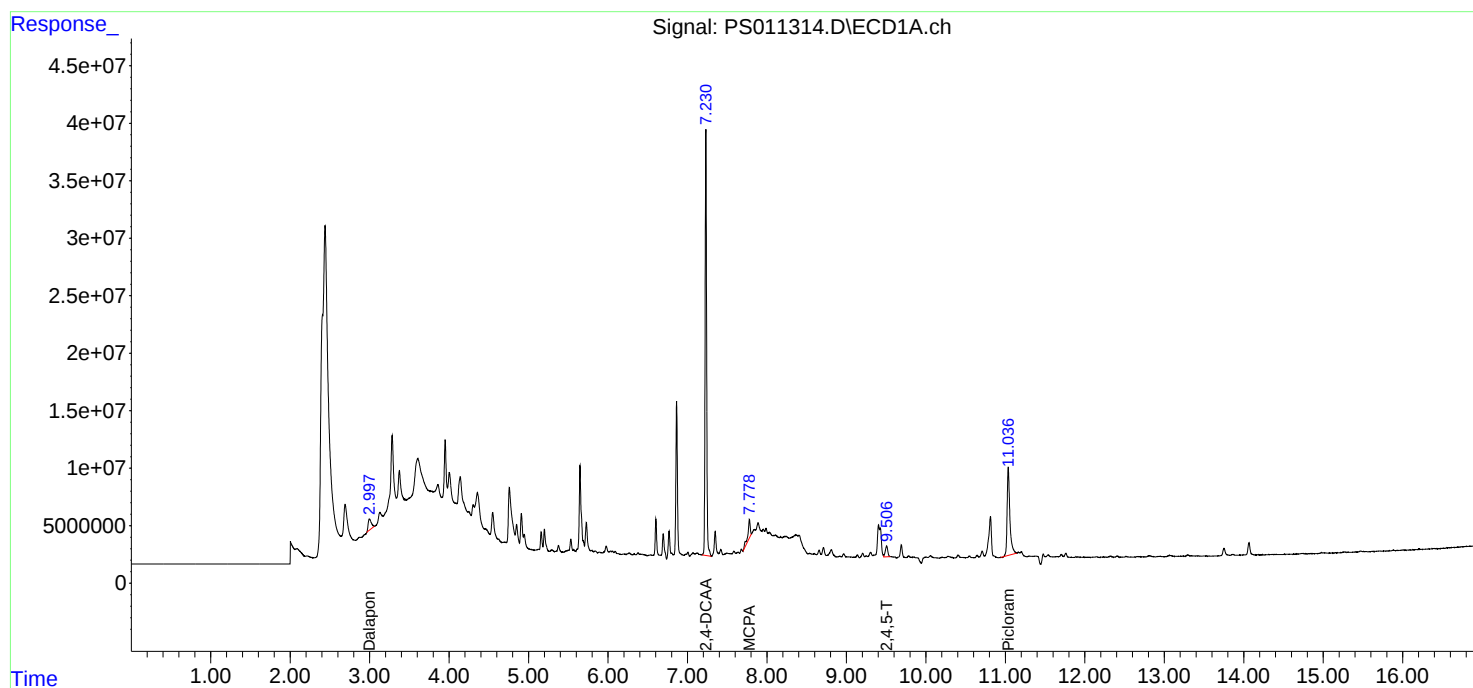


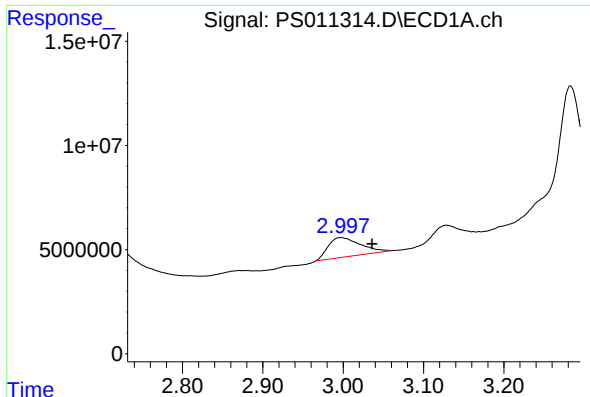

#1 Dalapon


R.T.: 2.997 min
Delta R.T.: -0.039 min
Response: 26315196
Conc: 21.87 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB130341BL

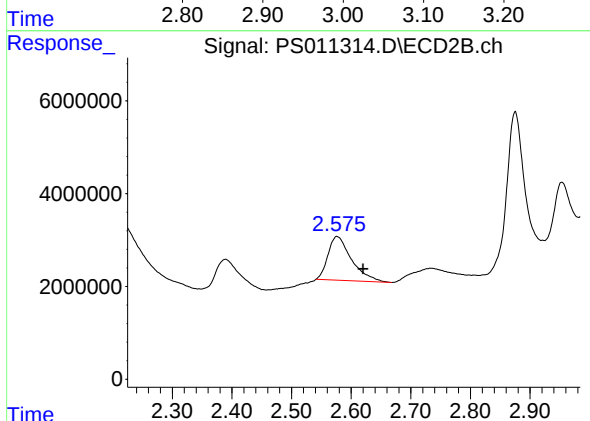


#1 Dalapon

R.T.: 2.577 min
Delta R.T.: -0.044 min
Response: 25789442
Conc: 33.59 ng/ml

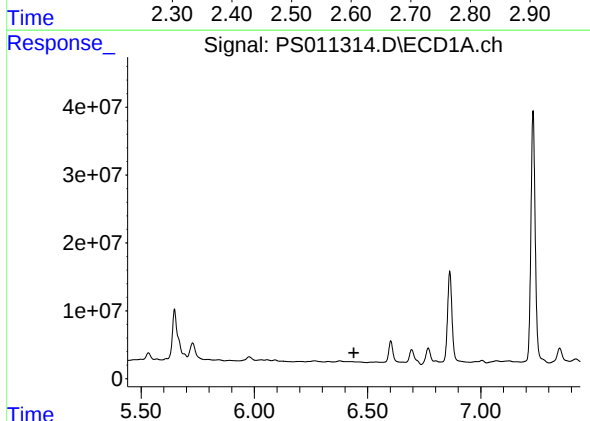


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.439 min
Response: 0
Conc: N.D.

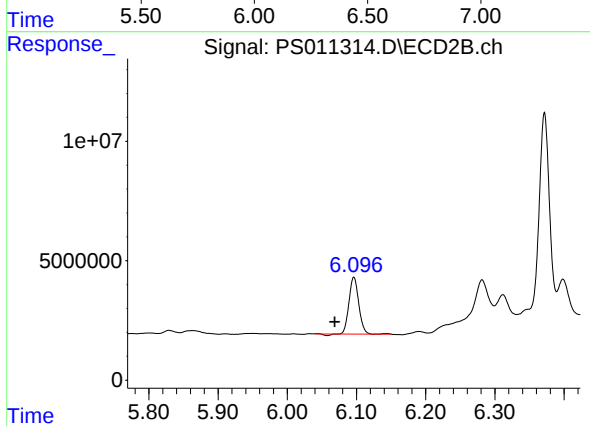

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.096 min
Delta R.T.: 0.028 min
Response: 23187917
Conc: 27.61 ng/ml

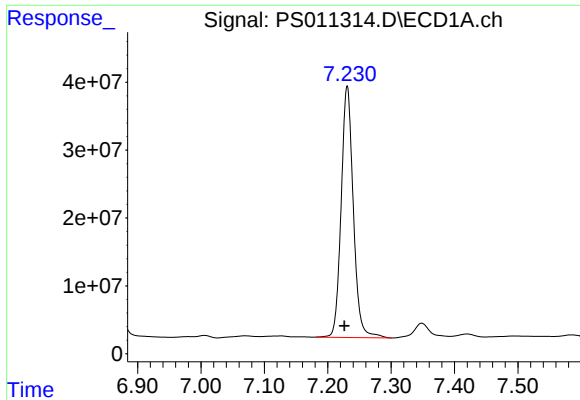

#4 2,4-DCAA


R.T.: 7.231 min
Delta R.T.: 0.004 min
Response: 493147783
Conc: 508.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB130341BL

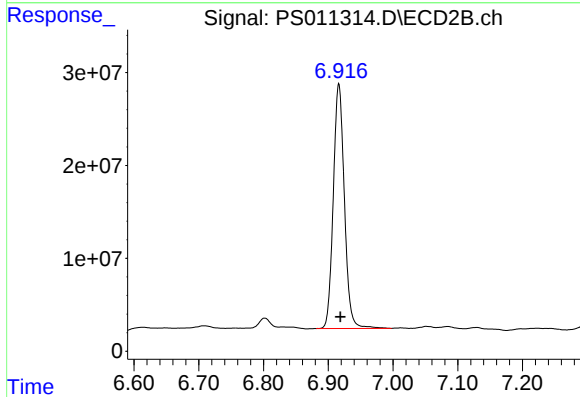


#4 2,4-DCAA

R.T.: 6.916 min
Delta R.T.: -0.002 min
Response: 313524358
Conc: 556.86 ng/ml

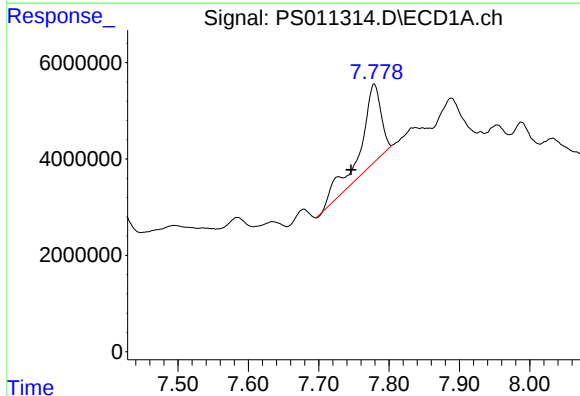


#7 MCPA

R.T.: 7.779 min
Delta R.T.: 0.033 min
Response: 33480489
Conc: 7.85 ug/ml

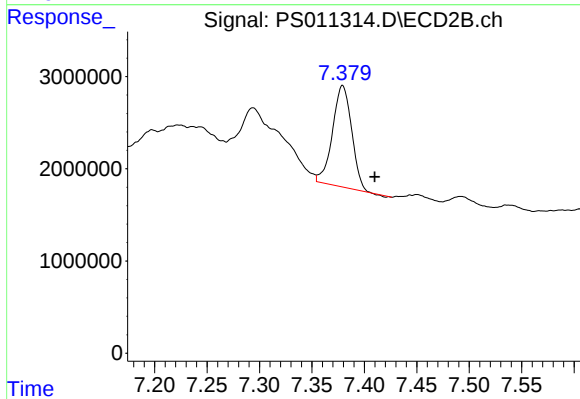

#7 MCPA


R.T.: 7.379 min
Delta R.T.: -0.031 min
Response: 13989808
Conc: 4.85 ug/ml

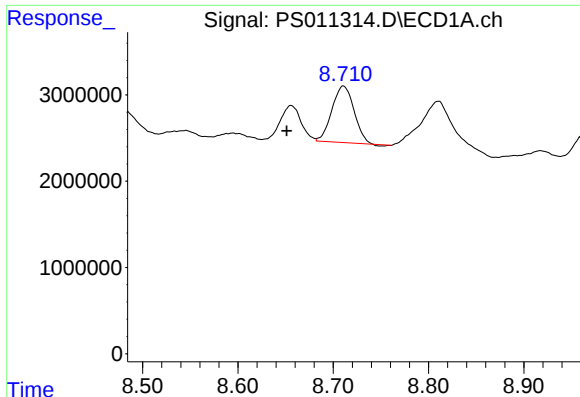

#10 Pentachlorophenol


R.T.: 8.711 min
Delta R.T.: 0.059 min
Response: 10461527
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB130341BL

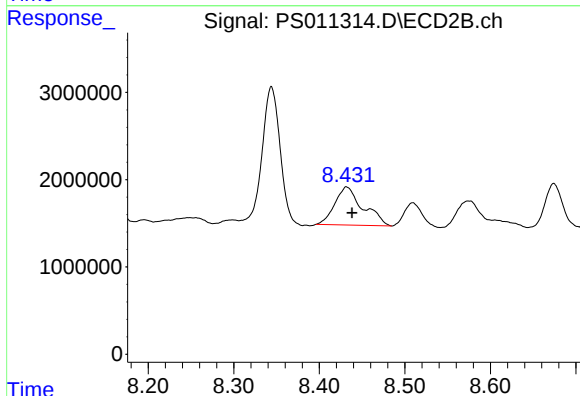


#10 Pentachlorophenol

R.T.: 8.432 min
Delta R.T.: -0.006 min
Response: 9953882
Conc: 1.43 ng/ml

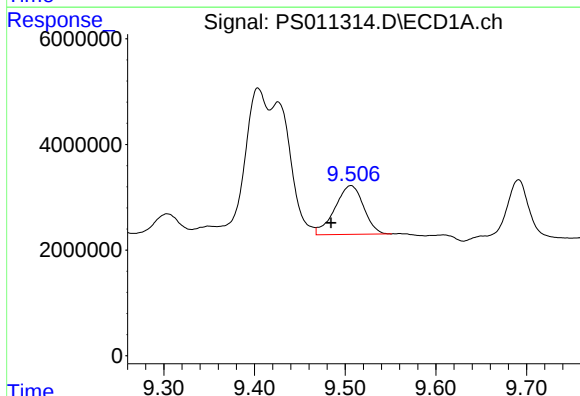


#12 2,4,5-T

R.T.: 9.506 min
Delta R.T.: 0.022 min
Response: 20371349
Conc: 4.04 ng/ml

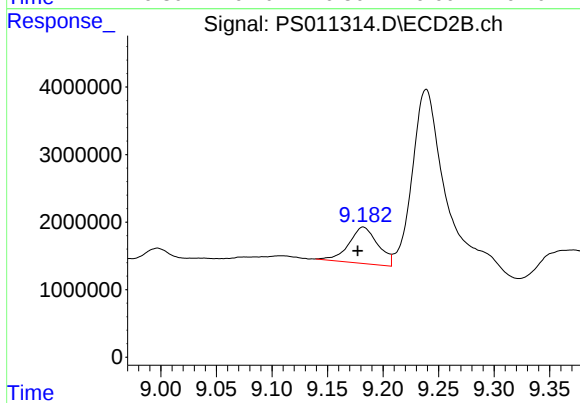

#12 2,4,5-T


R.T.: 9.182 min
Delta R.T.: 0.005 min
Response: 9856512
Conc: 3.25 ng/ml

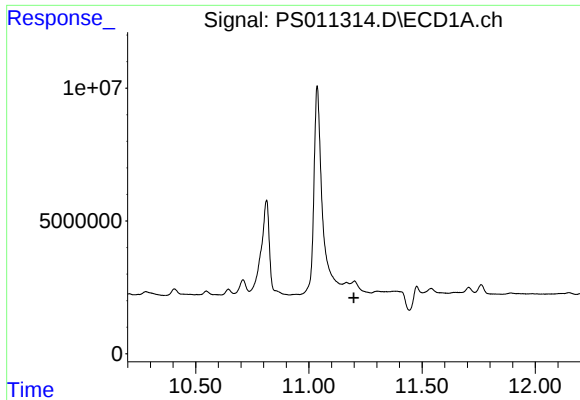

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.199 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB130341BL

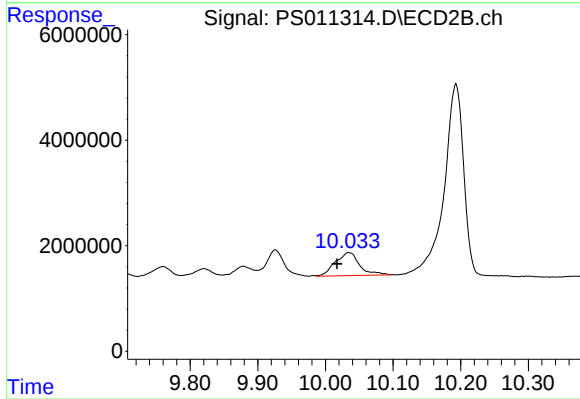


#14 DINOSEB

R.T.: 10.035 min
Delta R.T.: 0.018 min
Response: 10805160
Conc: 5.04 ng/ml

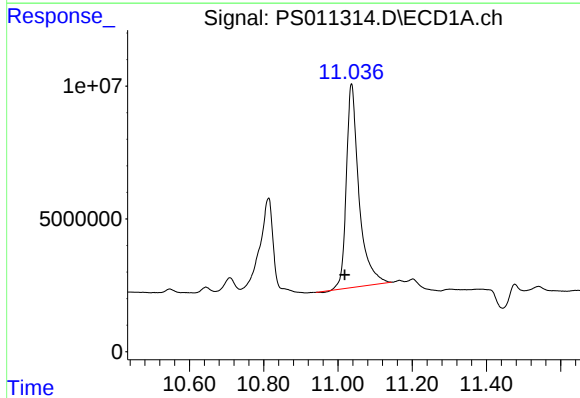


#15 Picloram

R.T.: 11.037 min
Delta R.T.: 0.018 min
Response: 181481268
Conc: 28.76 ng/ml

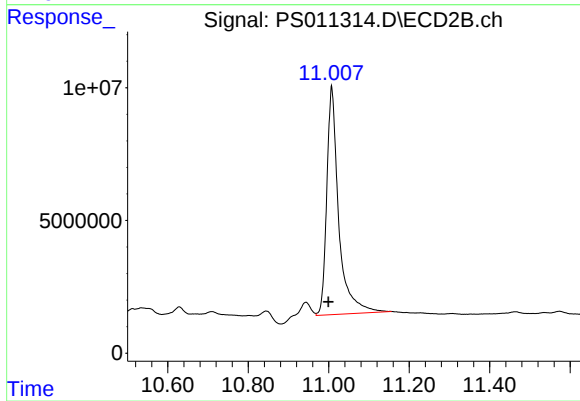

#15 Picloram


R.T.: 11.007 min
Delta R.T.: 0.008 min
Response: 177210412
Conc: 40.52 ng/ml

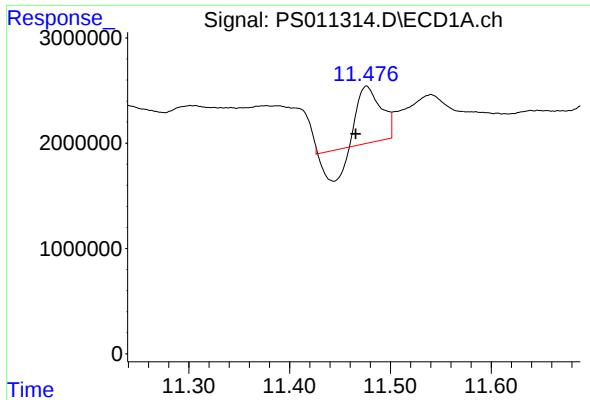

#16 DCPA

R.T.: 11.477 min
Delta R.T.: 0.011 min
Response: 5783628
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB130341BL

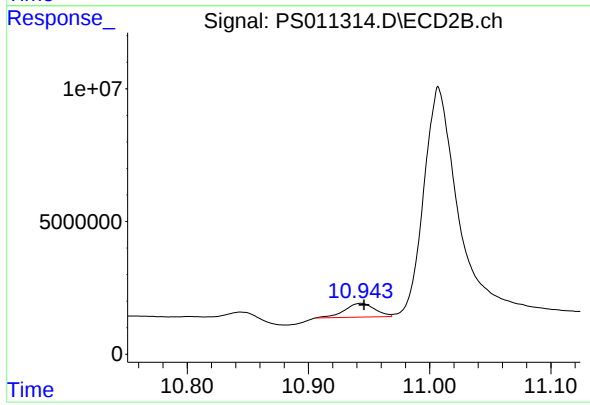

#16 DCPA

R.T.: 10.943 min
Delta R.T.: -0.003 min
Response: 9005811
Conc: 2.38 ng/ml