

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072220\
 Data File : PS011323.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2020 17:29
 Operator : DD\AJ
 Sample : L3360-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 02:46:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.225	6.918	287.2E6	180.8E6	295.937	321.142
Target Compounds							
1) T	Dalapon	2.996	0.000	25942749	0	21.558	N.D. #
2) T	3,5-DICHL...	0.000	6.098	0	53301706	N.D.	63.466
3) T	4-Nitroph...	7.060	6.529	10995202	8991159	24.941	27.422
6) T	MCP	7.581	0.000	9716031	0	3.209	N.D. #
7) T	MCPA	7.774	7.380	19602715	46240344	4.596	16.043 #
10) T	Pentachlo...	8.647	8.434	13312624	21886888	1.007	3.140 #
12) T	2,4,5-T	9.504	9.167	12236693	10101009	2.425	3.330 #
13) T	2,4-DB	9.987	9.687	7650584	16427701	11.870	38.428 #
14) T	DINOSEB	11.192	10.033	38463032	63568348	9.978	29.637 #
15) T	Picloram	10.991	11.024	30334036	15739779	4.807	3.599 #
16) T	DCPA	11.532	0.000	26914070	0	4.177	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072220\
Data File : PS011323.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2020 17:29
Operator : DD\AJ
Sample : L3360-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 02:46:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
Quant Title : 8080.M
QLast Update : Mon Jul 13 16:10:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

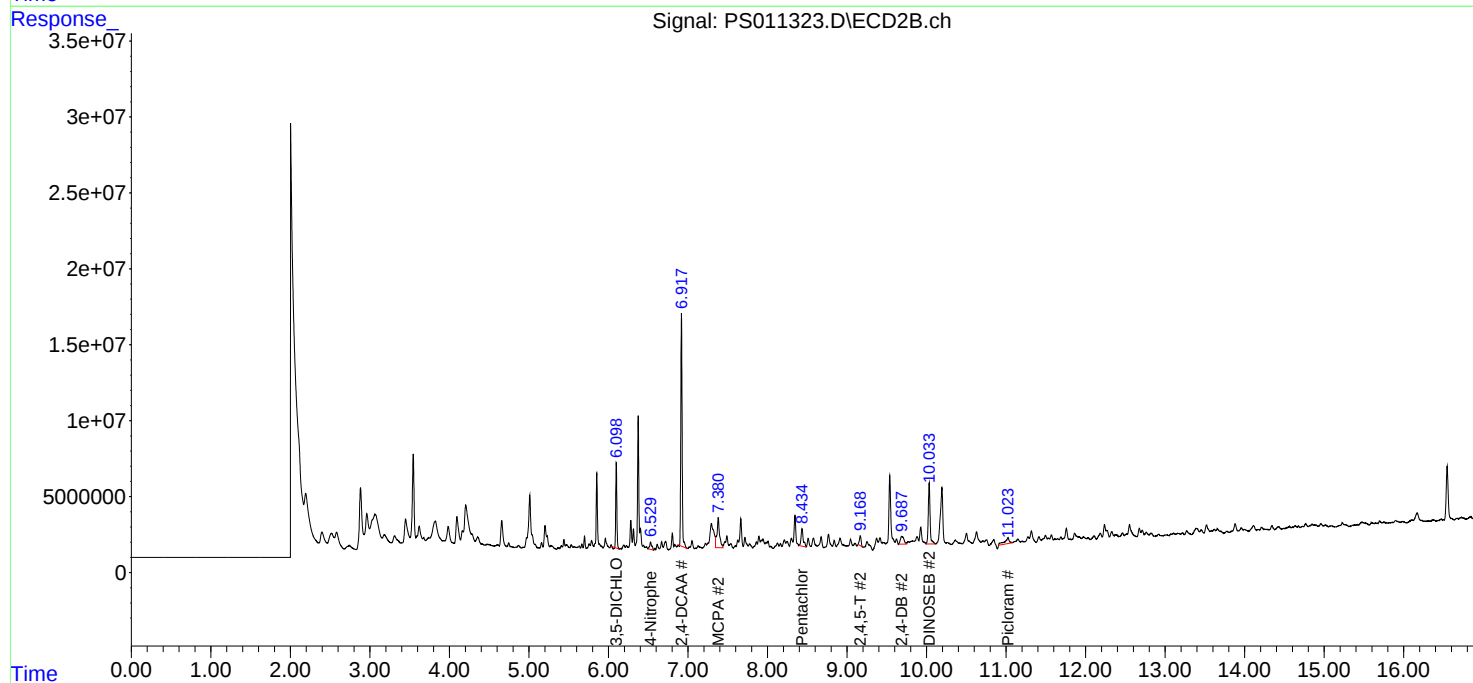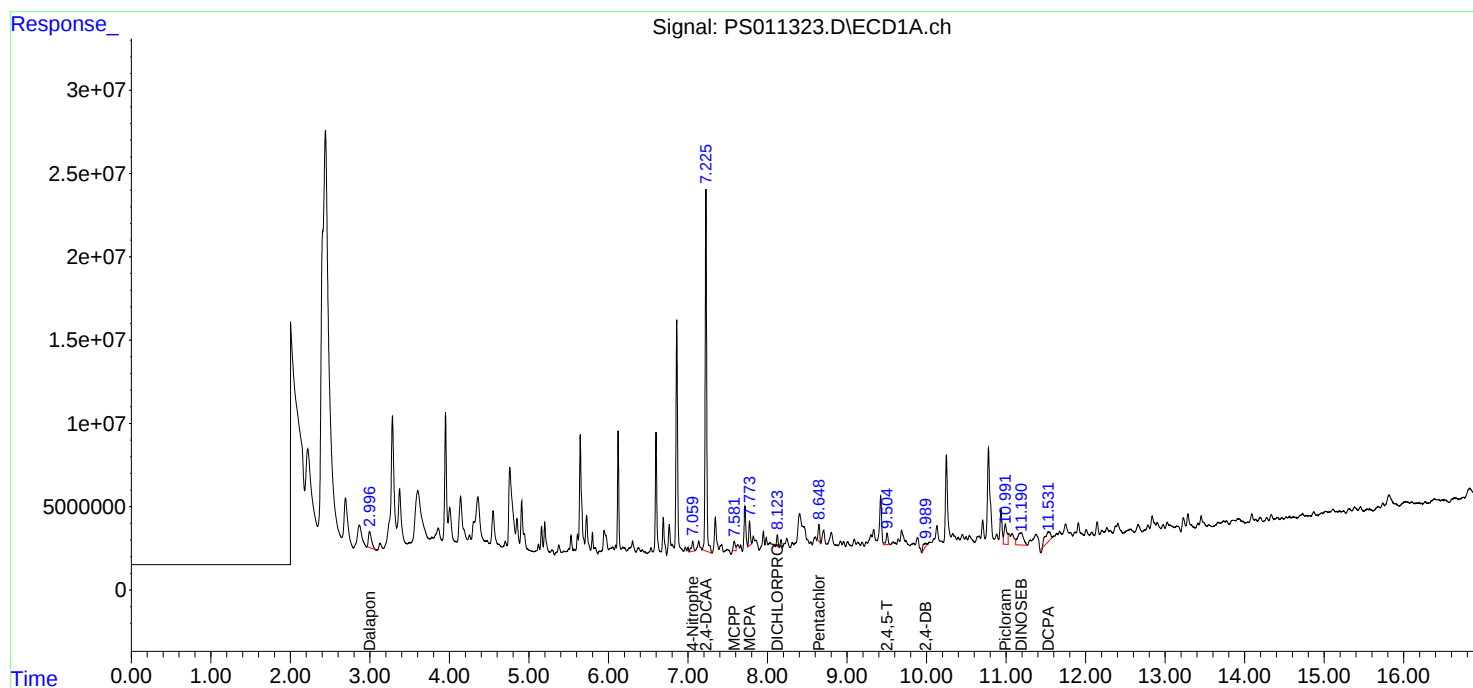


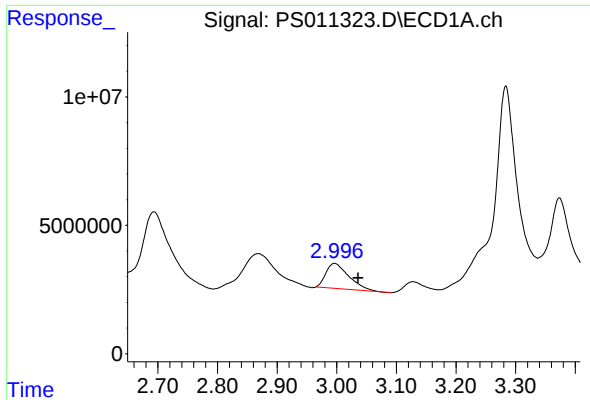

#1 Dalapon


R.T.: 2.996 min
Delta R.T.: -0.040 min
Response: 25942749
Conc: 21.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

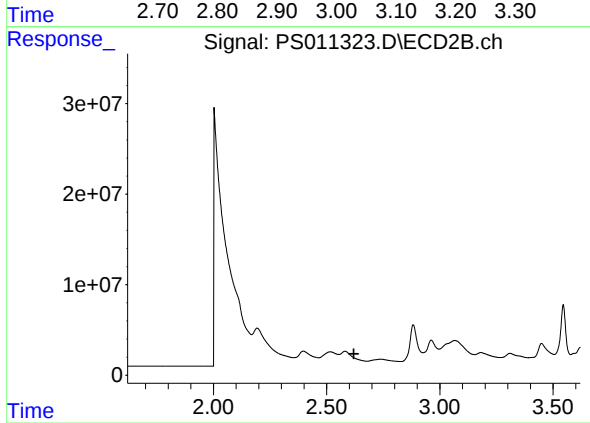


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.620 min
Response: 0
Conc: N.D.

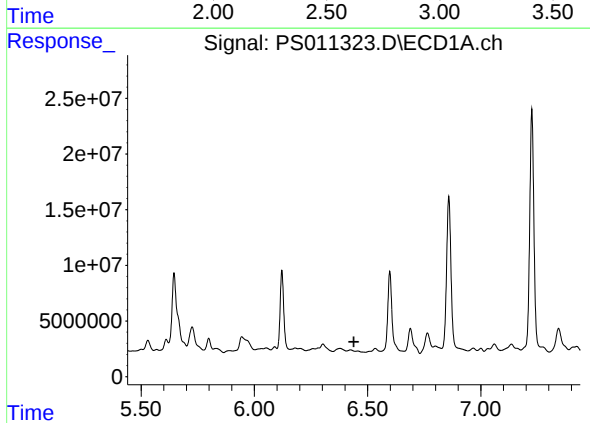


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.439 min
Response: 0
Conc: N.D.

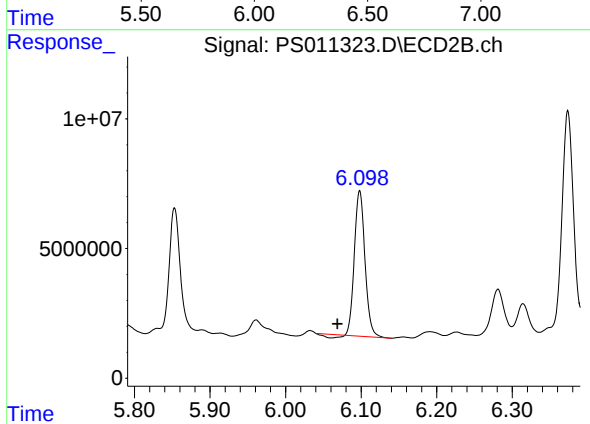

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.098 min
Delta R.T.: 0.030 min
Response: 53301706
Conc: 63.47 ng/ml

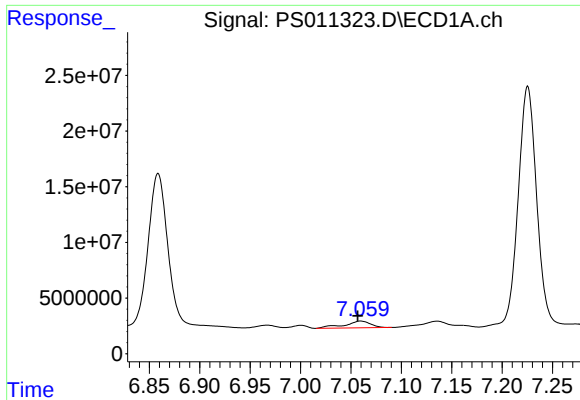

#3 4-Nitrophenol


R.T.: 7.060 min
Delta R.T.: 0.003 min
Response: 10995202
Conc: 24.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

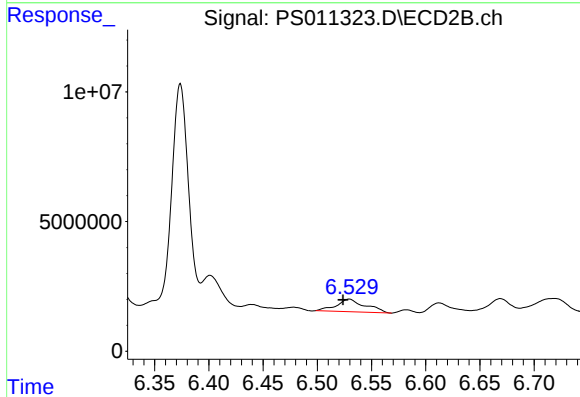


#3 4-Nitrophenol

R.T.: 6.529 min
Delta R.T.: 0.006 min
Response: 8991159
Conc: 27.42 ng/ml

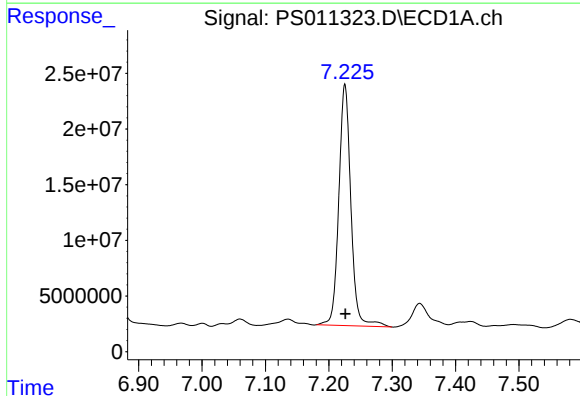


#4 2,4-DCAA

R.T.: 7.225 min
Delta R.T.: 0.000 min
Response: 287158466
Conc: 295.94 ng/ml

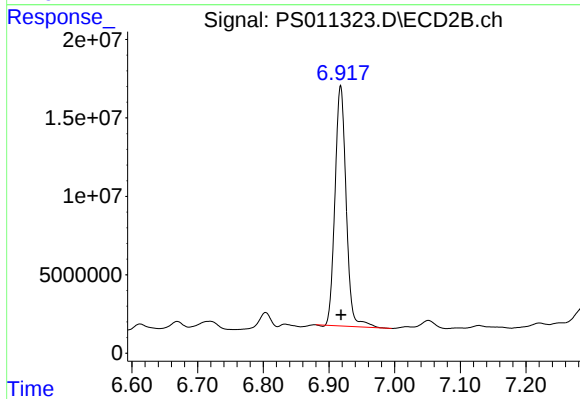

#4 2,4-DCAA


R.T.: 6.918 min
Delta R.T.: 0.000 min
Response: 180810149
Conc: 321.14 ng/ml

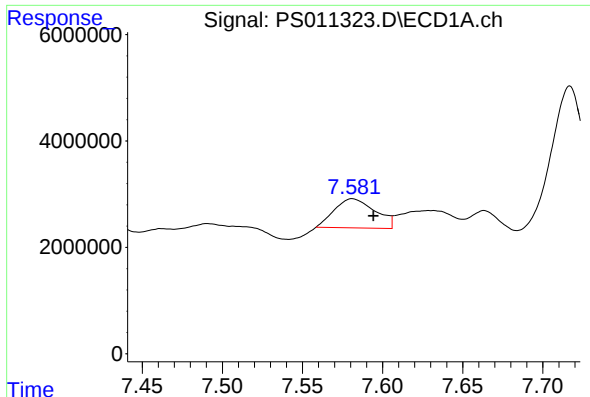

#6 MCPP


R.T.: 7.581 min
Delta R.T.: -0.013 min
Response: 9716031
Conc: 3.21 ug/ml

Instrument :
ECD_S
ClientSampleId :

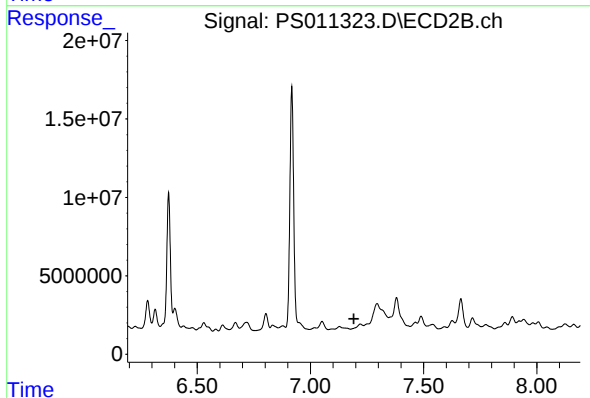


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.192 min
Response: 0
Conc: N.D.

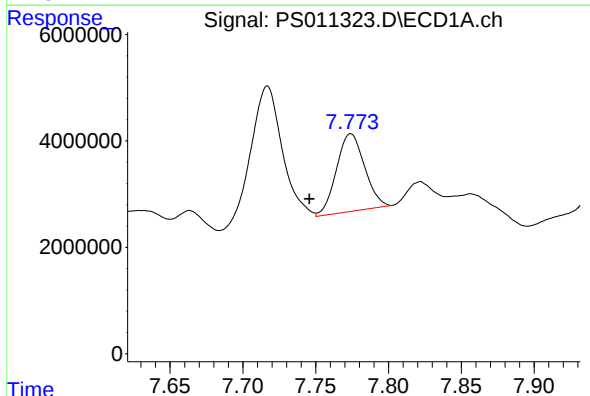


#7 MCPA

R.T.: 7.774 min
Delta R.T.: 0.028 min
Response: 19602715
Conc: 4.60 ug/ml

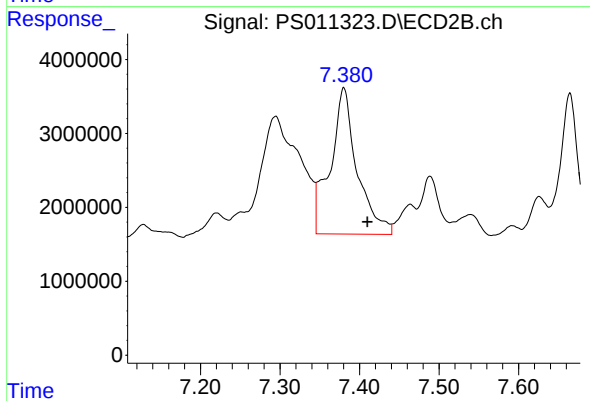

#7 MCPA


R.T.: 7.380 min
Delta R.T.: -0.030 min
Response: 46240344
Conc: 16.04 ug/ml

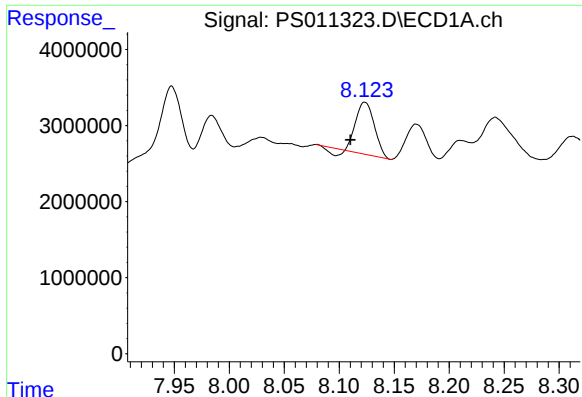

#8 DICHLORPROP


R.T.: 8.123 min
Delta R.T.: 0.013 min
Response: 7425282
Conc: 7.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

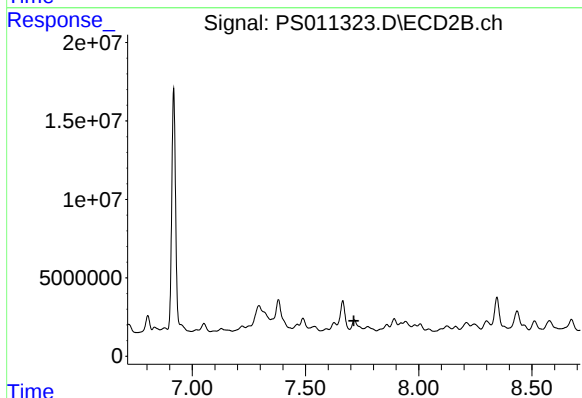


#8 DICHLORPROP

R.T.: 7.716 min
Delta R.T.: 0.002 min
Response: -9213077
Conc: N.D.

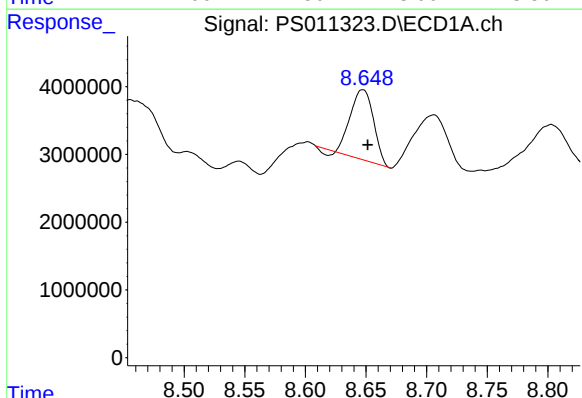


#10 Pentachlorophenol

R.T.: 8.647 min
Delta R.T.: -0.004 min
Response: 13312624
Conc: 1.01 ng/ml

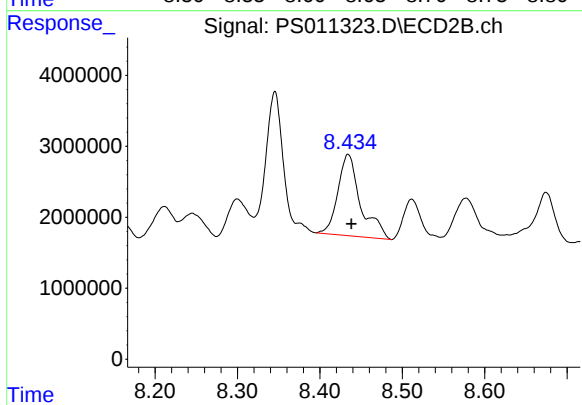

#10 Pentachlorophenol


R.T.: 8.434 min
Delta R.T.: -0.004 min
Response: 21886888
Conc: 3.14 ng/ml

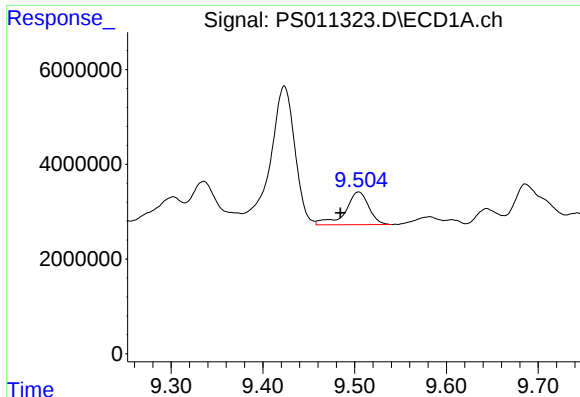

#12 2,4,5-T


R.T.: 9.504 min
Delta R.T.: 0.020 min
Response: 12236693
Conc: 2.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

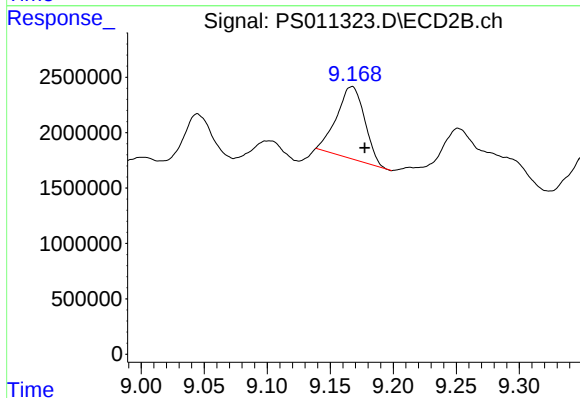


#12 2,4,5-T

R.T.: 9.167 min
Delta R.T.: -0.010 min
Response: 10101009
Conc: 3.33 ng/ml

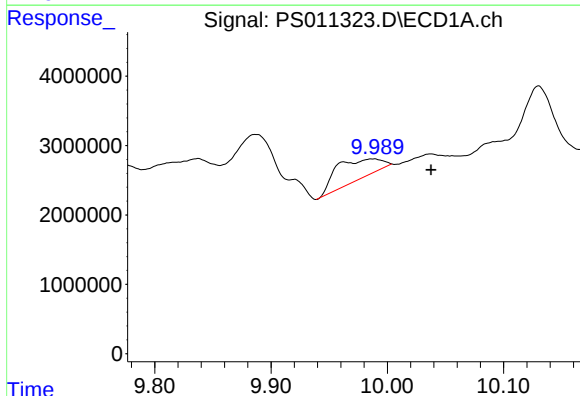


#13 2,4-DB

R.T.: 9.987 min
Delta R.T.: -0.050 min
Response: 7650584
Conc: 11.87 ng/ml

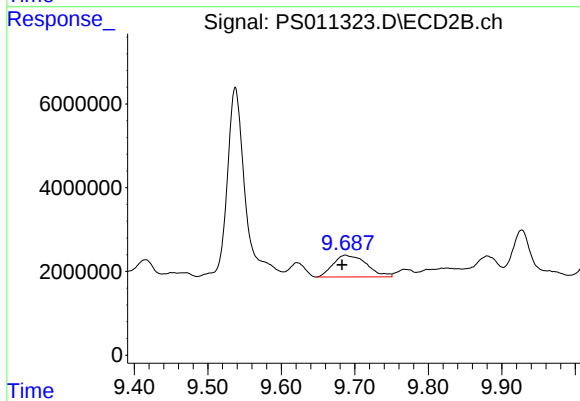

#13 2,4-DB


R.T.: 9.687 min
Delta R.T.: 0.004 min
Response: 16427701
Conc: 38.43 ng/ml

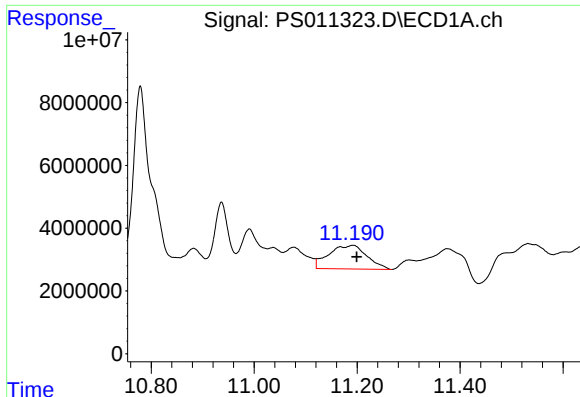

#14 DINOSEB


R.T.: 11.192 min
Delta R.T.: -0.007 min
Response: 38463032
Conc: 9.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

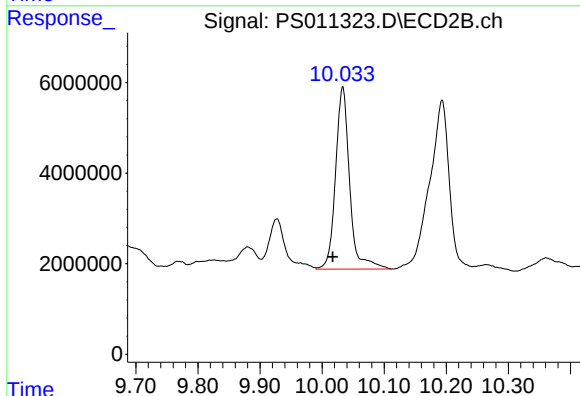


#14 DINOSEB

R.T.: 10.033 min
Delta R.T.: 0.016 min
Response: 63568348
Conc: 29.64 ng/ml

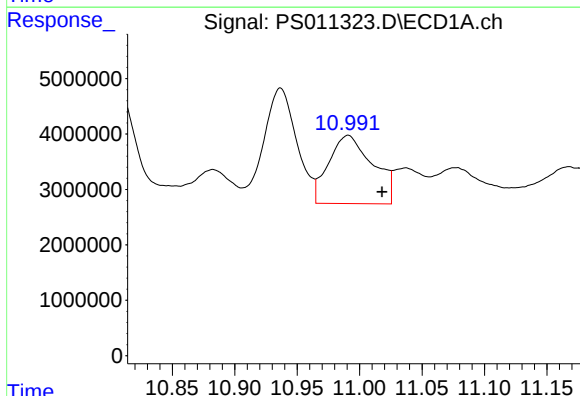


#15 Picloram

R.T.: 10.991 min
Delta R.T.: -0.027 min
Response: 30334036
Conc: 4.81 ng/ml

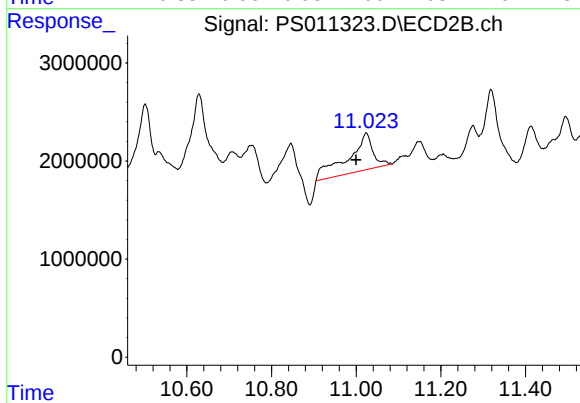

#15 Picloram


R.T.: 11.024 min
Delta R.T.: 0.024 min
Response: 15739779
Conc: 3.60 ng/ml

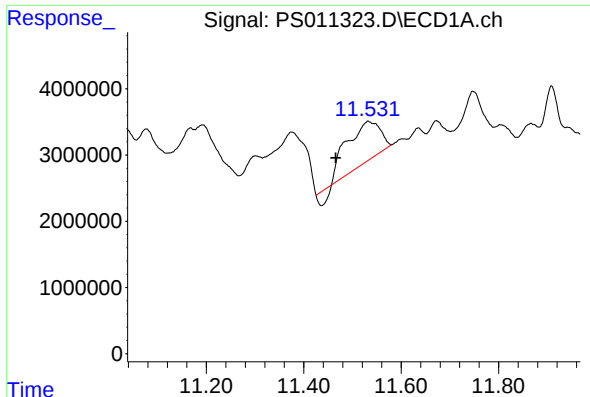

#16 DCPA

R.T.: 11.532 min
Delta R.T.: 0.067 min
Response: 26914070
Conc: 4.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

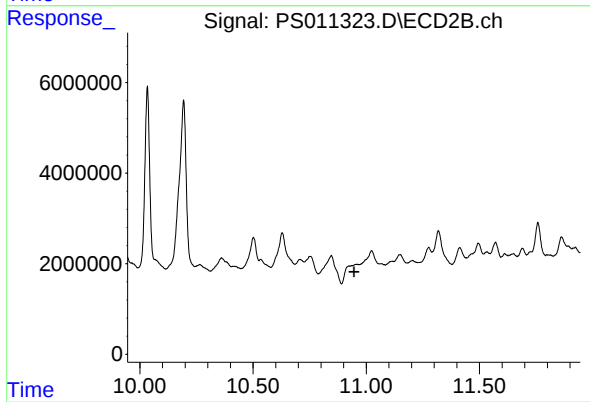

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.946 min
Response: 0
Conc: N.D.