

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072220\
 Data File : PS011328.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2020 19:24
 Operator : DD\AJ
 Sample : PB130394BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB130394BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 02:47:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.225	6.917	455.1E6	296.3E6	469.047	526.298
Target Compounds							
1) T	Dalapon	2.995	2.583	36869075	64847442	30.638	84.473 #
2) T	3,5-DICHL...	0.000	6.098	0	30945585	N.D.	36.847
3) T	4-Nitroph...	7.000	0.000	9851383	0	22.347	N.D. #
7) T	MCPA	7.773	7.380	21420322	27504230	5.023	9.542 #
10) T	Pentachlo...	8.704	0.000	12694845	0	<MDL	N.D. #
12) T	2,4,5-T	9.504	0.000	8597434	0	1.704	N.D. #
13) T	2,4-DB	0.000	9.623	0	8022406	N.D.	18.766
14) T	DINOSEB	0.000	10.034	0	6896344	N.D.	3.215
16) T	DCPA	11.532	0.000	11691609	0	1.815	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072220\
Data File : PS011328.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2020 19:24
Operator : DD\AJ
Sample : PB130394BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
PB130394BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 02:47:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
Quant Title : 8080.M
QLast Update : Mon Jul 13 16:10:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

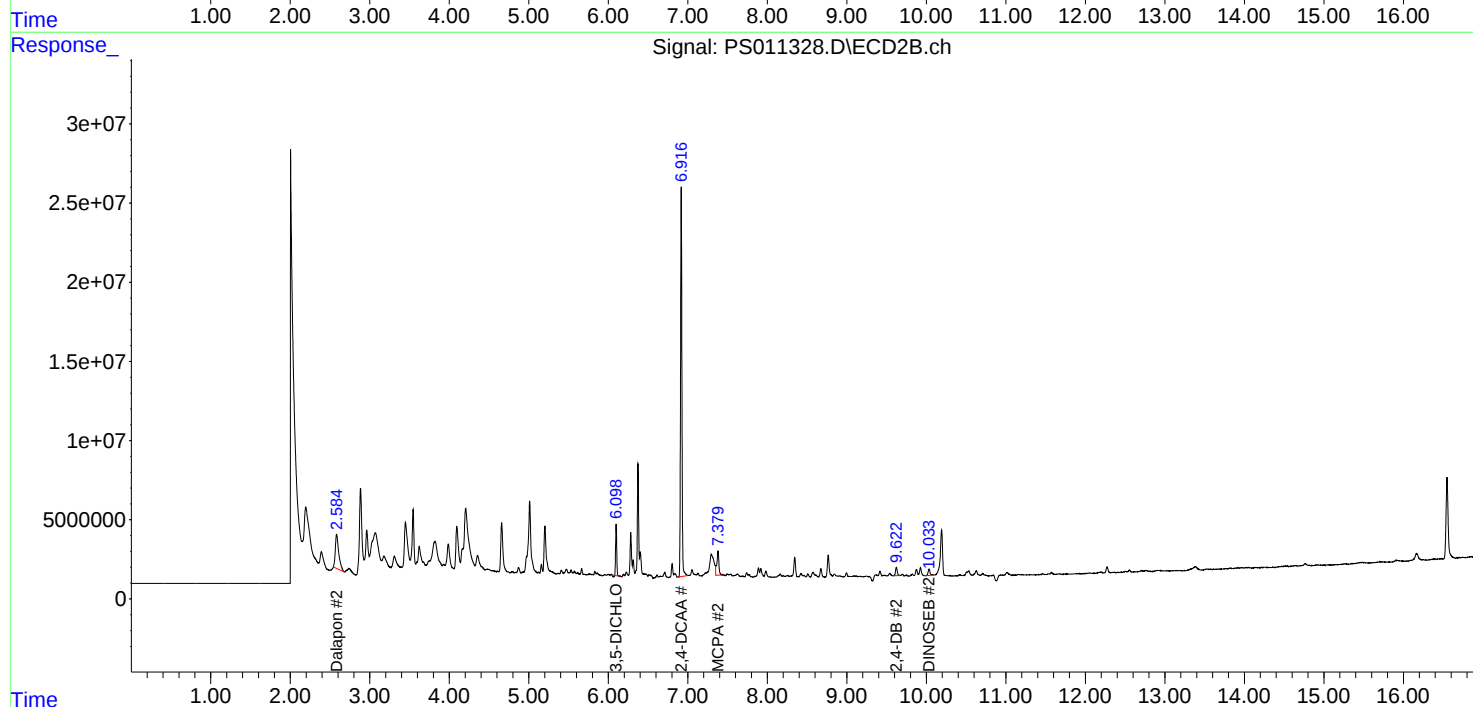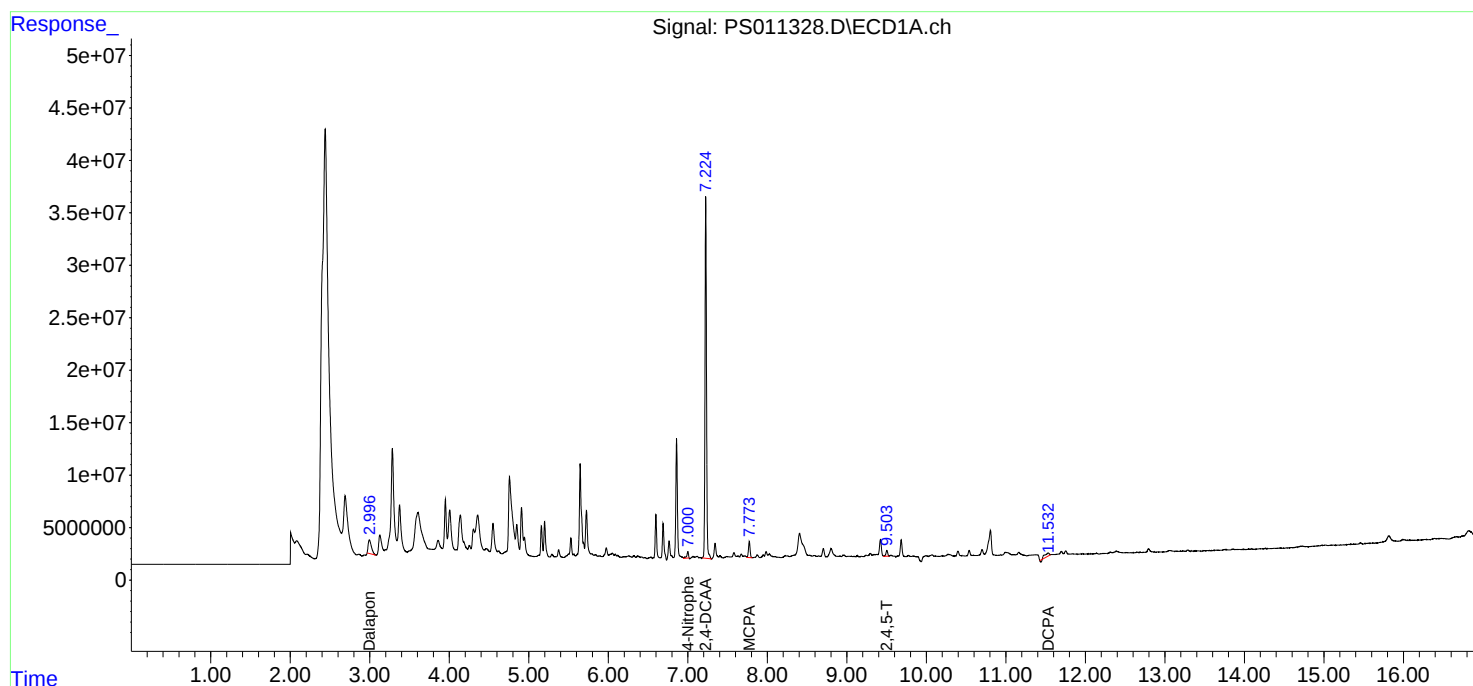


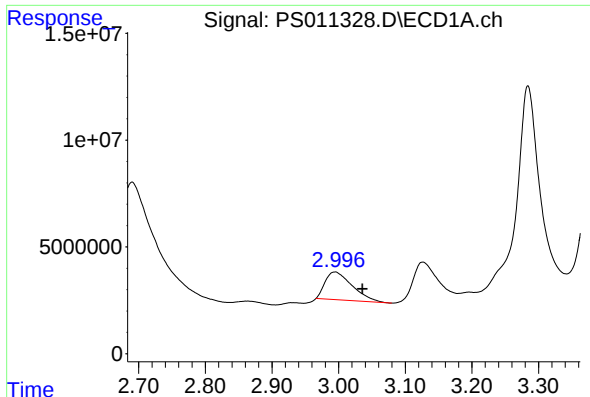

#1 Dalapon


R.T.: 2.995 min
Delta R.T.: -0.041 min
Response: 36869075
Conc: 30.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB130394BL

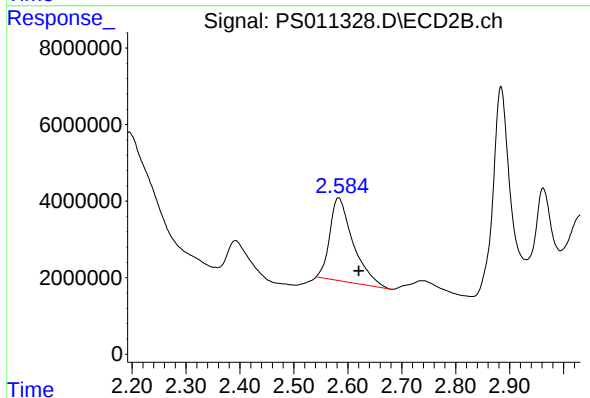


#1 Dalapon

R.T.: 2.583 min
Delta R.T.: -0.038 min
Response: 64847442
Conc: 84.47 ng/ml

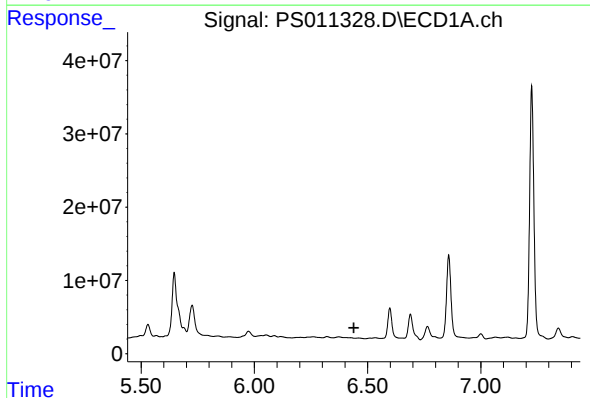


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.439 min
Response: 0
Conc: N.D.

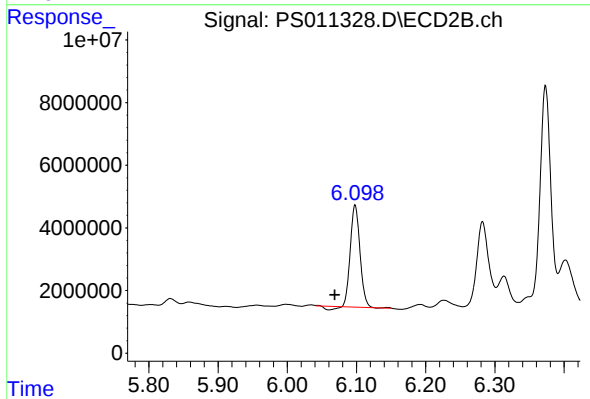

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.098 min
Delta R.T.: 0.030 min
Response: 30945585
Conc: 36.85 ng/ml

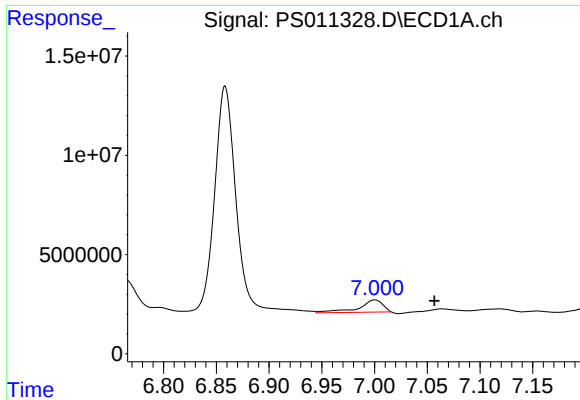

#3 4-Nitrophenol


R.T.: 7.000 min

Delta R.T.: -0.057 min

Response: 9851383

Conc: 22.35 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB130394BL

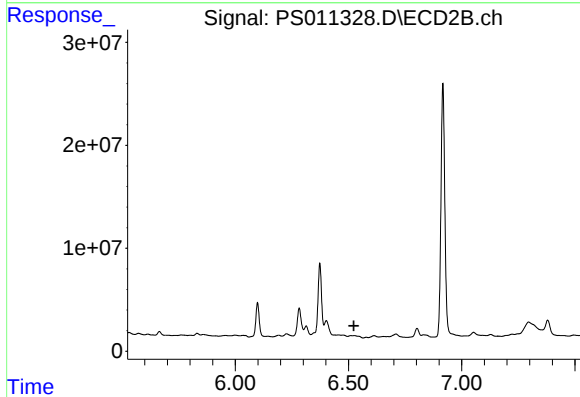


#3 4-Nitrophenol

R.T.: 0.000 min

Exp R.T. : 6.524 min

Response: 0

Conc: N.D.

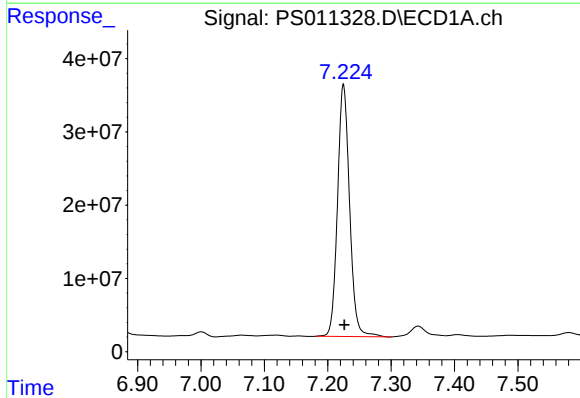


#4 2,4-DCAA

R.T.: 7.225 min

Delta R.T.: -0.002 min

Response: 455134254

Conc: 469.05 ng/ml

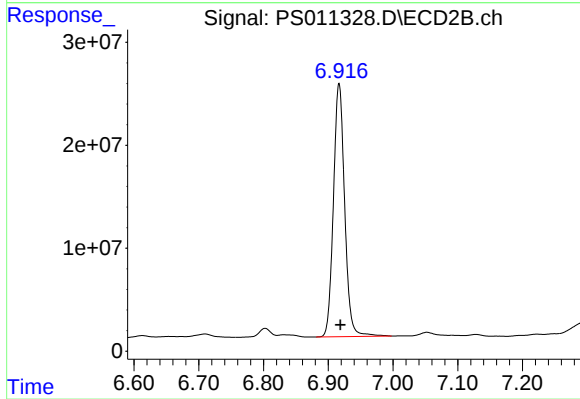


#4 2,4-DCAA

R.T.: 6.917 min

Delta R.T.: -0.002 min

Response: 296317509


Conc: 526.30 ng/ml

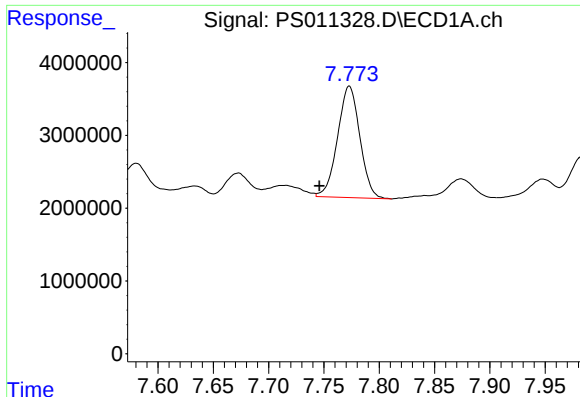

#7 MCPA


R.T.: 7.773 min
Delta R.T.: 0.027 min
Response: 21420322
Conc: 5.02 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB130394BL

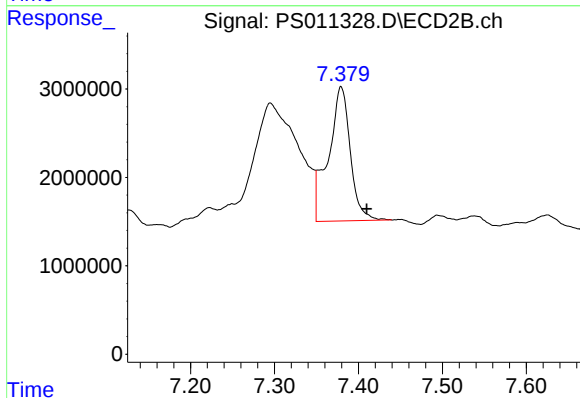


#7 MCPA

R.T.: 7.380 min
Delta R.T.: -0.030 min
Response: 27504230
Conc: 9.54 ug/ml

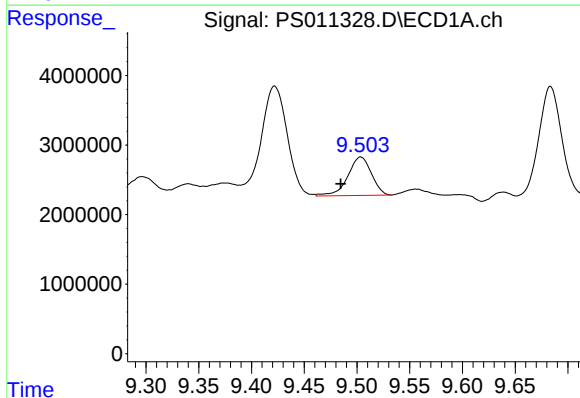


#12 2,4,5-T

R.T.: 9.504 min
Delta R.T.: 0.019 min
Response: 8597434
Conc: 1.70 ng/ml

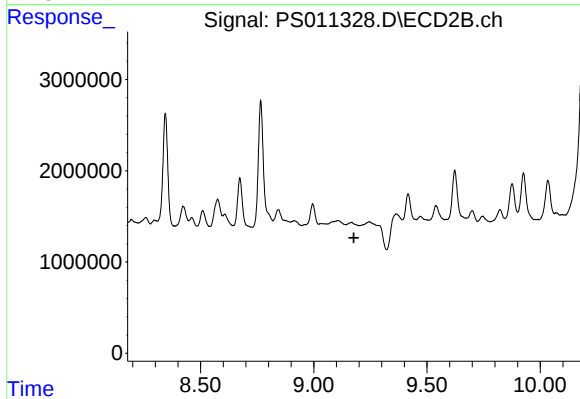

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.177 min
Response: 0
Conc: N.D.

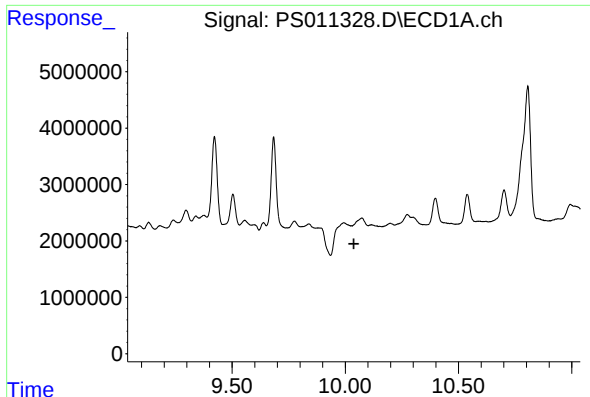

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.038 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB130394BL

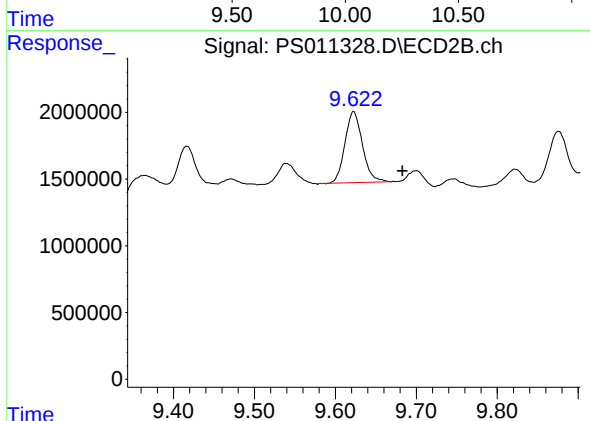


#13 2,4-DB

R.T.: 9.623 min
Delta R.T.: -0.060 min
Response: 8022406
Conc: 18.77 ng/ml

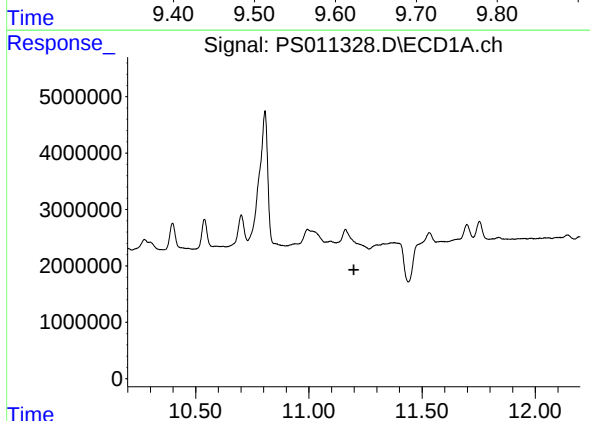


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.199 min
Response: 0
Conc: N.D.

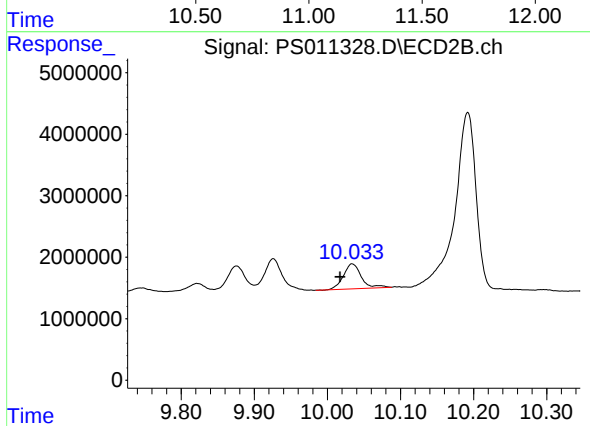

#14 DINOSEB


R.T.: 10.034 min
Delta R.T.: 0.017 min
Response: 6896344
Conc: 3.22 ng/ml

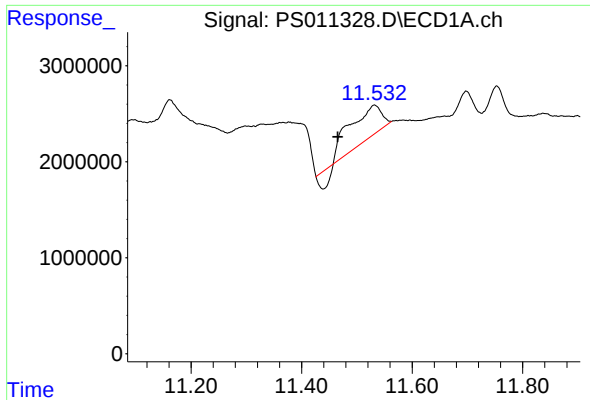

#16 DCPA

R.T.: 11.532 min
Delta R.T.: 0.066 min
Response: 11691609
Conc: 1.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB130394BL

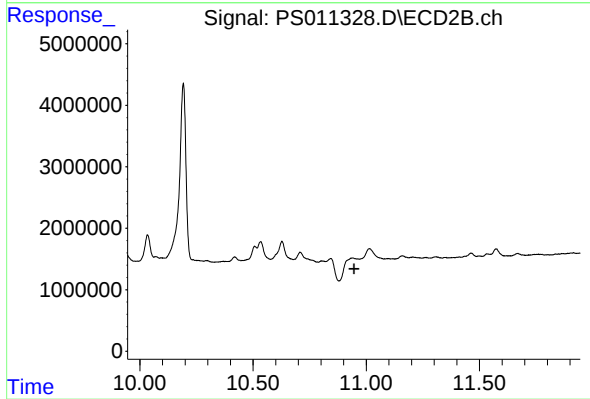

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.946 min
Response: 0
Conc: N.D.