

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072220\
 Data File : PS011330.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2020 20:10
 Operator : DD\AJ
 Sample : PB130394TB
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB130394TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 02:48:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.225	6.917	289.6E6	196.3E6	298.415	348.728
Target Compounds							
1) T	Dalapon	2.996	2.584	39016907	56256850	32.423	73.282 #
2) T	3,5-DICHL...	0.000	6.098	0	83377308	N.D.	99.277
3) T	4-Nitroph...	6.996	0.000	6001633	0	13.614	N.D. #
5) T	DICAMBA	7.405	7.052	9522807	5124180	2.457	2.238
6) T	MCPD	7.636	0.000	6771057	0	2.236	N.D. #
7) T	MCPA	7.691	7.464	115.4E6	96367850	27.056	33.434
10) T	Pentachlo...	8.704	8.430	9918136	8298858	<MDL	1.191 #
12) T	2,4,5-T	9.422	0.000	49244538	0	9.759	N.D. #
13) T	2,4-DB	0.000	9.622	0	8089054	N.D.	18.922
15) T	Picloram	11.023	0.000	21112554	0	3.346	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072220\
Data File : PS011330.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2020 20:10
Operator : DD\AJ
Sample : PB130394TB
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
PB130394TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 02:48:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
Quant Title : 8080.M
QLast Update : Mon Jul 13 16:10:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

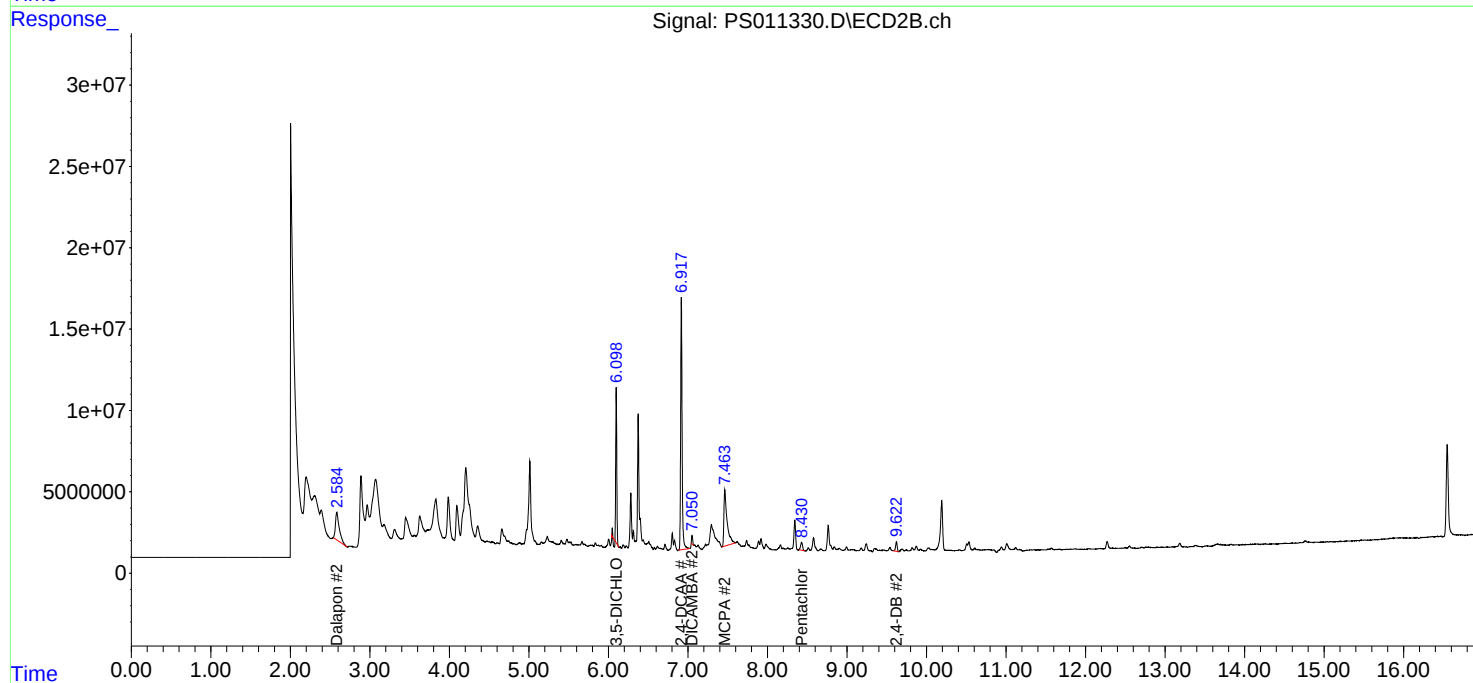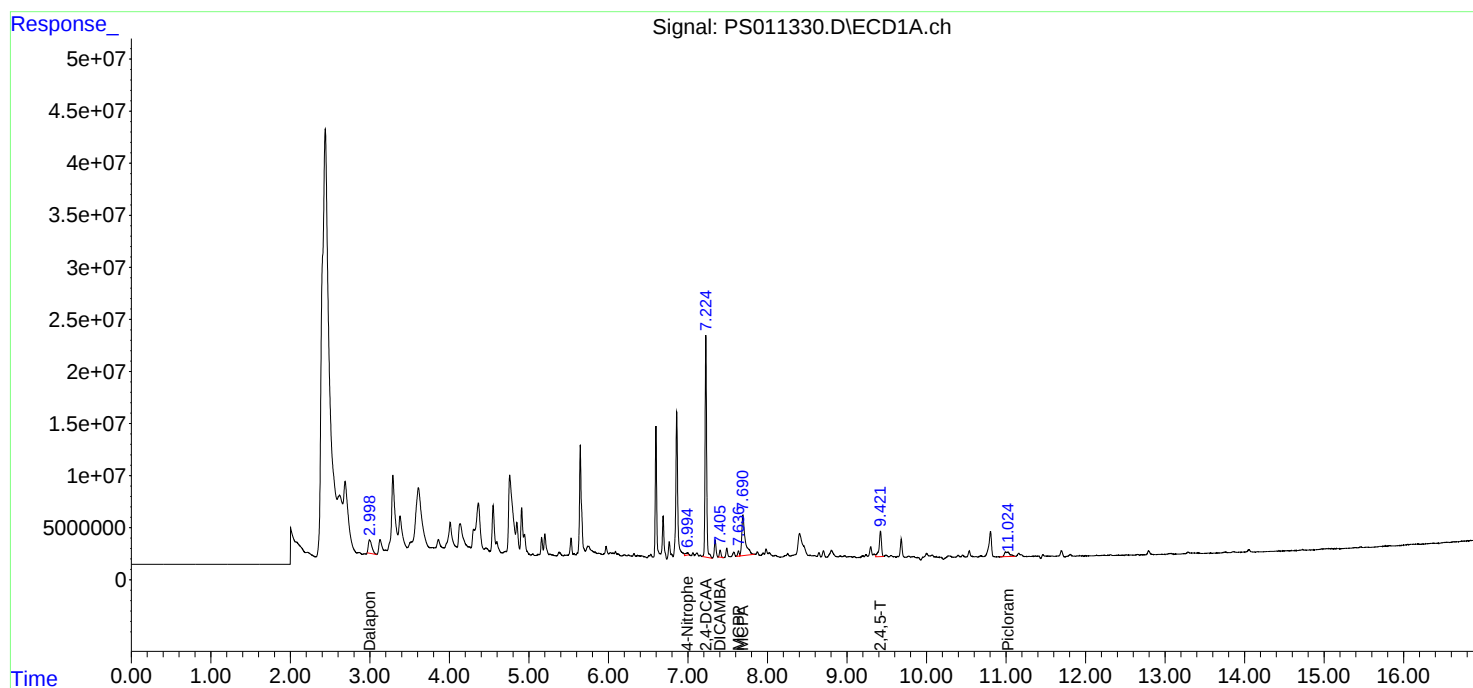


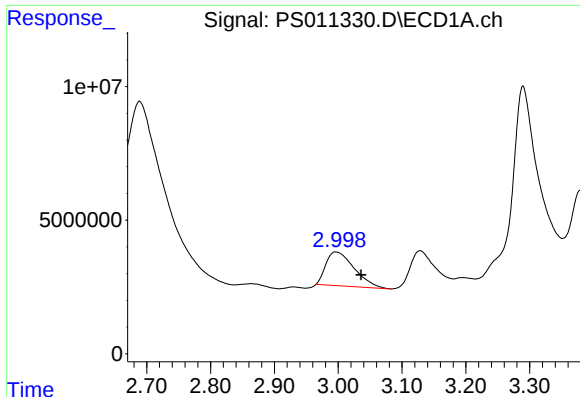

#1 Dalapon


R.T.: 2.996 min
Delta R.T.: -0.040 min
Response: 39016907
Conc: 32.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB130394TB

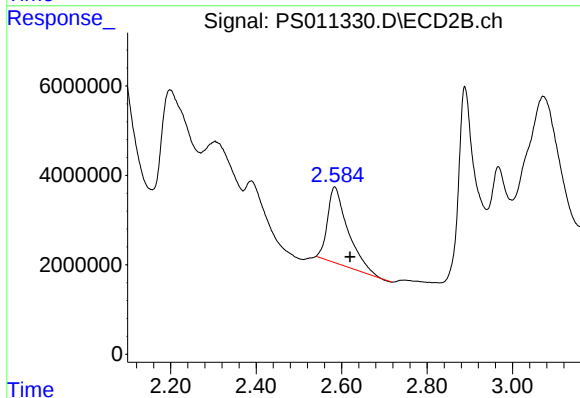


#1 Dalapon

R.T.: 2.584 min
Delta R.T.: -0.036 min
Response: 56256850
Conc: 73.28 ng/ml

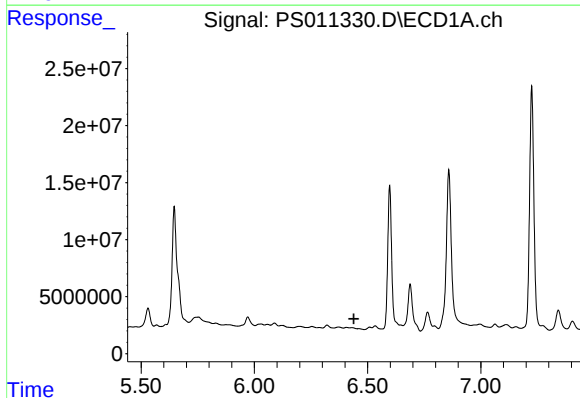


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.439 min
Response: 0
Conc: N.D.

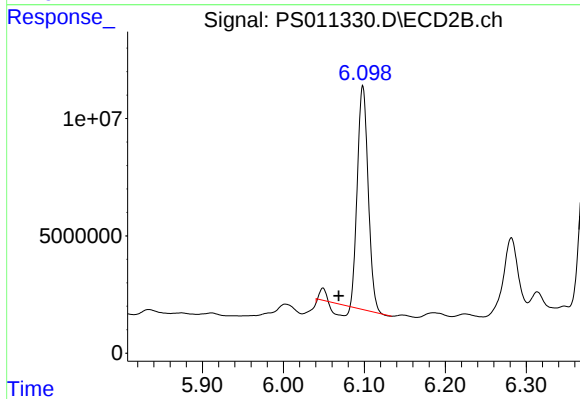

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.098 min
Delta R.T.: 0.030 min
Response: 83377308
Conc: 99.28 ng/ml

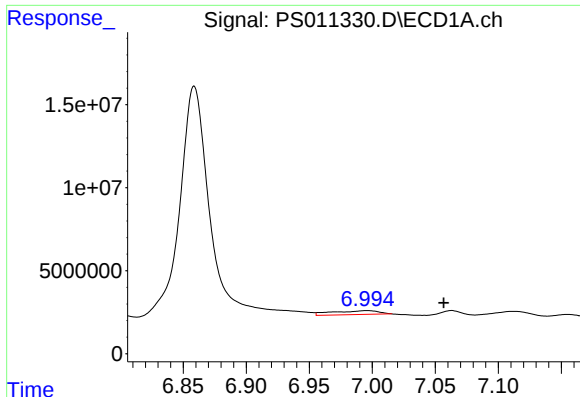

#3 4-Nitrophenol


R.T.: 6.996 min
Delta R.T.: -0.061 min
Response: 6001633
Conc: 13.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB130394TB

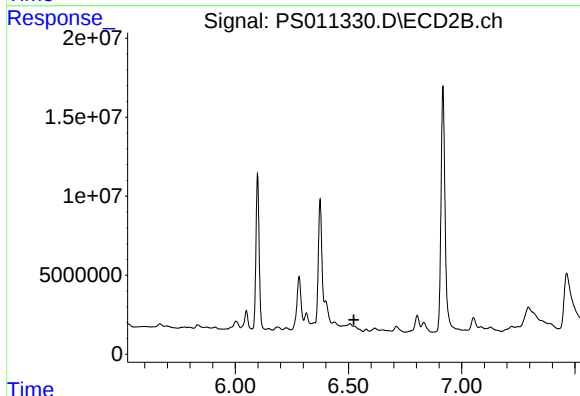


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.524 min
Response: 0
Conc: N.D.

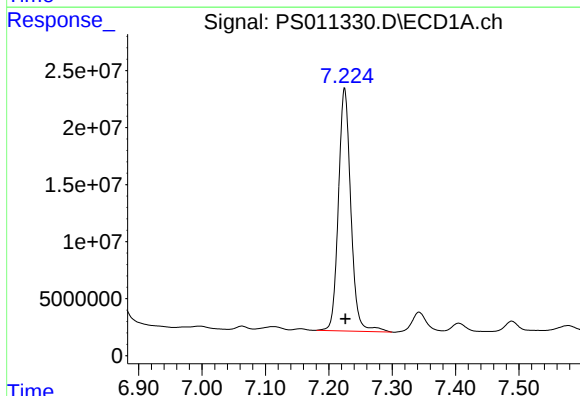


#4 2,4-DCAA

R.T.: 7.225 min
Delta R.T.: -0.001 min
Response: 289563351
Conc: 298.41 ng/ml

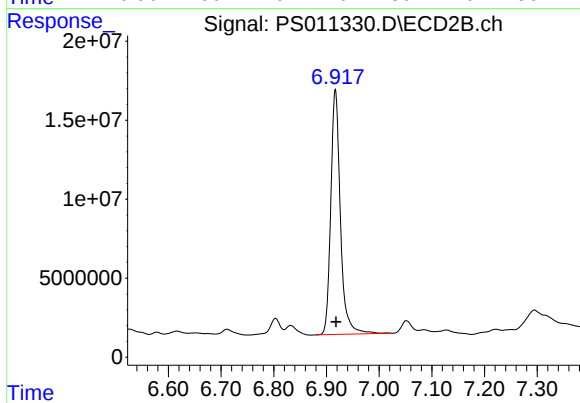

#4 2,4-DCAA


R.T.: 6.917 min
Delta R.T.: -0.001 min
Response: 196341507
Conc: 348.73 ng/ml

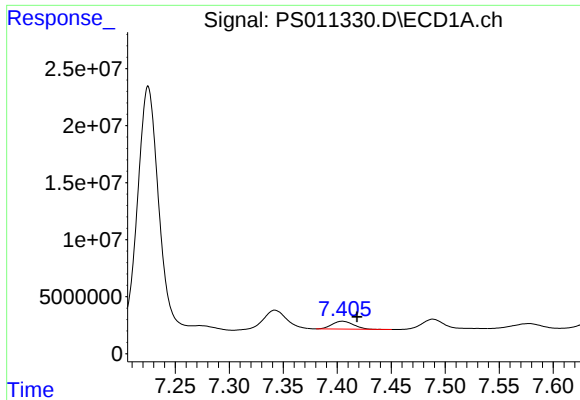

#5 DICAMBA


R.T.: 7.405 min
Delta R.T.: -0.014 min
Response: 9522807
Conc: 2.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB130394TB

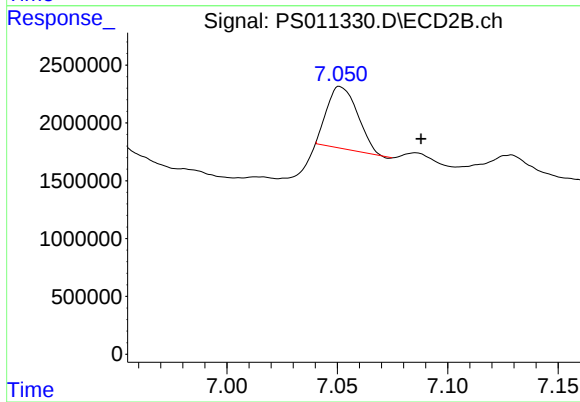


#5 DICAMBA

R.T.: 7.052 min
Delta R.T.: -0.036 min
Response: 5124180
Conc: 2.24 ng/ml

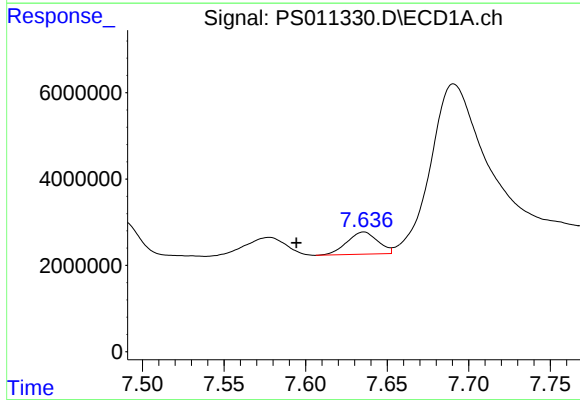


#6 MCP

R.T.: 7.636 min
Delta R.T.: 0.041 min
Response: 6771057
Conc: 2.24 ug/ml

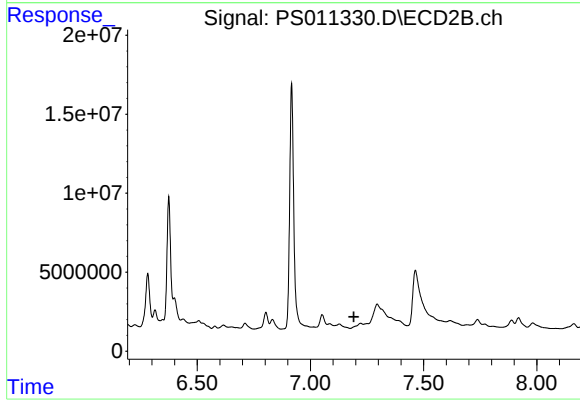

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.192 min
Response: 0
Conc: N.D.

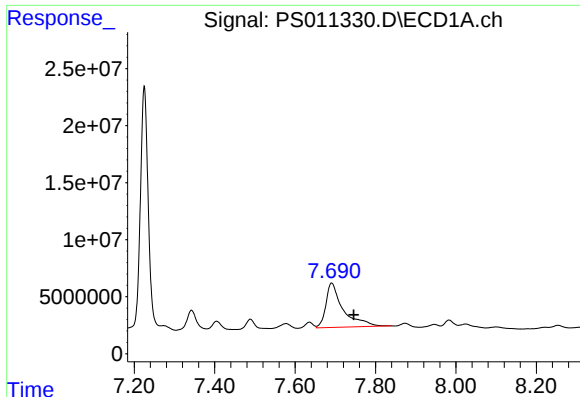

#7 MCPA


R.T.: 7.691 min
Delta R.T.: -0.055 min
Response: 115387229
Conc: 27.06 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB130394TB

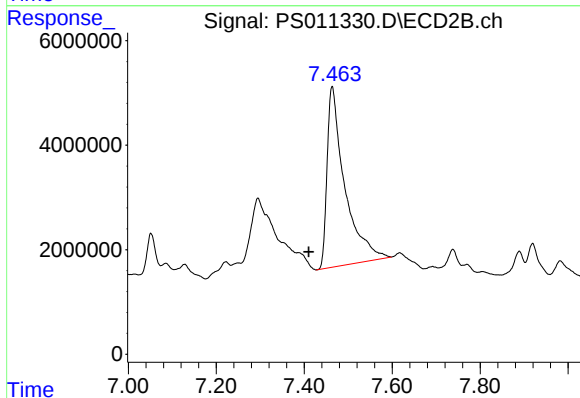


#7 MCPA

R.T.: 7.464 min
Delta R.T.: 0.054 min
Response: 96367850
Conc: 33.43 ug/ml

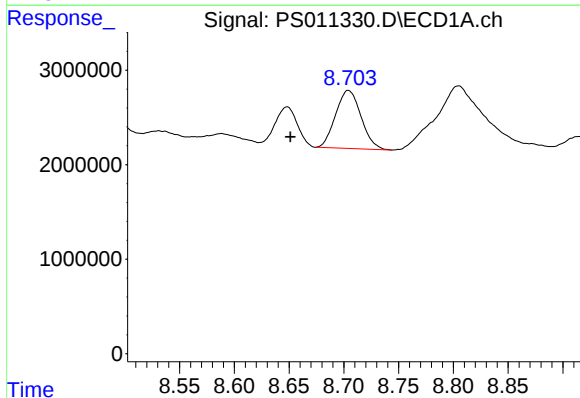


#10 Pentachlorophenol

R.T.: 8.704 min
Delta R.T.: 0.053 min
Response: 9918136
Conc: N.D.

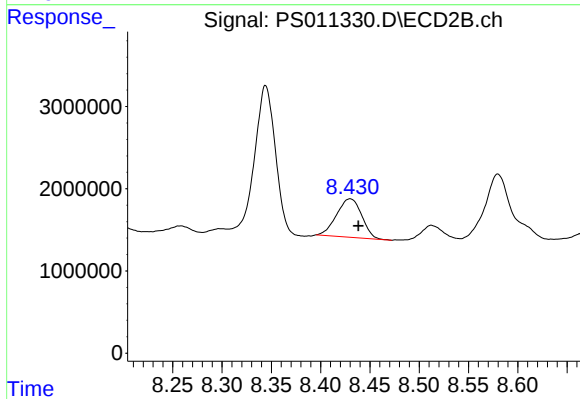

#10 Pentachlorophenol


R.T.: 8.430 min
Delta R.T.: -0.008 min
Response: 8298858
Conc: 1.19 ng/ml

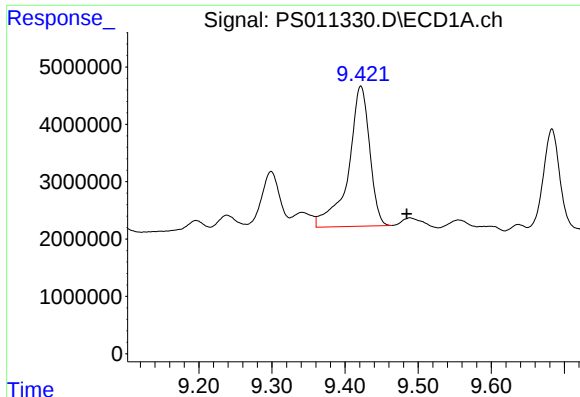

#12 2,4,5-T


R.T.: 9.422 min
Delta R.T.: -0.063 min
Response: 49244538
Conc: 9.76 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB130394TB

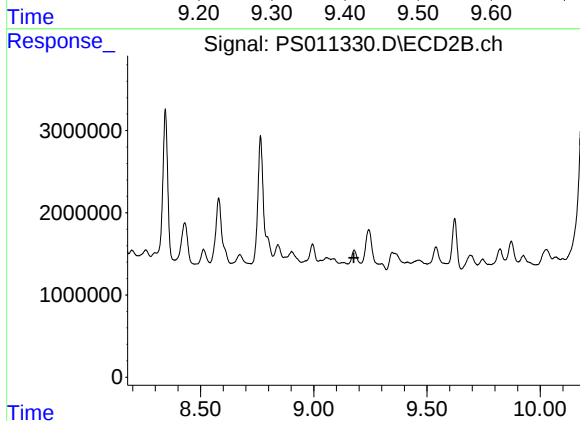


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.177 min
Response: 0
Conc: N.D.

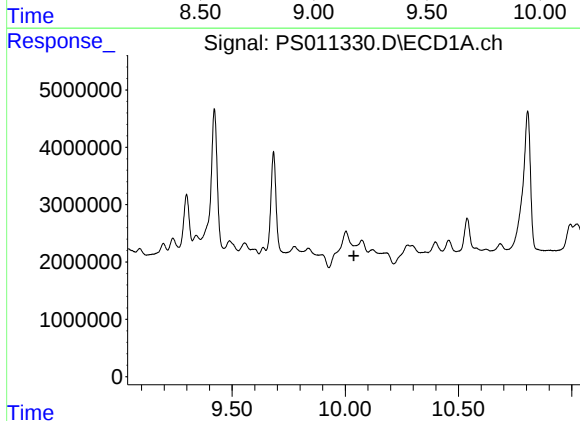


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.038 min
Response: 0
Conc: N.D.

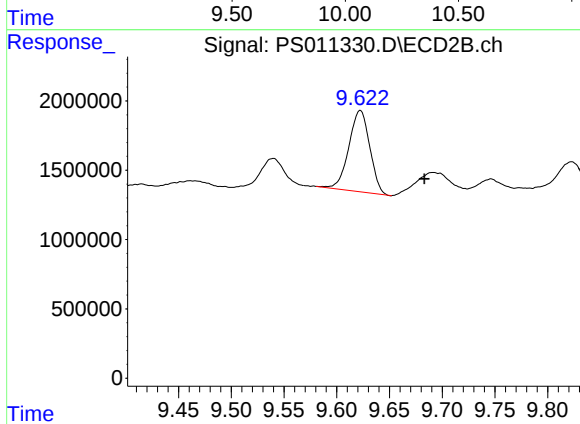

#13 2,4-DB


R.T.: 9.622 min
Delta R.T.: -0.061 min
Response: 8089054
Conc: 18.92 ng/ml

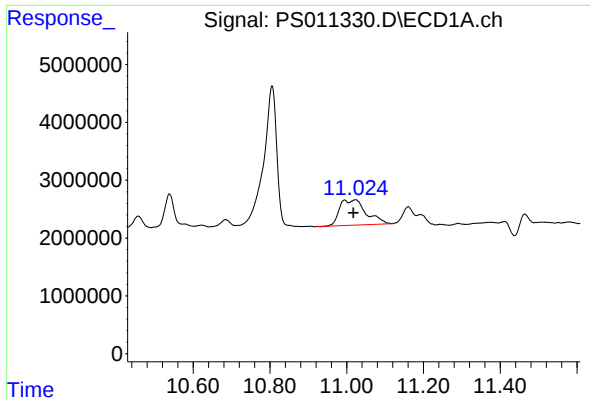

#15 Picloram

R.T.: 11.023 min
Delta R.T.: 0.005 min
Response: 21112554
Conc: 3.35 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB130394TB

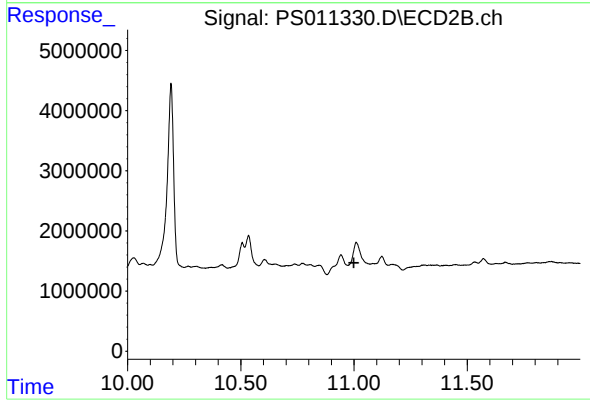

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.999 min
Response: 0
Conc: N.D.