

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072220\
 Data File : PS011334.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2020 21:42
 Operator : DD\AJ
 Sample : L3186-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 02:49:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.225	6.918	236.1E6	160.2E6	243.352	284.487
Target Compounds							
1) T	Dalapon	2.997	2.583	29365578	22357521	24.403	29.124
2) T	3,5-DICHL...	0.000	6.098	0	47149605	N.D.	56.141
5) T	DICAMBA	7.405	0.000	6724090	0	1.735	N.D. #
6) T	MCP	7.636	0.000	5236275	0	1.729	N.D. #
7) T	MCPA	7.692	7.466	156.8E6	136.0E6	36.777	47.193 #
10) T	Pentachlo...	8.704	0.000	7928989	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.789	0	31764744	N.D.	10.390
12) T	2,4,5-T	9.422	0.000	48934190	0	9.698	N.D. #
14) T	DINOSEB	0.000	10.061	0	12402302	N.D.	5.782
15) T	Picloram	10.993	0.000	29795031	0	4.722	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072220\
Data File : PS011334.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2020 21:42
Operator : DD\AJ
Sample : L3186-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 02:49:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
Quant Title : 8080.M
QLast Update : Mon Jul 13 16:10:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

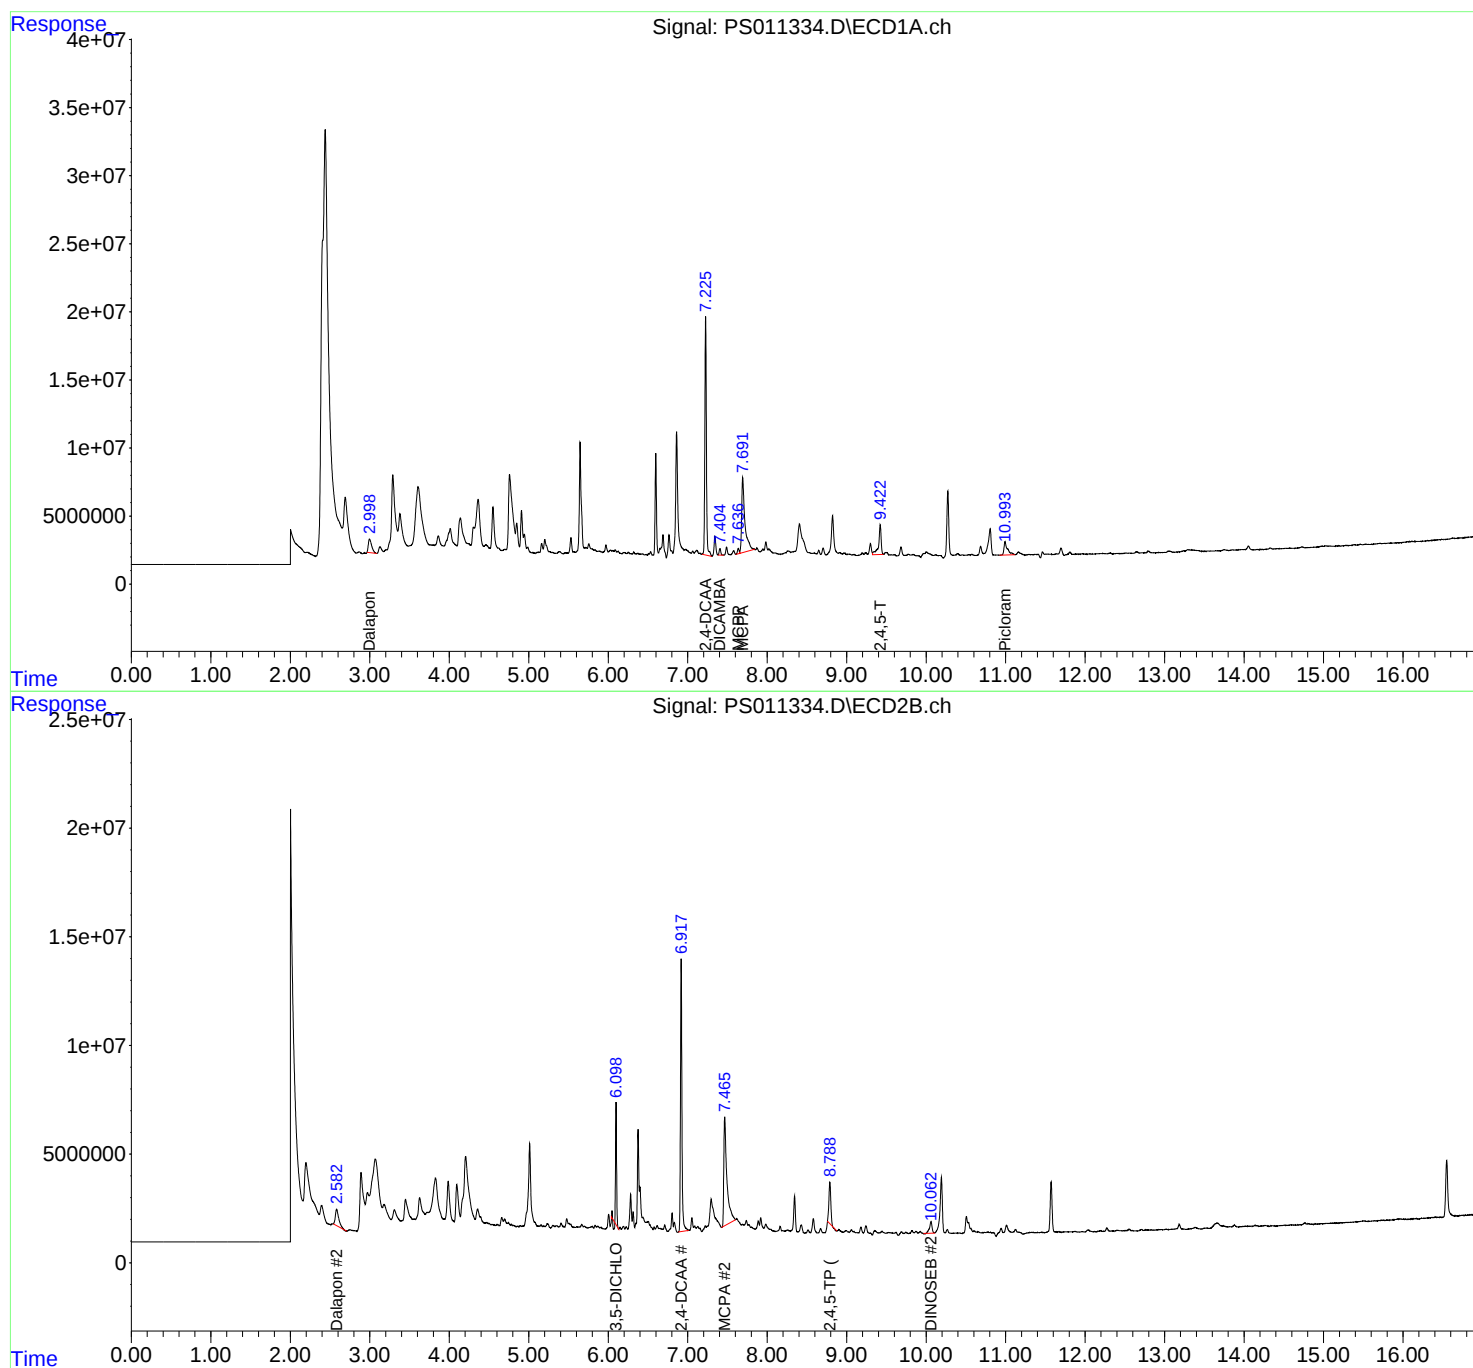


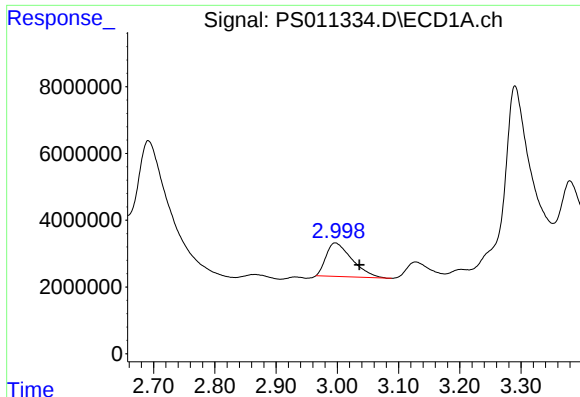

#1 Dalapon


R.T.: 2.997 min
Delta R.T.: -0.039 min
Response: 29365578
Conc: 24.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

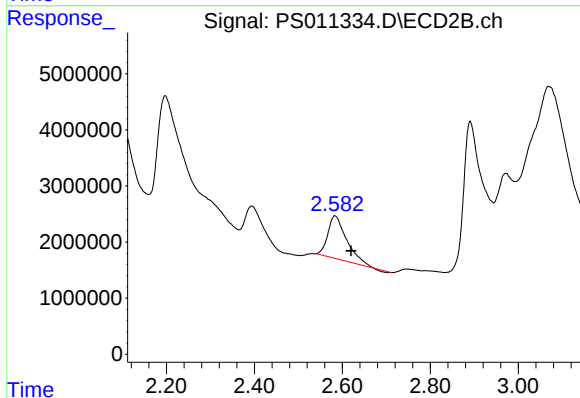


#1 Dalapon

R.T.: 2.583 min
Delta R.T.: -0.037 min
Response: 22357521
Conc: 29.12 ng/ml

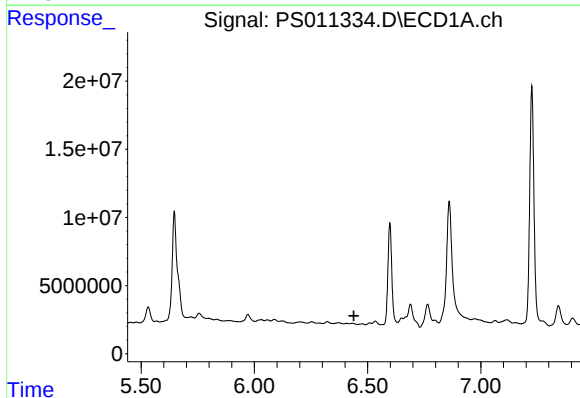


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.439 min
Response: 0
Conc: N.D.

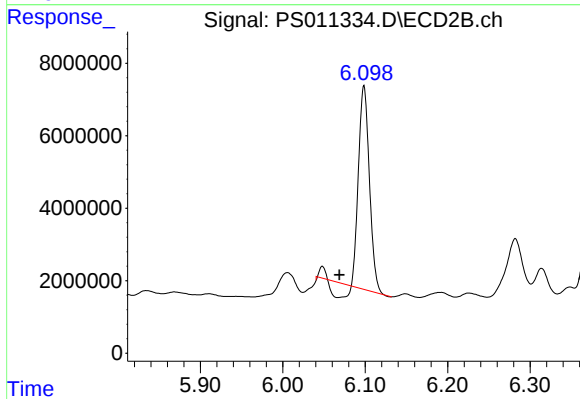

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.098 min
Delta R.T.: 0.030 min
Response: 47149605
Conc: 56.14 ng/ml

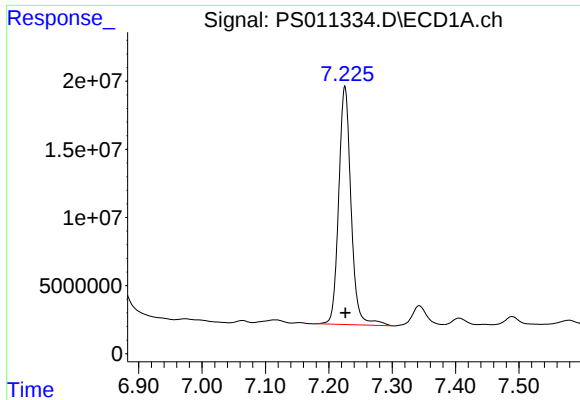

#4 2,4-DCAA


R.T.: 7.225 min
Delta R.T.: -0.001 min
Response: 236134129
Conc: 243.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

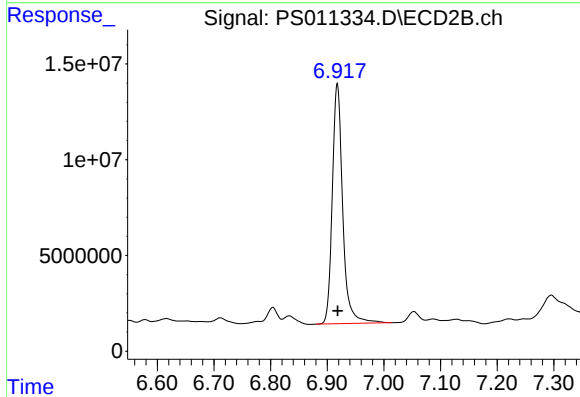


#4 2,4-DCAA

R.T.: 6.918 min
Delta R.T.: 0.000 min
Response: 160172459
Conc: 284.49 ng/ml

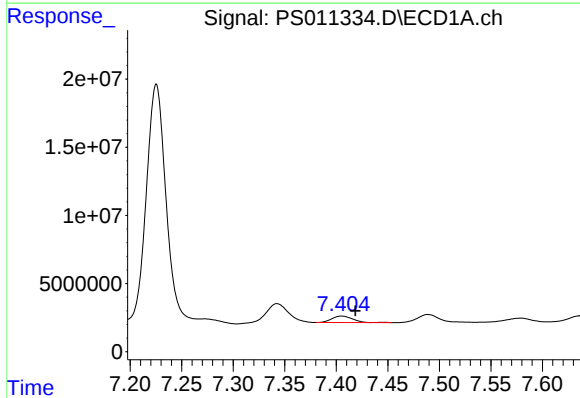


#5 DICAMBA

R.T.: 7.405 min
Delta R.T.: -0.013 min
Response: 6724090
Conc: 1.73 ng/ml

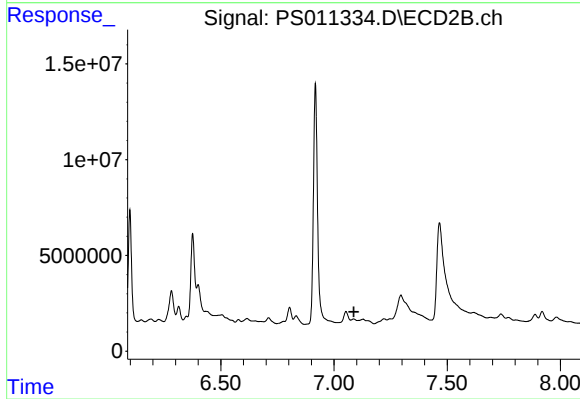

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

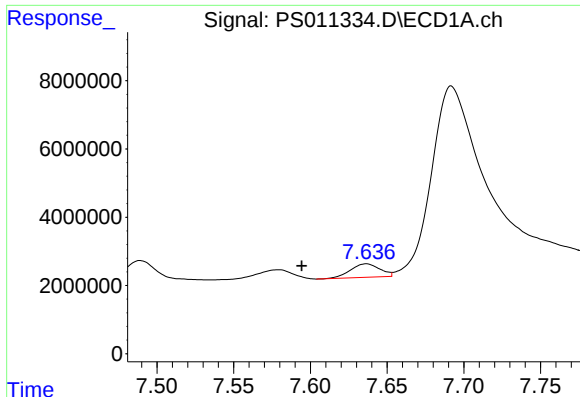

#6 MCPP


R.T.: 7.636 min
Delta R.T.: 0.042 min
Response: 5236275
Conc: 1.73 ug/ml

Instrument :
ECD_S
ClientSampleId :

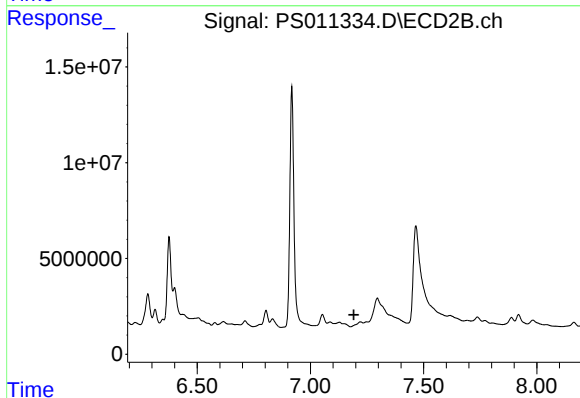


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.192 min
Response: 0
Conc: N.D.

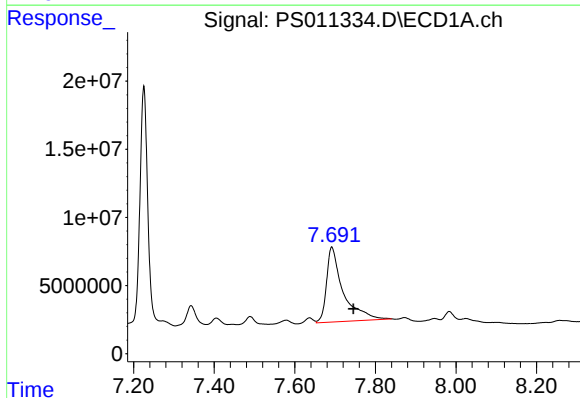


#7 MCPA

R.T.: 7.692 min
Delta R.T.: -0.054 min
Response: 156843545
Conc: 36.78 ug/ml

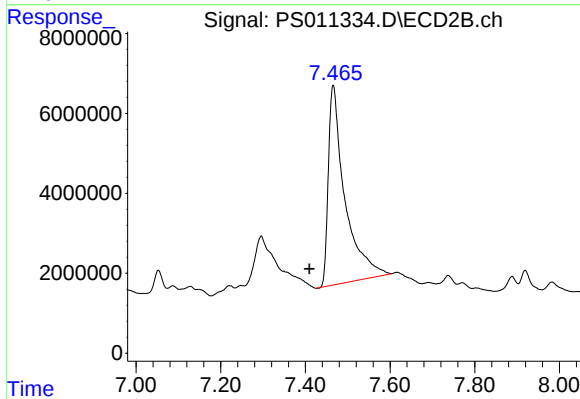

#7 MCPA


R.T.: 7.466 min
Delta R.T.: 0.056 min
Response: 136026430
Conc: 47.19 ug/ml

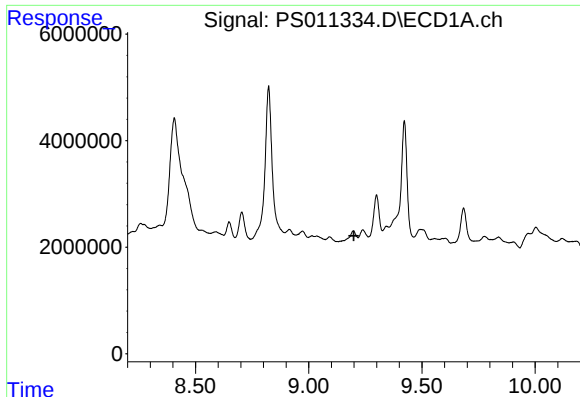

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.200 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

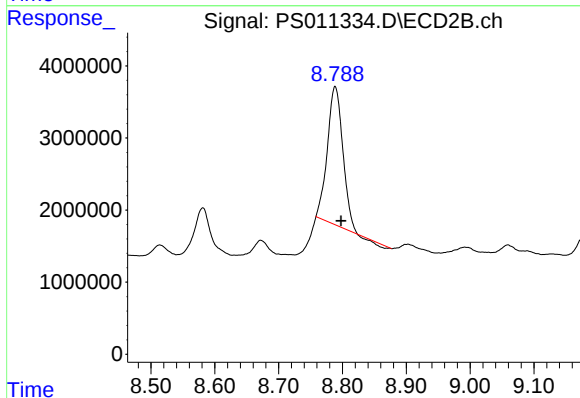


#11 2,4,5-TP (SILVEX)

R.T.: 8.789 min
Delta R.T.: -0.010 min
Response: 31764744
Conc: 10.39 ng/ml

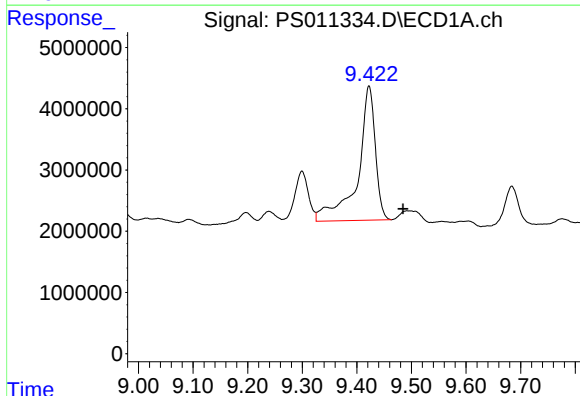


#12 2,4,5-T

R.T.: 9.422 min
Delta R.T.: -0.062 min
Response: 48934190
Conc: 9.70 ng/ml

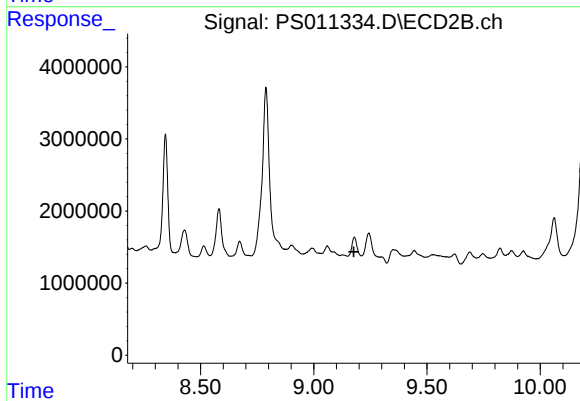

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.177 min
Response: 0
Conc: N.D.

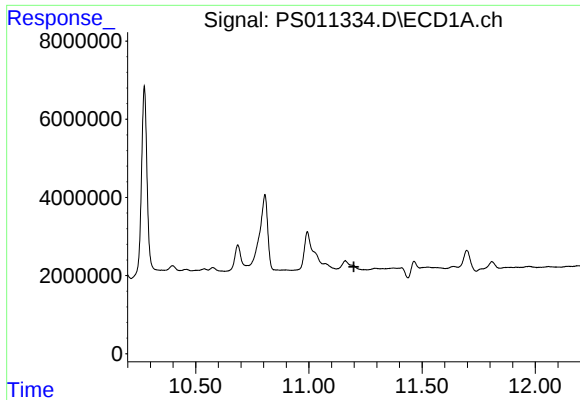

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.199 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

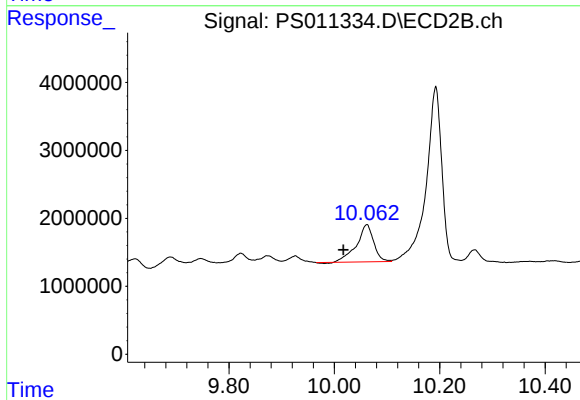


#14 DINOSEB

R.T.: 10.061 min
Delta R.T.: 0.044 min
Response: 12402302
Conc: 5.78 ng/ml

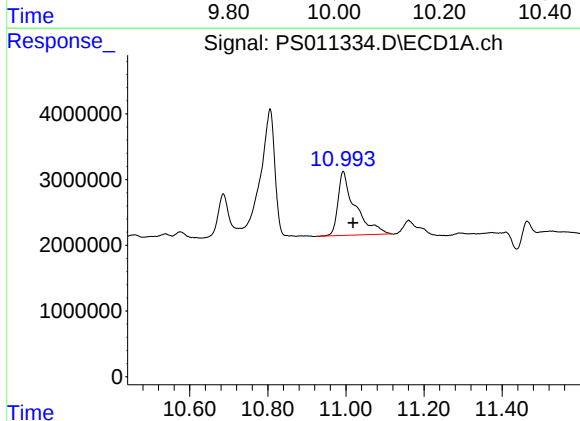

#15 Picloram

R.T.: 10.993 min
Delta R.T.: -0.025 min
Response: 29795031
Conc: 4.72 ng/ml

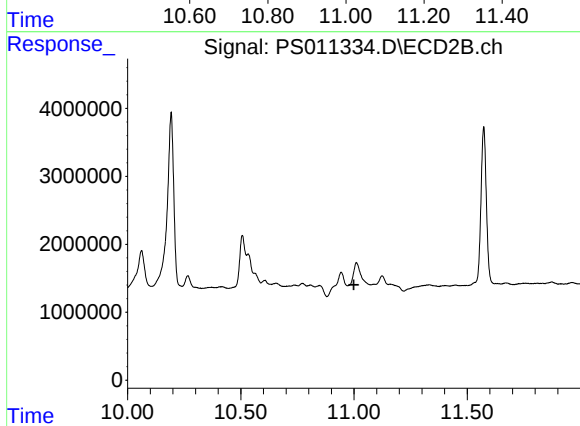

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 10.999 min
Response: 0
Conc: N.D.