

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072222\
 Data File : PS020049.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2022 18:00
 Operator : AJ\MA
 Sample : N3806-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 22:32:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072022.M
 Quant Title : 8080.M
 QLast Update : Wed Jul 20 17:52:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.190	6.775	1295.8E6	434.7E6	390.790	482.523
Target Compounds							
1) T	Dalapon	2.971	2.482f	188.3E6	51927912	34.116	43.453 #
2) T	3,5-DICHL...	6.372	5.981	-4929316	60173552	N.D.	43.394
3) T	4-Nitroph...	7.024	6.374	9327638	8277073	6.489	17.133 #
5) T	DICAMBA	7.373	6.943	17969629	41925812	1.370	10.228 #
6) T	MCPD	7.543	7.042	16023554	1147725	1.528	<MDL #
7) T	MCPA	7.738	7.233	30952800	10413372	2.072	2.442
8) T	DICHLORPROP	8.060	7.583	2146146	21877520	<MDL	21.089 #
9) T	2,4-D	8.367f	7.833	70207106	19726112	17.198	15.807
10) T	Pentachlo...	8.605	8.277	19836795	6557830	<MDL	<MDL #
11) T	2,4,5-TP ...	9.150	8.674	3625564	18568639	<MDL	3.128 #
12) T	2,4,5-T	9.428	9.019	7888837	10740913	<MDL	1.948 #
13) T	2,4-DB	9.957	9.529	37532726	57515549	8.617	80.575 #
14) T	DINOSEB	11.110	9.847	1689.8E6	155.6E6	94.026	37.442 #
15) T	Picloram	10.981	10.834	325.3E6	129.5E6	9.340	16.853 #
16) T	DCPA	11.431	10.772	-66229199	23805448	N.D.	3.296


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072222\
Data File : PS020049.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2022 18:00
Operator : AJ\MA
Sample : N3806-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 22:32:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072022.M
Quant Title : 8080.M
QLast Update : Wed Jul 20 17:52:40 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

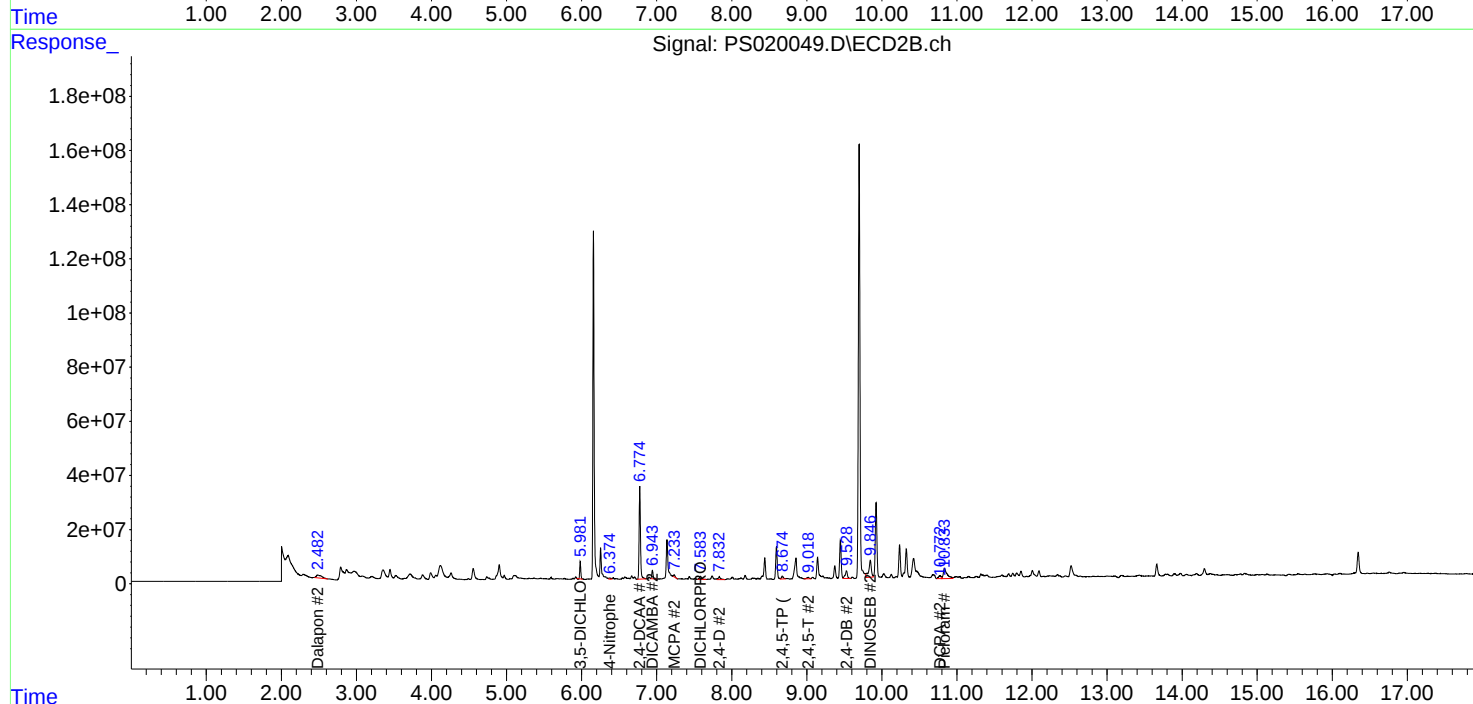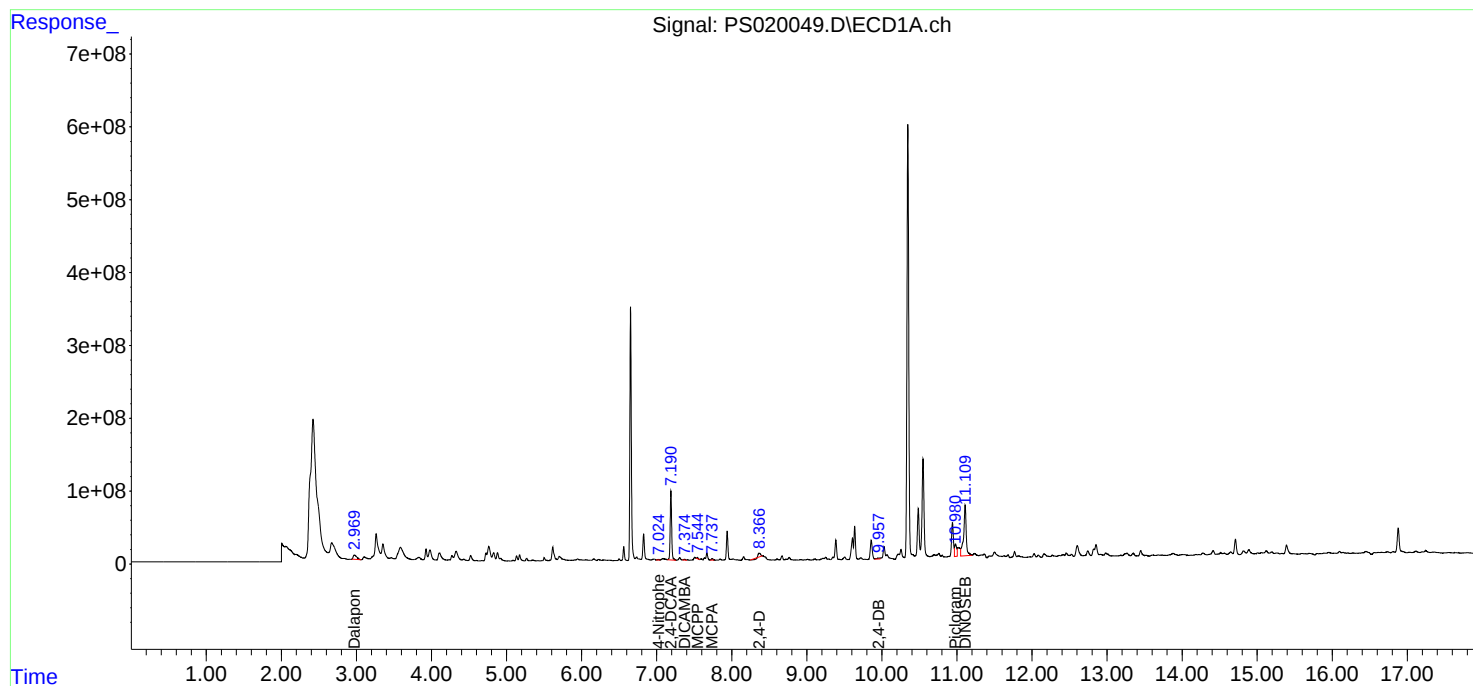

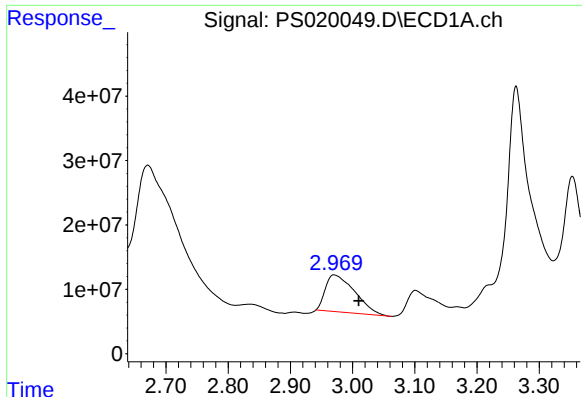


#1 Dalapon

R.T.: 2.971 min
Delta R.T.: -0.039 min
Response: 188280763
Conc: 34.12 ng/ml

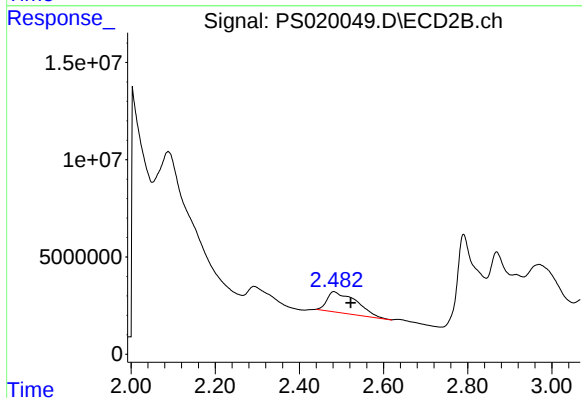


#1 Dalapon

R.T.: 2.482 min
Delta R.T.: -0.041 min
Response: 51927912
Conc: 43.45 ng/ml

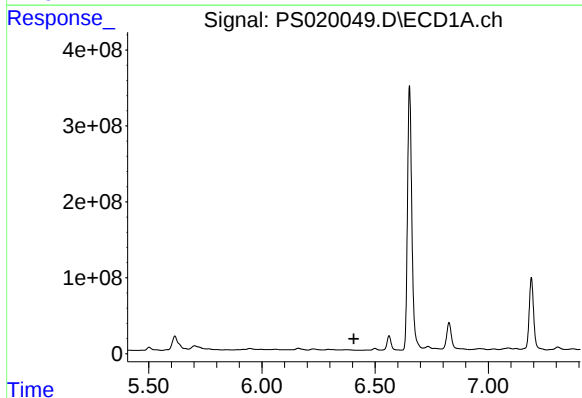


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.372 min
Delta R.T.: -0.034 min
Response: -4929316
Conc: N.D.

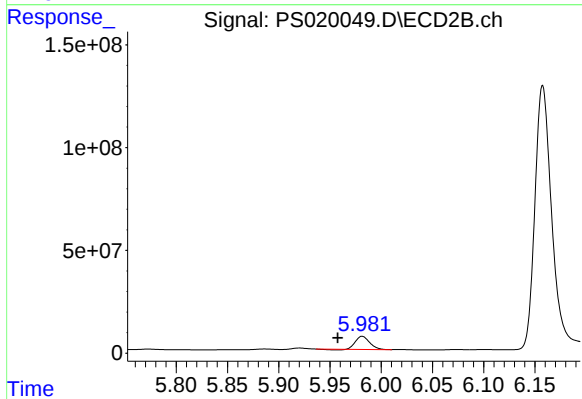


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.981 min
Delta R.T.: 0.024 min
Response: 60173552
Conc: 43.39 ng/ml

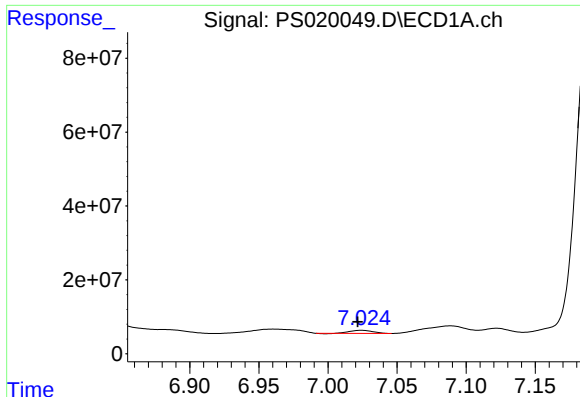


#3 4-Nitrophenol

R.T.: 7.024 min
Delta R.T.: 0.003 min
Response: 9327638
Conc: 6.49 ng/ml

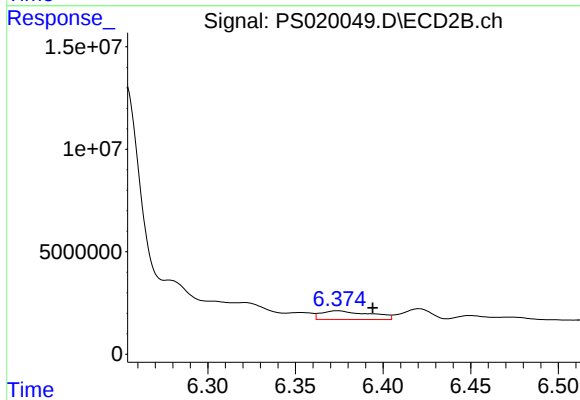


#3 4-Nitrophenol

R.T.: 6.374 min
Delta R.T.: -0.020 min
Response: 8277073
Conc: 17.13 ng/ml

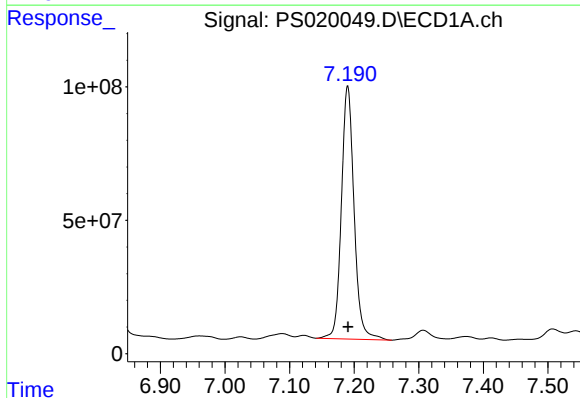


#4 2,4-DCAA

R.T.: 7.190 min
Delta R.T.: 0.000 min
Response: 1295800940
Conc: 390.79 ng/ml

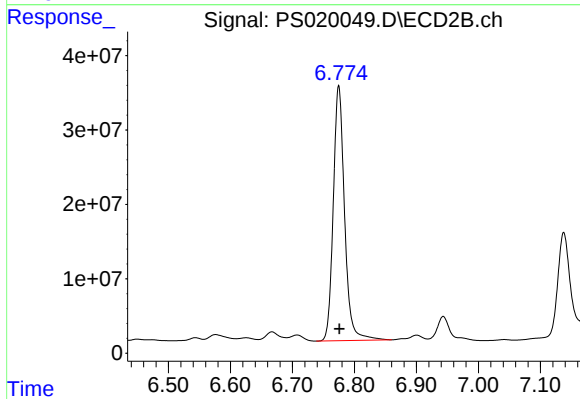


#4 2,4-DCAA

R.T.: 6.775 min
Delta R.T.: 0.000 min
Response: 434706748
Conc: 482.52 ng/ml

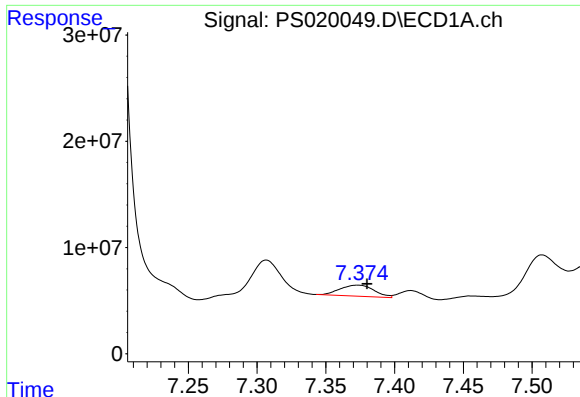


#5 DICAMBA

R.T.: 7.373 min
Delta R.T.: -0.007 min
Response: 17969629
Conc: 1.37 ng/ml

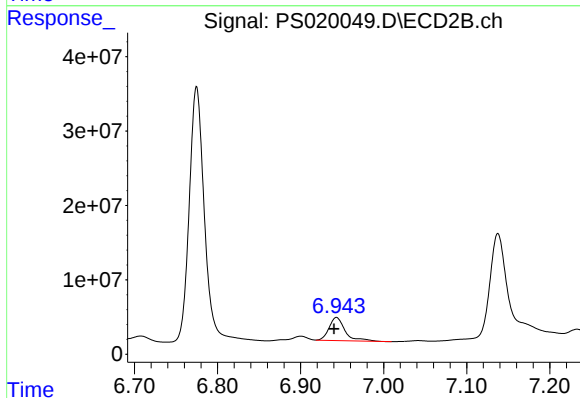


#5 DICAMBA

R.T.: 6.943 min
Delta R.T.: 0.003 min
Response: 41925812
Conc: 10.23 ng/ml

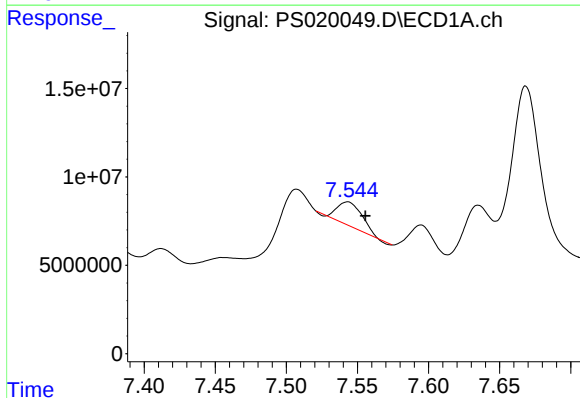


#6 MCP

R.T.: 7.543 min
Delta R.T.: -0.013 min
Response: 16023554
Conc: 1.53 ug/ml

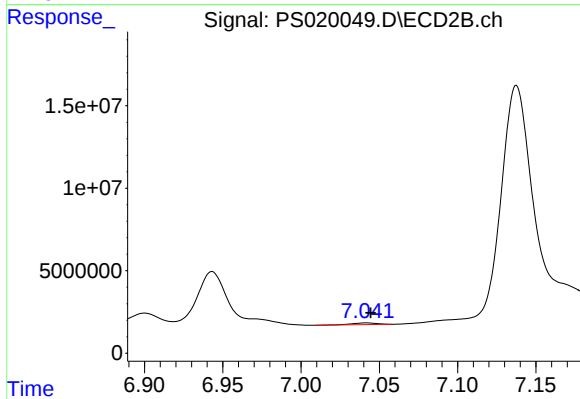


#6 MCP

R.T.: 7.042 min
Delta R.T.: -0.003 min
Response: 1147725
Conc: N.D.

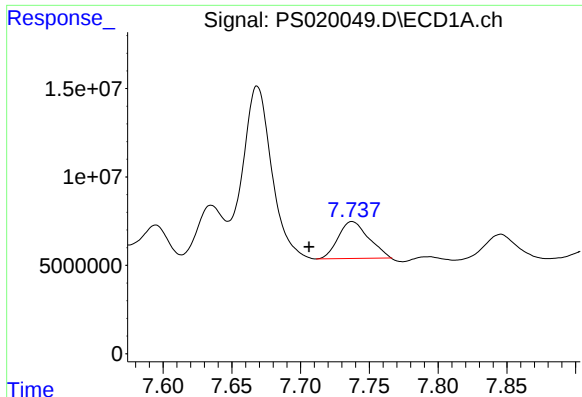


#7 MCPA

R.T.: 7.738 min
Delta R.T.: 0.032 min
Response: 30952800
Conc: 2.07 ug/ml

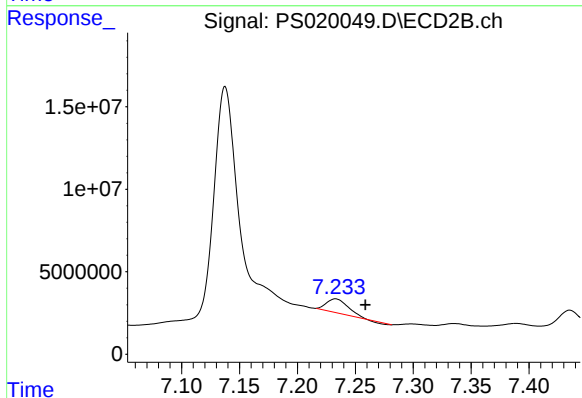


#7 MCPA

R.T.: 7.233 min
Delta R.T.: -0.026 min
Response: 10413372
Conc: 2.44 ug/ml

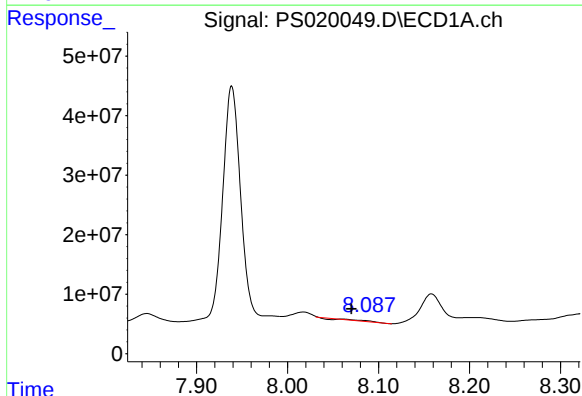


#8 DICHLORPROP

R.T.: 8.060 min
Delta R.T.: -0.010 min
Response: 2146146
Conc: N.D.

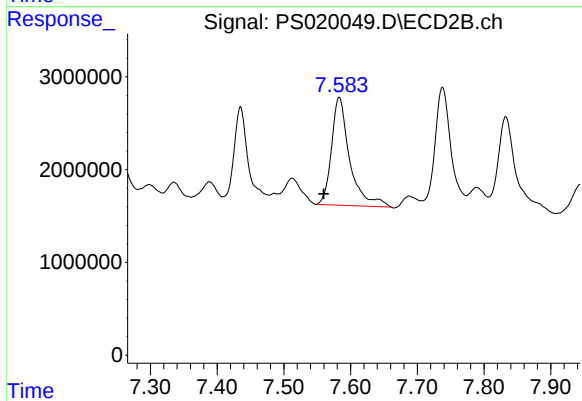


#8 DICHLORPROP

R.T.: 7.583 min
Delta R.T.: 0.023 min
Response: 21877520
Conc: 21.09 ng/ml

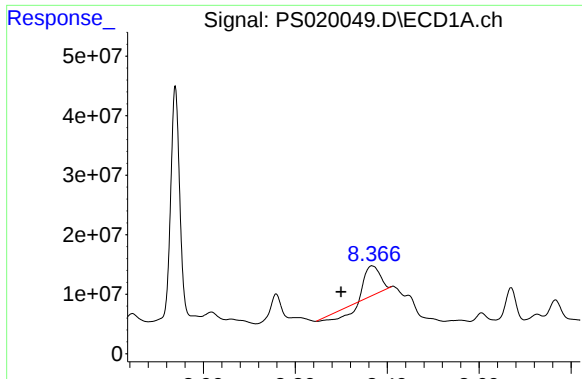


#9 2,4-D

R.T.: 8.367 min
Delta R.T.: 0.068 min
Response: 70207106
Conc: 17.20 ng/ml

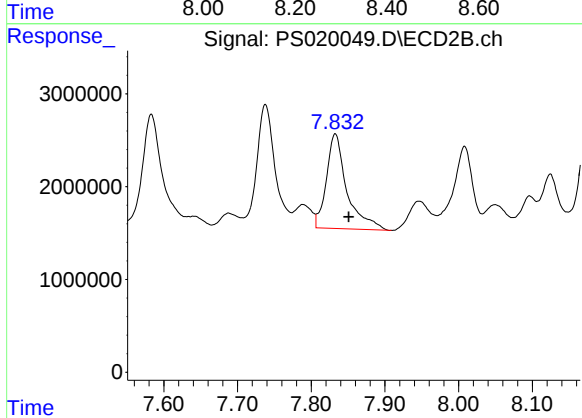


#9 2,4-D

R.T.: 7.833 min
Delta R.T.: -0.018 min
Response: 19726112
Conc: 15.81 ng/ml

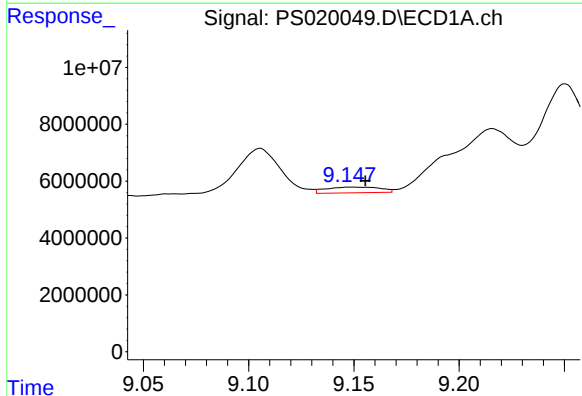


#11 2,4,5-TP (SILVEX)

R.T.: 9.150 min
Delta R.T.: -0.006 min
Response: 3625564
Conc: N.D.

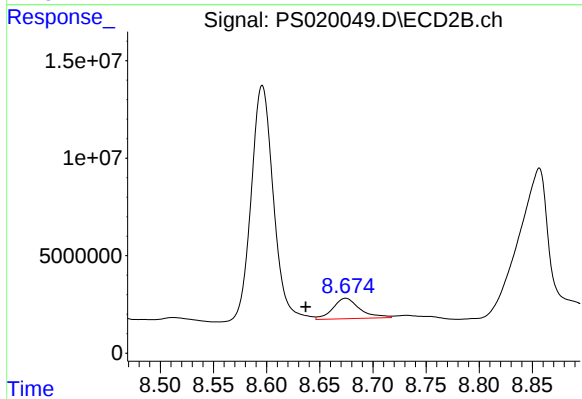


#11 2,4,5-TP (SILVEX)

R.T.: 8.674 min
Delta R.T.: 0.037 min
Response: 18568639
Conc: 3.13 ng/ml

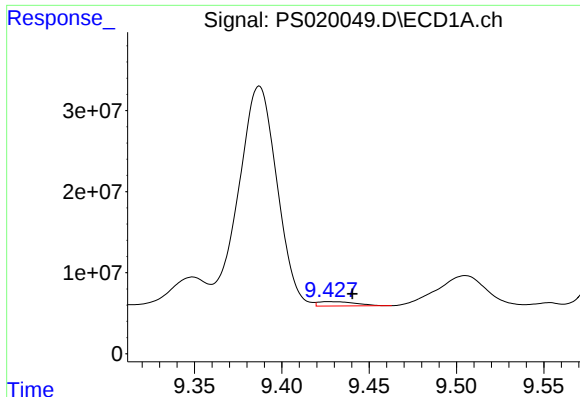


#12 2,4,5-T

R.T.: 9.428 min
Delta R.T.: -0.012 min
Response: 7888837
Conc: N.D.

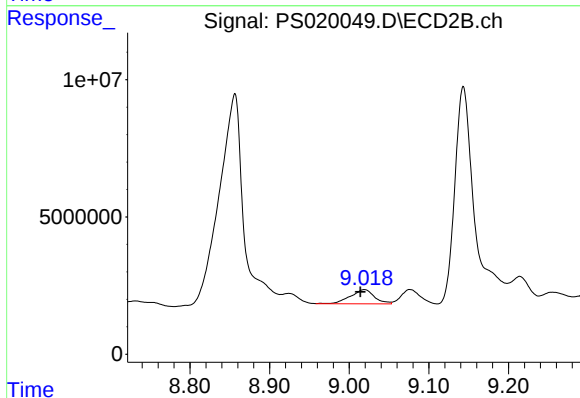


#12 2,4,5-T

R.T.: 9.019 min
Delta R.T.: 0.005 min
Response: 10740913
Conc: 1.95 ng/ml

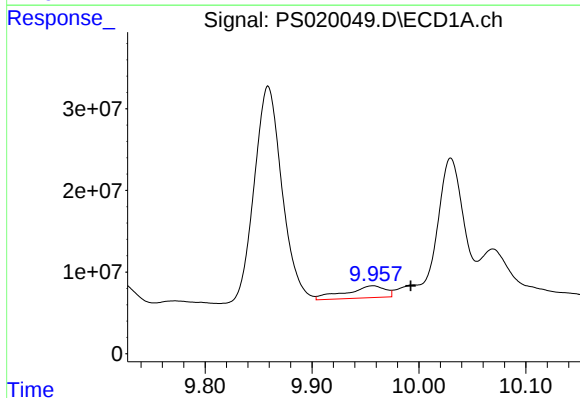


#13 2,4-DB

R.T.: 9.957 min
Delta R.T.: -0.036 min
Response: 37532726
Conc: 8.62 ng/ml

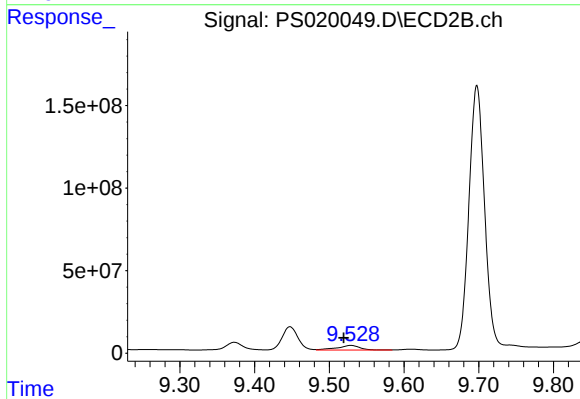


#13 2,4-DB

R.T.: 9.529 min
Delta R.T.: 0.009 min
Response: 57515549
Conc: 80.58 ng/ml

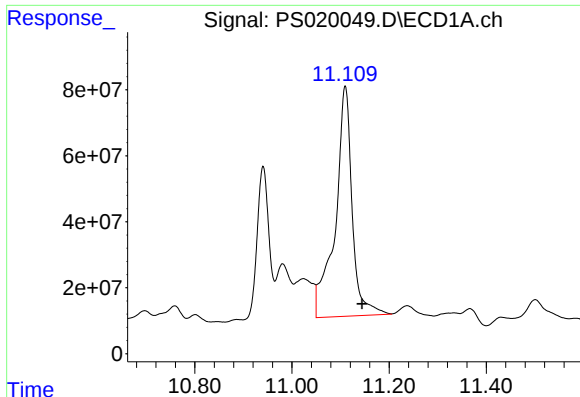


#14 DINOSEB

R.T.: 11.110 min
Delta R.T.: -0.035 min
Response: 1689778260
Conc: 94.03 ng/ml

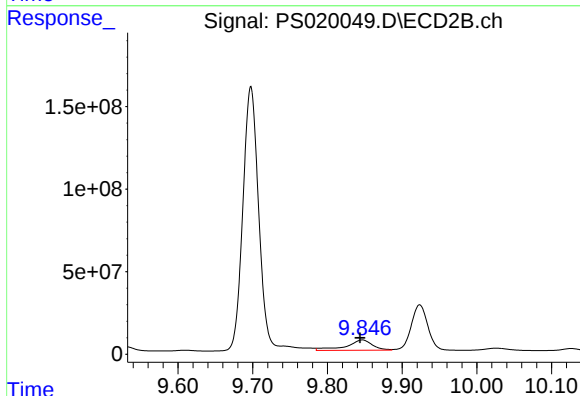


#14 DINOSEB

R.T.: 9.847 min
Delta R.T.: 0.003 min
Response: 155555493
Conc: 37.44 ng/ml

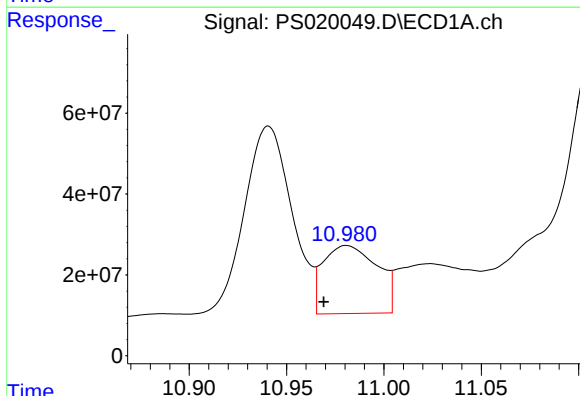


#15 Picloram

R.T.: 10.981 min
Delta R.T.: 0.012 min
Response: 325344942
Conc: 9.34 ng/ml

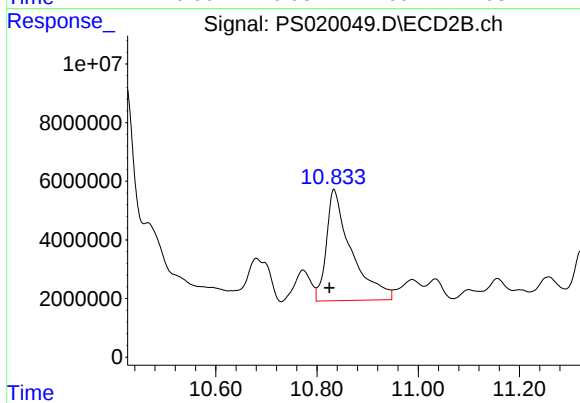


#15 Picloram

R.T.: 10.834 min
Delta R.T.: 0.010 min
Response: 129511799
Conc: 16.85 ng/ml

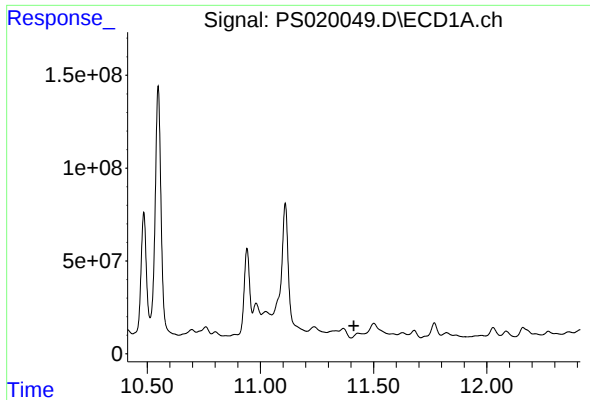

#16 DCPA

R.T.: 11.431 min
Delta R.T.: 0.018 min
Response: -66229199
Conc: N.D.

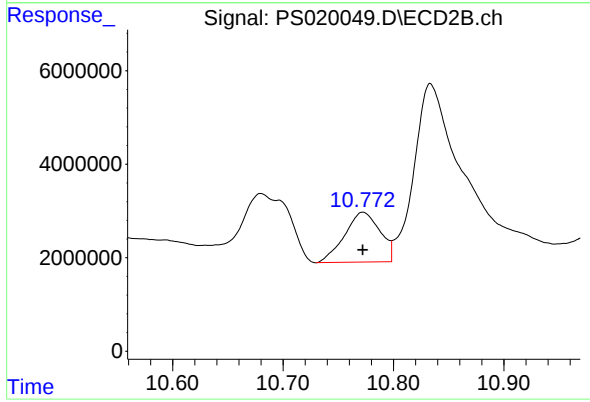

#16 DCPA

R.T.: 10.772 min
Delta R.T.: 0.000 min
Response: 23805448
Conc: 3.30 ng/ml