

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072320\
 Data File : PS011343.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2020 09:57
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 10:38:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.226	6.918	422.7E6	291.8E6	435.669	518.208
Target Compounds							
2) T	3,5-DICHL...	6.483	0.000	8800665	0	6.577	N.D. #
5) T	DICAMBA	0.000	7.153	0	6139672	N.D.	2.681
6) T	MCP	0.000	7.153	0	6139672	N.D.	3.218
15) T	Picloram	0.000	11.033	0	17656149	N.D.	4.037



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072320\
Data File : PS011343.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2020 09:57
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 10:38:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
Quant Title : 8080.M
QLast Update : Mon Jul 13 16:10:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

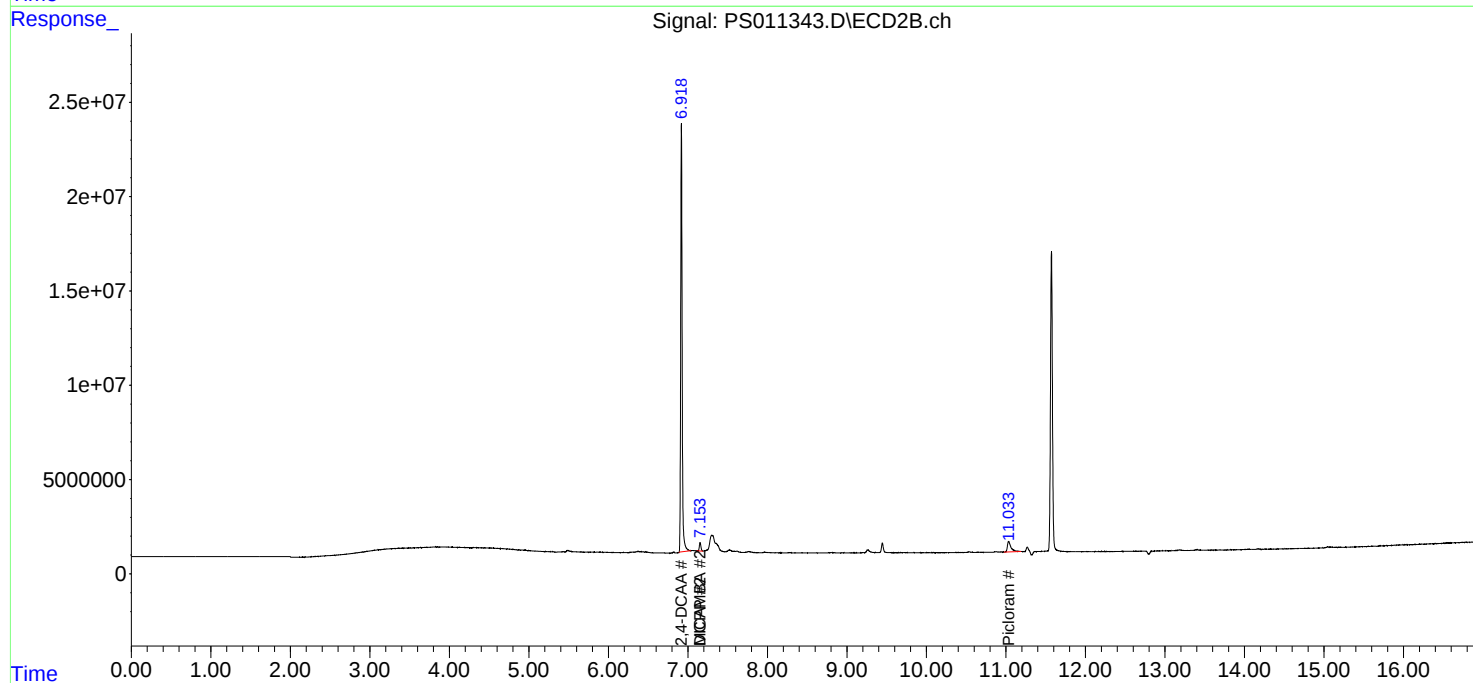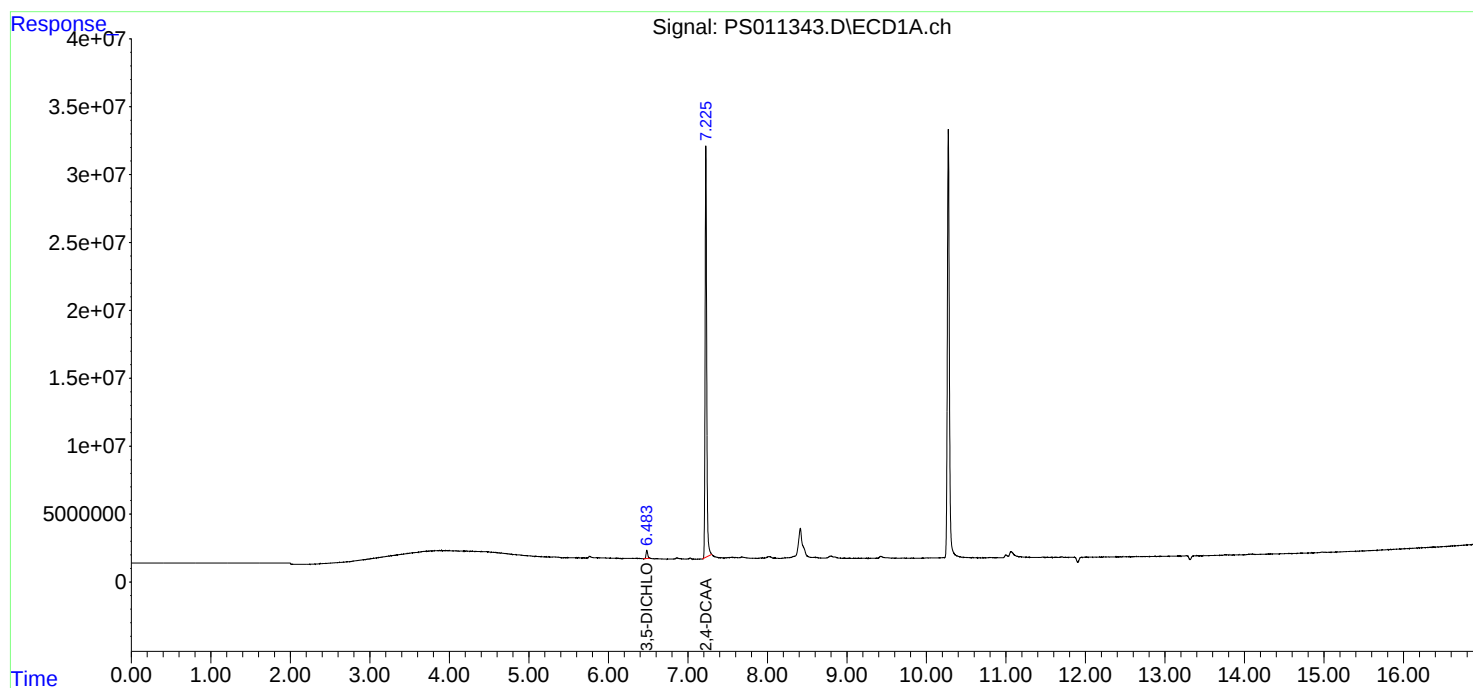


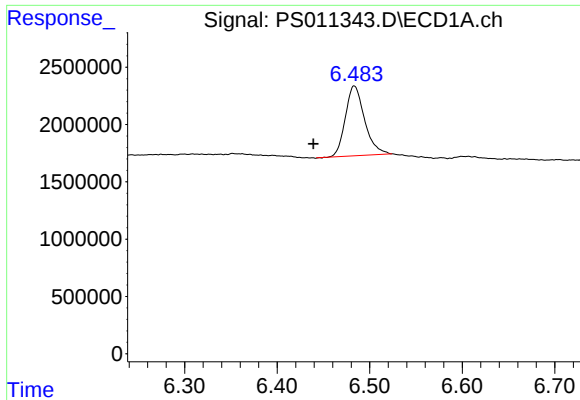

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.483 min
Delta R.T.: 0.044 min
Response: 8800665
Conc: 6.58 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

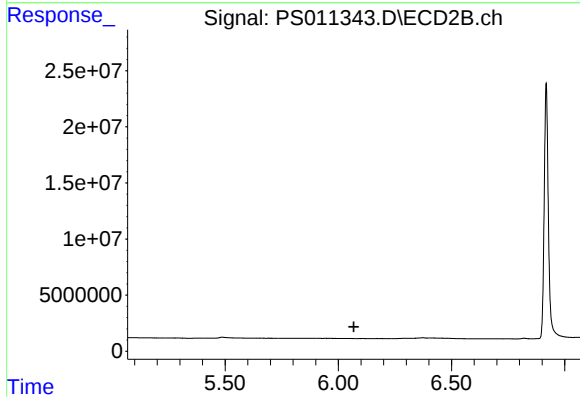


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.069 min
Response: 0
Conc: N.D.

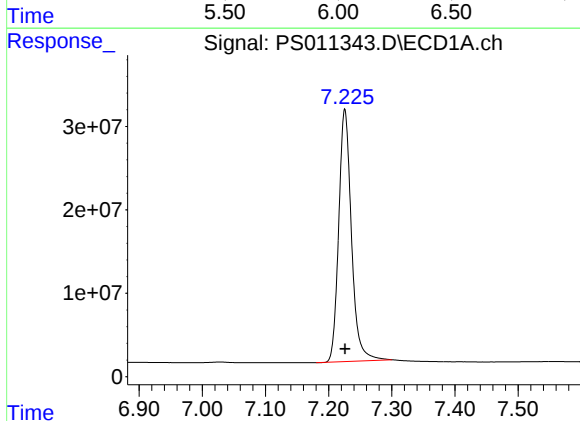


#4 2,4-DCAA

R.T.: 7.226 min
Delta R.T.: 0.000 min
Response: 422746253
Conc: 435.67 ng/ml

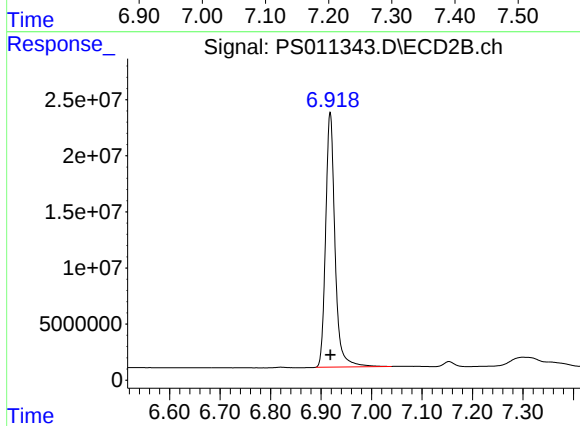

#4 2,4-DCAA


R.T.: 6.918 min
Delta R.T.: 0.000 min
Response: 291762677
Conc: 518.21 ng/ml

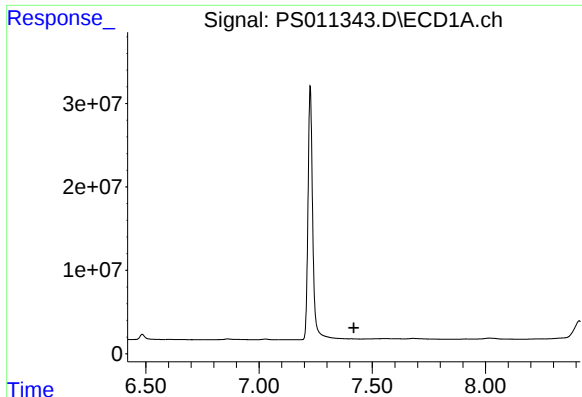

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

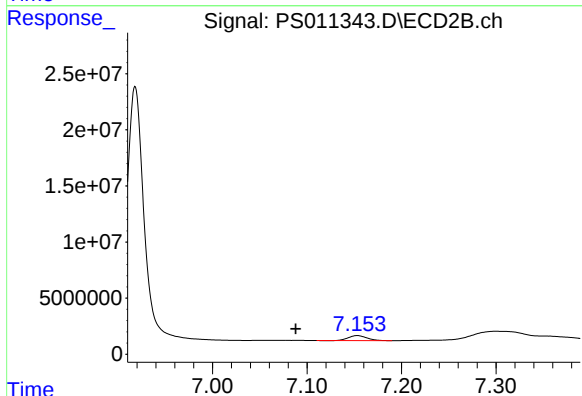


#5 DICAMBA

R.T.: 7.153 min
Delta R.T.: 0.065 min
Response: 6139672
Conc: 2.68 ng/ml

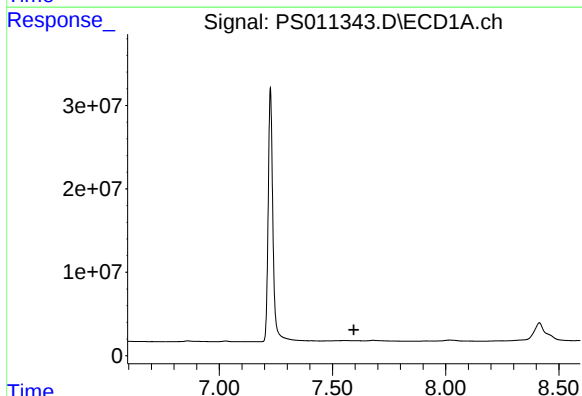


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 7.594 min
Response: 0
Conc: N.D.

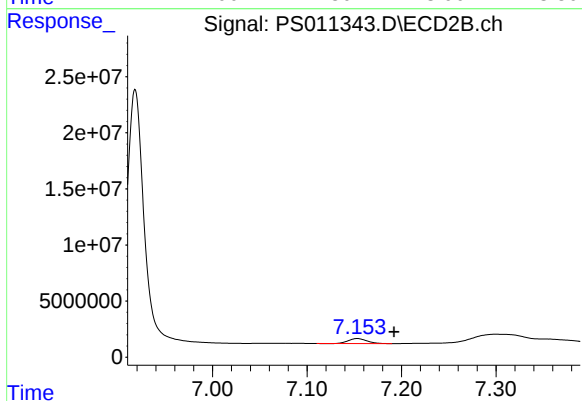

#6 MCPP


R.T.: 7.153 min
Delta R.T.: -0.039 min
Response: 6139672
Conc: 3.22 ug/ml

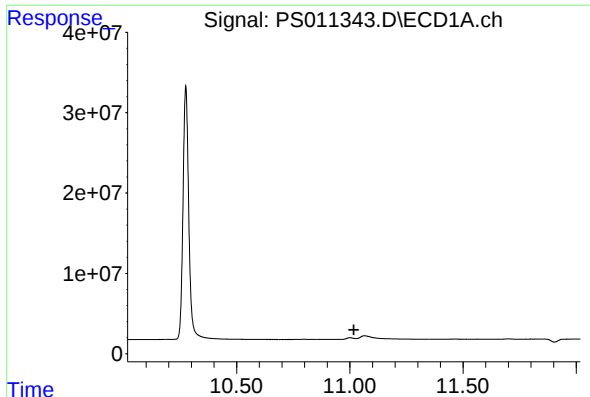

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.018 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

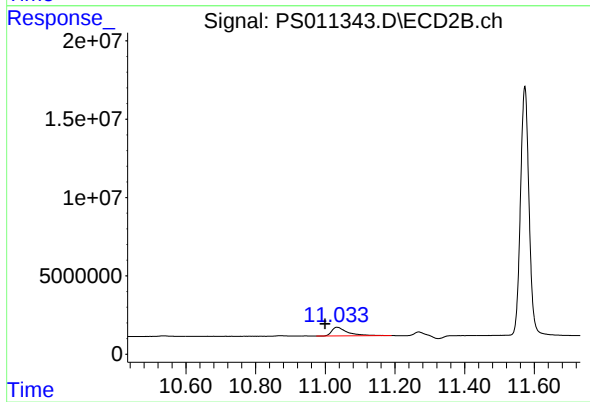

#15 Picloram

R.T.: 11.033 min
Delta R.T.: 0.034 min
Response: 17656149
Conc: 4.04 ng/ml