

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072320\
 Data File : PS011355.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2020 20:26
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 03:45:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.225	6.917	439.1E6	300.2E6	452.483	533.210
Target Compounds							
2) T	3,5-DICHL...	6.483	0.000	6835067	0	5.108	N.D. #
5) T	DICAMBA	0.000	7.153	0	4899041	N.D.	2.139
6) T	MCP	0.000	7.153	0	4899041	N.D.	2.568



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072320\
Data File : PS011355.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2020 20:26
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 03:45:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
Quant Title : 8080.M
QLast Update : Mon Jul 13 16:10:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

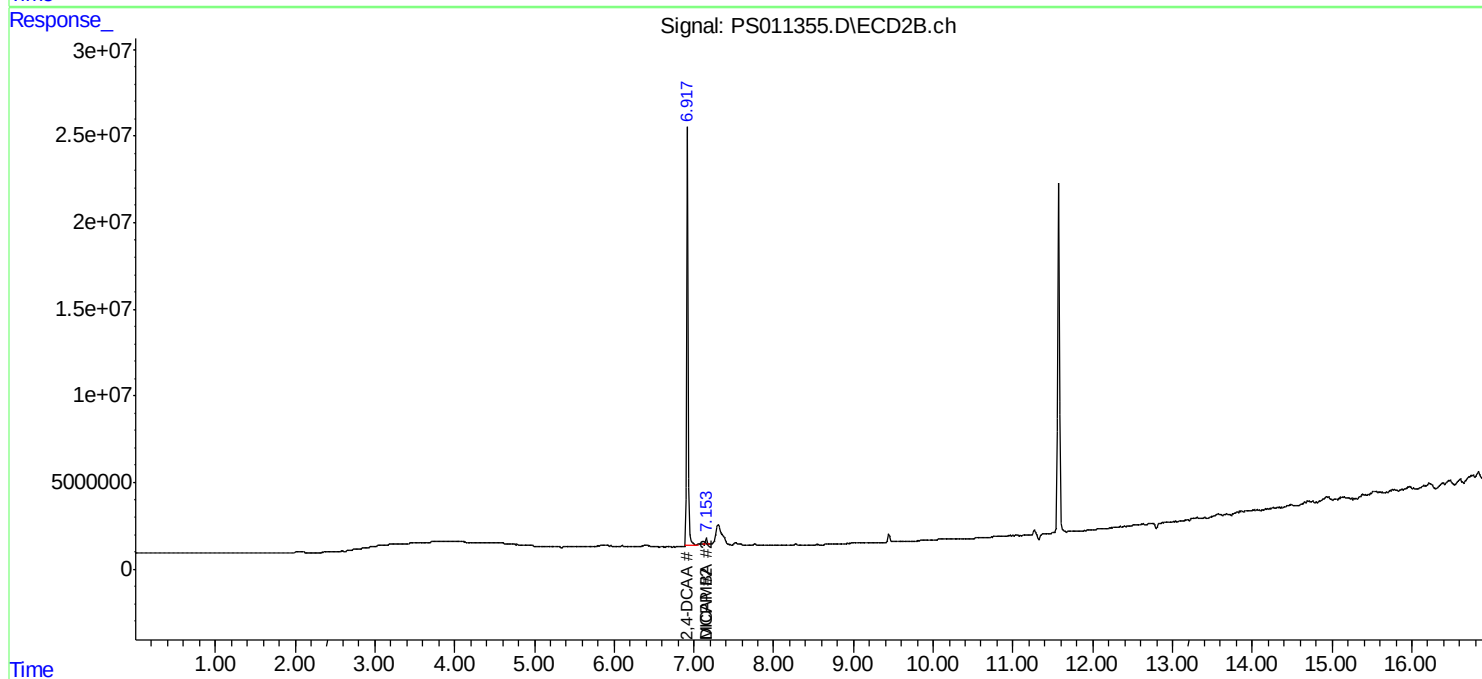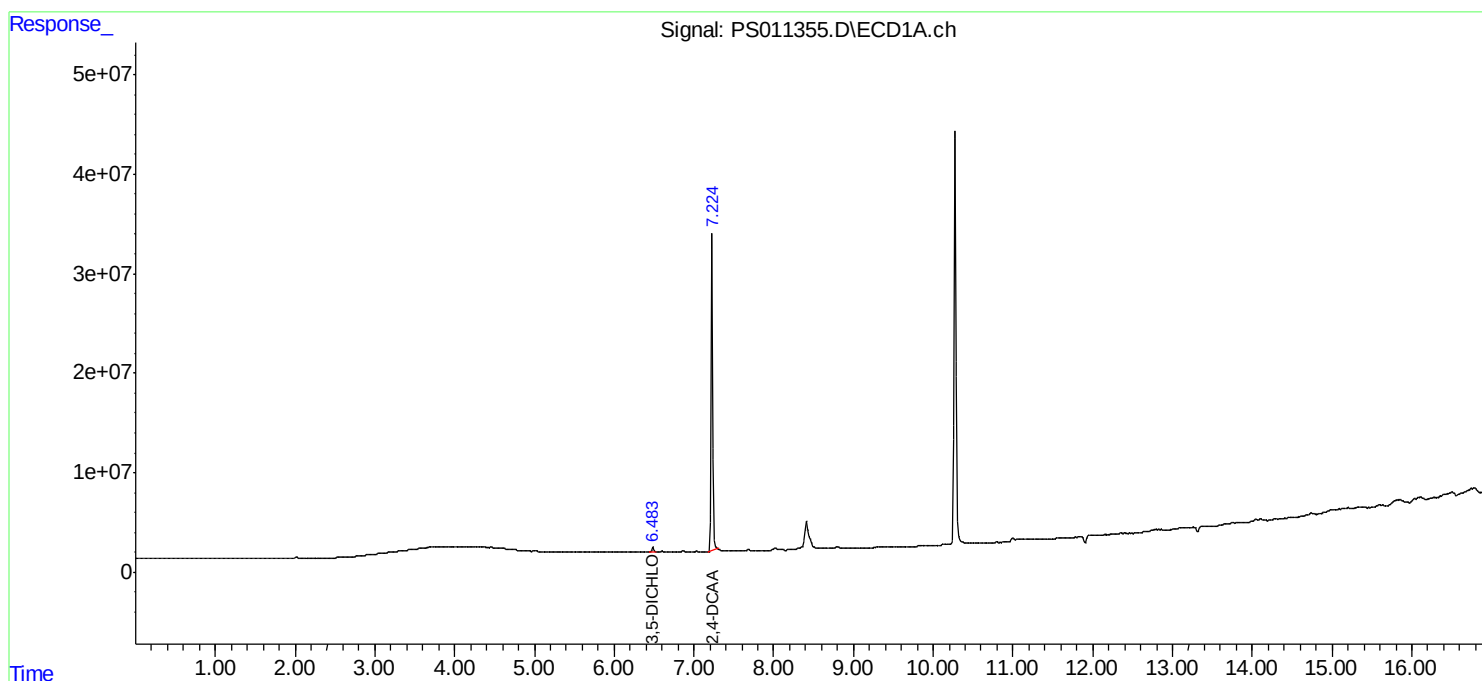


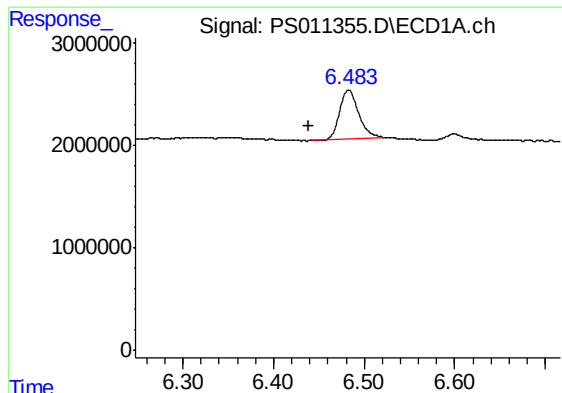

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.483 min
Delta R.T.: 0.044 min
Response: 6835067
Conc: 5.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

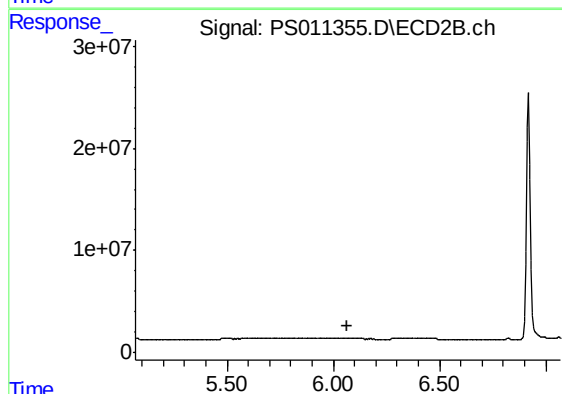


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.069 min
Response: 0
Conc: N.D.

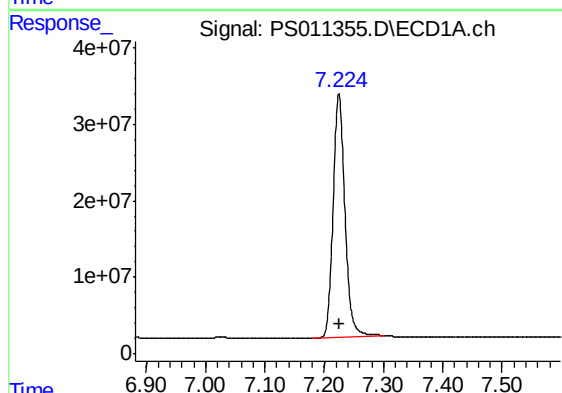


#4 2,4-DCAA

R.T.: 7.225 min
Delta R.T.: -0.002 min
Response: 439061334
Conc: 452.48 ng/ml

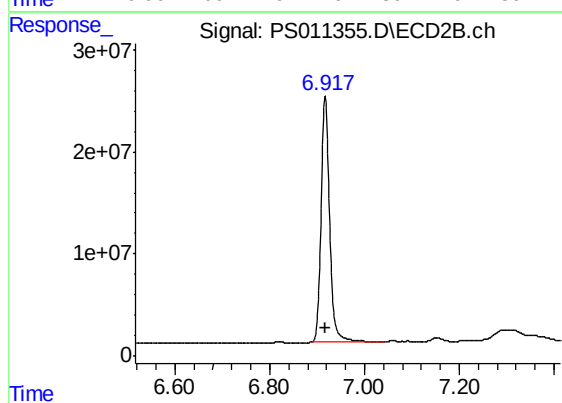

#4 2,4-DCAA


R.T.: 6.917 min
Delta R.T.: -0.002 min
Response: 300209174
Conc: 533.21 ng/ml

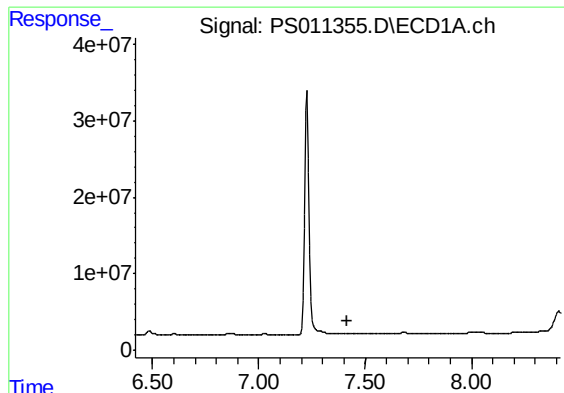

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

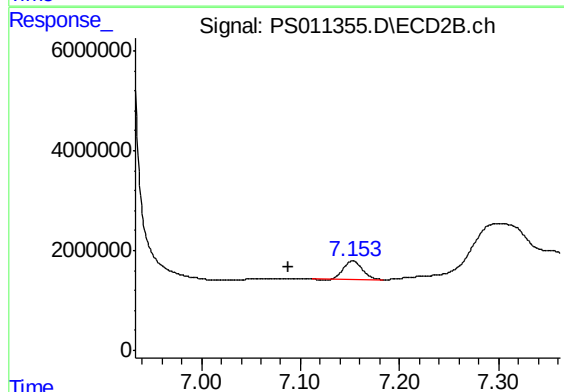


#5 DICAMBA

R.T.: 7.153 min
Delta R.T.: 0.065 min
Response: 4899041
Conc: 2.14 ng/ml

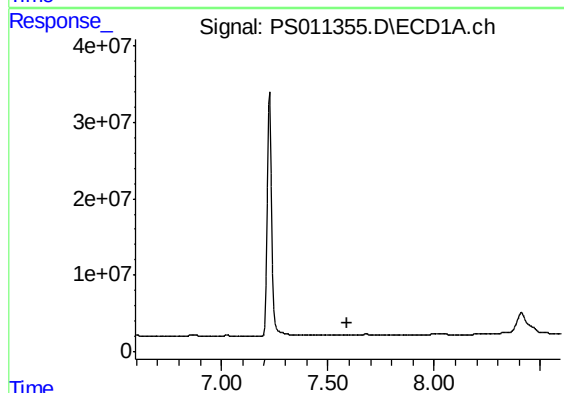

#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.594 min
Response: 0
Conc: N.D.

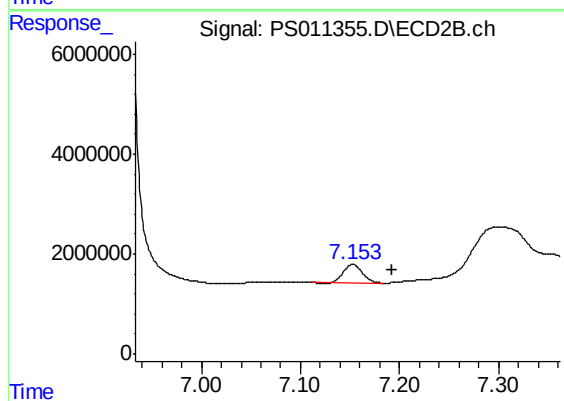

#6 MCPP

R.T.: 7.153 min
Delta R.T.: -0.039 min
Response: 4899041
Conc: 2.57 ug/ml