

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072320\
 Data File : PS011359.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2020 21:58
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 03:46:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.225	6.917	442.3E6	303.2E6	455.849	538.537
Target Compounds							
2) T	3,5-DICHL...	6.483	0.000	8074617	0	6.034	N.D. #
5) T	DICAMBA	0.000	7.153	0	6199450	N.D.	2.707
6) T	MCP	0.000	7.153	0	6199450	N.D.	3.249
10) T	Pentachlo...	0.000	8.437	0	3124745	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.799	0	1223939	N.D.	<MDL
15) T	Picloram	10.993	11.026	2544884	5718766	<MDL	1.308 #
16) T	DCPA	0.000	10.943	0	1512344	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072320\
Data File : PS011359.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2020 21:58
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 03:46:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
Quant Title : 8080.M
QLast Update : Mon Jul 13 16:10:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

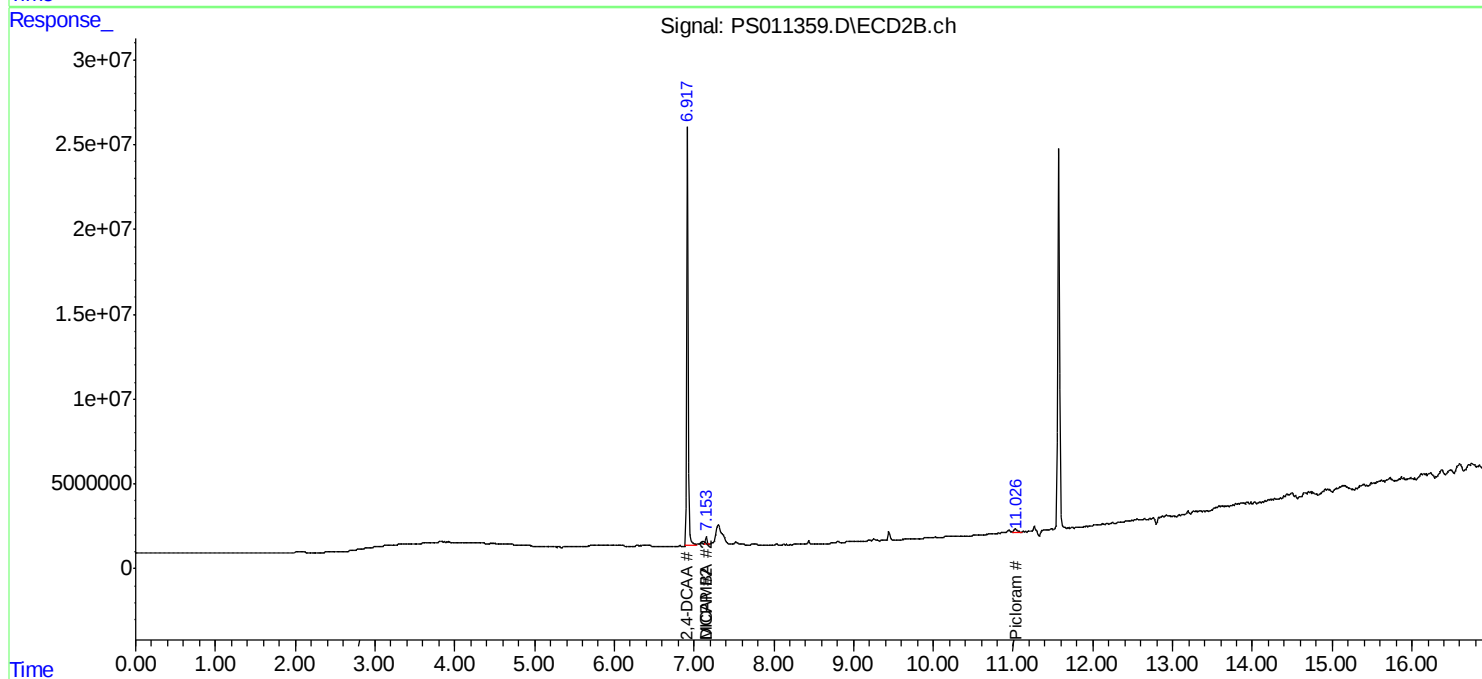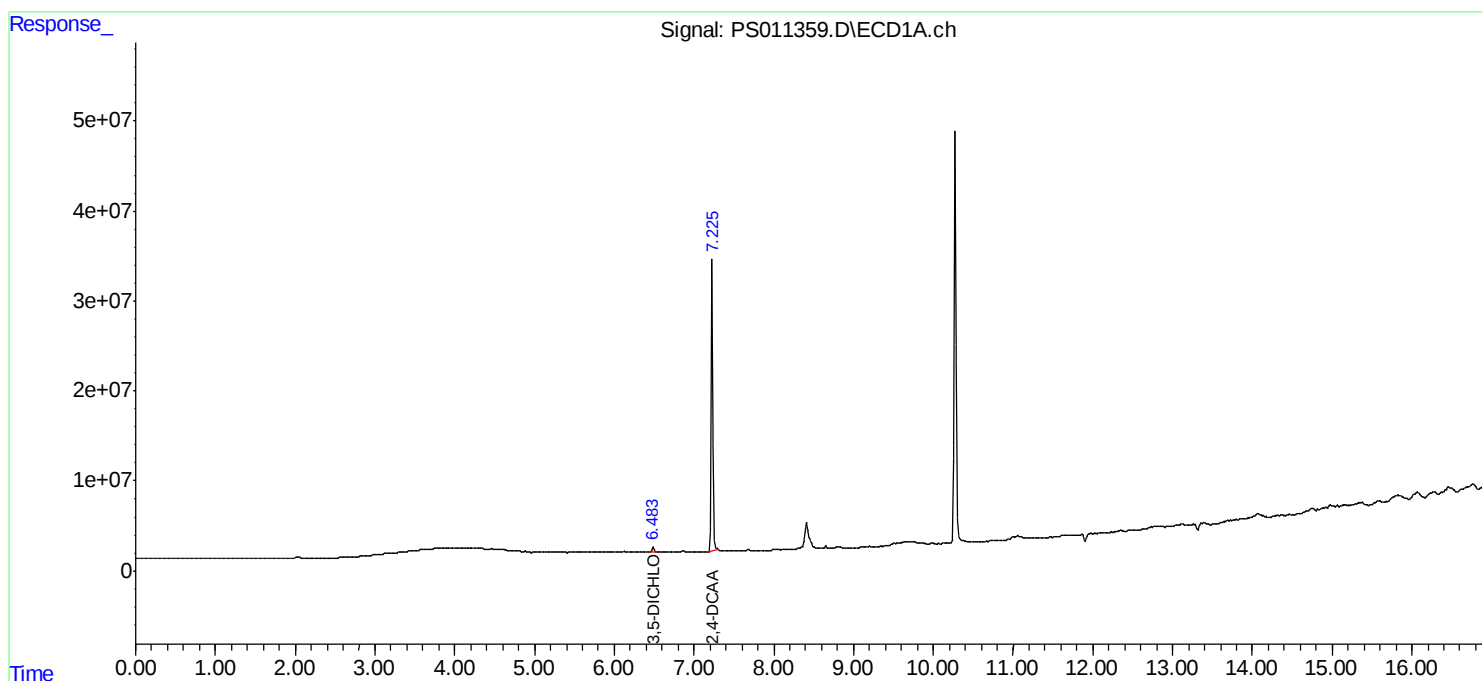


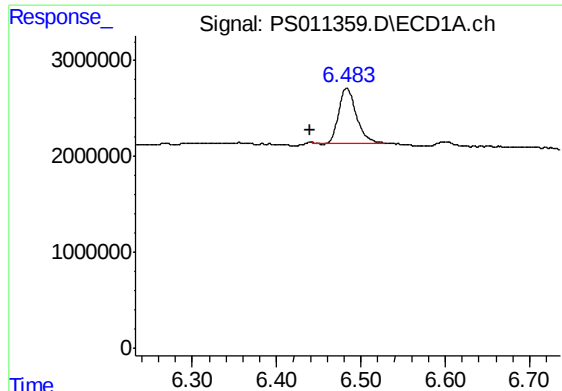

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.483 min
Delta R.T.: 0.044 min
Response: 8074617
Conc: 6.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

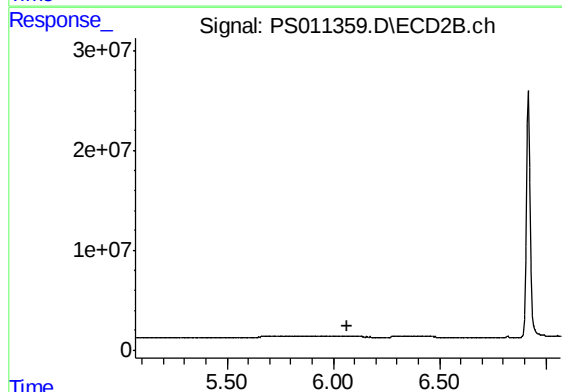


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.069 min
Response: 0
Conc: N.D.

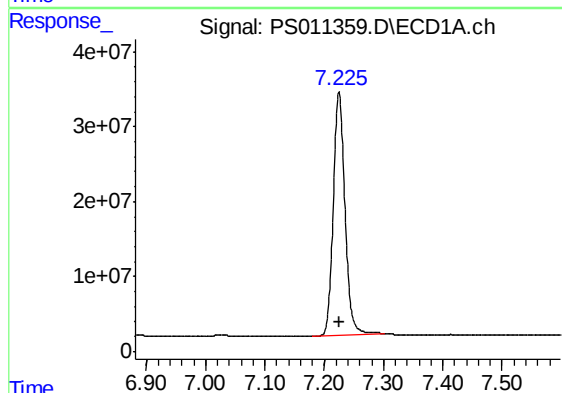


#4 2,4-DCAA

R.T.: 7.225 min
Delta R.T.: -0.001 min
Response: 442327546
Conc: 455.85 ng/ml

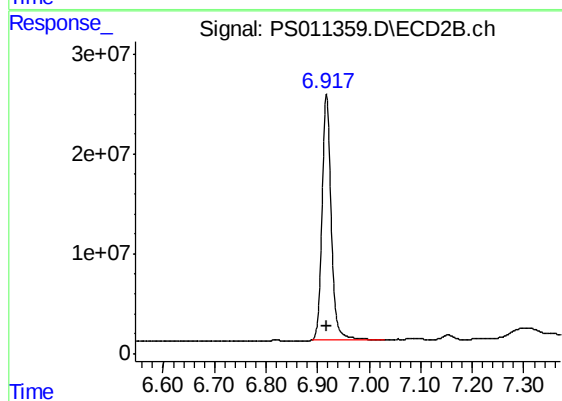

#4 2,4-DCAA


R.T.: 6.917 min
Delta R.T.: -0.002 min
Response: 303208218
Conc: 538.54 ng/ml

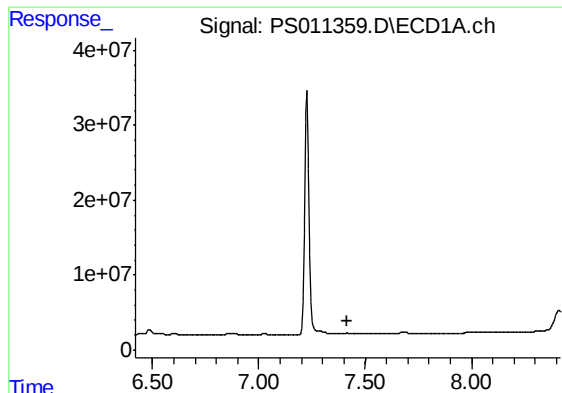

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

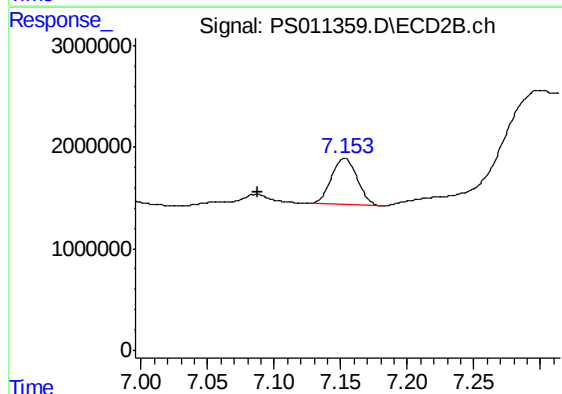


#5 DICAMBA

R.T.: 7.153 min
Delta R.T.: 0.065 min
Response: 6199450
Conc: 2.71 ng/ml

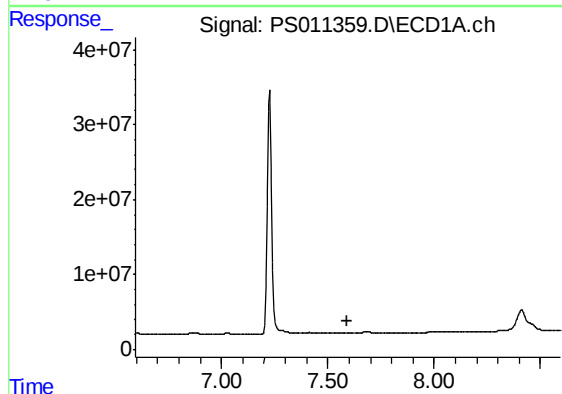


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.594 min
Response: 0
Conc: N.D.

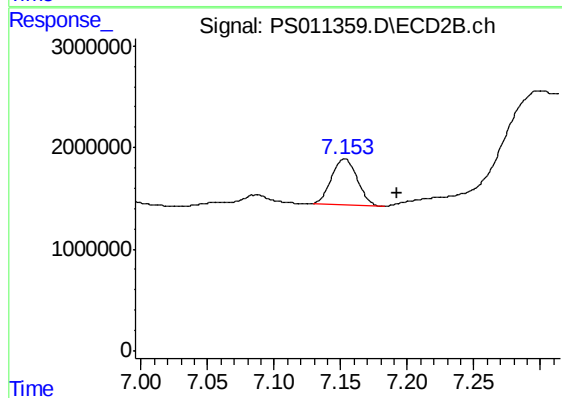

#6 MCPP


R.T.: 7.153 min
Delta R.T.: -0.039 min
Response: 6199450
Conc: 3.25 ug/ml

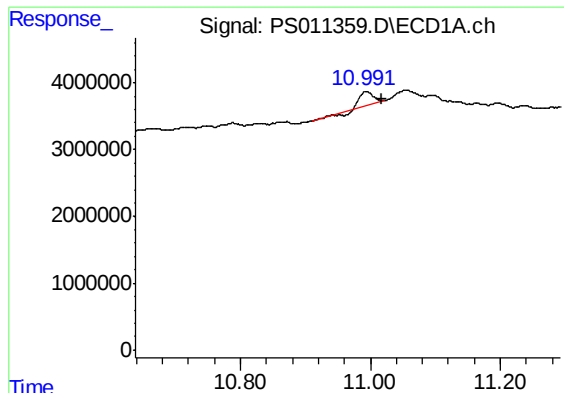

#15 Picloram

R.T.: 10.993 min
Delta R.T.: -0.026 min
Response: 2544884
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

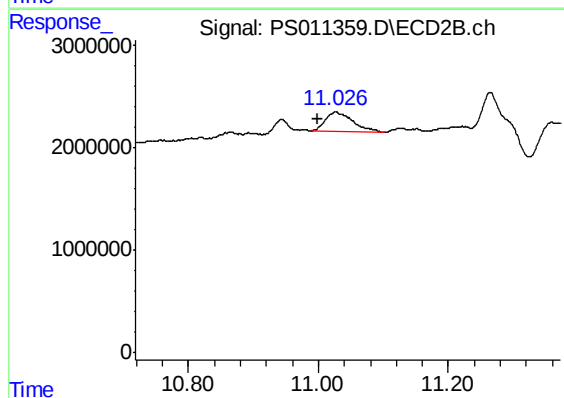

#15 Picloram

R.T.: 11.026 min
Delta R.T.: 0.027 min
Response: 5718766
Conc: 1.31 ng/ml