

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072420\
 Data File : PS011362.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2020 08:36
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 12:24:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.226	6.917	418.9E6	288.7E6	431.662	512.805
Target Compounds							
9) T	2,4-D	0.000	7.963	0	7211199	N.D.	9.619
12) T	2,4,5-T	9.421	0.000	17822204	0	3.532	N.D. #
15) T	Picloram	11.051	11.021	93799678	98959517	14.866	22.628 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072420\
Data File : PS011362.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2020 08:36
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 12:24:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
Quant Title : 8080.M
QLast Update : Mon Jul 13 16:10:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

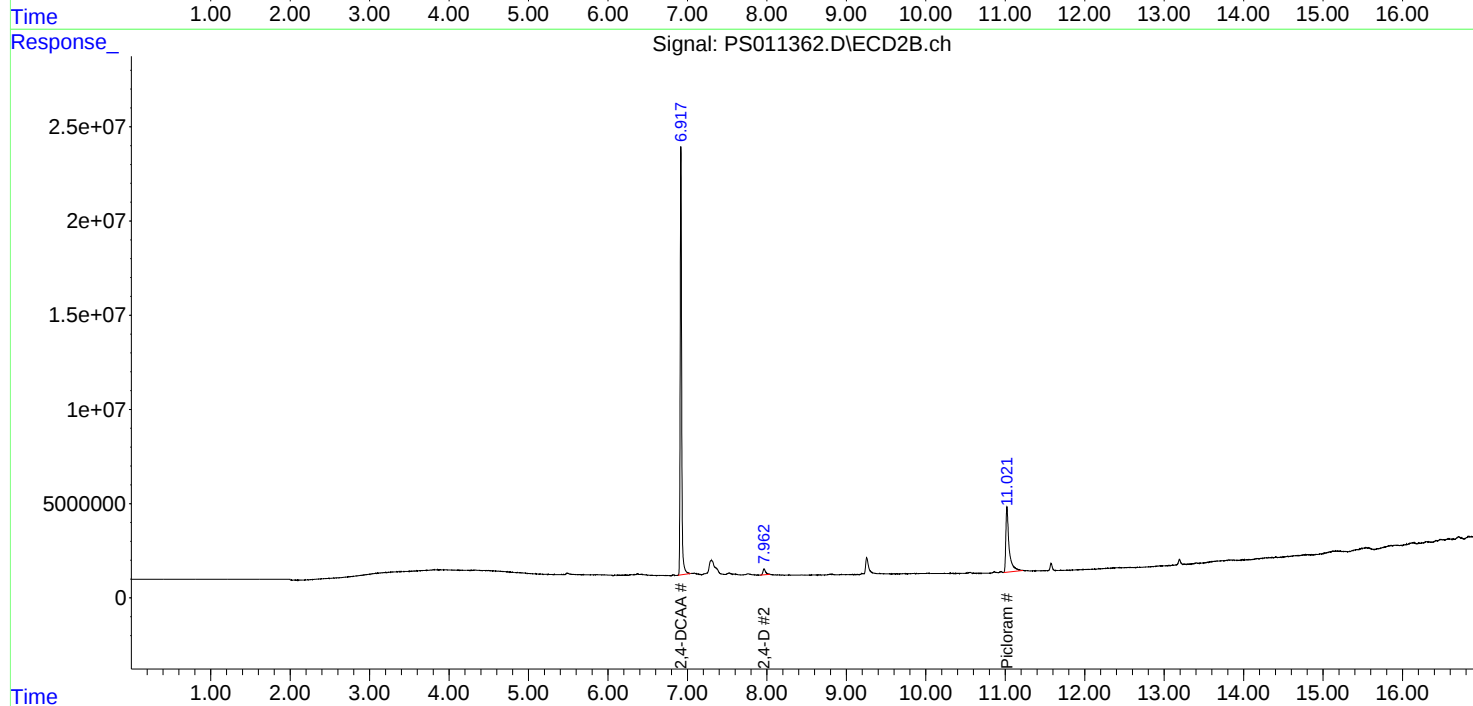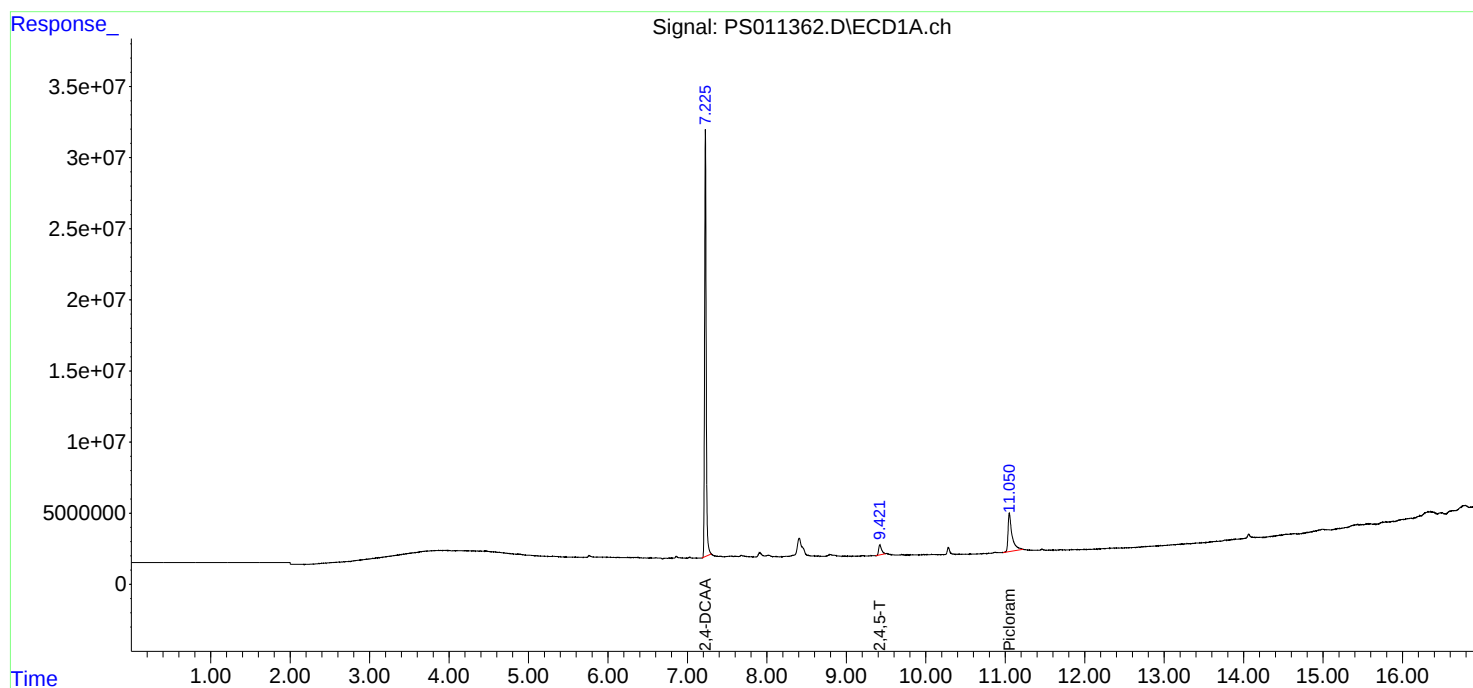


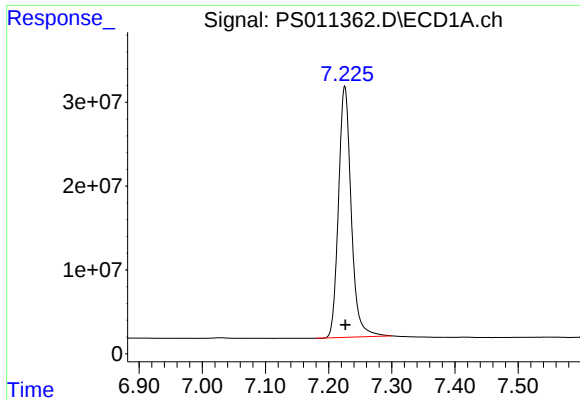

#4 2,4-DCAA


R.T.: 7.226 min
Delta R.T.: 0.000 min
Response: 418858072
Conc: 431.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

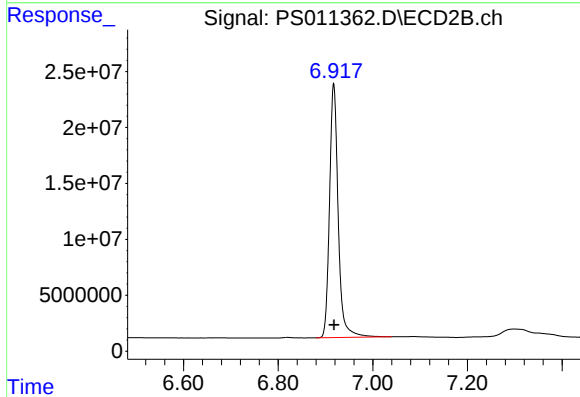


#4 2,4-DCAA

R.T.: 6.917 min
Delta R.T.: -0.001 min
Response: 288720823
Conc: 512.81 ng/ml

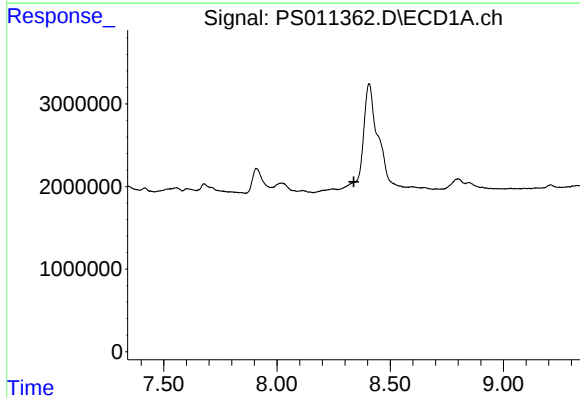


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.339 min
Response: 0
Conc: N.D.

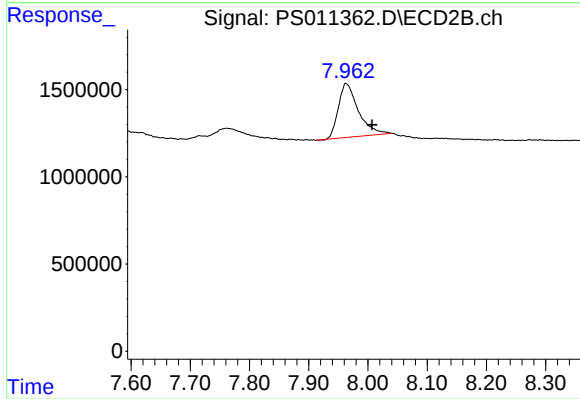

#9 2,4-D


R.T.: 7.963 min
Delta R.T.: -0.044 min
Response: 7211199
Conc: 9.62 ng/ml

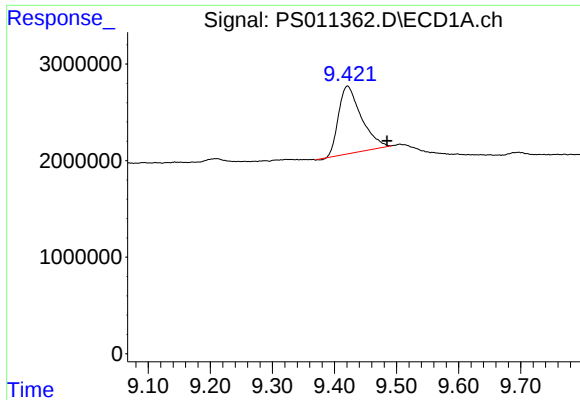

#12 2,4,5-T


R.T.: 9.421 min
Delta R.T.: -0.063 min
Response: 17822204
Conc: 3.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

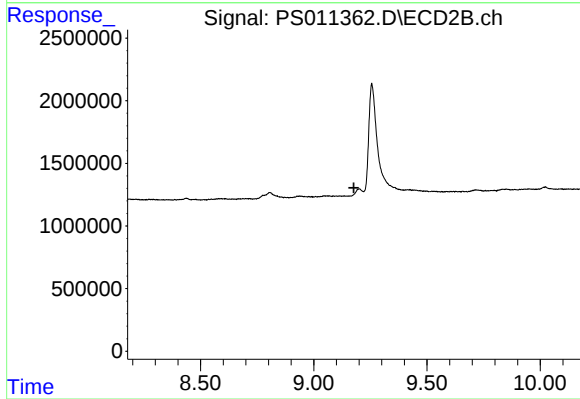


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.177 min
Response: 0
Conc: N.D.

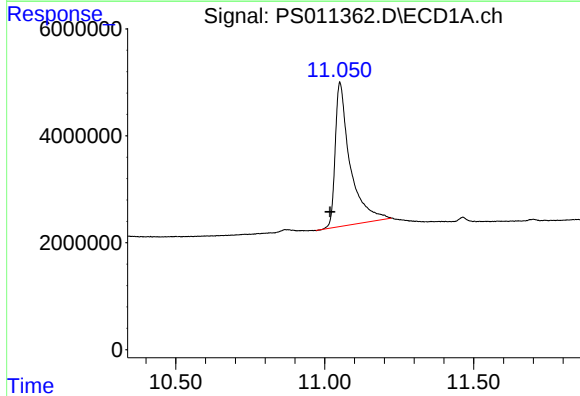

#15 Picloram

R.T.: 11.051 min
Delta R.T.: 0.033 min
Response: 93799678
Conc: 14.87 ng/ml

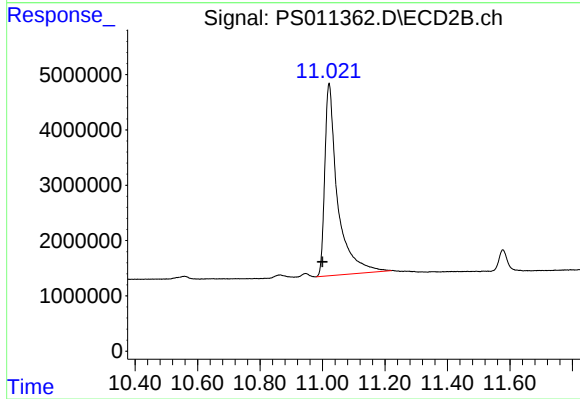

#15 Picloram

R.T.: 11.021 min
Delta R.T.: 0.022 min
Response: 98959517
Conc: 22.63 ng/ml