

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072423\
 Data File : PS023811.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2023 10:51
 Operator : AR\AJ
 Sample : 03670-01 (Sig #1); 003670-01 (Sig #2)
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 N48909

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/25/2023
 Supervised By : Ankita Jodhani 07/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 14:00:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072023.M
 Quant Title : 8080.M
 QLast Update : Thu Jul 20 19:21:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.373	6.809	1013.1E6	343.7E6	510.997m	505.405

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072423\
Data File : PS023811.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2023 10:51
Operator : AR\AJ
Sample : 03670-01 (Sig #1); 003670-01 (Sig #2)
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
N48909


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/25/2023
Supervised By : Ankita Jodhani 07/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 14:00:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072023.M
Quant Title : 8080.M
QLast Update : Thu Jul 20 19:21:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

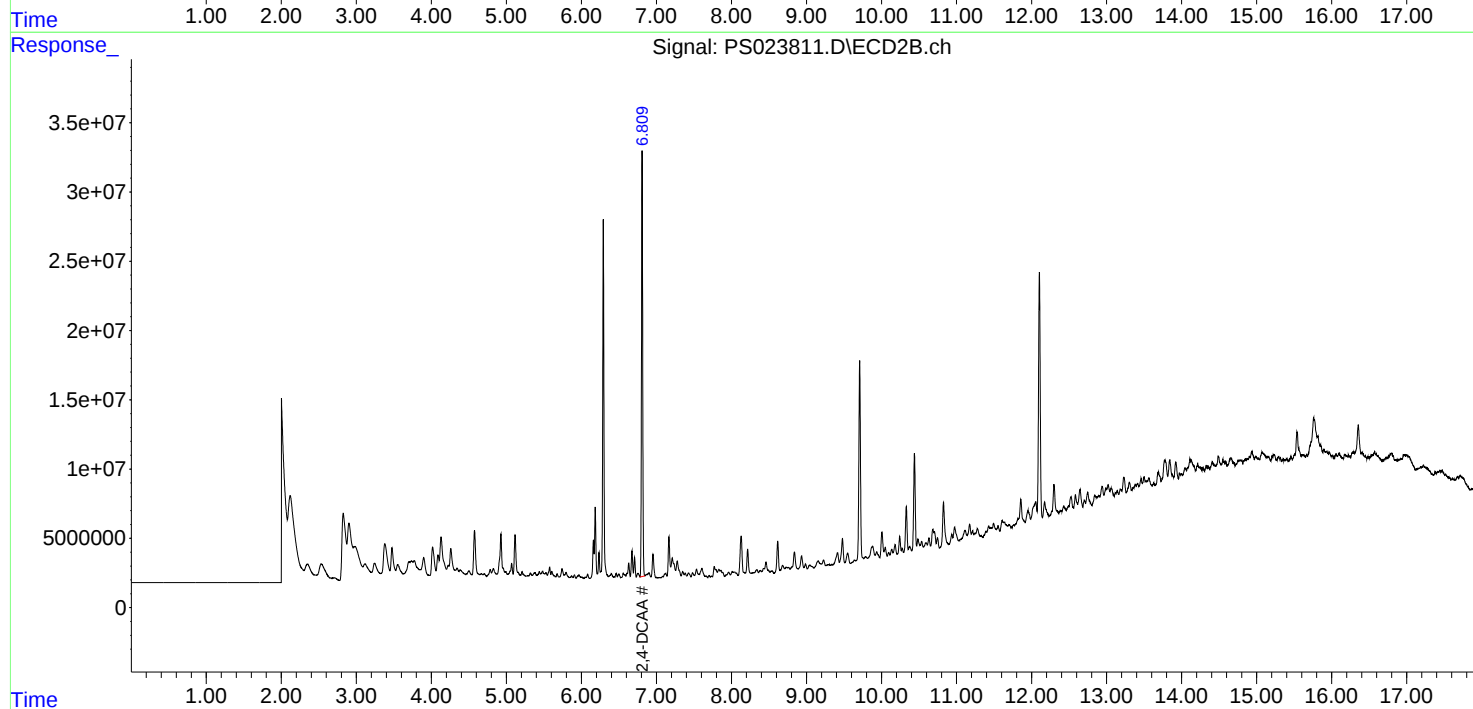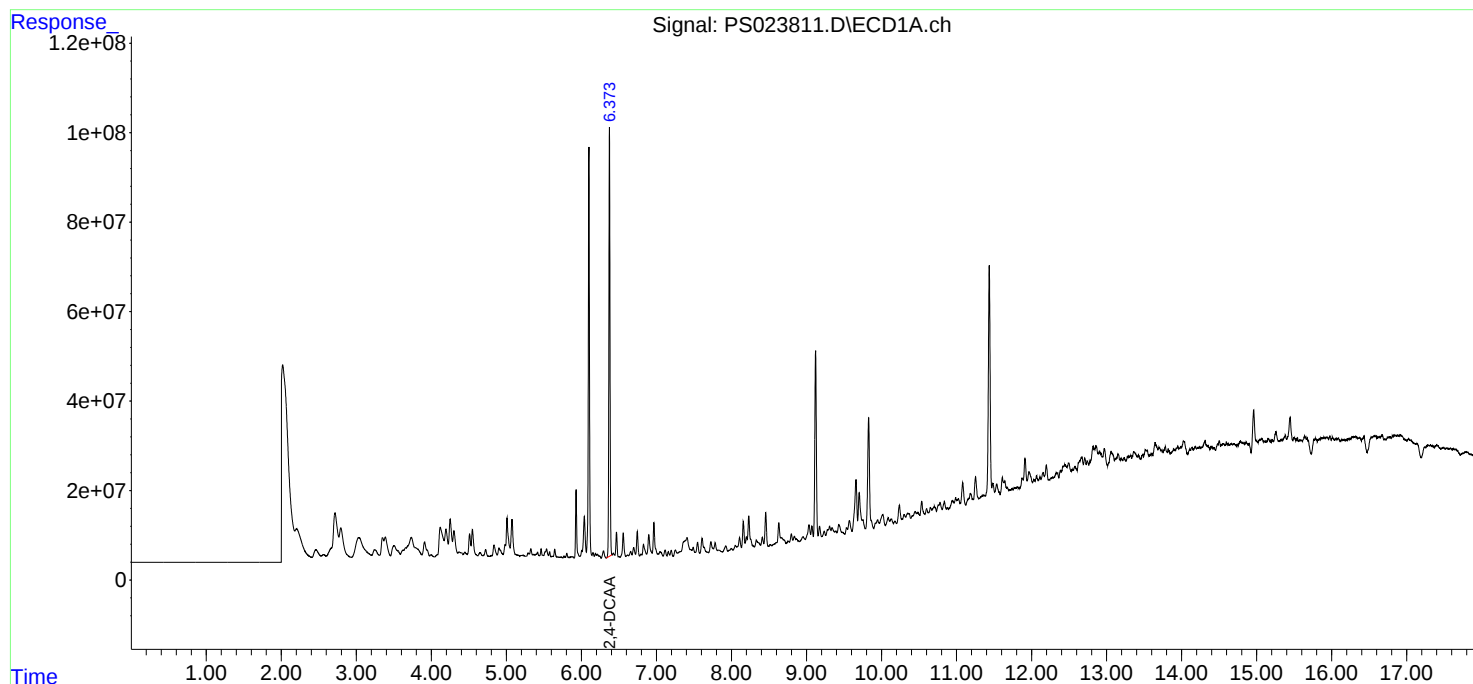

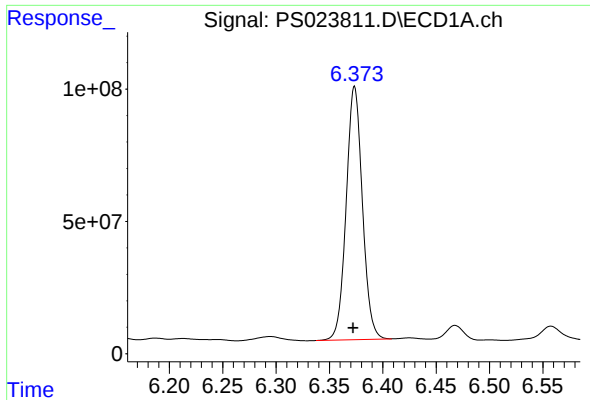


#4 2,4-DCAA

R.T.: 6.373 min
Delta R.T.: 0.001 min
Response: 1013122285
Conc: 511.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
N48909

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/25/2023
Supervised By :Ankita Jodhani 07/25/2023

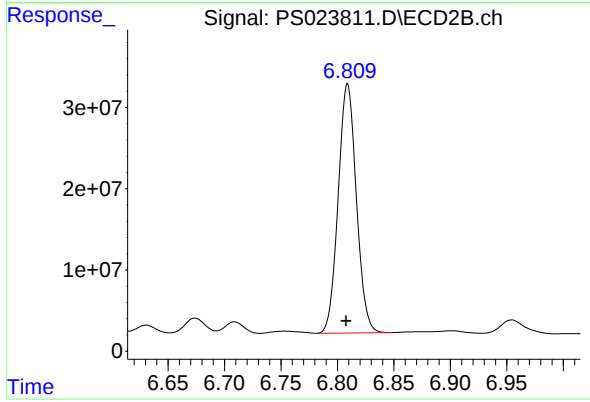

#4 2,4-DCAA

R.T.: 6.809 min
Delta R.T.: 0.001 min
Response: 343725051
Conc: 505.40 ng/ml