

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072425\
 Data File : PS031242.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2025 22:17
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 03:46:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072125.M
 Quant Title : 8080.M
 QLast Update : Tue Jul 22 03:18:42 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.320	7.764	1834.3E6	505.9E6	421.850	498.392
Target Compounds							
1) T	Dalapon	2.734f	2.663f	38732294	64965506	6.175	22.901 #
2) T	3,5-DICHL...	6.476	0.000	2269244	0	<MDL	N.D. #
3) T	4-Nitroph...	7.115	0.000	8601397	0	5.217	N.D. #
5) T	DICAMBA	7.505	7.984	1779545	4944556	<MDL	<MDL #
7) T	MCPA	7.867	8.282f	900079	63828080	<MDL	20.229 #
8) T	DICHLORPROP	0.000	8.683	0	2784932	N.D.	1.838
10) T	Pentachlo...	8.756	9.544	7827390	4131006	<MDL	<MDL #
11) T	2,4,5-TP ...	9.335	9.926	18866181	7250708	<MDL	<MDL #
12) T	2,4,5-T	9.634	10.366	4319331	5184874	<MDL	<MDL #
13) T	2,4-DB	10.241f	0.000	852407	0	<MDL	N.D. #
14) T	DINOSEB	11.417	11.308	3165740	2413059	<MDL	<MDL #
15) T	Picloram	11.235	0.000	10212721	0	<MDL	N.D. #
16) T	DCPA	11.717	0.000	8379553	0	<MDL	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072425\
Data File : PS031242.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2025 22:17
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 03:46:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072125.M
Quant Title : 8080.M
QLast Update : Tue Jul 22 03:18:42 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

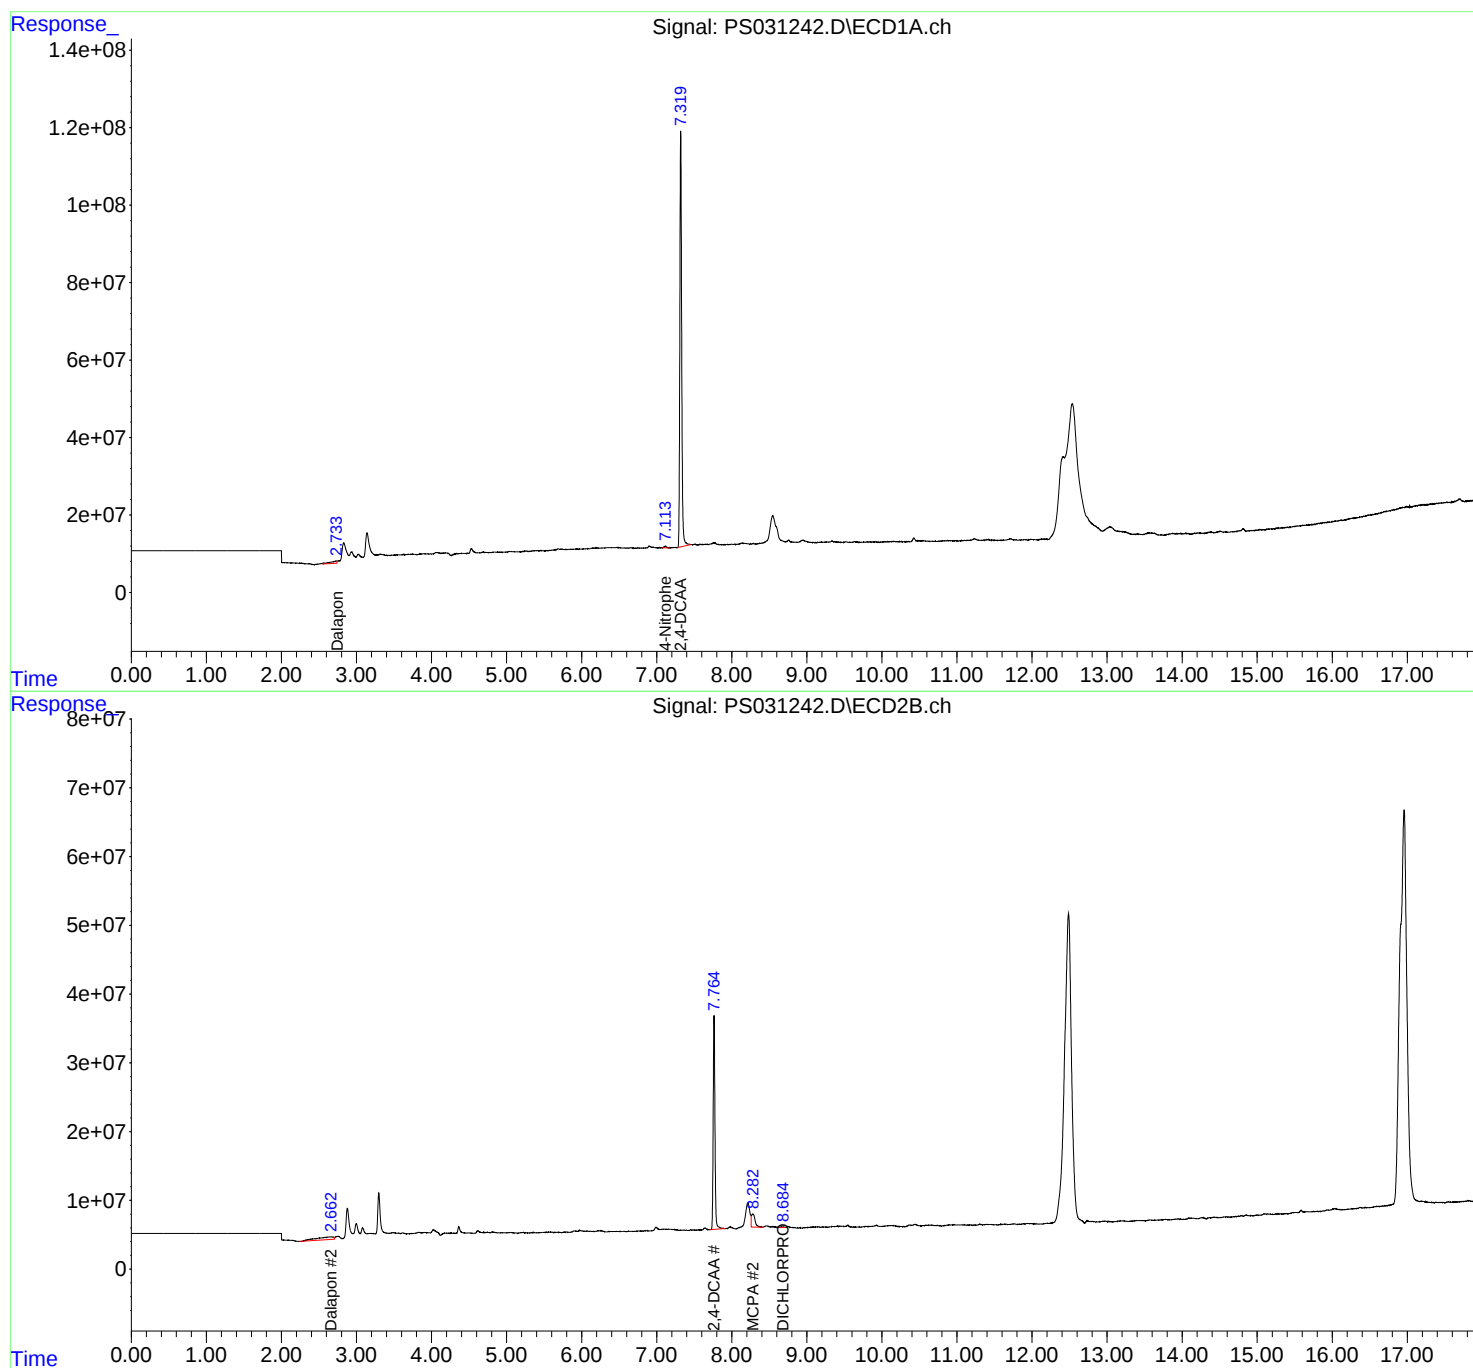


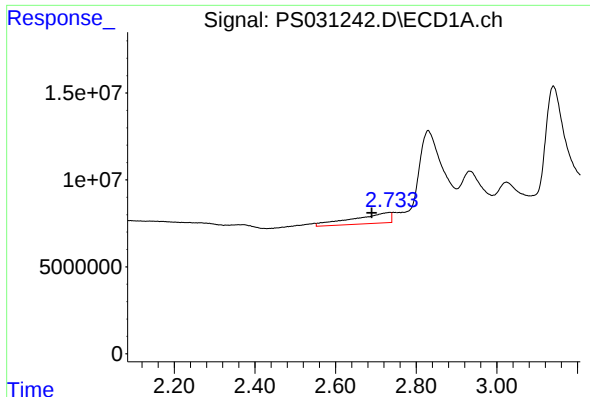

#1 Dalapon


R.T.: 2.734 min
Delta R.T.: 0.044 min
Response: 38732294
Conc: 6.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

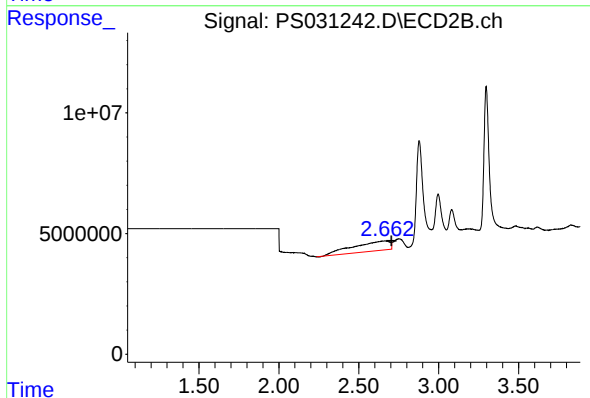


#1 Dalapon

R.T.: 2.663 min
Delta R.T.: -0.040 min
Response: 64965506
Conc: 22.90 ng/ml

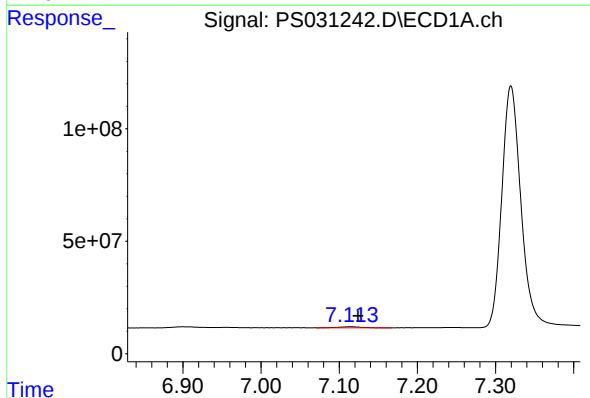


#3 4-Nitrophenol

R.T.: 7.115 min
Delta R.T.: -0.009 min
Response: 8601397
Conc: 5.22 ng/ml

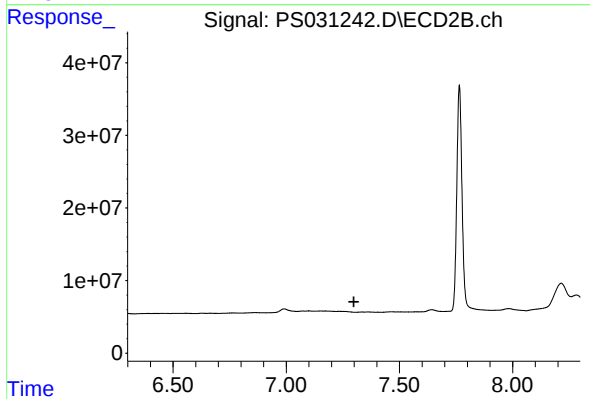

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.299 min
Response: 0
Conc: N.D.

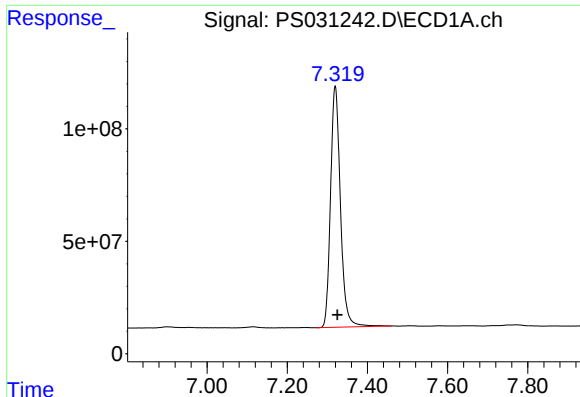

#4 2,4-DCAA


R.T.: 7.320 min
Delta R.T.: -0.005 min
Response: 1834308835
Conc: 421.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

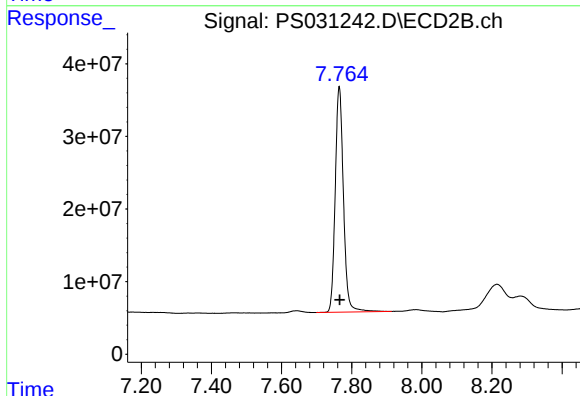


#4 2,4-DCAA

R.T.: 7.764 min
Delta R.T.: -0.002 min
Response: 505852351
Conc: 498.39 ng/ml

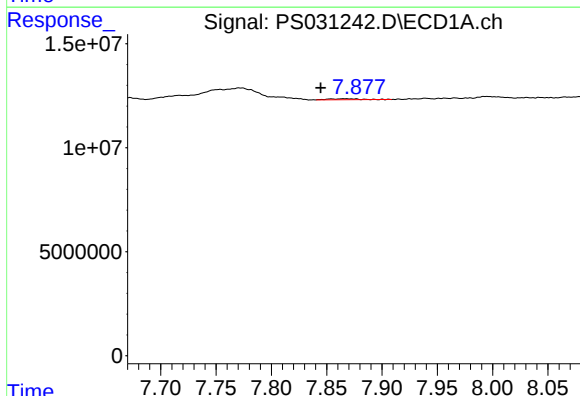


#7 MCPA

R.T.: 7.867 min
Delta R.T.: 0.022 min
Response: 900079
Conc: N.D.

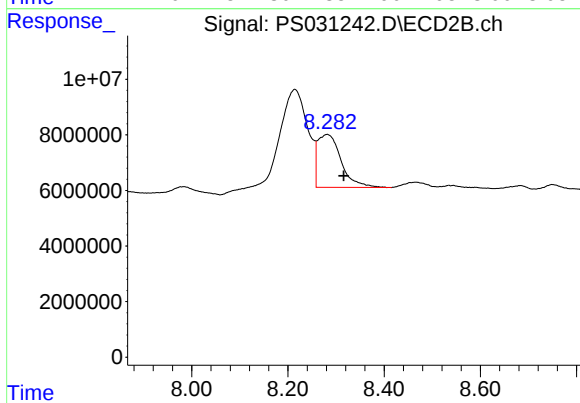

#7 MCPA


R.T.: 8.282 min
Delta R.T.: -0.034 min
Response: 63828080
Conc: 20.23 ug/ml

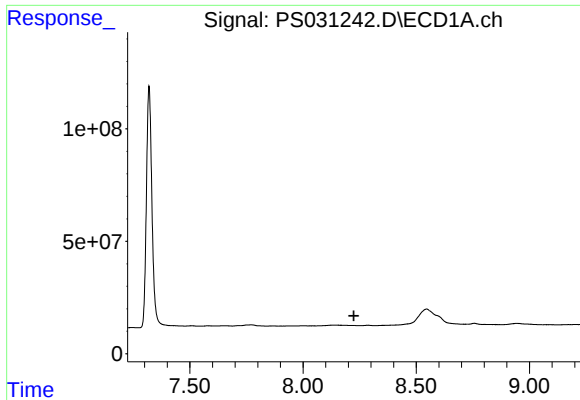

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.224 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

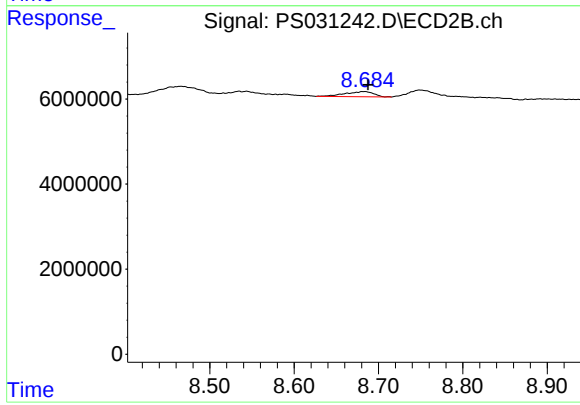

#8 DICHLORPROP

R.T.: 8.683 min
Delta R.T.: -0.005 min
Response: 2784932
Conc: 1.84 ng/ml