

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072425\
 Data File : PS031245.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2025 00:17
 Operator : AR\AJ
 Sample : Q2481-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CC0627-AOXL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/25/2025
 Supervised By :mohammad ahmed 07/26/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 03:49:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072125.M
 Quant Title : 8080.M
 QLast Update : Tue Jul 22 03:18:42 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.319	7.763	1731.3E6	562.6E6	398.169	554.293m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072425\
Data File : PS031245.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2025 00:17
Operator : AR\AJ
Sample : Q2481-15
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
CC0627-AOXL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2025
Supervised By :mohammad ahmed 07/26/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 03:49:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072125.M
Quant Title : 8080.M
QLast Update : Tue Jul 22 03:18:42 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

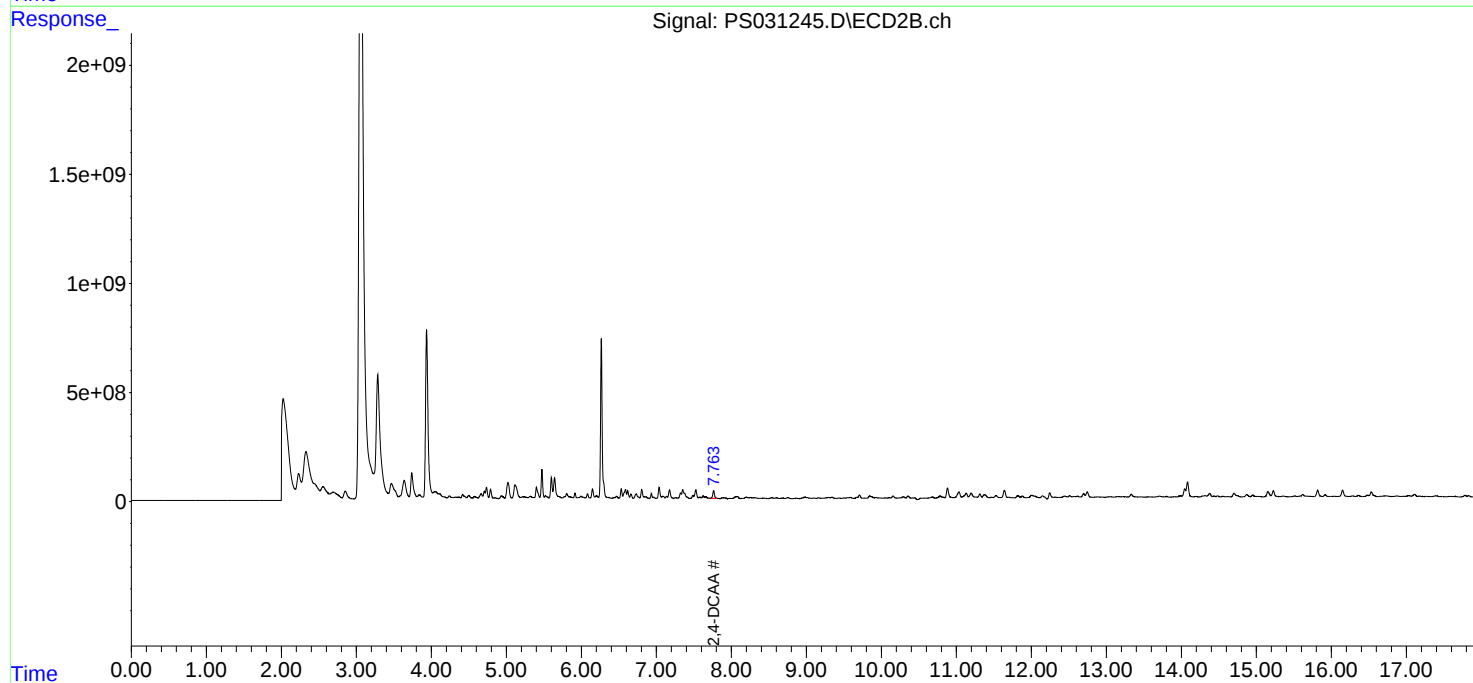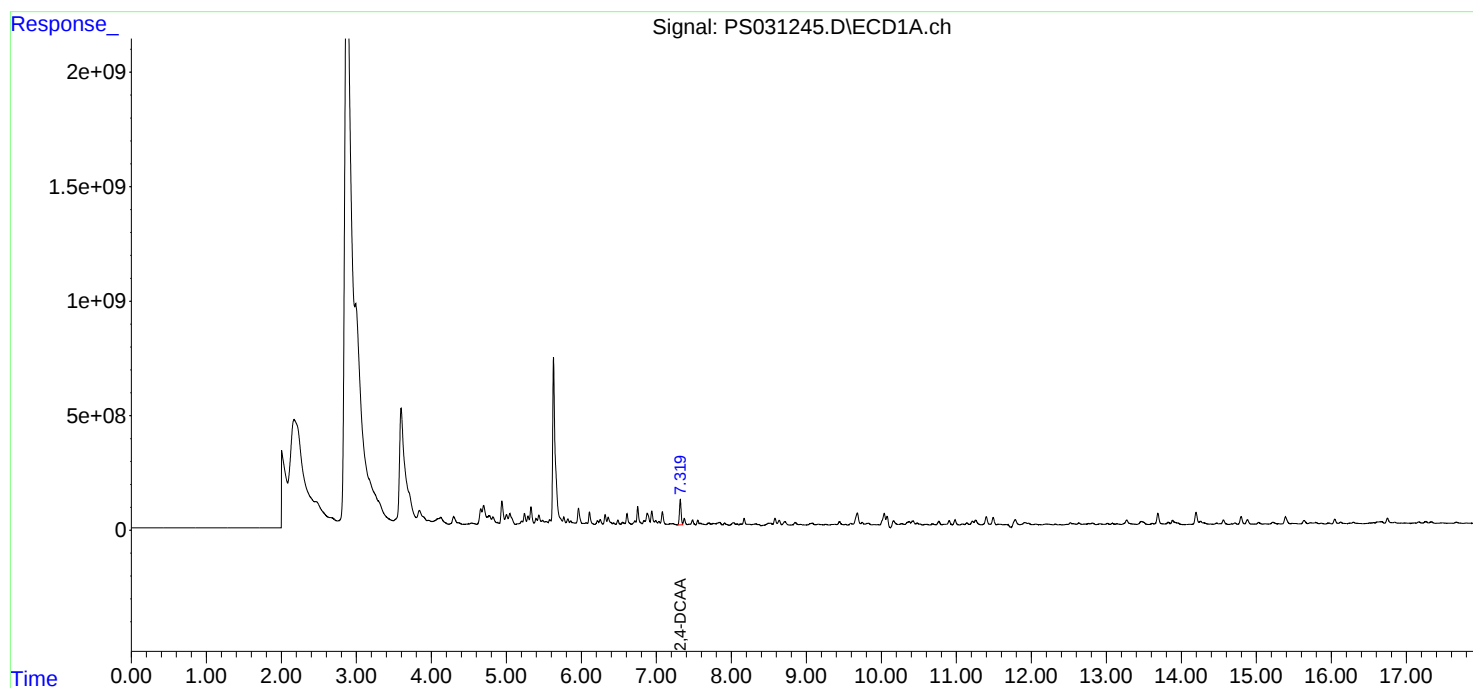

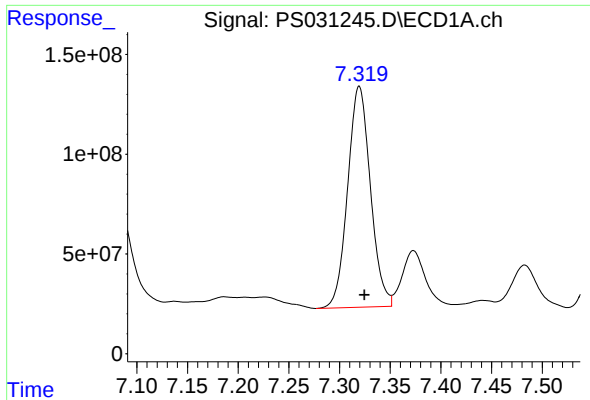


#4 2,4-DCAA

R.T.: 7.319 min
Delta R.T.: -0.005 min
Response: 1731339920
Conc: 398.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
CC0627-AOXL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2025
Supervised By :mohammad ahmed 07/26/2025

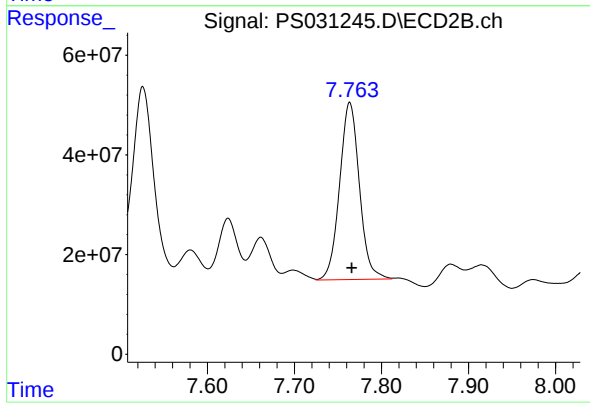

#4 2,4-DCAA

R.T.: 7.763 min
Delta R.T.: -0.003 min
Response: 562590080
Conc: 554.29 ng/ml m