

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS072425\  
Data File : PS031253.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 25 Jul 2025 04:18  
Operator : AR\AJ  
Sample : Q2481-13 10X  
Misc :  
ALS Vial : 28 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
CC0627-CLOXPL

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jul 25 07:10:59 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS072125.M  
Quant Title : 8080.M  
QLast Update : Tue Jul 22 03:18:42 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

-----  
System Monitoring Compounds

Target Compounds  
-----



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS072425\  
Data File : PS031253.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 25 Jul 2025 04:18  
Operator : AR\AJ  
Sample : Q2481-13 10X  
Misc :  
ALS Vial : 28 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
CC0627-CLOXPL

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jul 25 07:10:59 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS072125.M  
Quant Title : 8080.M  
QLast Update : Tue Jul 22 03:18:42 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

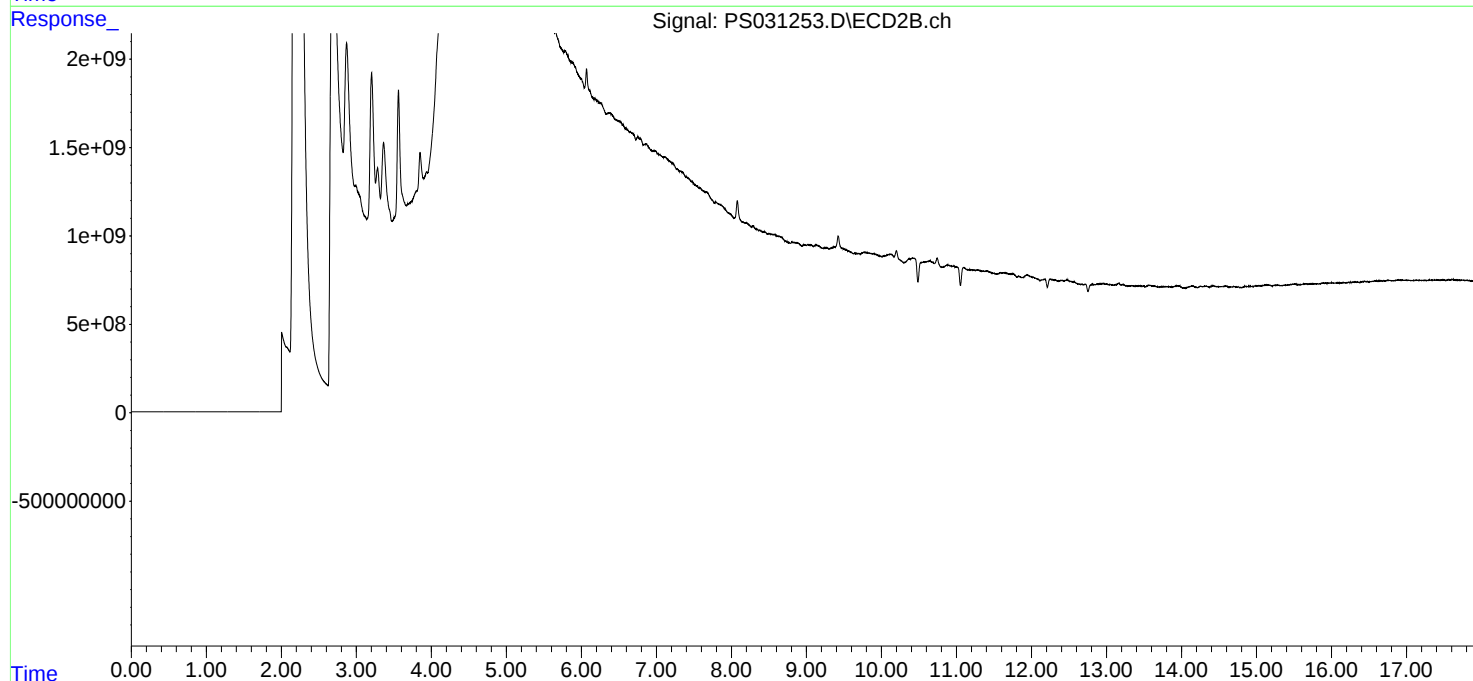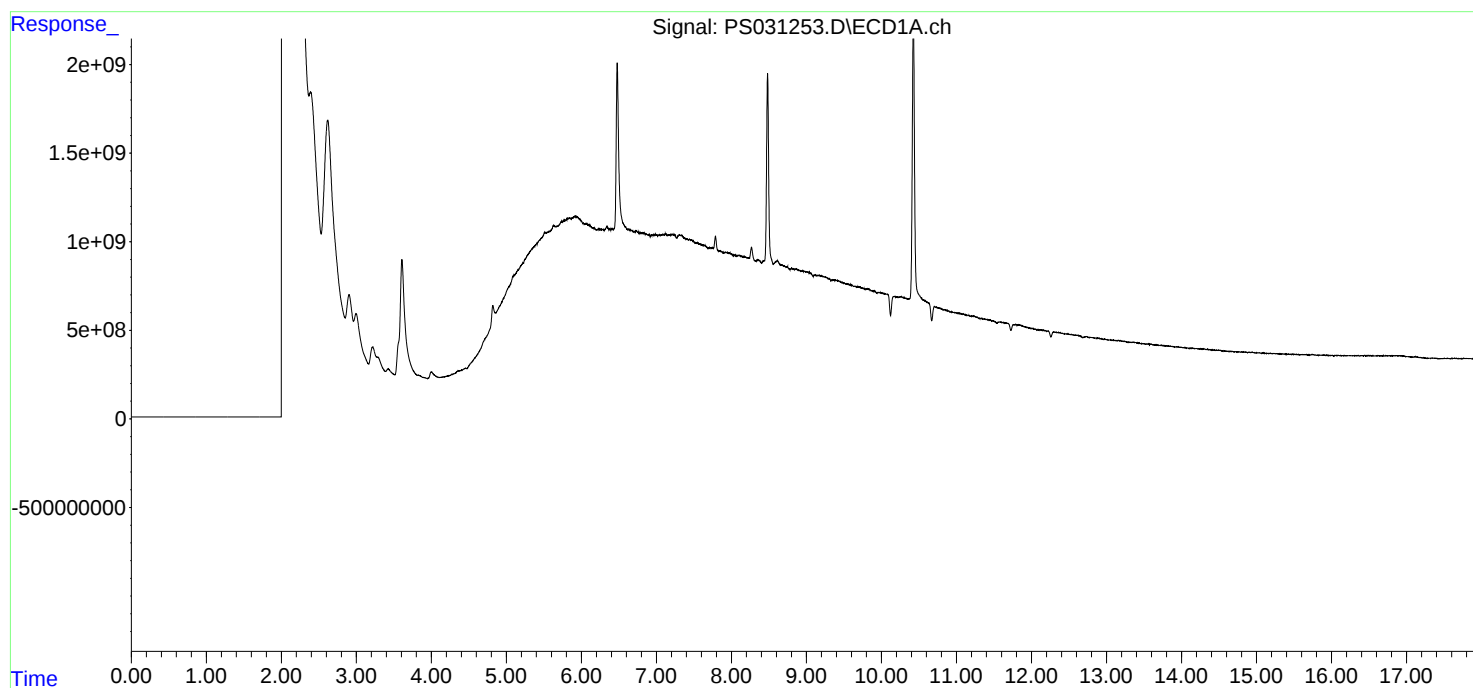


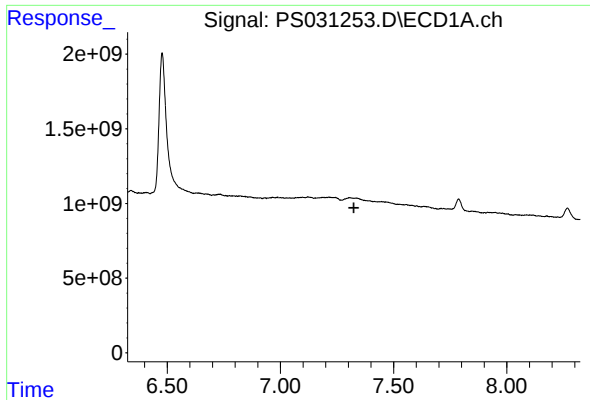

#4 2,4-DCAA

R.T.: 0.000 min  
Exp R.T. : 7.325 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
CC0627-CLOXPL

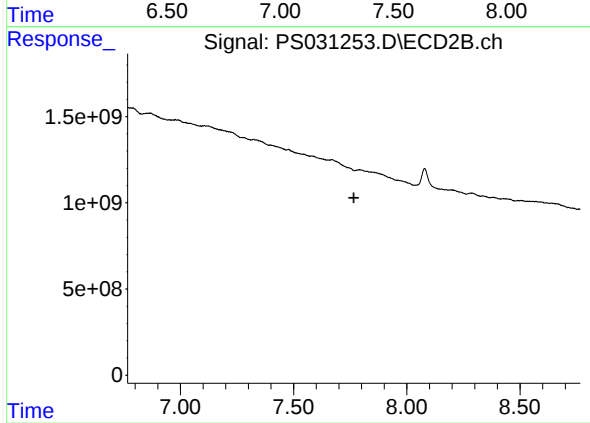

#4 2,4-DCAA

R.T.: 0.000 min  
Exp R.T. : 7.766 min  
Response: 0  
Conc: N.D.