

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072618\
 Data File : PS001255.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2018 15:24
 Operator : UA
 Sample : J4140-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 00:45:32 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.619	11.038	84095913	82916643	453.225	455.899
Target Compounds							
1) T	Dalapon	2.965	2.398	2890030	3484916	12.188	15.293 #
5) T	DICAMBA	11.986	11.283	2403167	11579149	3.342	16.894 #
6) T	MCPD	12.313	0.000	12640620	0	25.150	N.D. #
7) T	MCPA	12.589	11.988	9493264	1253891	12.038	1.928 #
8) T	DICHLORPROP	13.125	0.000	3194562	0	17.501	N.D. #
9) T	2,4-D	0.000	12.879	0	1385861	N.D.	5.840 #
14) T	DINOSEB	0.000	15.735	0	21890570	N.D.	30.797 #
15) T	Picloram	0.000	16.982	0	37268126	N.D.	27.035 #
16) T	DCPA	17.764	16.982	15860843	37268126	11.748	25.804 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072618\
Data File : PS001255.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2018 15:24
Operator : UA
Sample : J4140-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 00:45:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

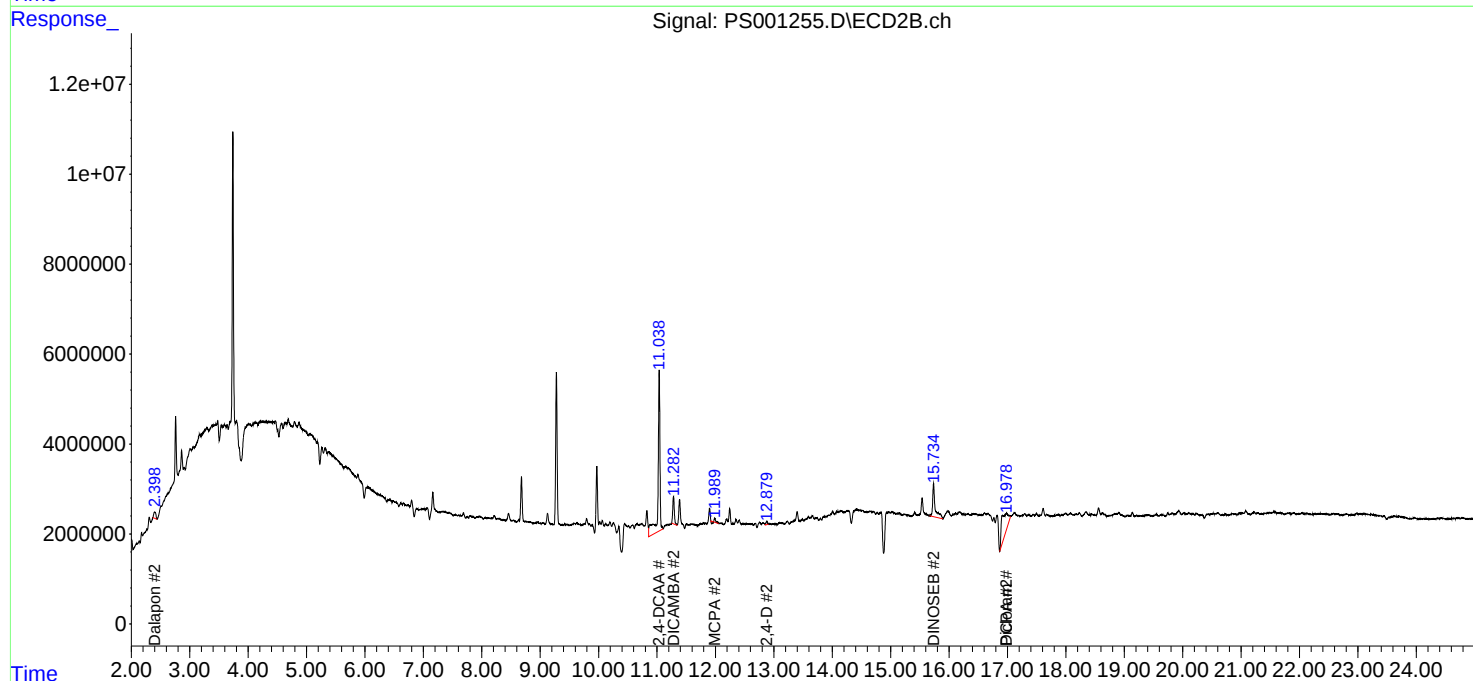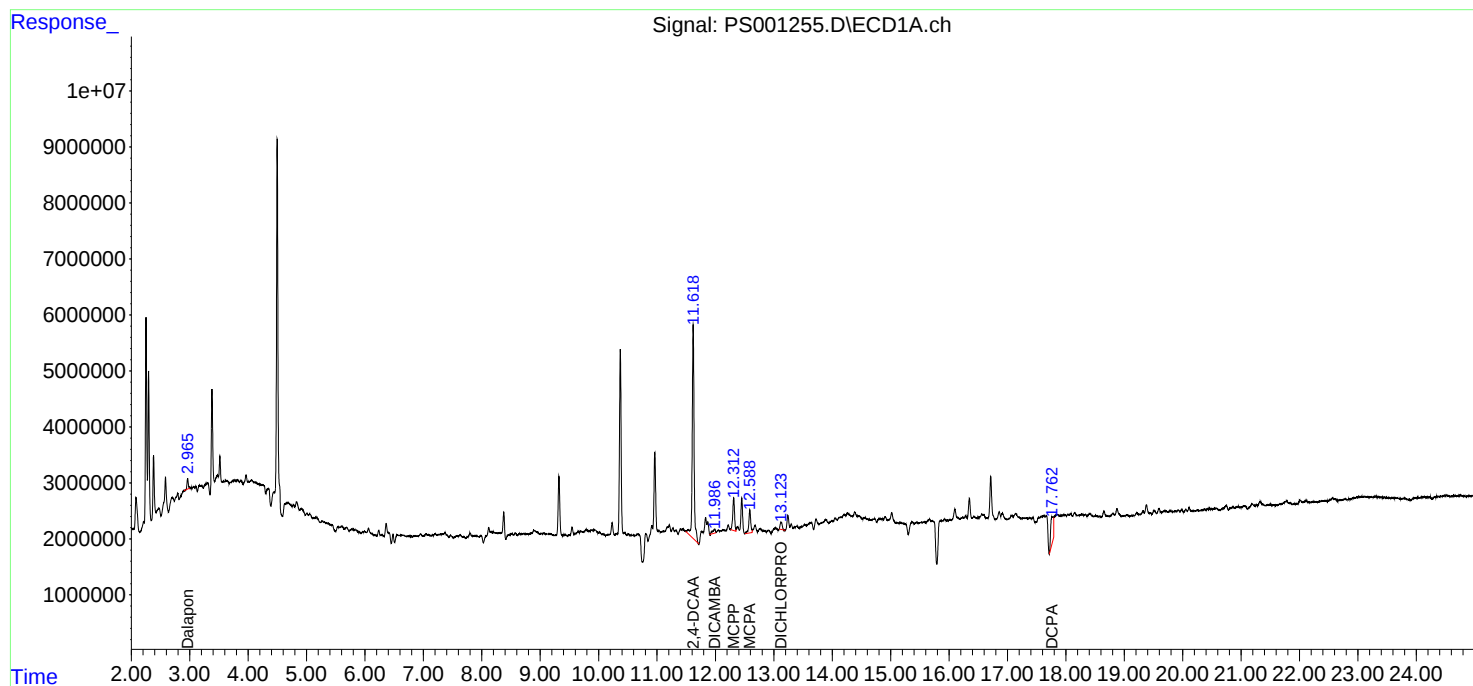


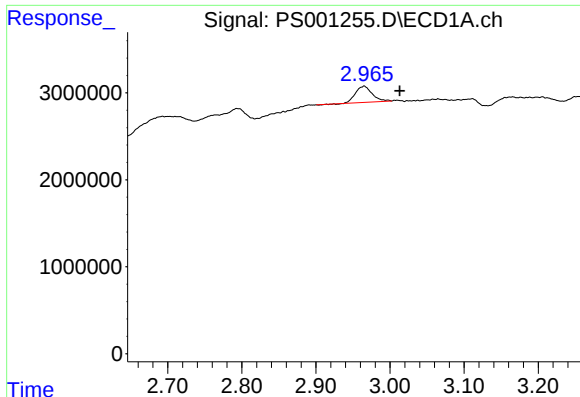

#1 Dalapon


R.T.: 2.965 min
Delta R.T.: -0.048 min
Response: 2890030
Conc: 12.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

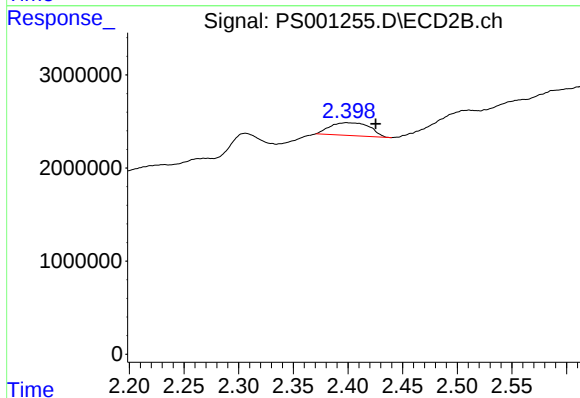


#1 Dalapon

R.T.: 2.398 min
Delta R.T.: -0.027 min
Response: 3484916
Conc: 15.29 ng/ml

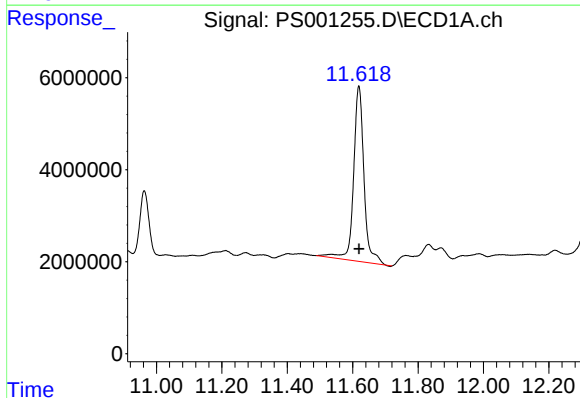


#4 2,4-DCAA

R.T.: 11.619 min
Delta R.T.: 0.000 min
Response: 84095913
Conc: 453.23 ng/ml

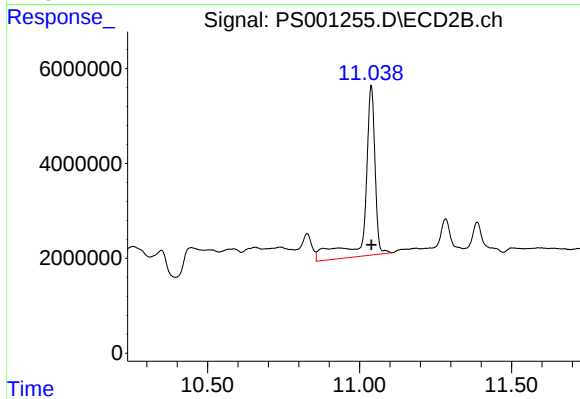

#4 2,4-DCAA


R.T.: 11.038 min
Delta R.T.: 0.000 min
Response: 82916643
Conc: 455.90 ng/ml

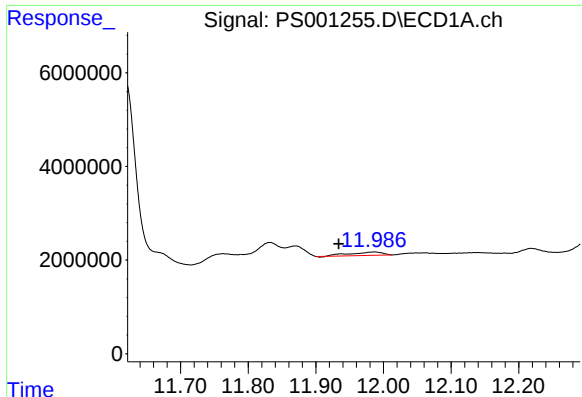

#5 DICAMBA


R.T.: 11.986 min
Delta R.T.: 0.053 min
Response: 2403167
Conc: 3.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

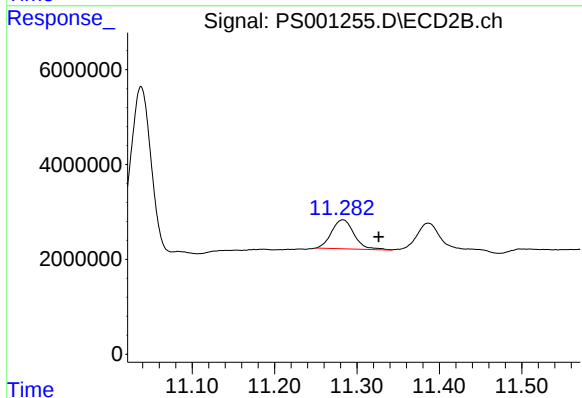


#5 DICAMBA

R.T.: 11.283 min
Delta R.T.: -0.044 min
Response: 11579149
Conc: 16.89 ng/ml

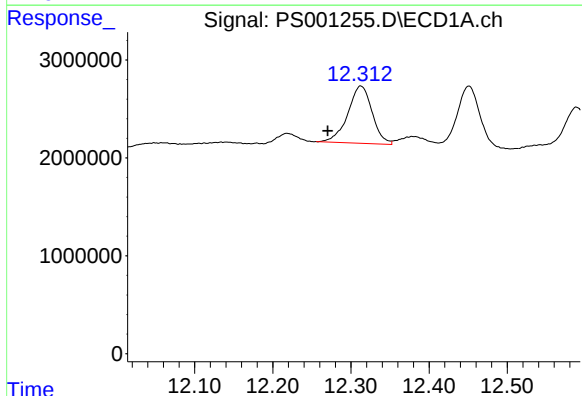


#6 MCP

R.T.: 12.313 min
Delta R.T.: 0.042 min
Response: 12640620
Conc: 25.15 ug/ml

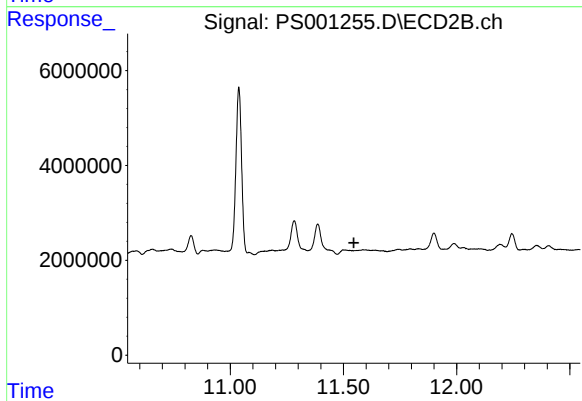

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.546 min
Response: 0
Conc: N.D.

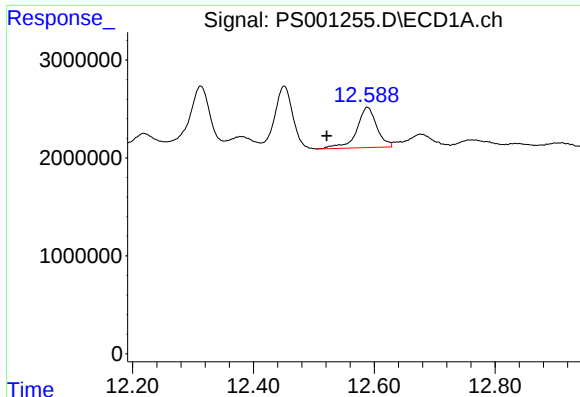

#7 MCPA


R.T.: 12.589 min
Delta R.T.: 0.067 min
Response: 9493264
Conc: 12.04 ug/ml

Instrument :
ECD_S
ClientSampleId :

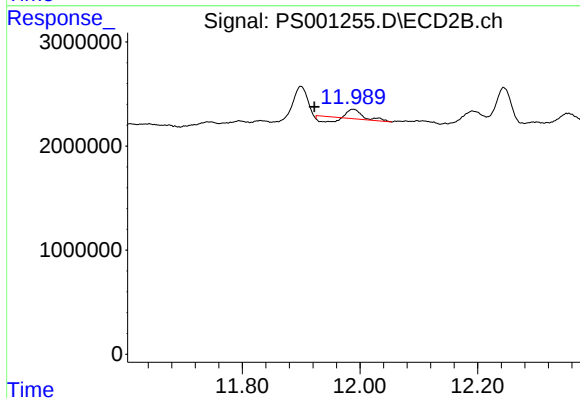


#7 MCPA

R.T.: 11.988 min
Delta R.T.: 0.066 min
Response: 1253891
Conc: 1.93 ug/ml

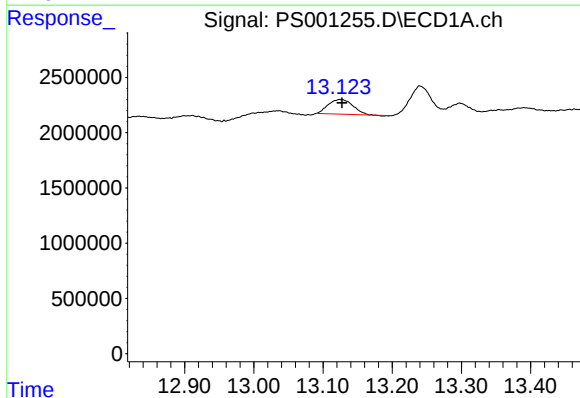


#8 DICHLORPROP

R.T.: 13.125 min
Delta R.T.: -0.003 min
Response: 3194562
Conc: 17.50 ng/ml

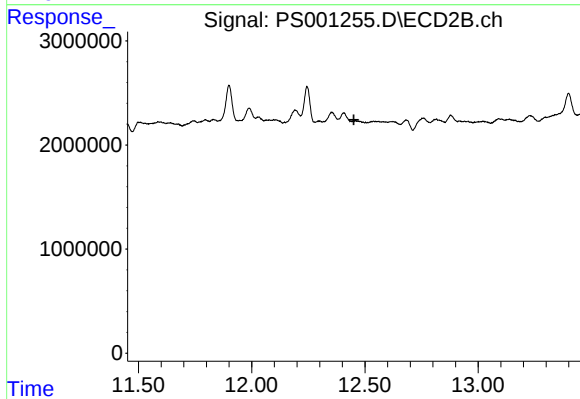

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.451 min
Response: 0
Conc: N.D.

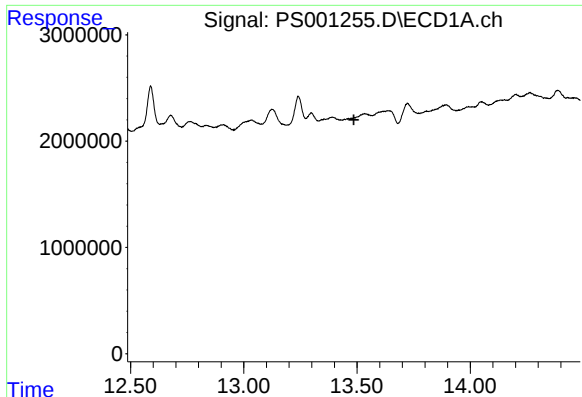

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

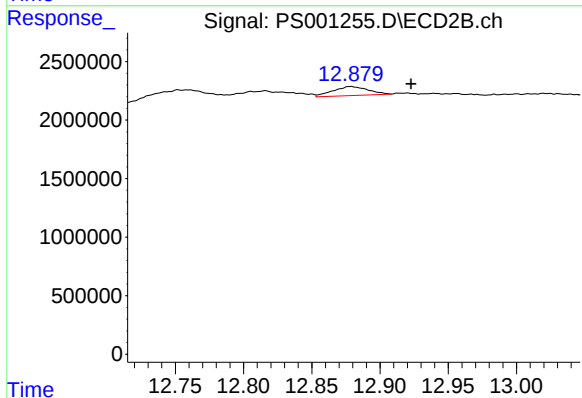


#9 2,4-D

R.T.: 12.879 min
Delta R.T.: -0.044 min
Response: 1385861
Conc: 5.84 ng/ml

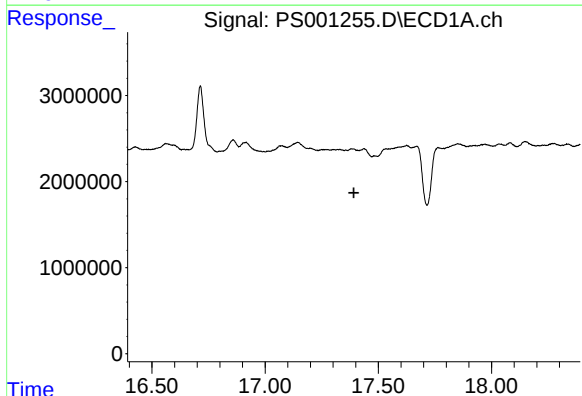


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.392 min
Response: 0
Conc: N.D.

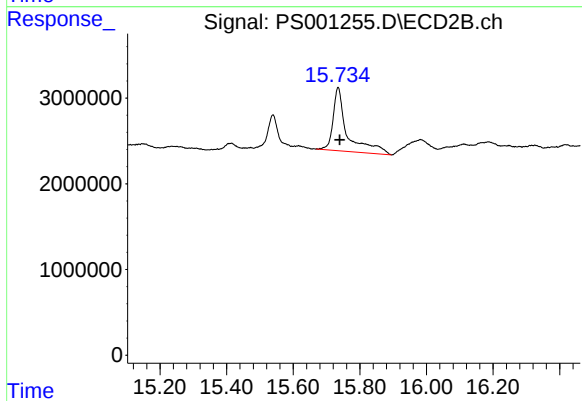

#14 DINOSEB


R.T.: 15.735 min
Delta R.T.: -0.005 min
Response: 21890570
Conc: 30.80 ng/ml

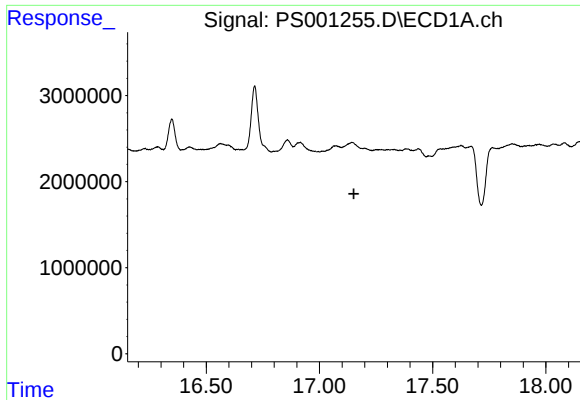

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 17.152 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

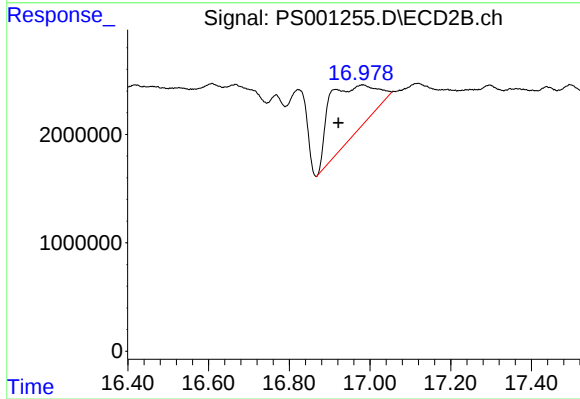


#15 Picloram

R.T.: 16.982 min
Delta R.T.: 0.060 min
Response: 37268126
Conc: 27.04 ng/ml

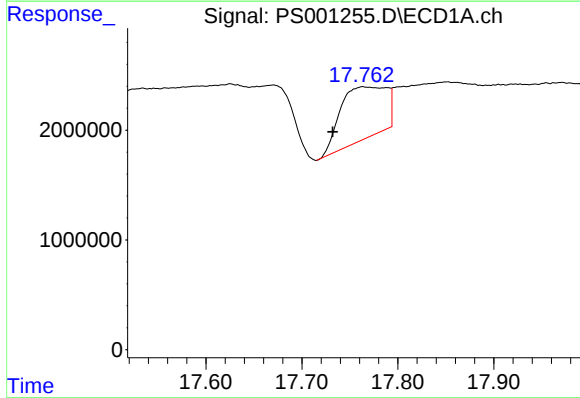

#16 DCPA

R.T.: 17.764 min
Delta R.T.: 0.032 min
Response: 15860843
Conc: 11.75 ng/ml

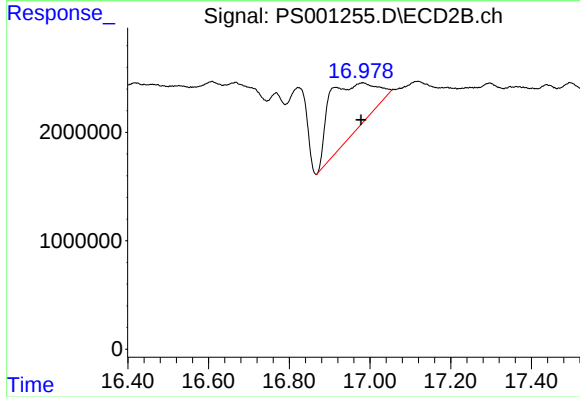

#16 DCPA

R.T.: 16.982 min
Delta R.T.: 0.004 min
Response: 37268126
Conc: 25.80 ng/ml