

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072618\
 Data File : PS001259.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2018 17:28
 Operator : UA
 Sample : J4140-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 00:47:06 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.623	11.042	66553246	43303296	358.681	238.094 #
Target Compounds							
1) T	Dalapon	2.968	2.407	4094567	4020171	17.268	17.642
5) T	DICAMBA	11.995	11.287	3517928	9589824	4.893	13.992 #
6) T	MCPD	12.317	0.000	10477944	0	20.847	N.D. #
7) T	MCPA	12.455	0.000	22709939	0	28.797	N.D. #
8) T	DICHLORPROP	13.127	12.413	4440760	1198825	24.328	6.767 #
9) T	2,4-D	0.000	12.944	0	2224140	N.D.	9.373 #
14) T	DINOSEB	0.000	15.739	0	15069848	N.D.	21.201 #
15) T	Picloram	0.000	16.917	0	19042754	N.D.	13.814 #
16) T	DCPA	0.000	16.984	0	18983334	N.D.	13.144 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072618\
Data File : PS001259.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2018 17:28
Operator : UA
Sample : J4140-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 00:47:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

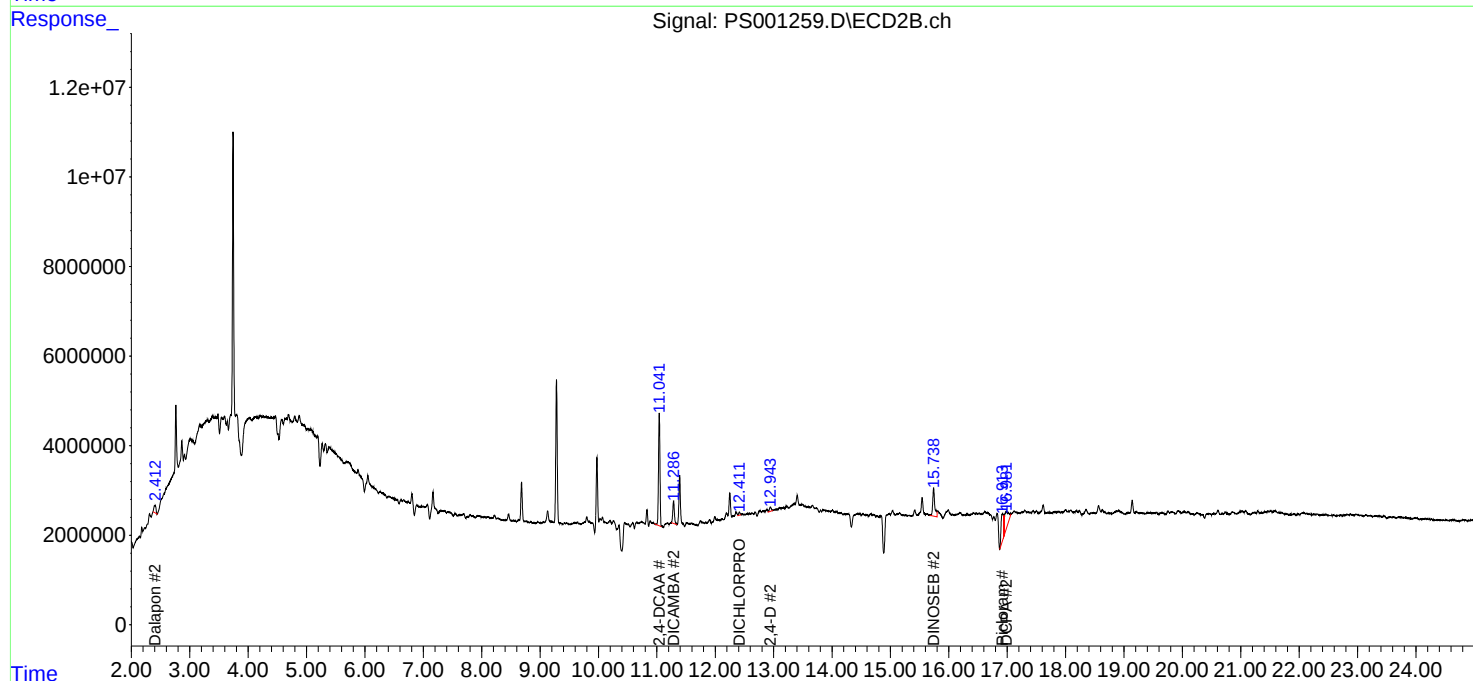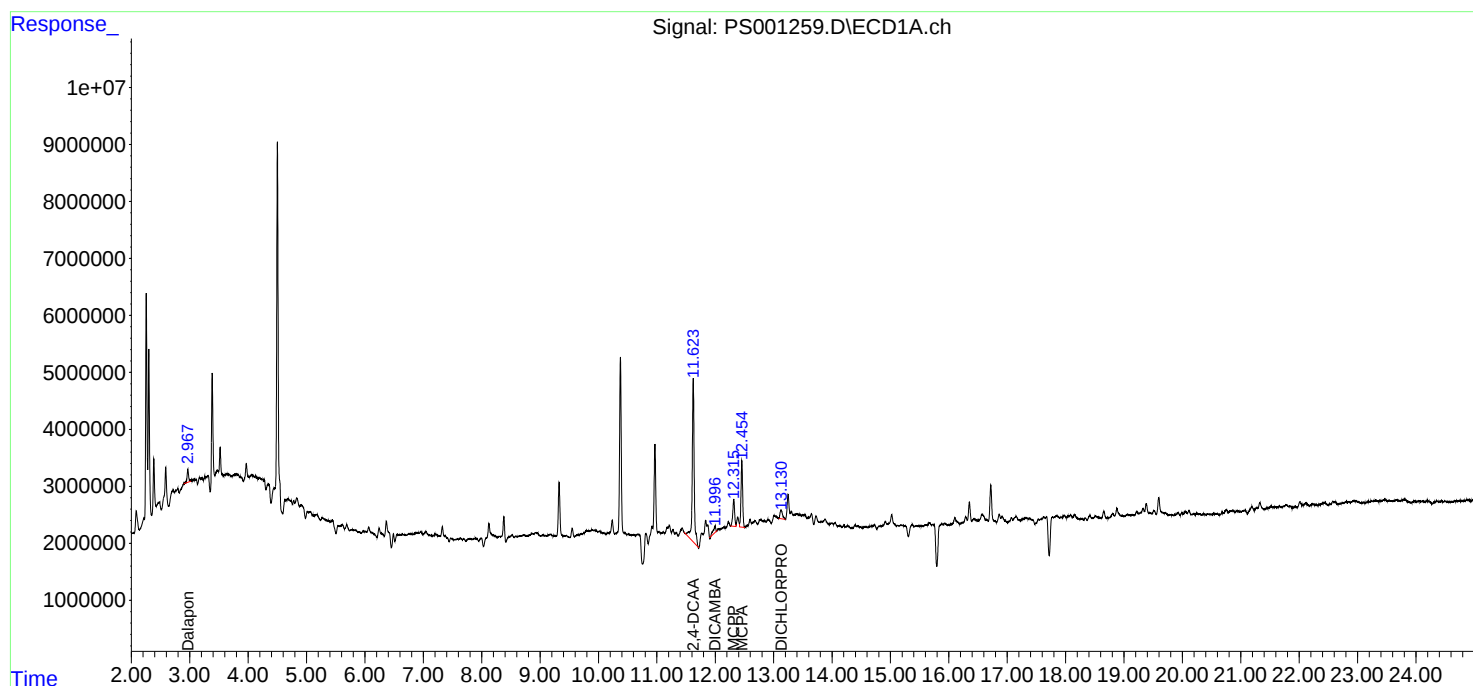


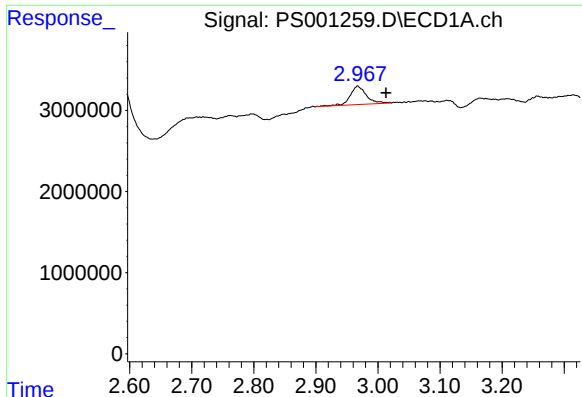

#1 Dalapon


R.T.: 2.968 min
Delta R.T.: -0.045 min
Response: 4094567
Conc: 17.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

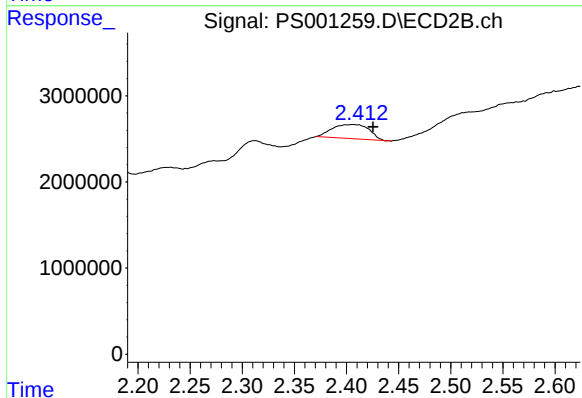


#1 Dalapon

R.T.: 2.407 min
Delta R.T.: -0.018 min
Response: 4020171
Conc: 17.64 ng/ml

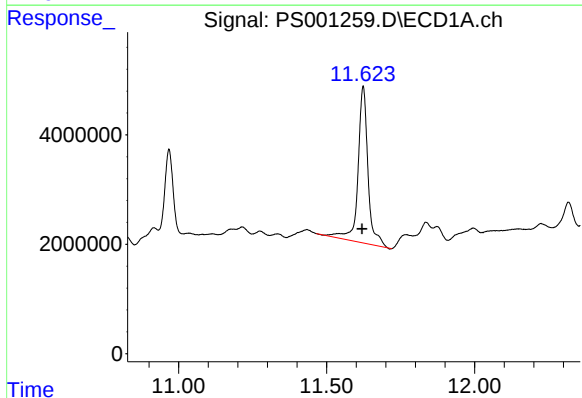


#4 2,4-DCAA

R.T.: 11.623 min
Delta R.T.: 0.004 min
Response: 66553246
Conc: 358.68 ng/ml

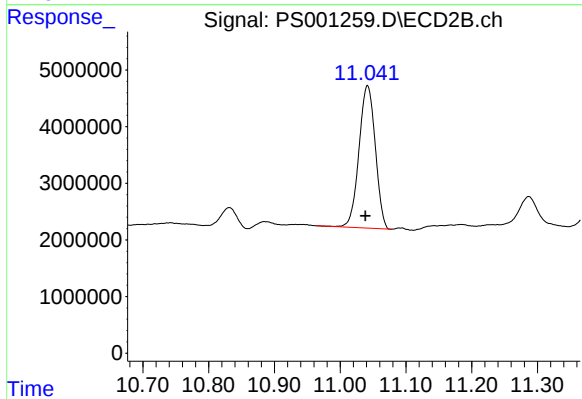

#4 2,4-DCAA


R.T.: 11.042 min
Delta R.T.: 0.003 min
Response: 43303296
Conc: 238.09 ng/ml

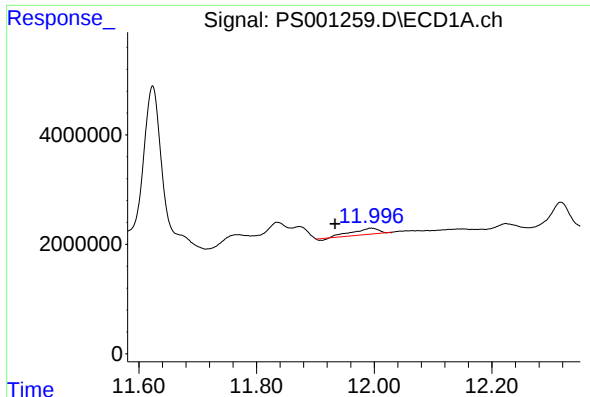

#5 DICAMBA


R.T.: 11.995 min
Delta R.T.: 0.061 min
Response: 3517928
Conc: 4.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

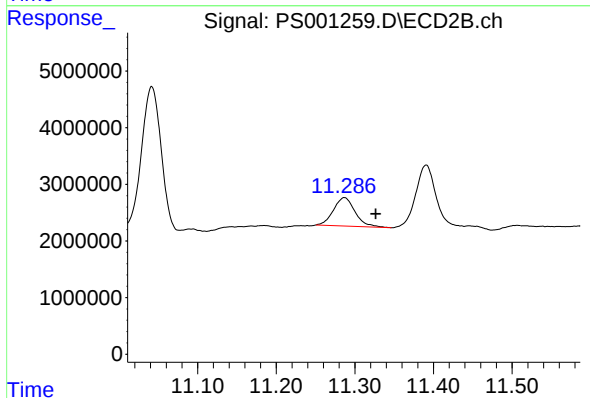


#5 DICAMBA

R.T.: 11.287 min
Delta R.T.: -0.040 min
Response: 9589824
Conc: 13.99 ng/ml

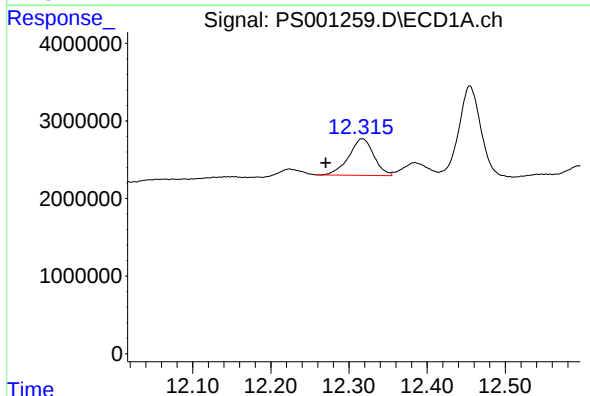


#6 MCP

R.T.: 12.317 min
Delta R.T.: 0.047 min
Response: 10477944
Conc: 20.85 ug/ml

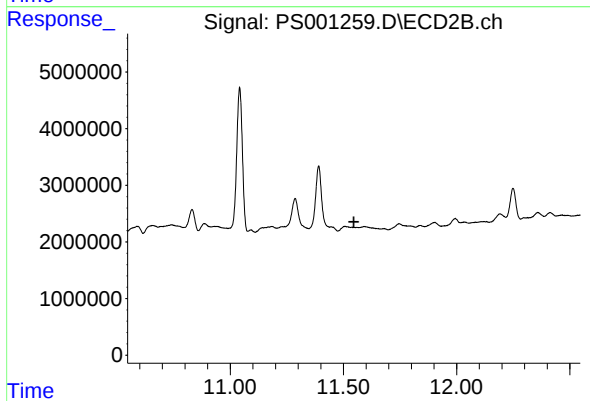

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.546 min
Response: 0
Conc: N.D.

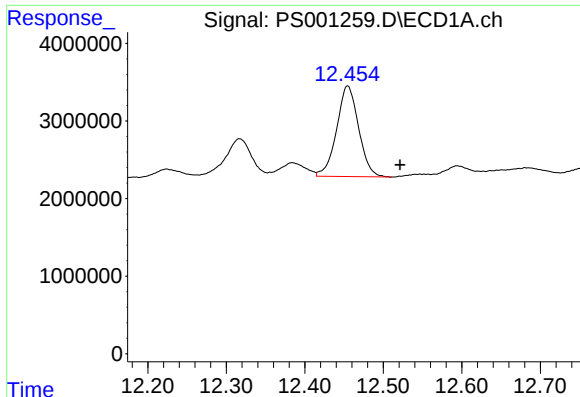

#7 MCPA


R.T.: 12.455 min
Delta R.T.: -0.067 min
Response: 22709939
Conc: 28.80 ug/ml

Instrument :
ECD_S
ClientSampleId :

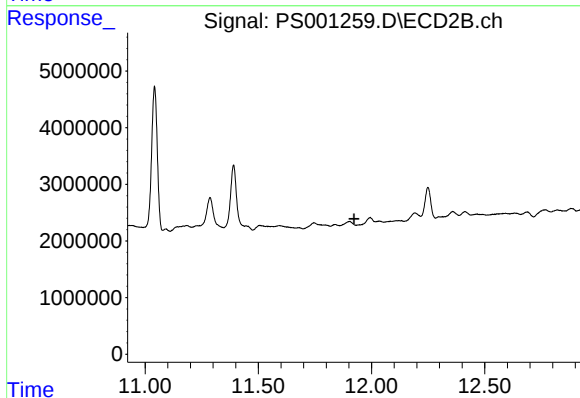


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.922 min
Response: 0
Conc: N.D.

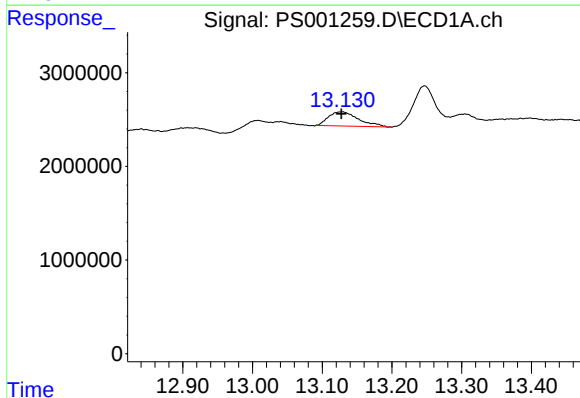


#8 DICHLORPROP

R.T.: 13.127 min
Delta R.T.: 0.000 min
Response: 4440760
Conc: 24.33 ng/ml

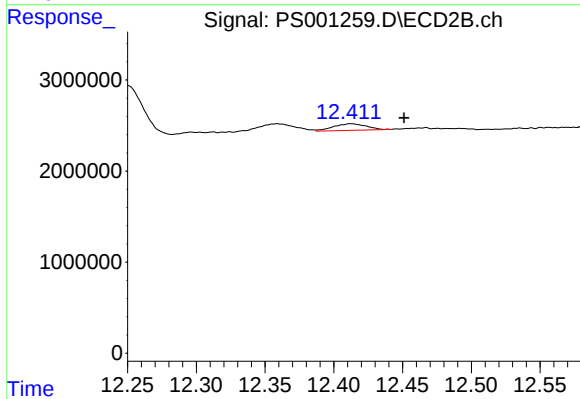

#8 DICHLORPROP


R.T.: 12.413 min
Delta R.T.: -0.038 min
Response: 1198825
Conc: 6.77 ng/ml

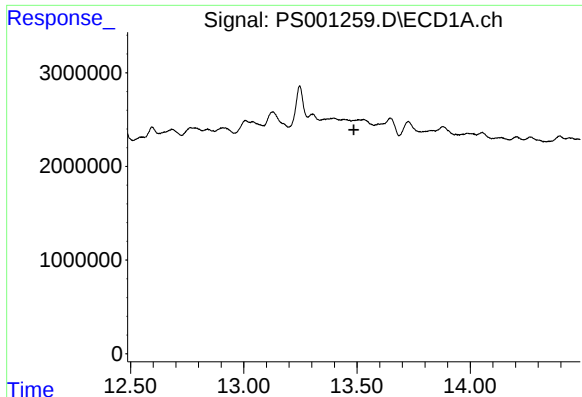

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

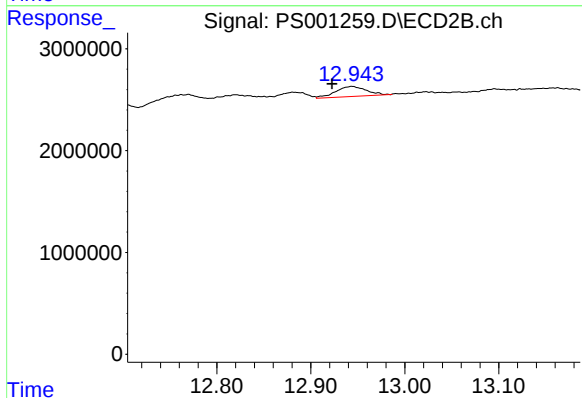


#9 2,4-D

R.T.: 12.944 min
Delta R.T.: 0.021 min
Response: 2224140
Conc: 9.37 ng/ml

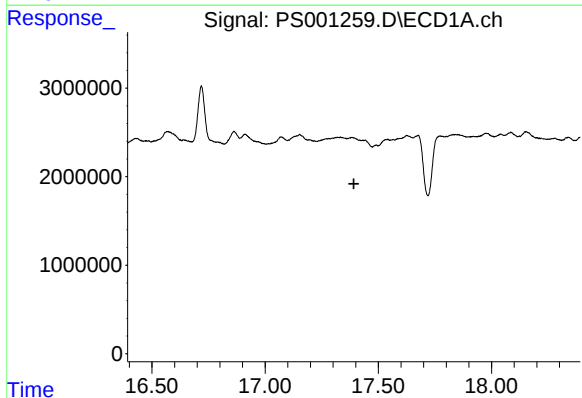


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.392 min
Response: 0
Conc: N.D.

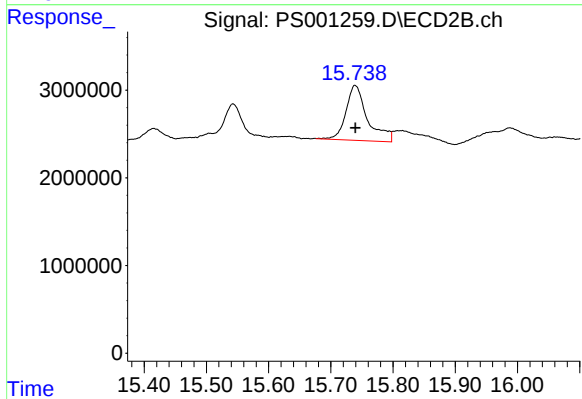

#14 DINOSEB


R.T.: 15.739 min
Delta R.T.: 0.000 min
Response: 15069848
Conc: 21.20 ng/ml

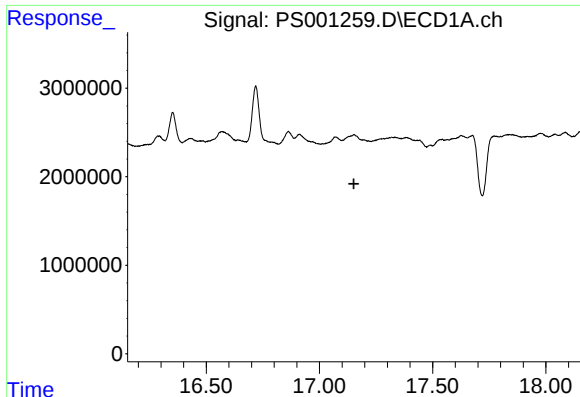

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 17.152 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

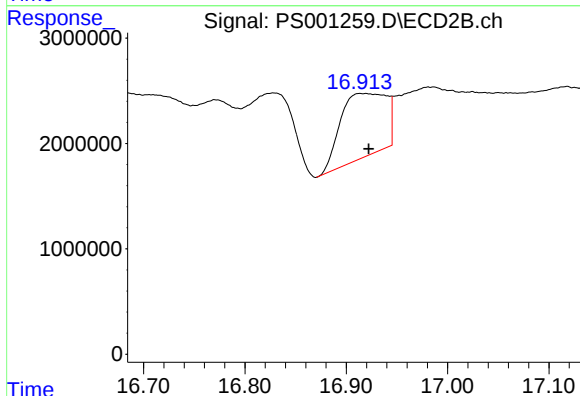


#15 Picloram

R.T.: 16.917 min
Delta R.T.: -0.005 min
Response: 19042754
Conc: 13.81 ng/ml

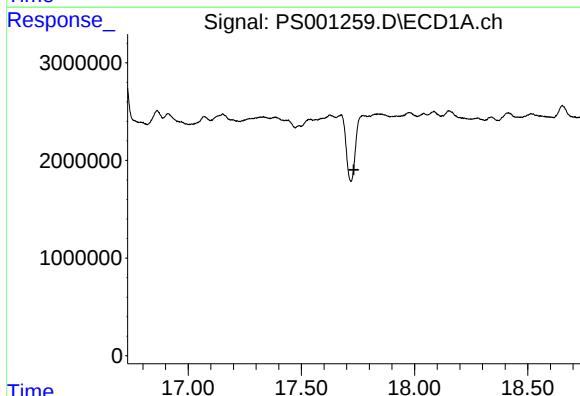

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.732 min
Response: 0
Conc: N.D.

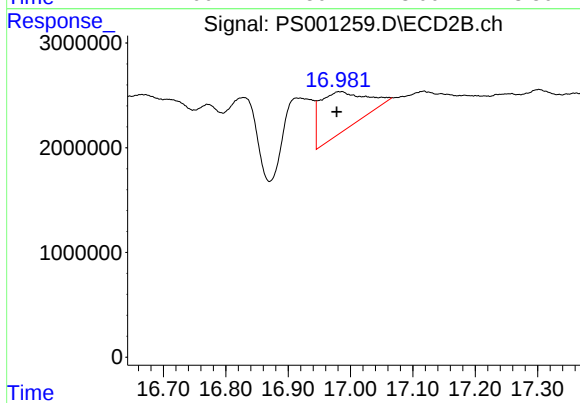

#16 DCPA

R.T.: 16.984 min
Delta R.T.: 0.006 min
Response: 18983334
Conc: 13.14 ng/ml