

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072618\
 Data File : PS001265.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2018 20:34
 Operator : UA
 Sample : J4140-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 00:49:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.616	11.036	49275833	43760398	265.566	240.607
Target Compounds							
1) T	Dalapon	2.961	2.398	6114100	4493789	25.784	19.721
2) T	3,5-DICHL...	0.000	9.123	0	33092	N.D.	0.130 #
5) T	DICAMBA	0.000	11.280	0	8201100	N.D.	11.966 #
6) T	MCP	12.311	0.000	10693061	0	21.275	N.D. #
7) T	MCPA	12.586	0.000	9169874	0	11.628	N.D. #
8) T	DICHLORPROP	0.000	12.405	0	1403610	N.D.	7.923 #
9) T	2,4-D	0.000	12.876	0	4516576	N.D.	19.034 #
14) T	DINOSEB	0.000	15.731	0	13031180	N.D.	18.333 #
15) T	Picloram	0.000	16.911	0	24121090	N.D.	17.498 #
16) T	DCPA	17.769	16.980	22356385	41283215	16.559	28.584 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072618\
Data File : PS001265.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2018 20:34
Operator : UA
Sample : J4140-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 00:49:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

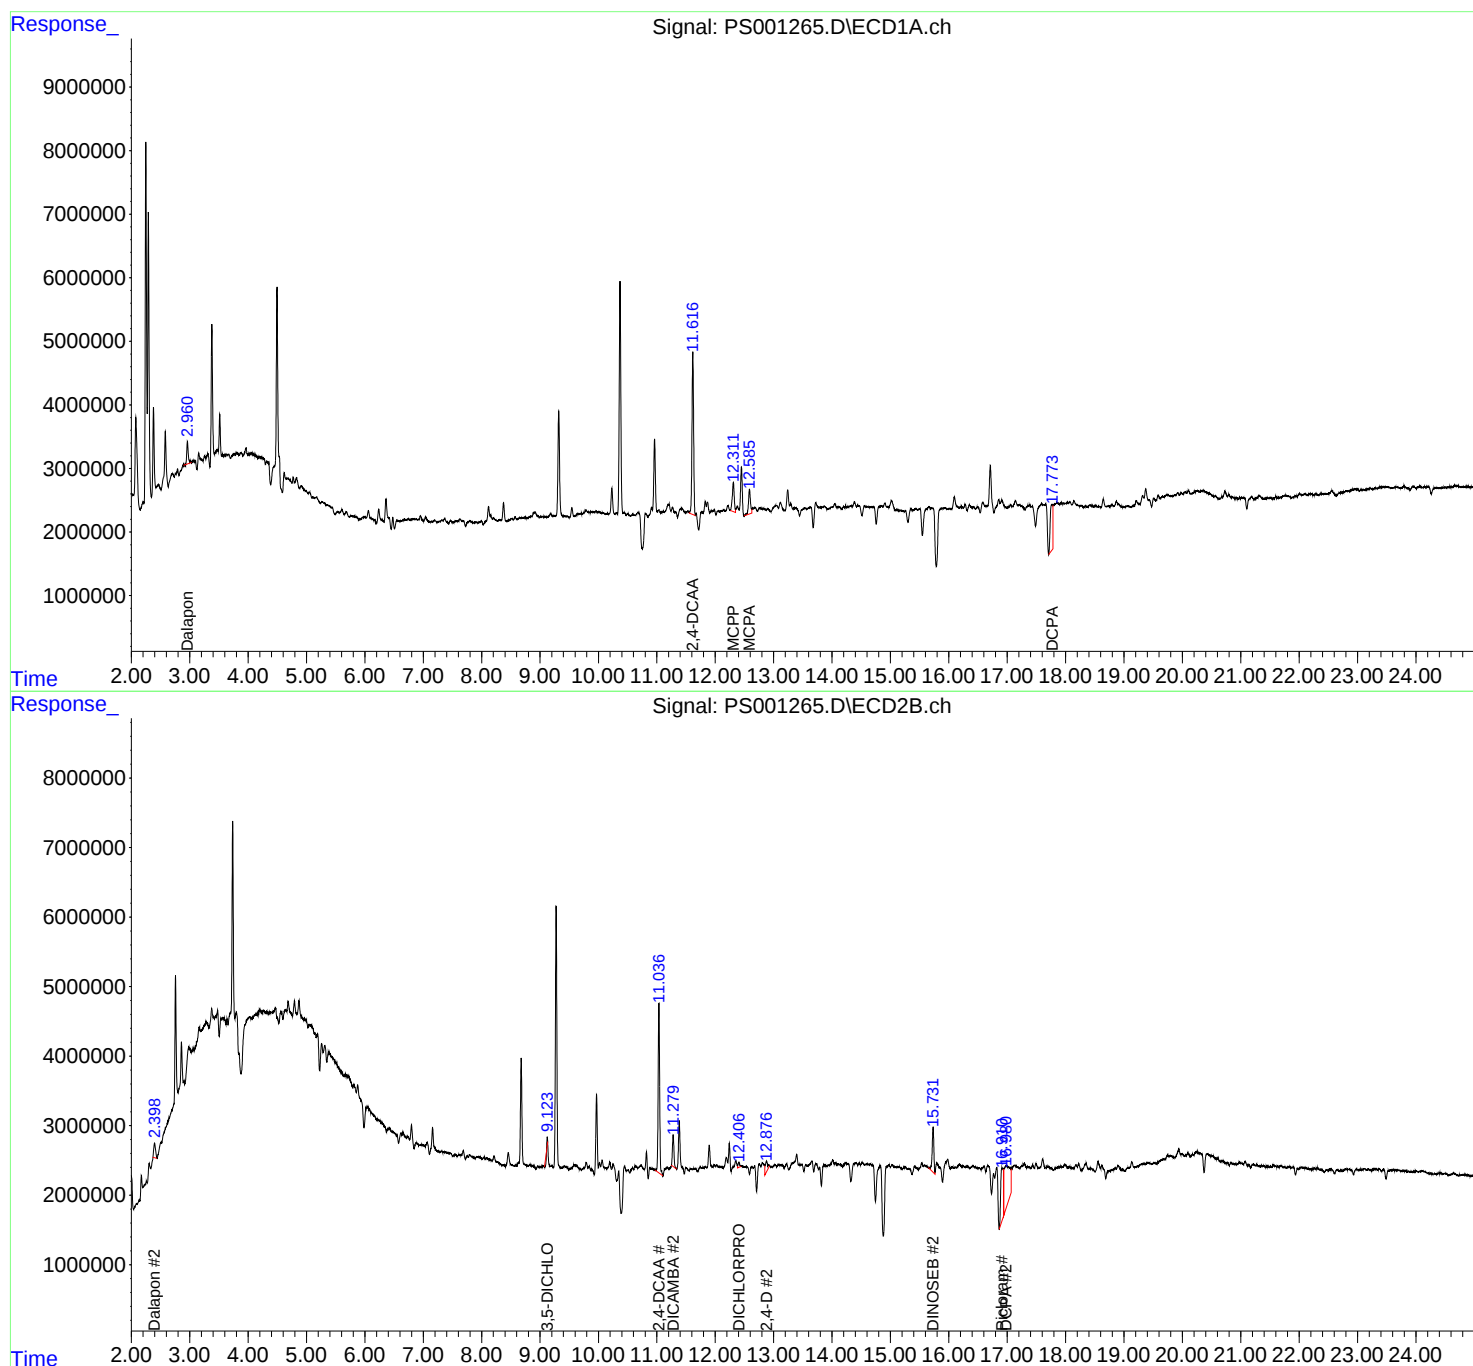


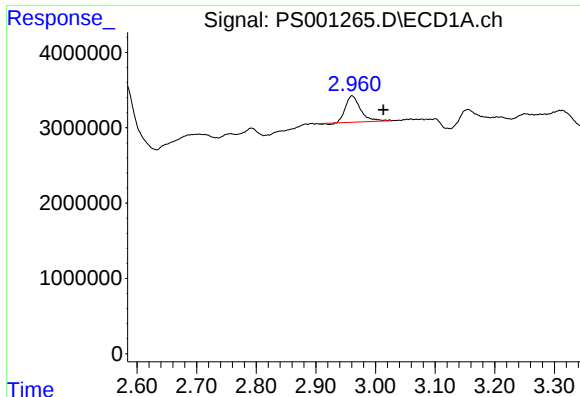

#1 Dalapon


R.T.: 2.961 min
Delta R.T.: -0.052 min
Response: 6114100
Conc: 25.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

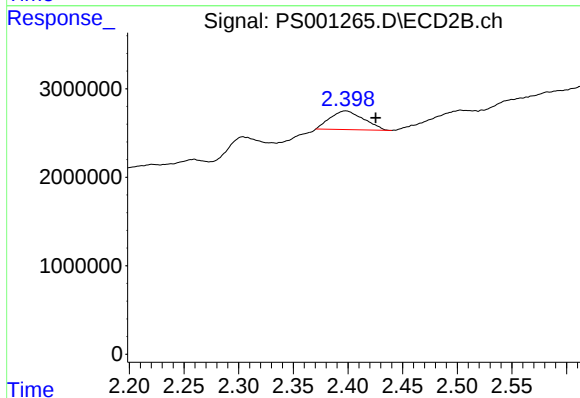


#1 Dalapon

R.T.: 2.398 min
Delta R.T.: -0.028 min
Response: 4493789
Conc: 19.72 ng/ml

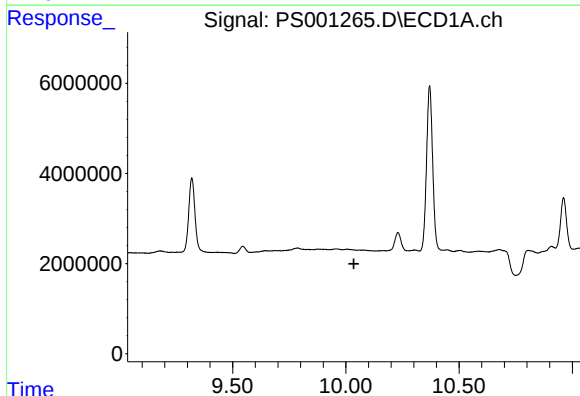


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.035 min
Response: 0
Conc: N.D.

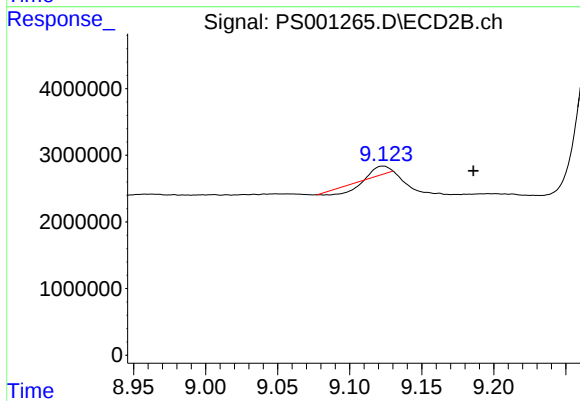

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.123 min
Delta R.T.: -0.063 min
Response: 33092
Conc: 0.13 ng/ml

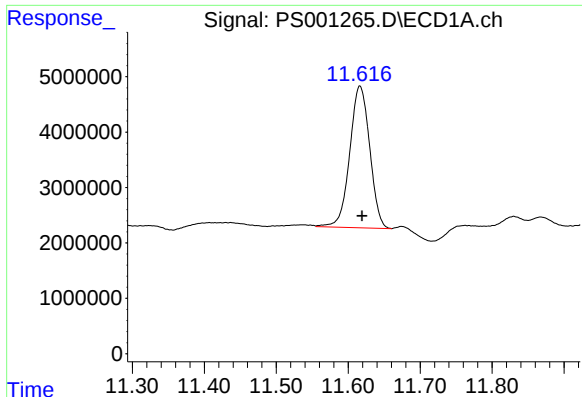

#4 2,4-DCAA


R.T.: 11.616 min
Delta R.T.: -0.003 min
Response: 49275833
Conc: 265.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

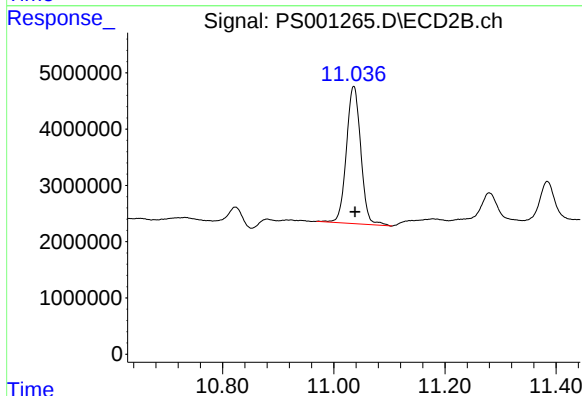


#4 2,4-DCAA

R.T.: 11.036 min
Delta R.T.: -0.003 min
Response: 43760398
Conc: 240.61 ng/ml

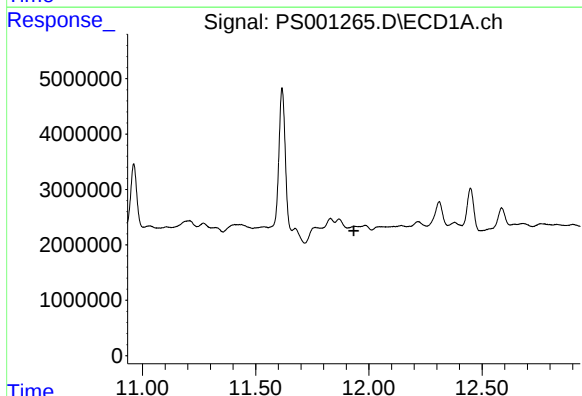


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.934 min
Response: 0
Conc: N.D.

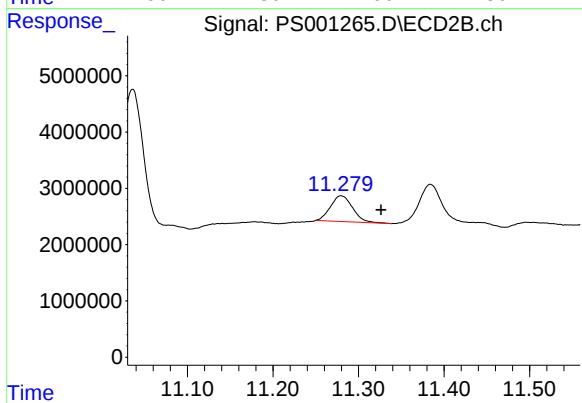

#5 DICAMBA


R.T.: 11.280 min
Delta R.T.: -0.047 min
Response: 8201100
Conc: 11.97 ng/ml

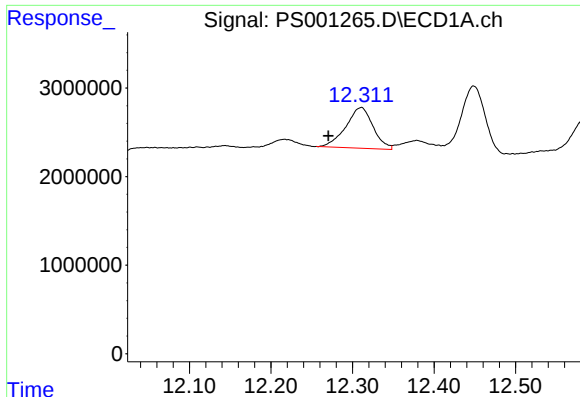

#6 MCPP


R.T.: 12.311 min
Delta R.T.: 0.040 min
Response: 10693061
Conc: 21.28 ug/ml

Instrument :
ECD_S
ClientSampleId :

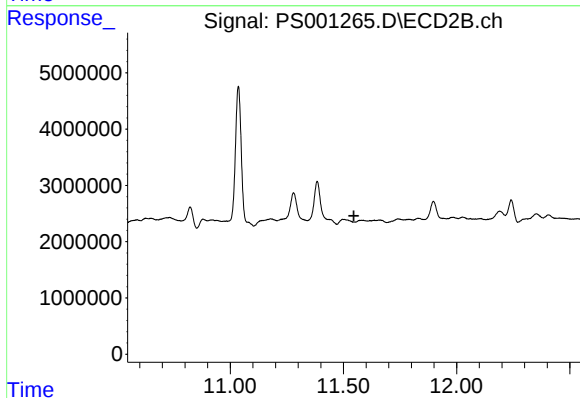


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.546 min
Response: 0
Conc: N.D.

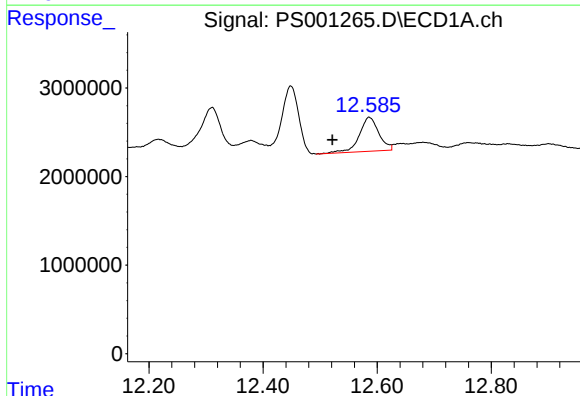


#7 MCPA

R.T.: 12.586 min
Delta R.T.: 0.065 min
Response: 9169874
Conc: 11.63 ug/ml

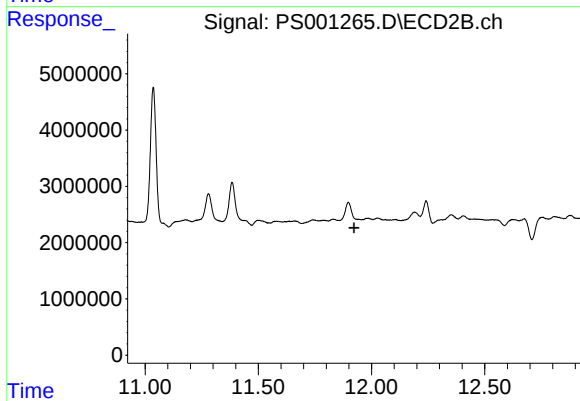

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 11.922 min
Response: 0
Conc: N.D.

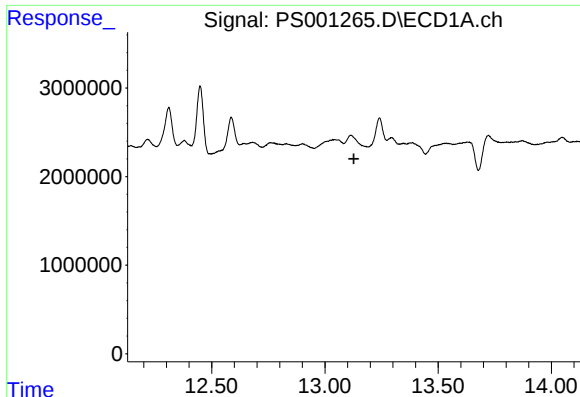

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.128 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

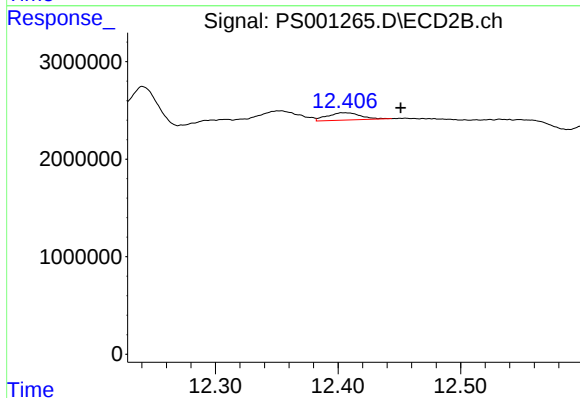


#8 DICHLORPROP

R.T.: 12.405 min
Delta R.T.: -0.046 min
Response: 1403610
Conc: 7.92 ng/ml

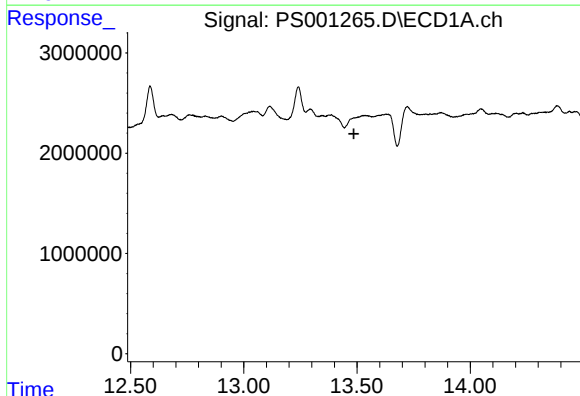


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.486 min
Response: 0
Conc: N.D.

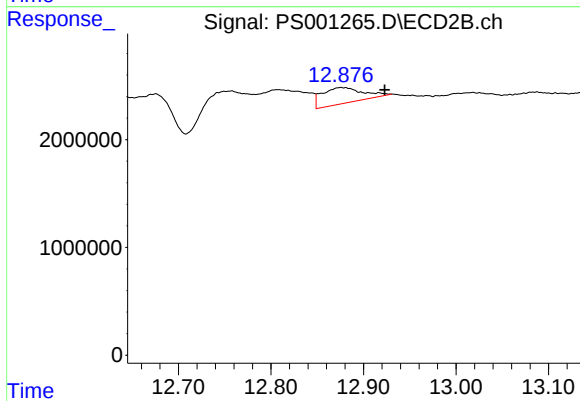

#9 2,4-D


R.T.: 12.876 min
Delta R.T.: -0.046 min
Response: 4516576
Conc: 19.03 ng/ml

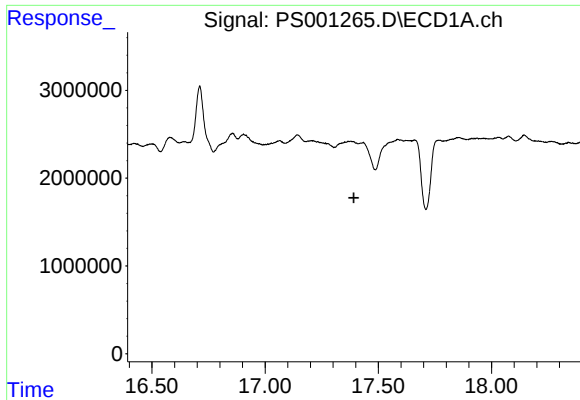

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.392 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

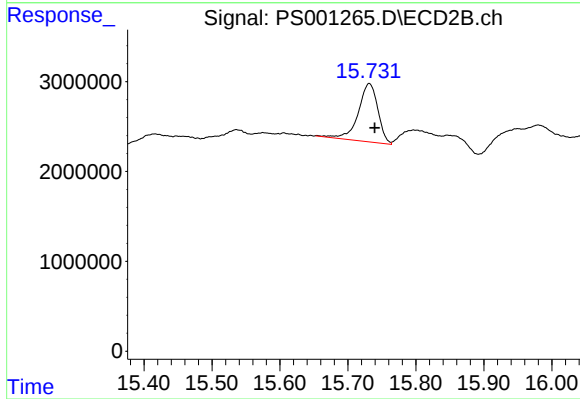


#14 DINOSEB

R.T.: 15.731 min
Delta R.T.: -0.008 min
Response: 13031180
Conc: 18.33 ng/ml

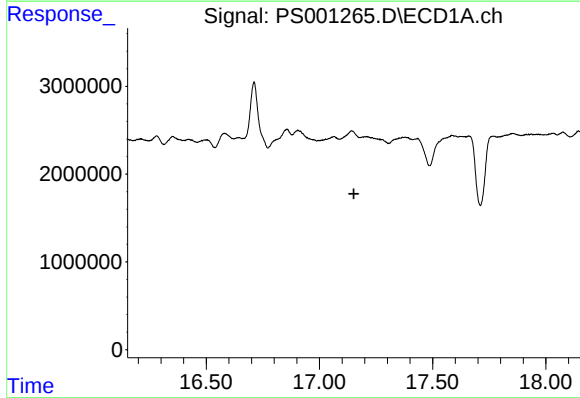


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.152 min
Response: 0
Conc: N.D.

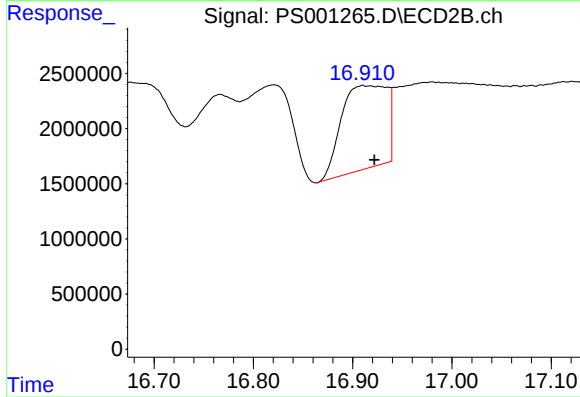

#15 Picloram


R.T.: 16.911 min
Delta R.T.: -0.011 min
Response: 24121090
Conc: 17.50 ng/ml

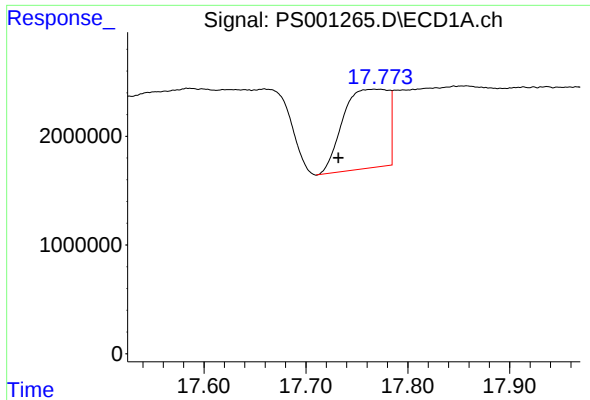

#16 DCPA

R.T.: 17.769 min
Delta R.T.: 0.037 min
Response: 22356385
Conc: 16.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

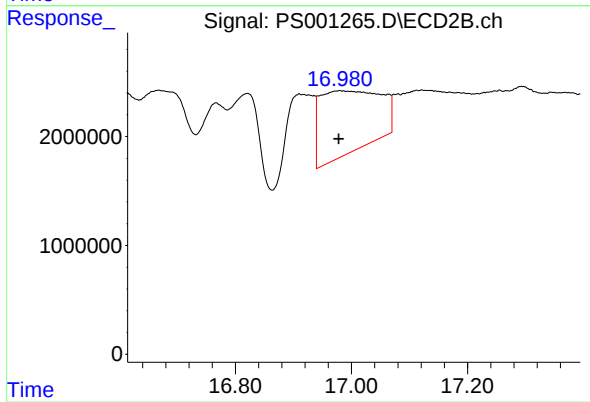

#16 DCPA

R.T.: 16.980 min
Delta R.T.: 0.002 min
Response: 41283215
Conc: 28.58 ng/ml