

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072618\
 Data File : PS001275.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2018 01:44
 Operator : UA
 Sample : J4152-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 06:37:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.633	11.053	85380153	77284379	460.147	424.932
Target Compounds							
1) T	Dalapon	2.979	2.416	4877810	3775540	20.571	16.569
2) T	3,5-DICHL...	0.000	9.140	0	1873765	N.D.	7.355 #
5) T	DICAMBA	0.000	11.296	0	8088640	N.D.	11.802 #
6) T	MCP	12.328	0.000	7376256	0	14.676	N.D. #
8) T	DICHLORPROP	0.000	12.422	0	2860887	N.D.	16.150 #
10) T	Pentachlo...	13.887	13.491	3757817	2863492	1.335	1.040
11) T	2,4,5-TP ...	0.000	14.031	0	9801776	N.D.	8.964 #
15) T	Picloram	17.180	0.000	25553563	0	16.167	N.D. #
16) T	DCPA	17.774	16.994	10038165	-764125	7.435	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072618\
Data File : PS001275.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2018 01:44
Operator : UA
Sample : J4152-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 06:37:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

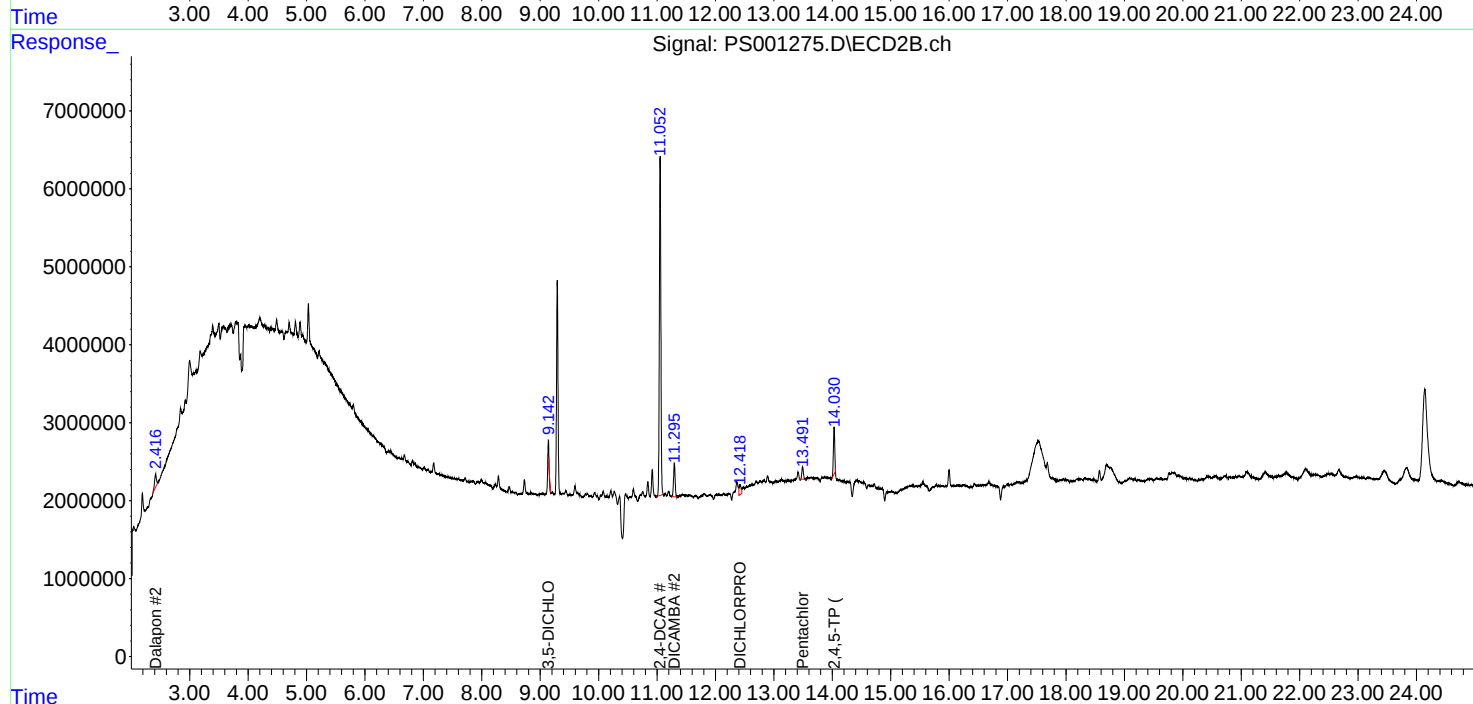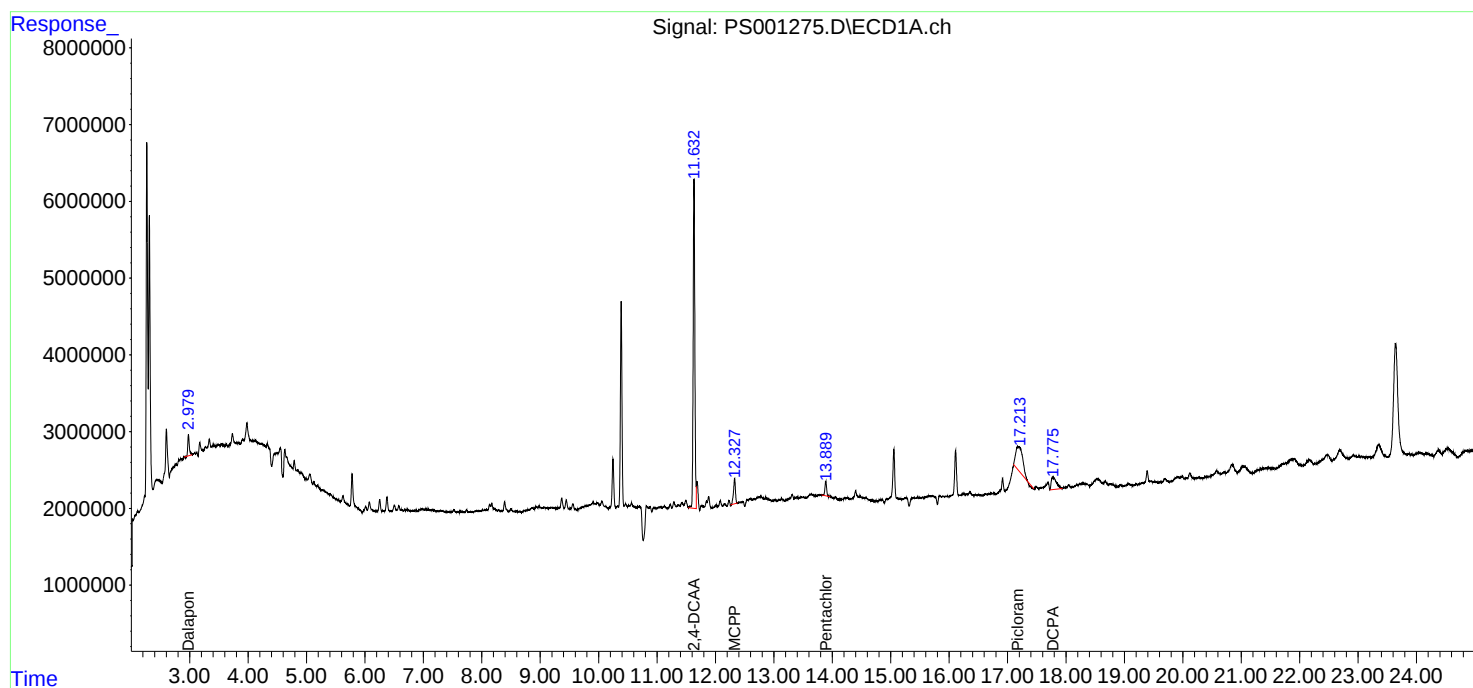


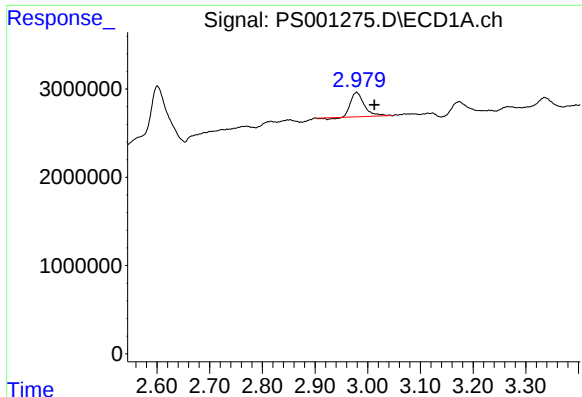

#1 Dalapon


R.T.: 2.979 min
Delta R.T.: -0.034 min
Response: 4877810
Conc: 20.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

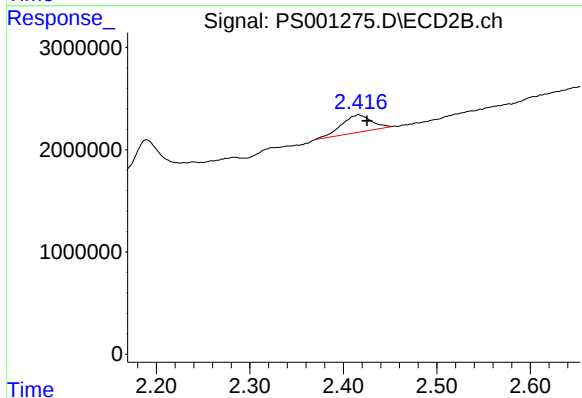


#1 Dalapon

R.T.: 2.416 min
Delta R.T.: -0.009 min
Response: 3775540
Conc: 16.57 ng/ml

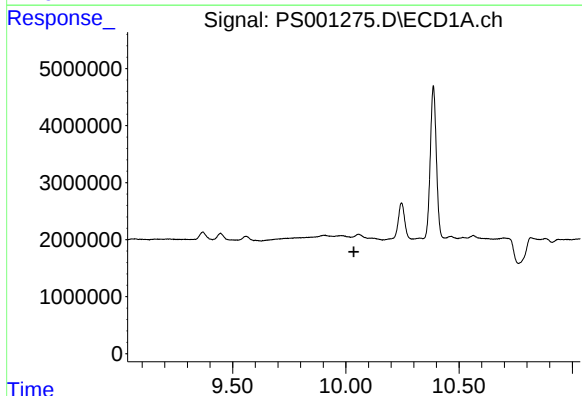


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.035 min
Response: 0
Conc: N.D.

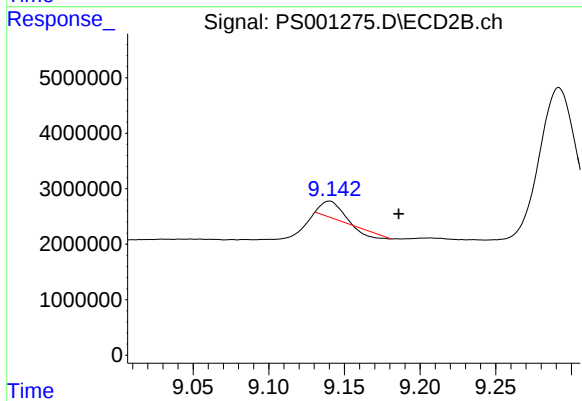

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.140 min
Delta R.T.: -0.046 min
Response: 1873765
Conc: 7.36 ng/ml

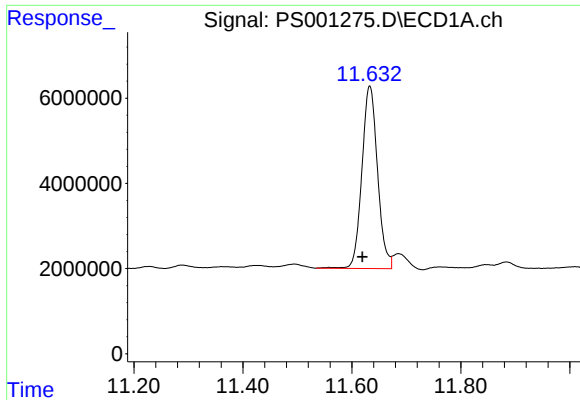

#4 2,4-DCAA


R.T.: 11.633 min
Delta R.T.: 0.014 min
Response: 85380153
Conc: 460.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

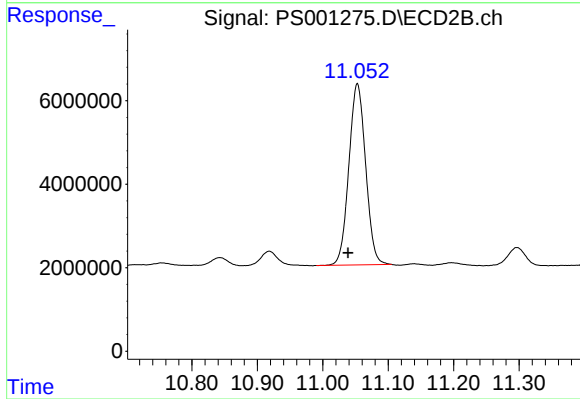


#4 2,4-DCAA

R.T.: 11.053 min
Delta R.T.: 0.014 min
Response: 77284379
Conc: 424.93 ng/ml

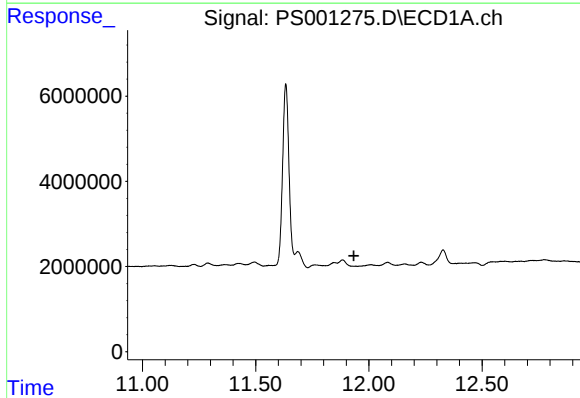


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.934 min
Response: 0
Conc: N.D.

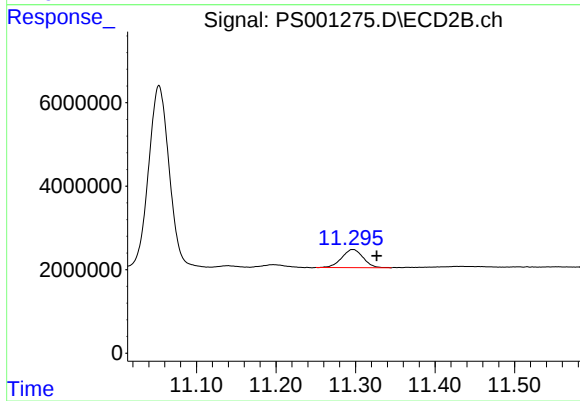

#5 DICAMBA


R.T.: 11.296 min
Delta R.T.: -0.030 min
Response: 8088640
Conc: 11.80 ng/ml

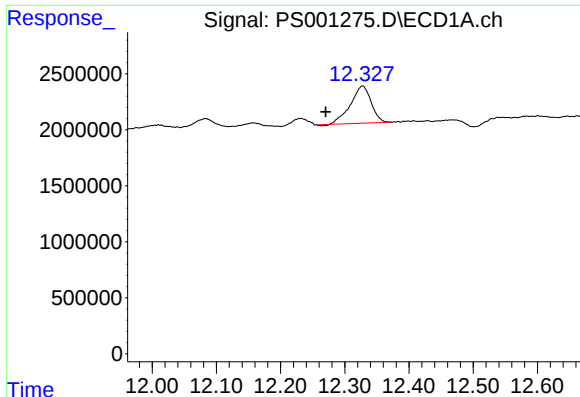

#6 MCP


R.T.: 12.328 min
Delta R.T.: 0.057 min
Response: 7376256
Conc: 14.68 ug/ml

Instrument :
ECD_S
ClientSampleId :

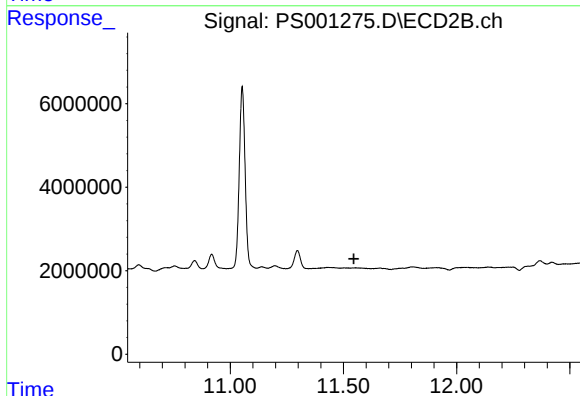


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.546 min
Response: 0
Conc: N.D.

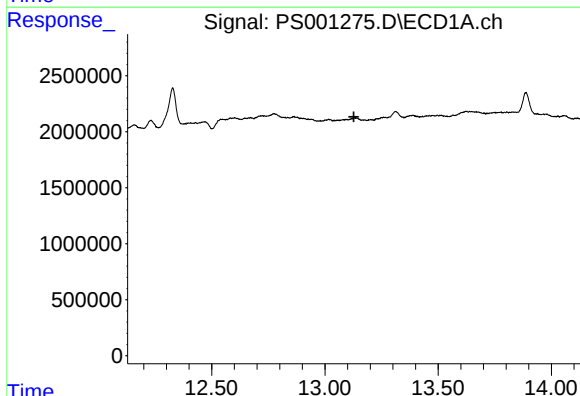


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.128 min
Response: 0
Conc: N.D.

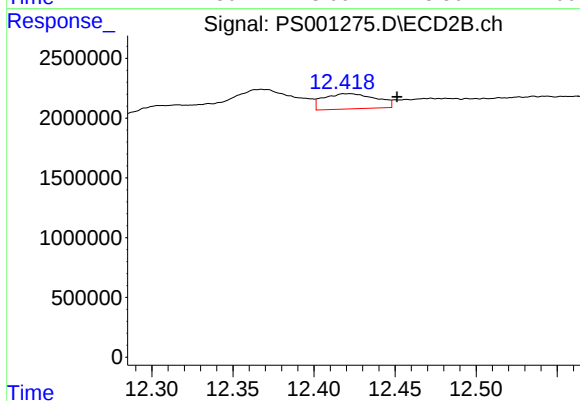

#8 DICHLORPROP


R.T.: 12.422 min
Delta R.T.: -0.029 min
Response: 2860887
Conc: 16.15 ng/ml

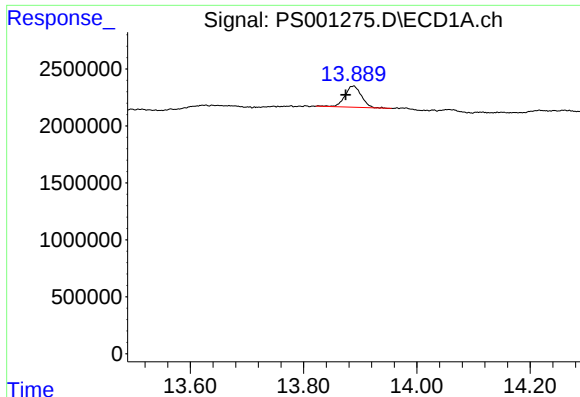

#10 Pentachlorophenol


R.T.: 13.887 min
Delta R.T.: 0.013 min
Response: 3757817
Conc: 1.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

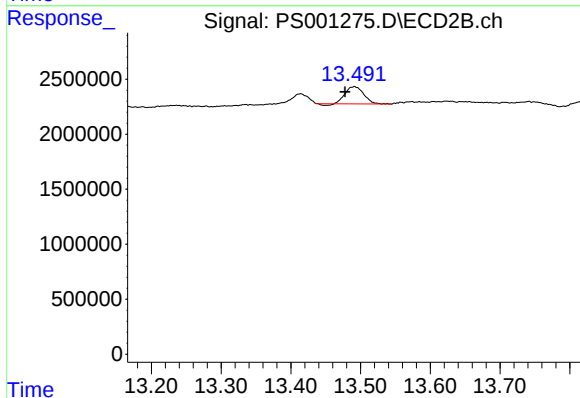


#10 Pentachlorophenol

R.T.: 13.491 min
Delta R.T.: 0.014 min
Response: 2863492
Conc: 1.04 ng/ml

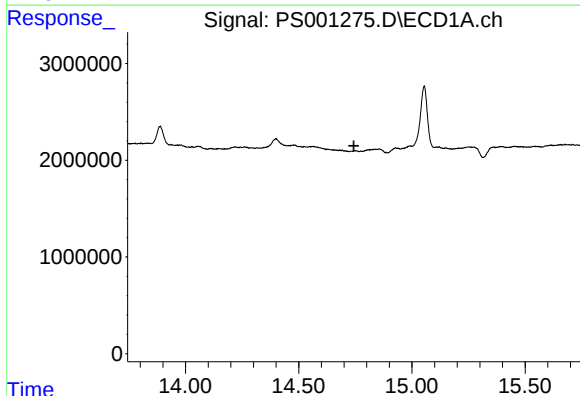


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.743 min
Response: 0
Conc: N.D.

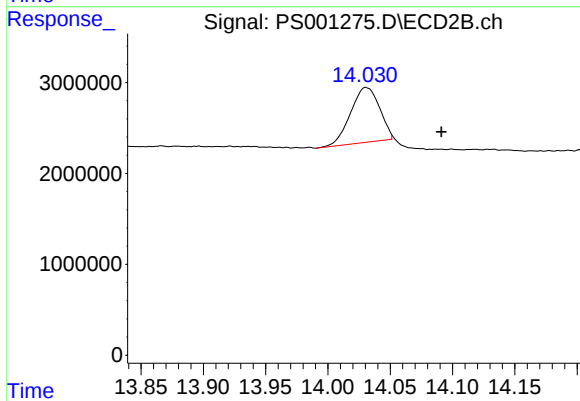

#11 2,4,5-TP (SILVEX)


R.T.: 14.031 min
Delta R.T.: -0.060 min
Response: 9801776
Conc: 8.96 ng/ml

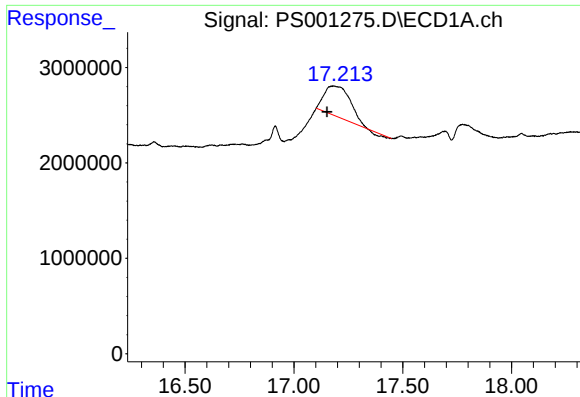

#15 Picloram


R.T.: 17.180 min
Delta R.T.: 0.029 min
Response: 25553563
Conc: 16.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

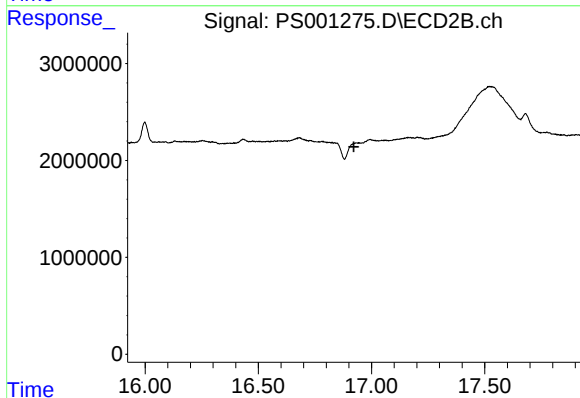


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.922 min
Response: 0
Conc: N.D.

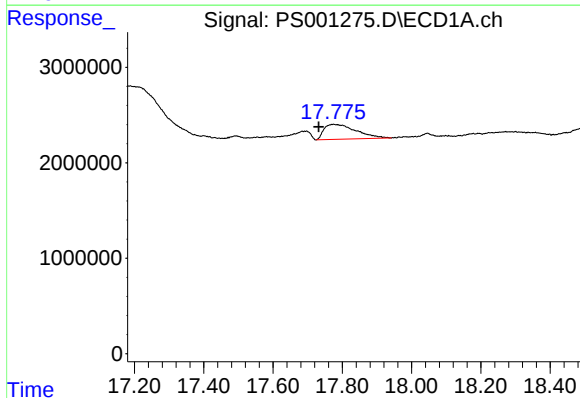

#16 DCPA

R.T.: 17.774 min
Delta R.T.: 0.042 min
Response: 10038165
Conc: 7.44 ng/ml

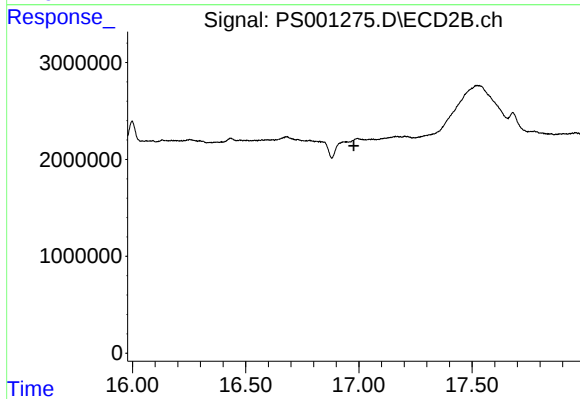

#16 DCPA

R.T.: 16.994 min
Delta R.T.: 0.016 min
Response: -764125
Conc: N.D.