

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072618\
 Data File : PS001276.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2018 02:15
 Operator : UA
 Sample : J4152-08
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 06:38:19 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.616	11.037	90076465	81563100	485.457	448.457
Target Compounds							
1) T	Dalapon	2.963	2.399	4948554	2749356	20.869	12.065 #
5) T	DICAMBA	0.000	11.280	0	7830174	N.D.	11.425 #
6) T	MCPD	12.310	0.000	8606292	0	17.123	N.D. #
8) T	DICHLORPROP	0.000	12.405	0	2267423	N.D.	12.800 #
12) T	2,4,5-T	0.000	14.700	0	24903388	N.D.	26.960 #
13) T	2,4-DB	15.823	0.000	3587544	0	24.920	N.D. #
15) T	Picloram	0.000	16.903	0	3247950	N.D.	2.356 #
16) T	DCPA	17.782	0.000	5967779	0	4.420	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072618\
Data File : PS001276.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2018 02:15
Operator : UA
Sample : J4152-08
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 06:38:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

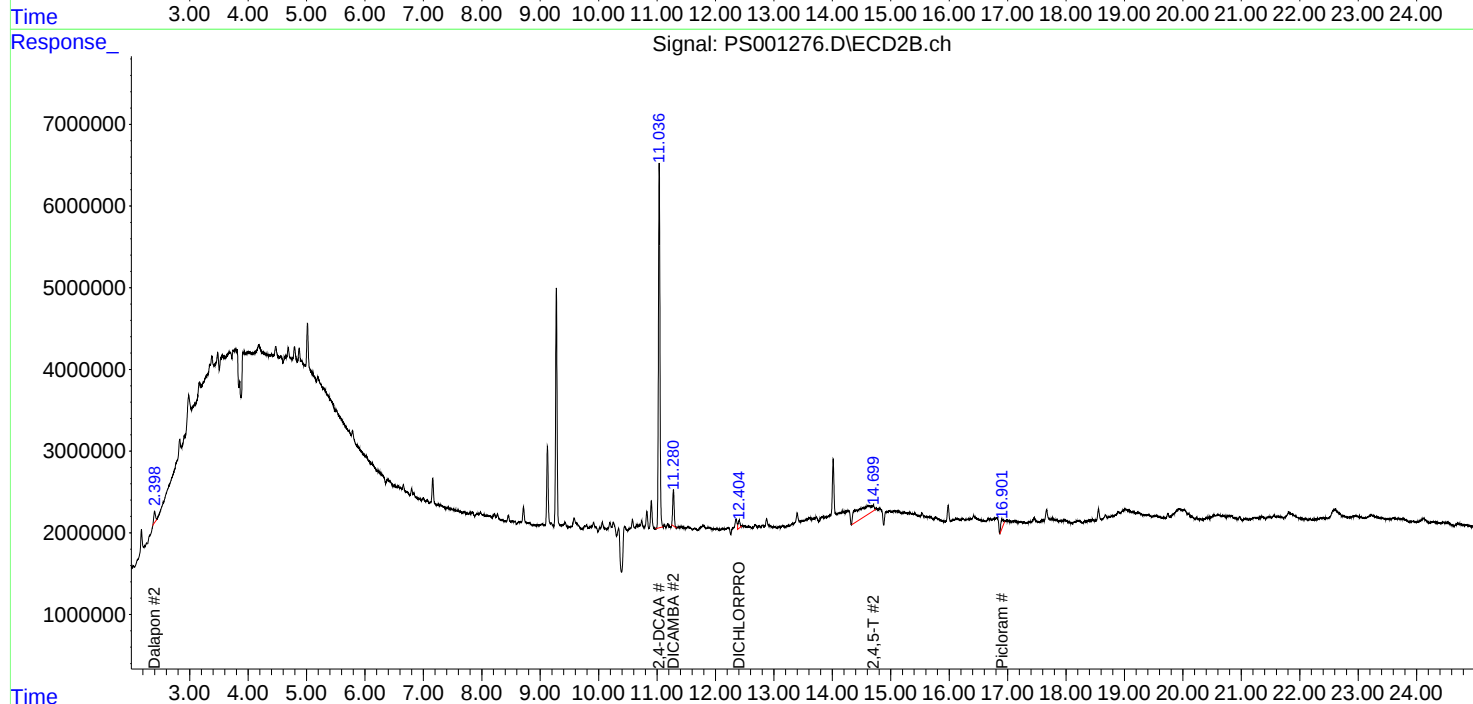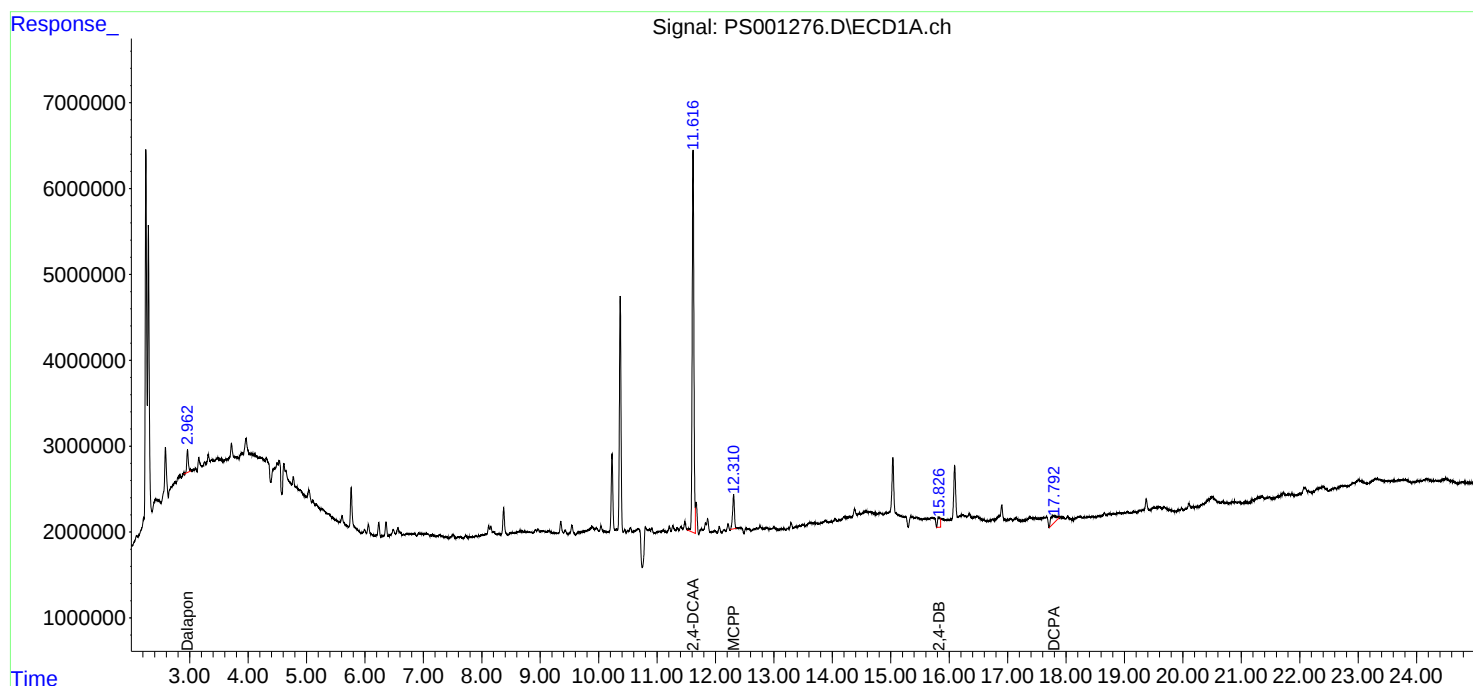


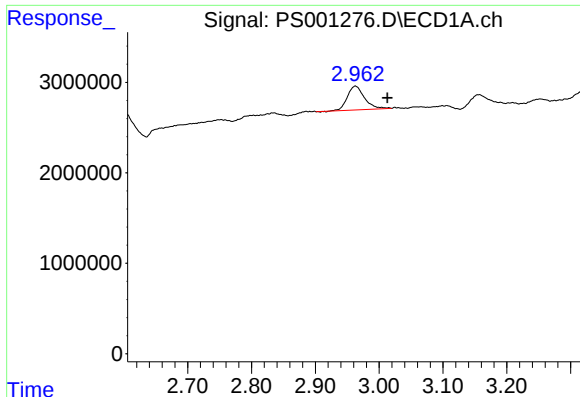

#1 Dalapon


R.T.: 2.963 min
Delta R.T.: -0.050 min
Response: 4948554
Conc: 20.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

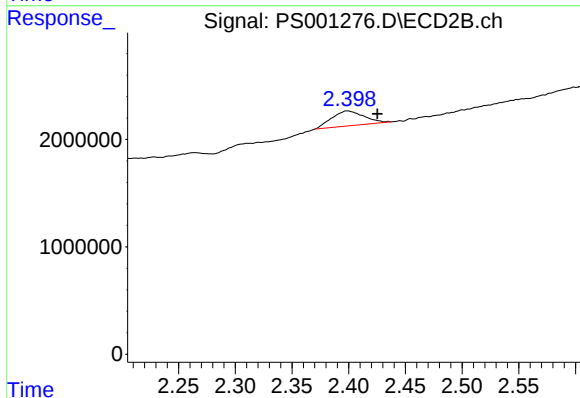


#1 Dalapon

R.T.: 2.399 min
Delta R.T.: -0.026 min
Response: 2749356
Conc: 12.07 ng/ml

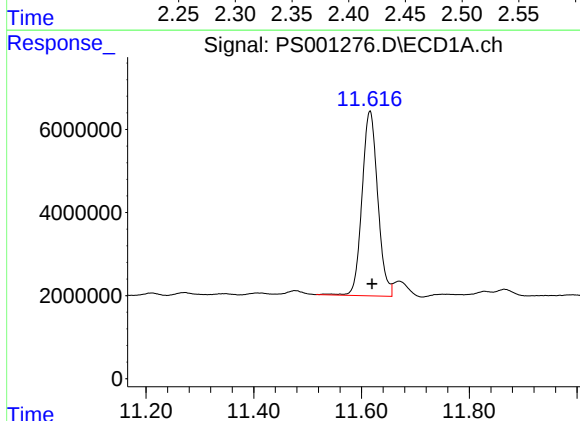


#4 2,4-DCAA

R.T.: 11.616 min
Delta R.T.: -0.004 min
Response: 90076465
Conc: 485.46 ng/ml

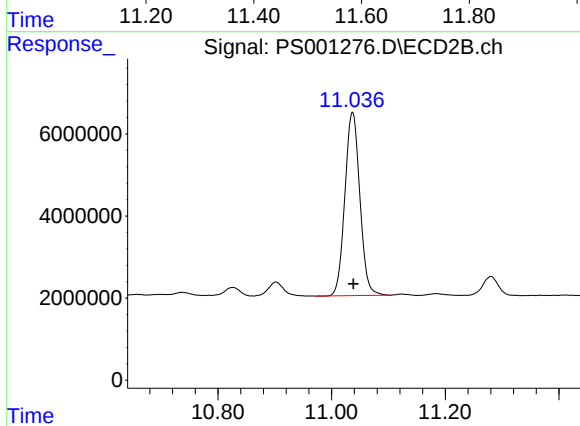

#4 2,4-DCAA


R.T.: 11.037 min
Delta R.T.: -0.002 min
Response: 81563100
Conc: 448.46 ng/ml

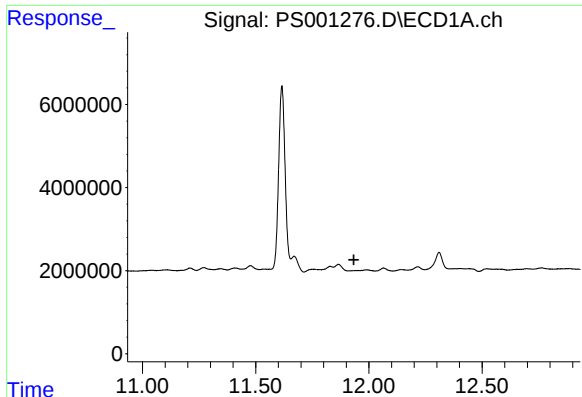

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.934 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

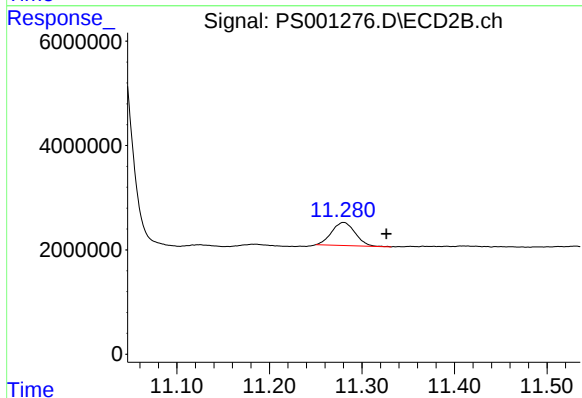


#5 DICAMBA

R.T.: 11.280 min
Delta R.T.: -0.046 min
Response: 7830174
Conc: 11.42 ng/ml

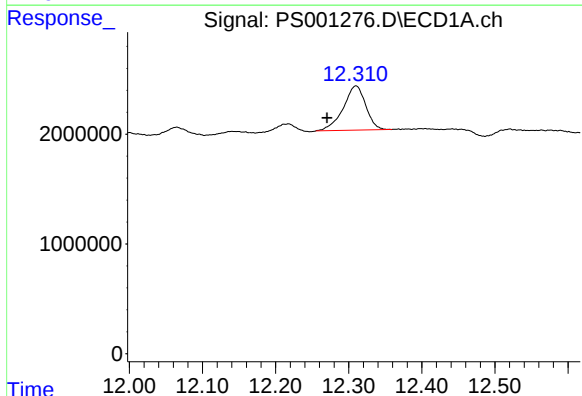


#6 MCP

R.T.: 12.310 min
Delta R.T.: 0.039 min
Response: 8606292
Conc: 17.12 ug/ml

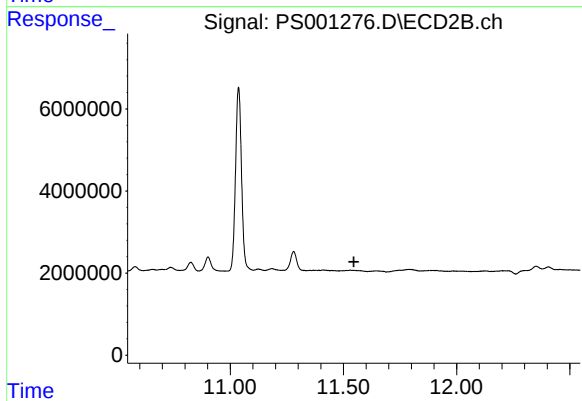

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.546 min
Response: 0
Conc: N.D.

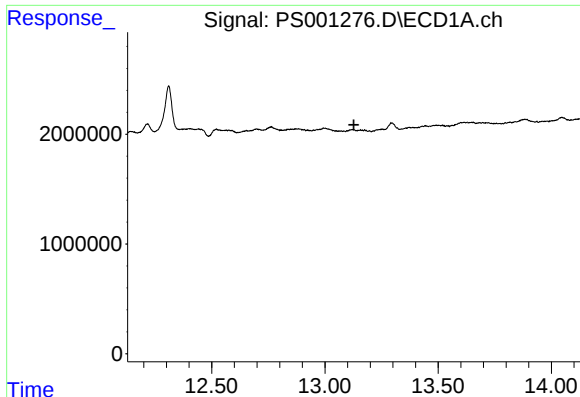

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.128 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

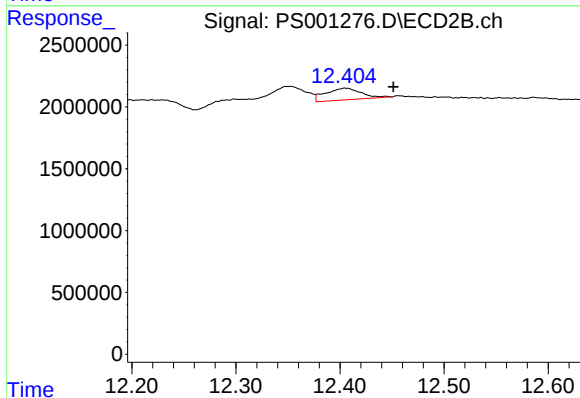


#8 DICHLORPROP

R.T.: 12.405 min
Delta R.T.: -0.046 min
Response: 2267423
Conc: 12.80 ng/ml

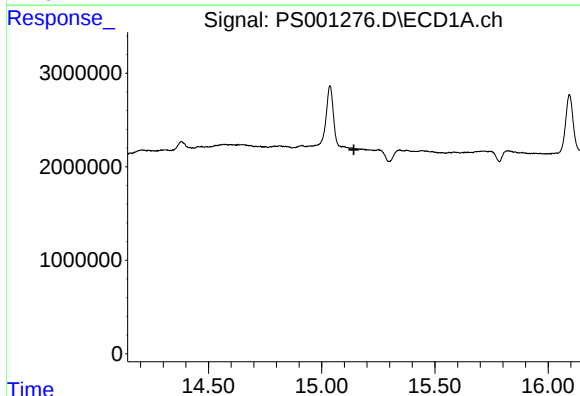


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.142 min
Response: 0
Conc: N.D.

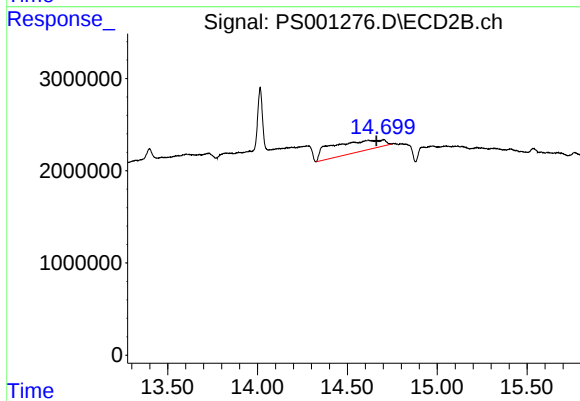

#12 2,4,5-T


R.T.: 14.700 min
Delta R.T.: 0.038 min
Response: 24903388
Conc: 26.96 ng/ml

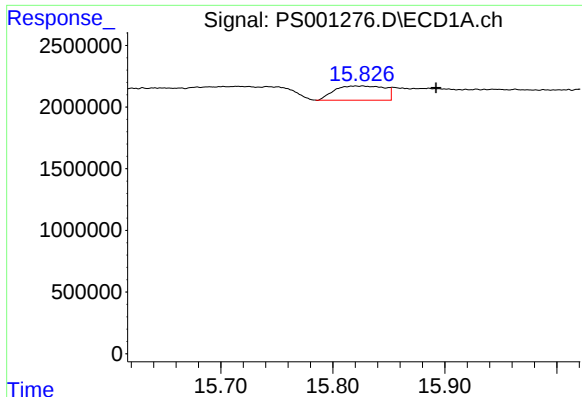

#13 2,4-DB


R.T.: 15.823 min
Delta R.T.: -0.069 min
Response: 3587544
Conc: 24.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

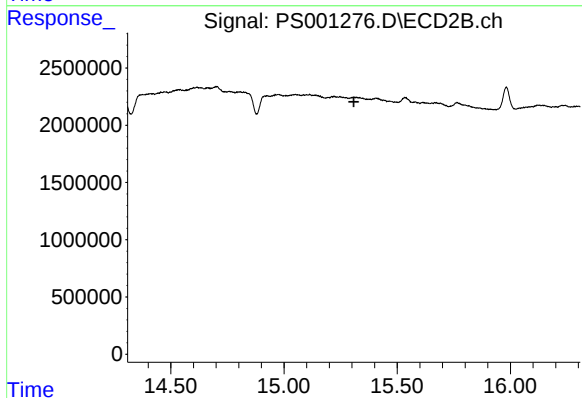


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 15.308 min
Response: 0
Conc: N.D.

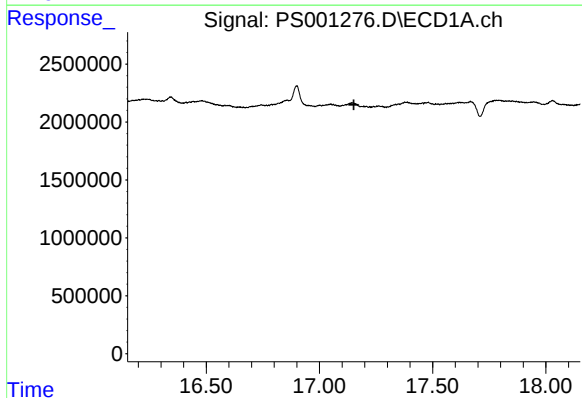


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.152 min
Response: 0
Conc: N.D.

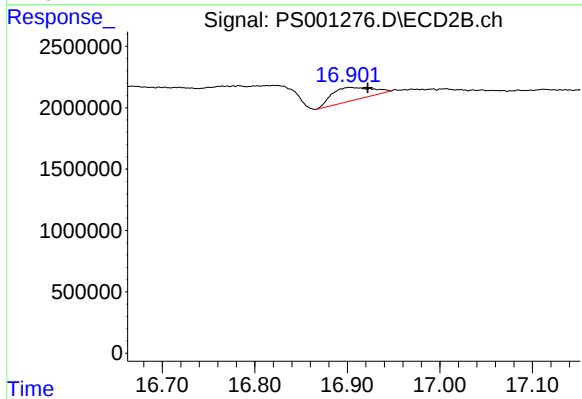

#15 Picloram


R.T.: 16.903 min
Delta R.T.: -0.019 min
Response: 3247950
Conc: 2.36 ng/ml

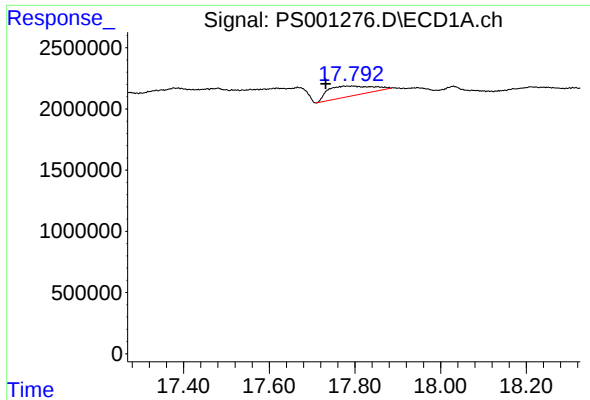

#16 DCPA

R.T.: 17.782 min
Delta R.T.: 0.050 min
Response: 5967779
Conc: 4.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

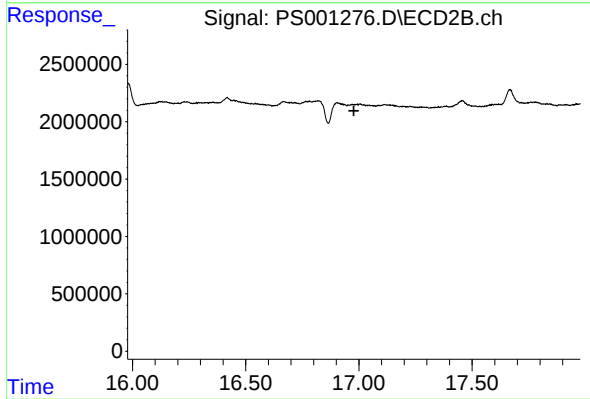

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 16.978 min
Response: 0
Conc: N.D.