

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072621\
 Data File : PS016181.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2021 09:16
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 02:36:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
 Quant Title : 8080.M
 QLast Update : Wed Jun 30 00:31:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.188	6.765	618.2E6	249.8E6	402.673	486.583
Target Compounds							
12) T	2,4,5-T	9.382f	0.000	14115083	0	1.808	N.D. #
15) T	Picloram	11.011f	10.836	86707464	33346075	7.882	8.015
16) T	DCPA	0.000	10.836f	0	33346075	N.D.	7.754



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072621\
Data File : PS016181.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2021 09:16
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 02:36:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
Quant Title : 8080.M
QLast Update : Wed Jun 30 00:31:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

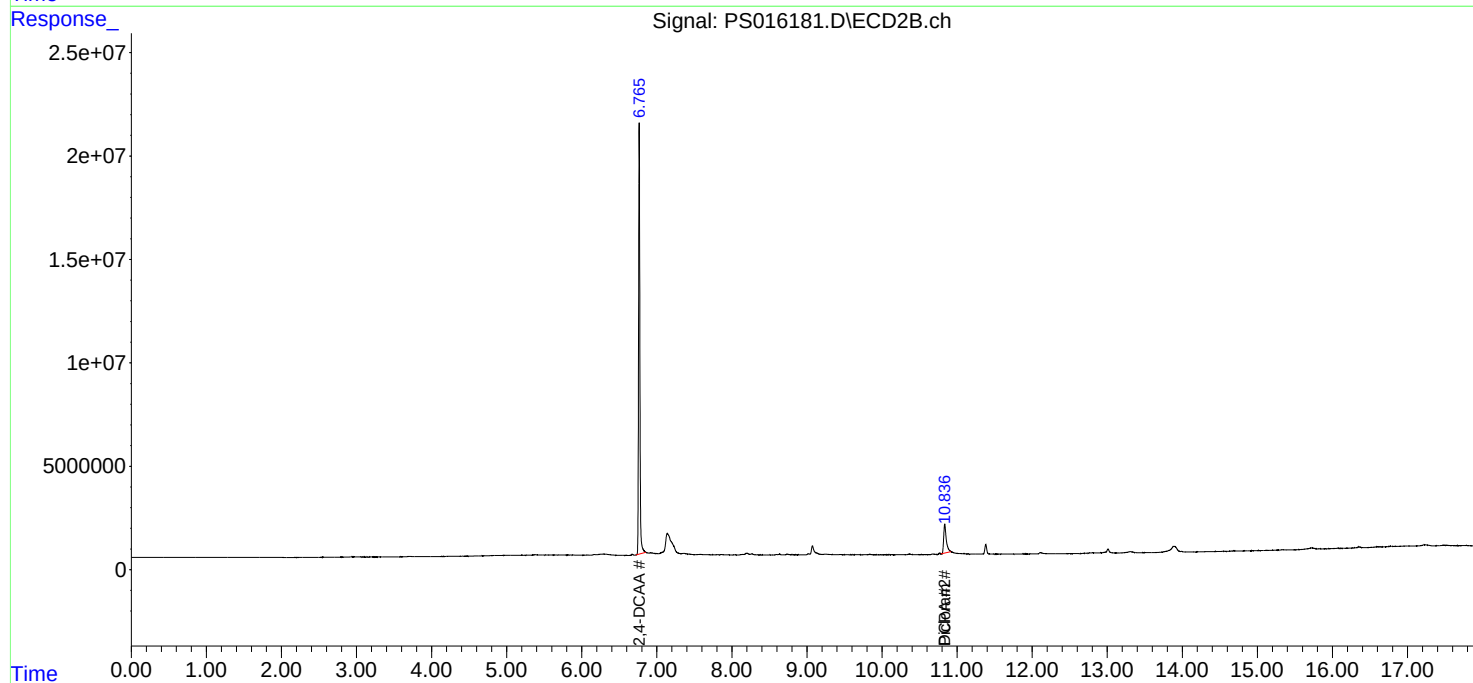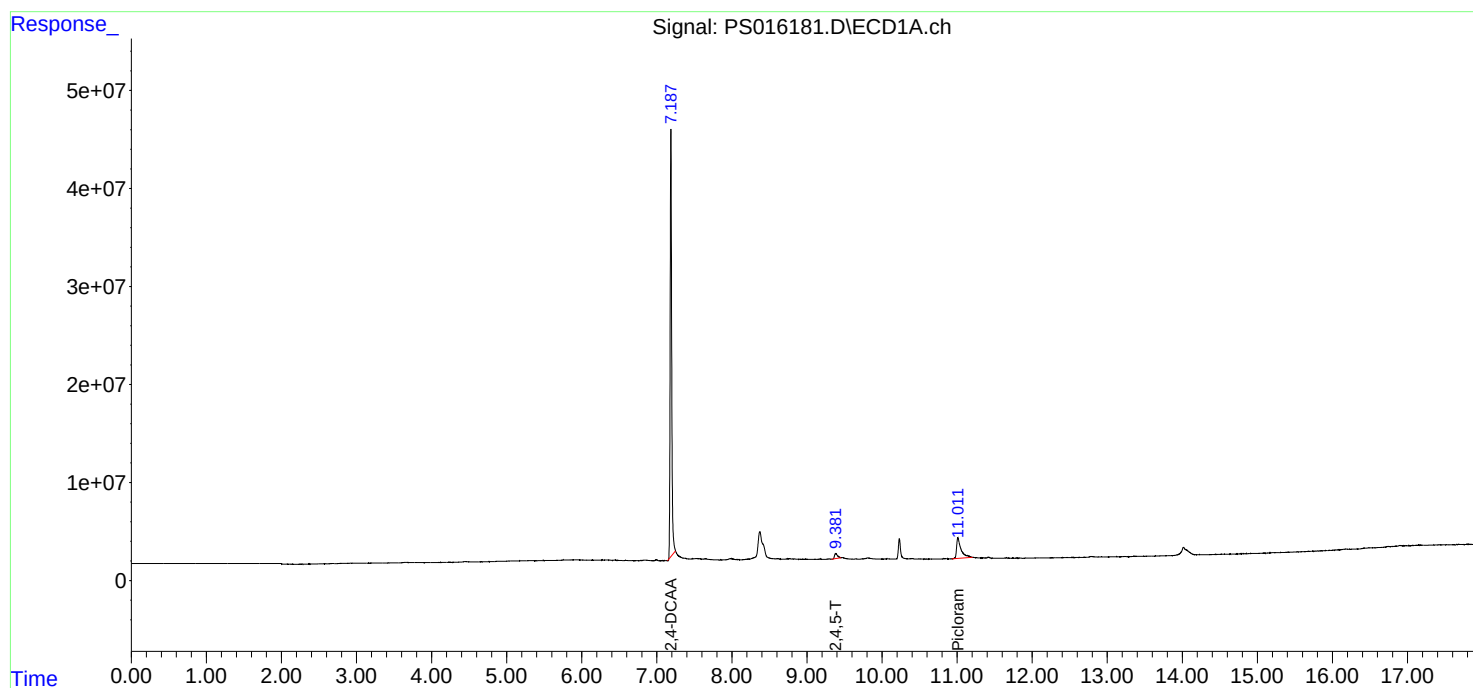


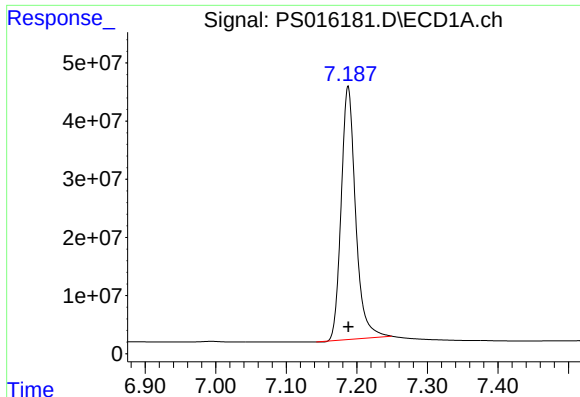

#4 2,4-DCAA


R.T.: 7.188 min
Delta R.T.: 0.000 min
Response: 618183753
Conc: 402.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

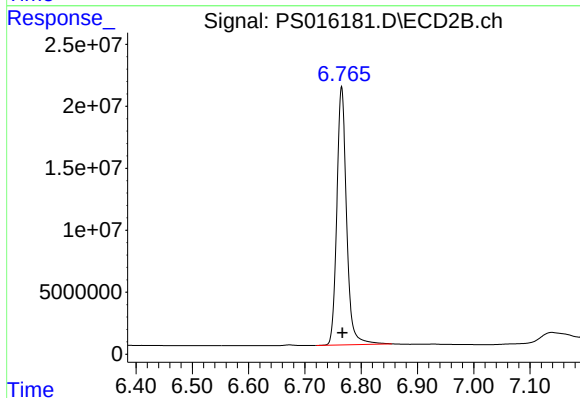


#4 2,4-DCAA

R.T.: 6.765 min
Delta R.T.: -0.001 min
Response: 249771371
Conc: 486.58 ng/ml

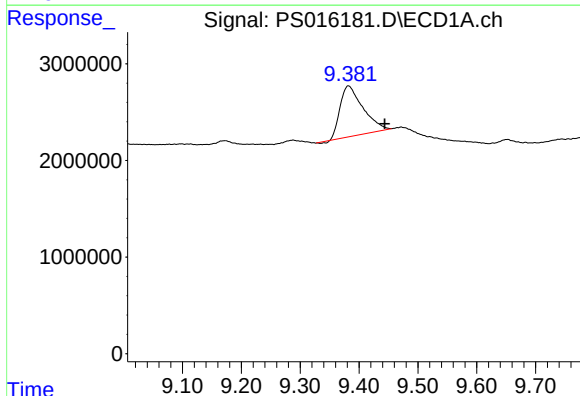


#12 2,4,5-T

R.T.: 9.382 min
Delta R.T.: -0.061 min
Response: 14115083
Conc: 1.81 ng/ml

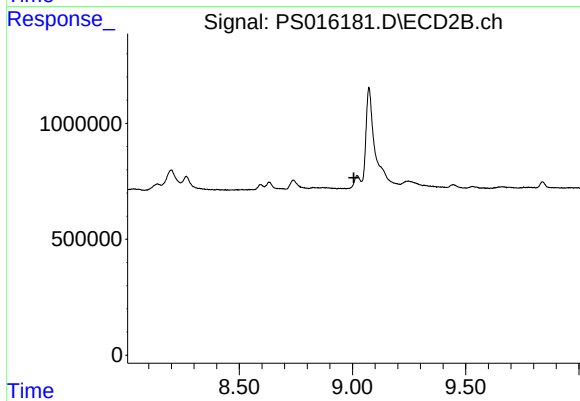

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.006 min
Response: 0
Conc: N.D.

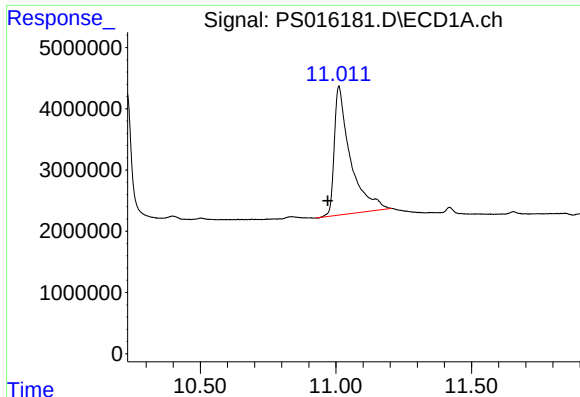

#15 Picloram


R.T.: 11.011 min
Delta R.T.: 0.041 min
Response: 86707464
Conc: 7.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

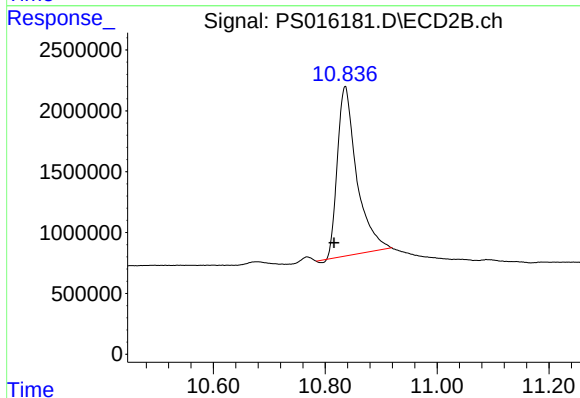


#15 Picloram

R.T.: 10.836 min
Delta R.T.: 0.020 min
Response: 33346075
Conc: 8.01 ng/ml

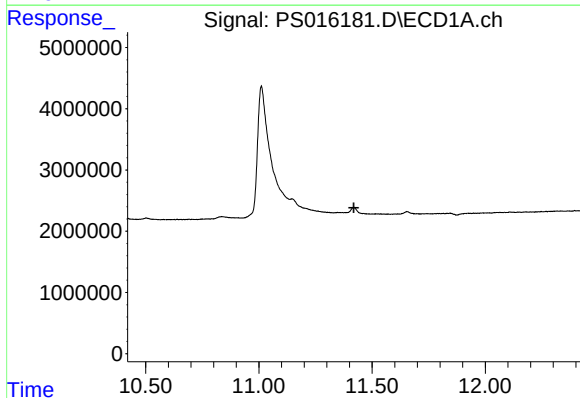

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.420 min
Response: 0
Conc: N.D.

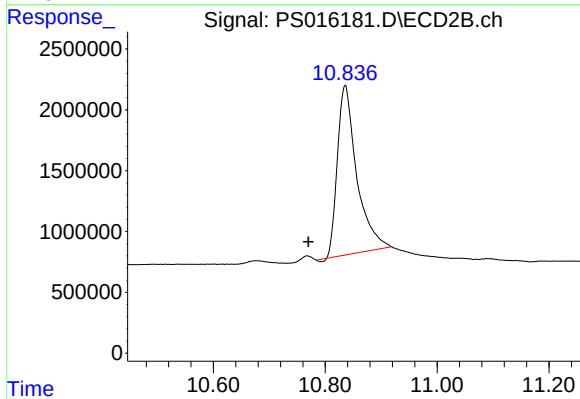

#16 DCPA

R.T.: 10.836 min
Delta R.T.: 0.066 min
Response: 33346075
Conc: 7.75 ng/ml