

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072624\
 Data File : PS027211.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2024 09:13
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 00:24:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071224.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	7.771	0	1144729	N.D.	<MDL
Target Compounds							
1) T	Dalapon	2.667f	2.669f	3472260	1293233	1.044	<MDL #
2) T	3,5-DICHL...	6.349f	0.000	6652749	0	1.682	N.D. #
3) T	4-Nitroph...	6.990	7.251f	3559069	1297469	2.220	<MDL #
5) T	DICAMBA	0.000	7.946	0	5120068	N.D.	<MDL
6) T	MCP	7.520f	8.048	11957969	23294	1.558	<MDL #
10) T	Pentachlo...	8.636f	9.515	5809022	381768	<MDL	<MDL #
12) T	2,4,5-T	0.000	10.325	0	3655847	N.D.	<MDL
13) T	2,4-DB	10.066f	10.913f	9364622	206579	4.334	<MDL #
14) T	DINOSEB	11.214	11.297f	14145880	269495	1.256	<MDL #
15) T	Picloram	11.059	12.359	82775204	15372858	4.249	<MDL #
16) T	DCPA	11.497f	12.261f	31411030	5784032	1.750	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072624\
Data File : PS027211.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2024 09:13
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 00:24:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071224.M
Quant Title : 8080.M
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

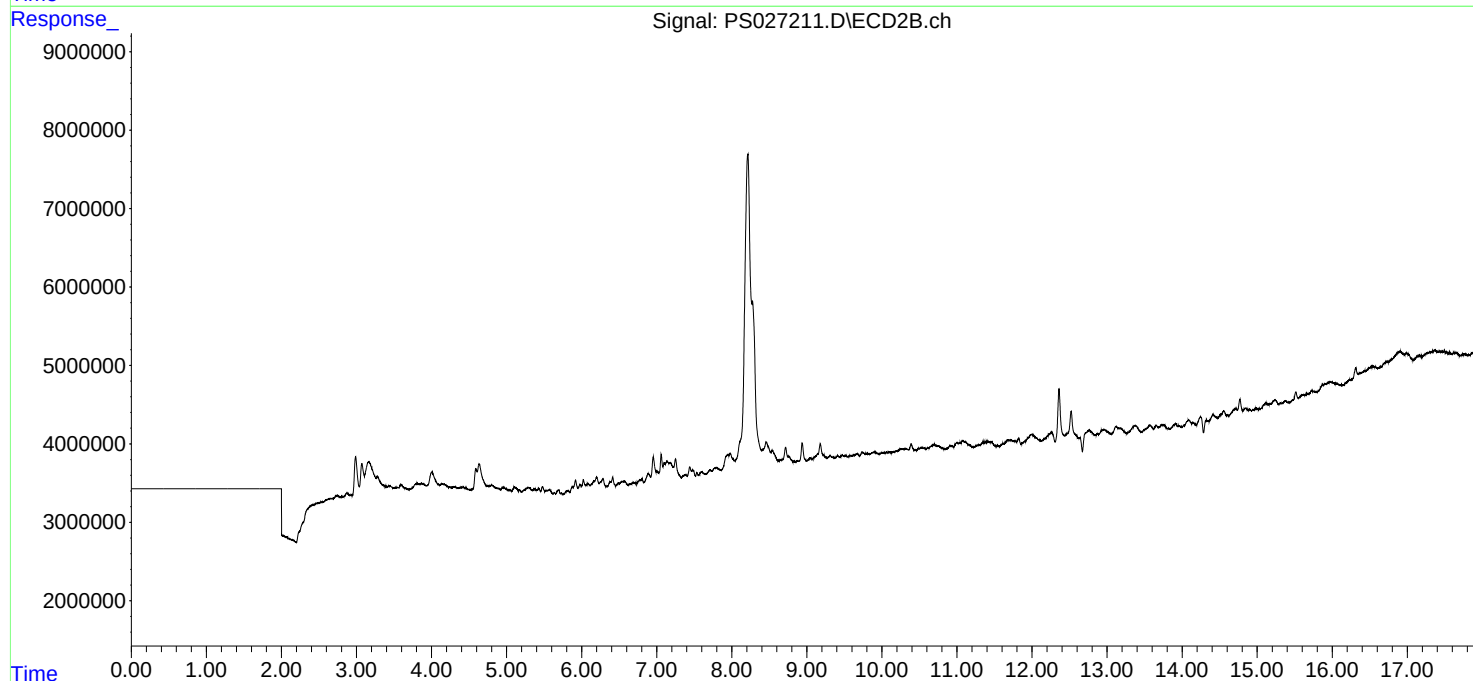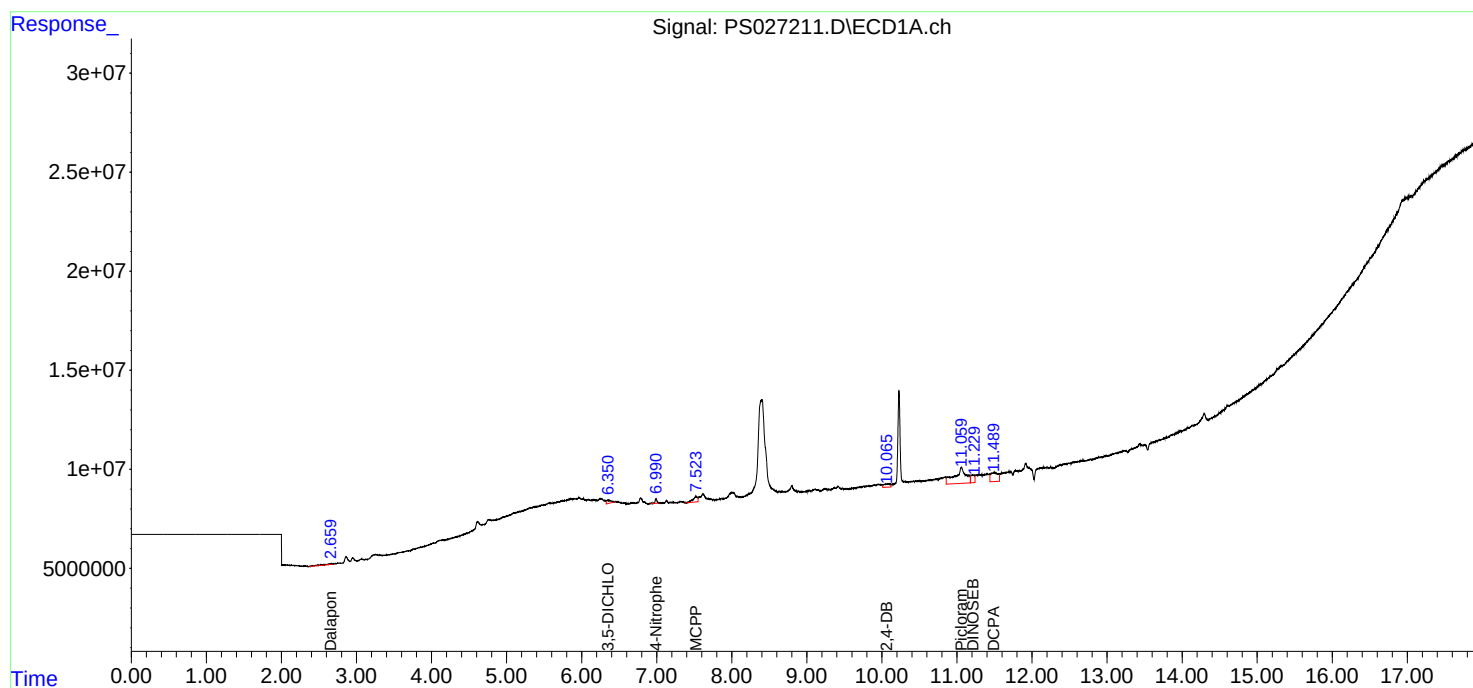


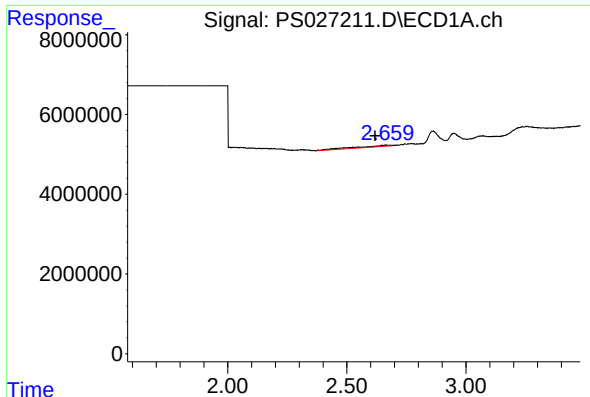

#1 Dalapon


R.T.: 2.667 min
Delta R.T.: 0.048 min
Response: 3472260
Conc: 1.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

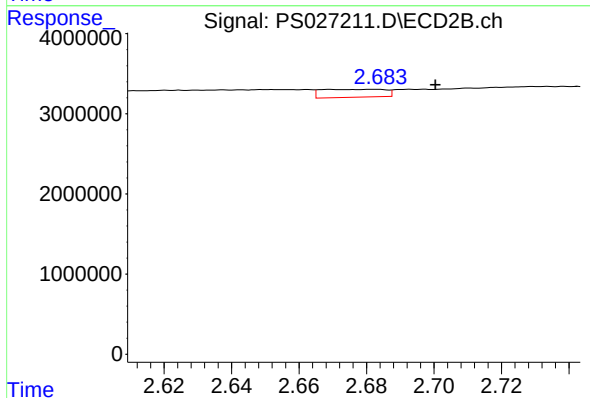


#1 Dalapon

R.T.: 2.669 min
Delta R.T.: -0.031 min
Response: 1293233
Conc: N.D.

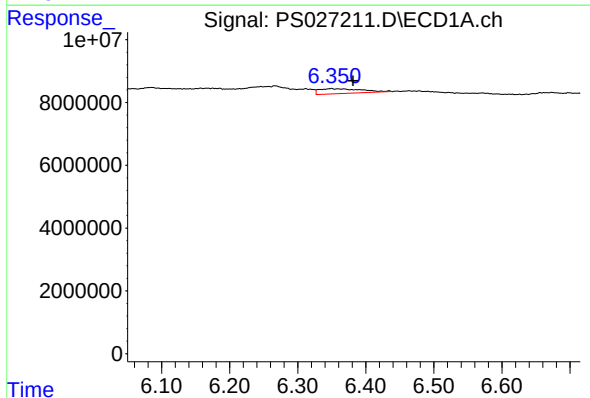


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.349 min
Delta R.T.: -0.032 min
Response: 6652749
Conc: 1.68 ng/ml

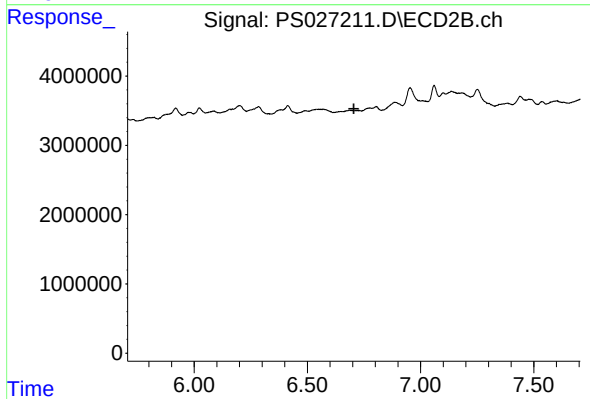

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.705 min
Response: 0
Conc: N.D.

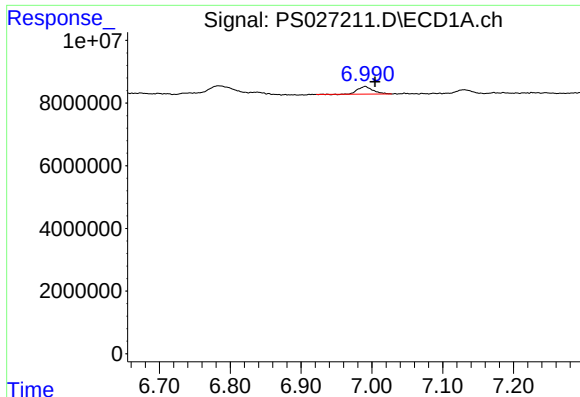

#3 4-Nitrophenol


R.T.: 6.990 min
Delta R.T.: -0.014 min
Response: 3559069
Conc: 2.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

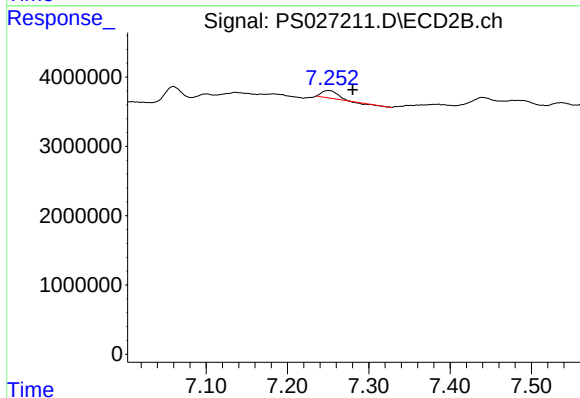


#3 4-Nitrophenol

R.T.: 7.251 min
Delta R.T.: -0.029 min
Response: 1297469
Conc: N.D.

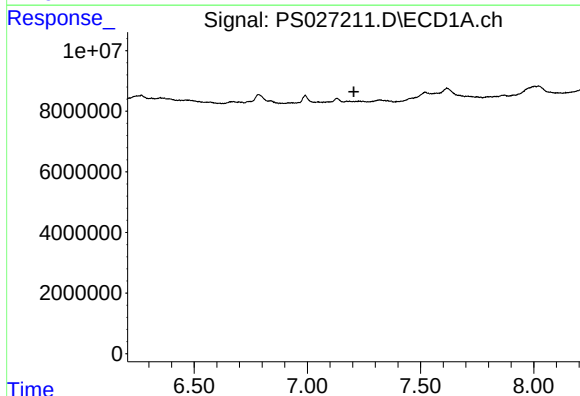


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.205 min
Response: 0
Conc: N.D.

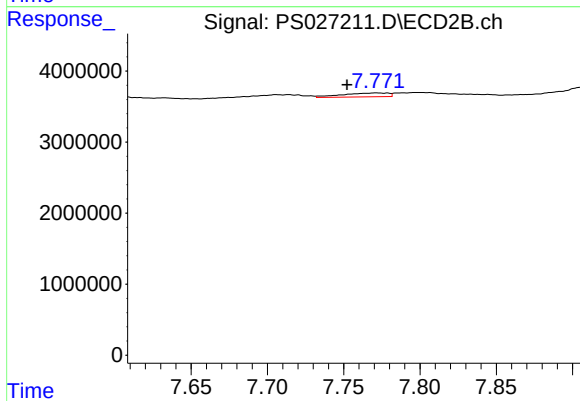

#4 2,4-DCAA


R.T.: 7.771 min
Delta R.T.: 0.019 min
Response: 1144729
Conc: N.D.

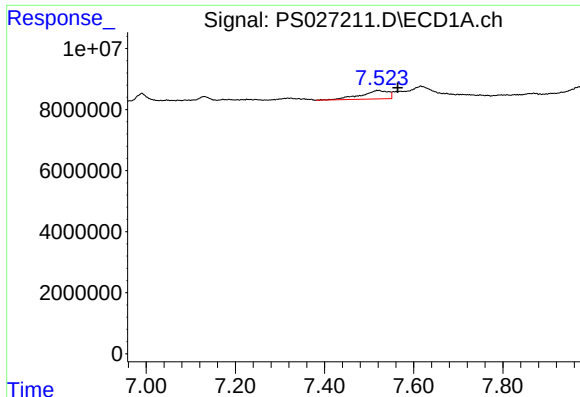

#6 MCPP


R.T.: 7.520 min
Delta R.T.: -0.044 min
Response: 11957969
Conc: 1.56 ug/ml

Instrument :
ECD_S
ClientSampleId :

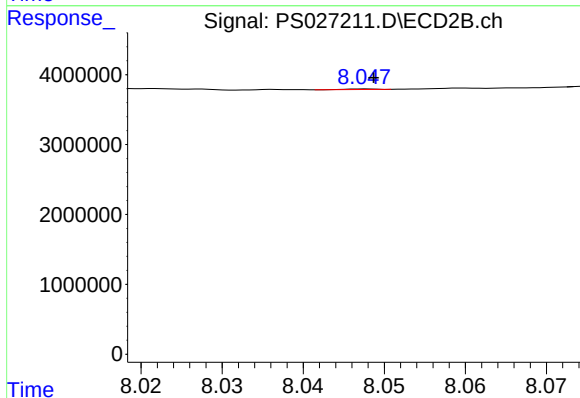


#6 MCPP

R.T.: 8.048 min
Delta R.T.: -0.001 min
Response: 23294
Conc: N.D.

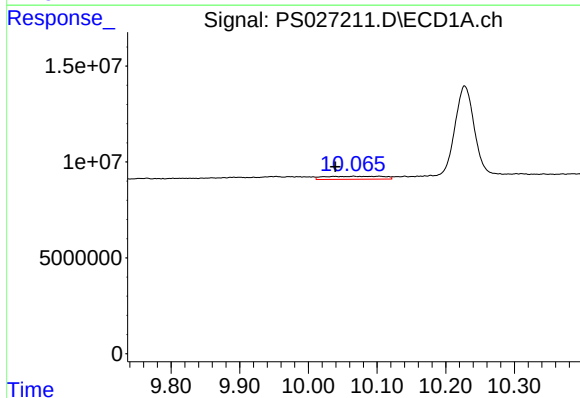


#13 2,4-DB

R.T.: 10.066 min
Delta R.T.: 0.027 min
Response: 9364622
Conc: 4.33 ng/ml

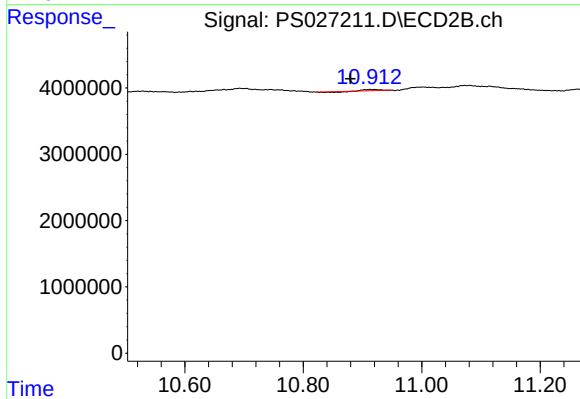

#13 2,4-DB


R.T.: 10.913 min
Delta R.T.: 0.033 min
Response: 206579
Conc: N.D.

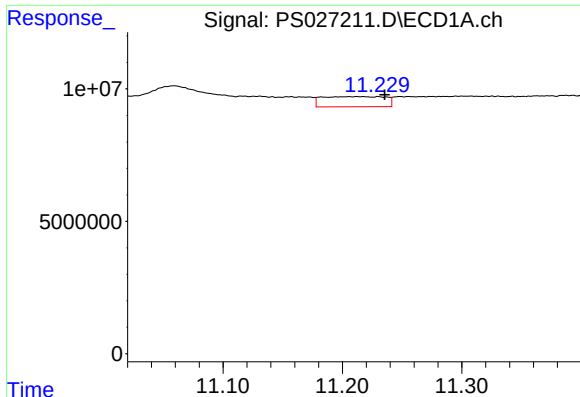

#14 DINOSEB


R.T.: 11.214 min
Delta R.T.: -0.022 min
Response: 14145880
Conc: 1.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

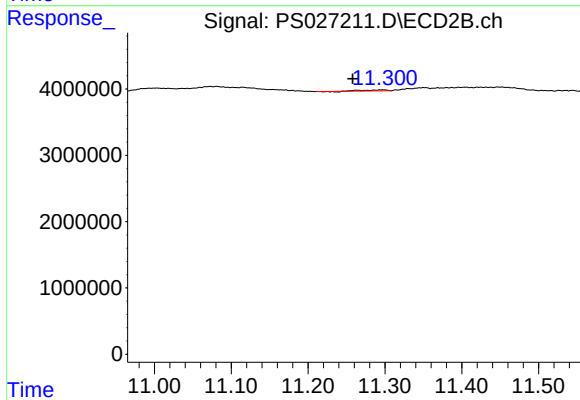


#14 DINOSEB

R.T.: 11.297 min
Delta R.T.: 0.039 min
Response: 269495
Conc: N.D.

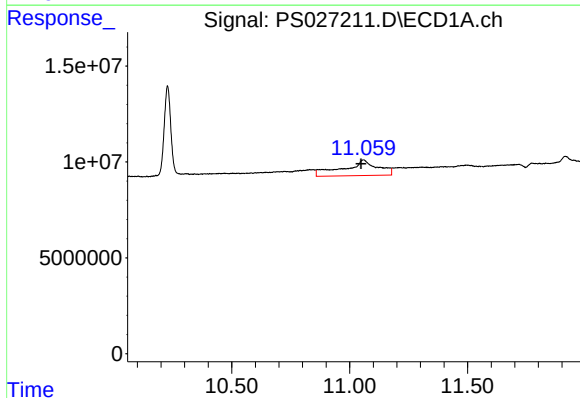


#15 Picloram

R.T.: 11.059 min
Delta R.T.: 0.009 min
Response: 82775204
Conc: 4.25 ng/ml

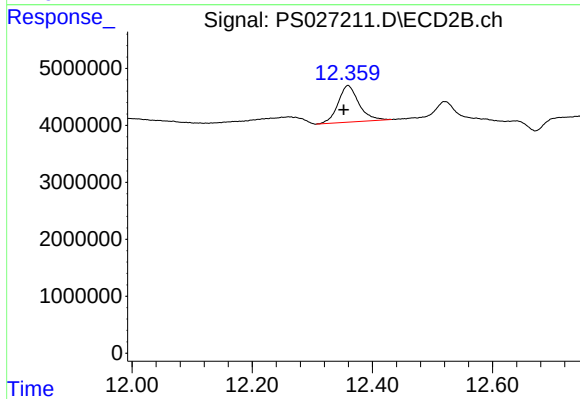

#15 Picloram


R.T.: 12.359 min
Delta R.T.: 0.007 min
Response: 15372858
Conc: N.D.

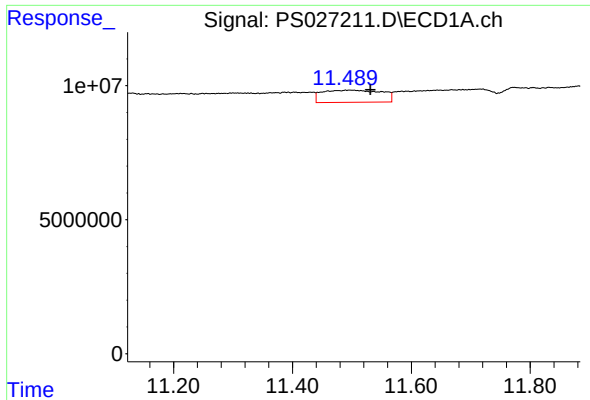

#16 DCPA

R.T.: 11.497 min
Delta R.T.: -0.034 min
Response: 31411030
Conc: 1.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

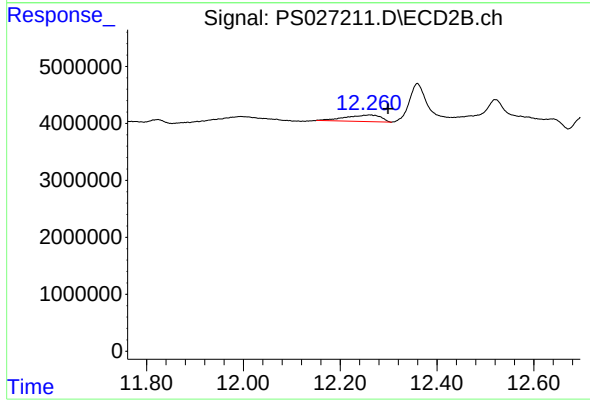

#16 DCPA

R.T.: 12.261 min
Delta R.T.: -0.038 min
Response: 5784032
Conc: N.D.