

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072624\
 Data File : PS027221.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2024 19:33
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 00:32:38 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071224.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.196	7.750	1264.3E6	1096.3E6	499.971	472.805
Target Compounds							
1) T	Dalapon	0.000	2.733f	0	3877156	N.D.	<MDL
2) T	3,5-DICHL...	6.351f	0.000	15309214	0	3.871	N.D. #
3) T	4-Nitroph...	6.993	0.000	5943070	0	3.707	N.D. #
5) T	DICAMBA	0.000	7.934	0	4717759	N.D.	<MDL
6) T	MCP	7.569	8.034	22540644	33885	2.936	<MDL #
8) T	DICHLORPROP	8.091	8.713f	2419024	-1649467	<MDL	N.D. #
9) T	2,4-D	0.000	9.042f	0	52228	N.D.	<MDL
10) T	Pentachlo...	8.598	0.000	15166078	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.151f	9.902	5324502	655407	<MDL	<MDL #
12) T	2,4,5-T	9.471	10.314	8081732	1789238	<MDL	<MDL #
13) T	2,4-DB	10.050	0.000	18647388	0	8.629	N.D. #
15) T	Picloram	11.061	12.359	30973537	3257702	1.590	<MDL #
16) T	DCPA	0.000	12.268f	0	4848437	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072624\
Data File : PS027221.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2024 19:33
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 00:32:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071224.M
Quant Title : 8080.M
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

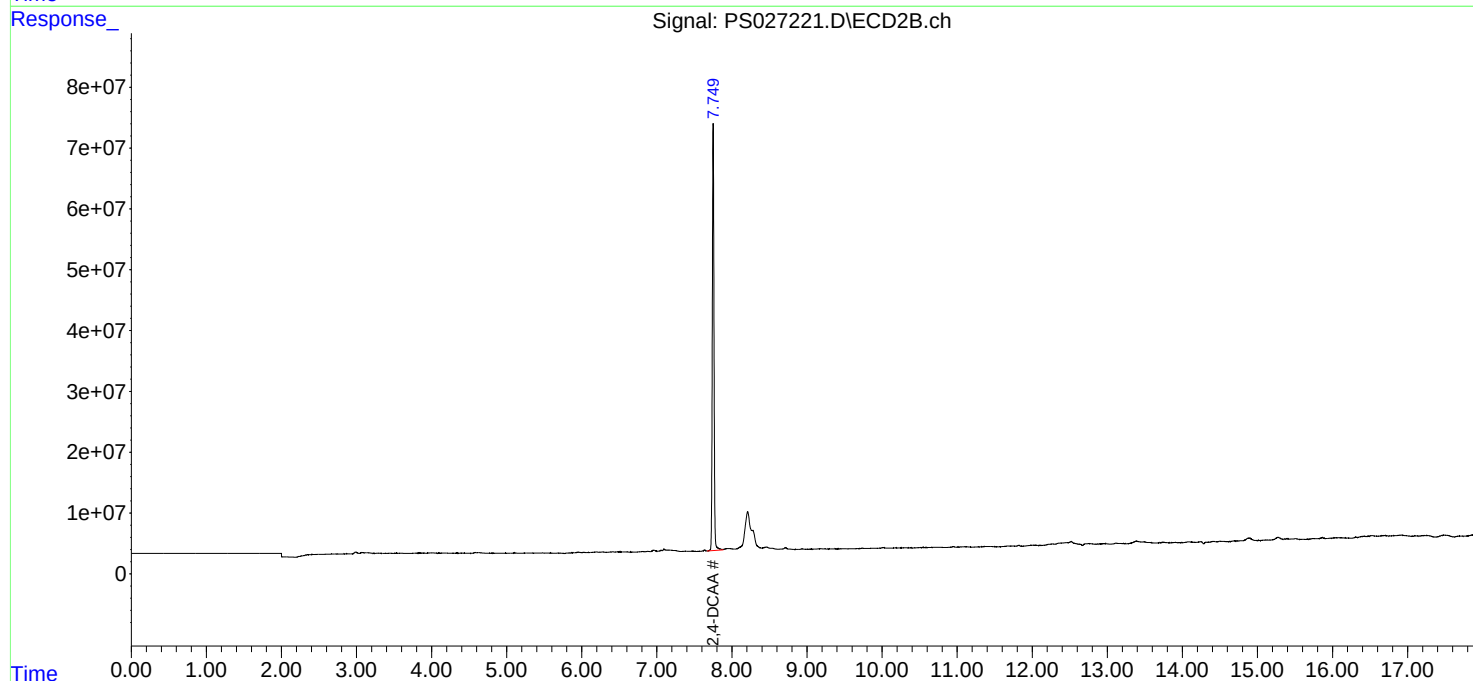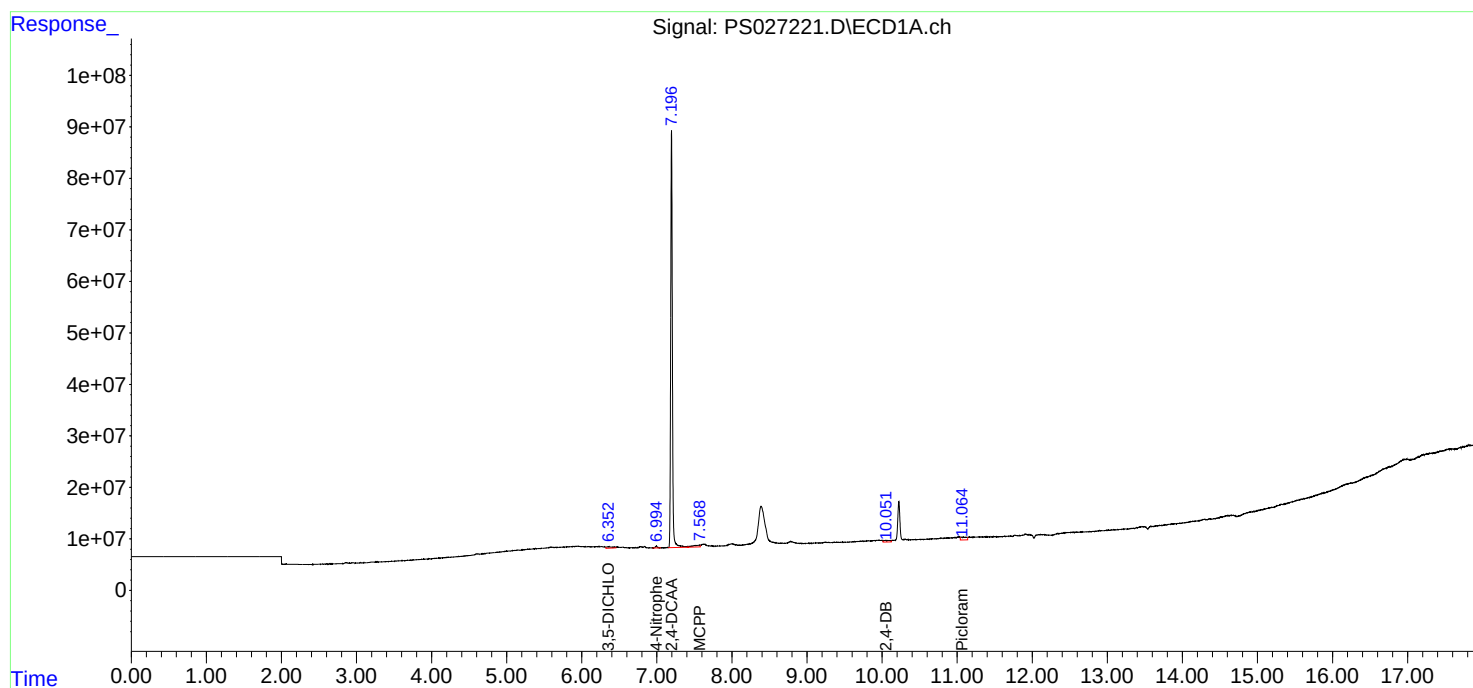


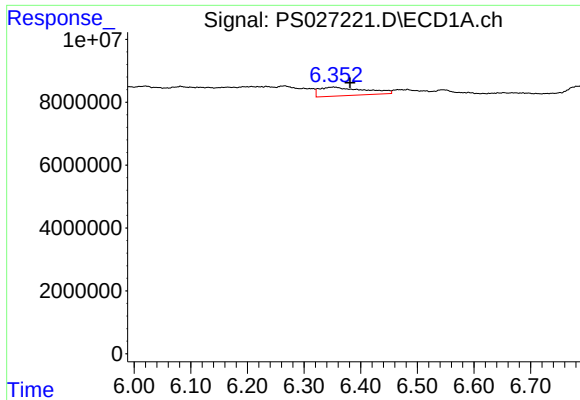

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.351 min
Delta R.T.: -0.030 min
Response: 15309214
Conc: 3.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

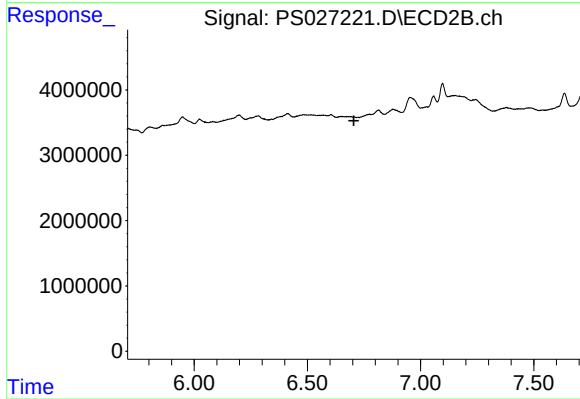


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.705 min
Response: 0
Conc: N.D.

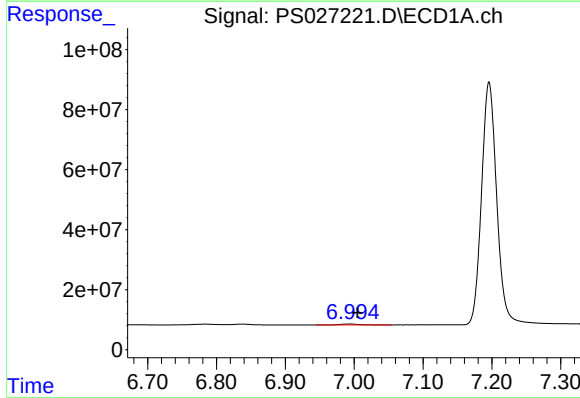


#3 4-Nitrophenol

R.T.: 6.993 min
Delta R.T.: -0.011 min
Response: 5943070
Conc: 3.71 ng/ml

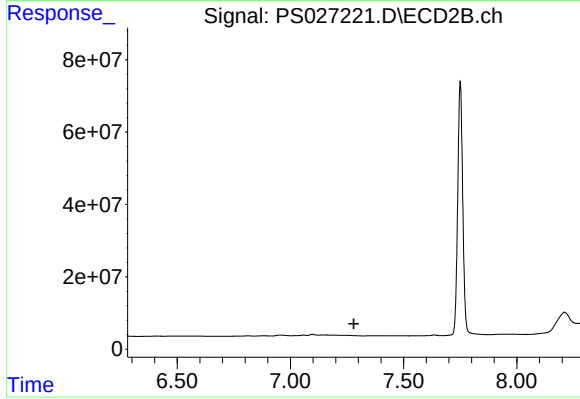

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.280 min
Response: 0
Conc: N.D.

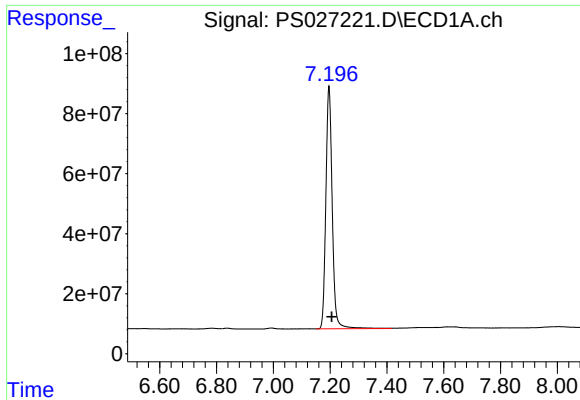

#4 2,4-DCAA


R.T.: 7.196 min
Delta R.T.: -0.009 min
Response: 1264308761
Conc: 499.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

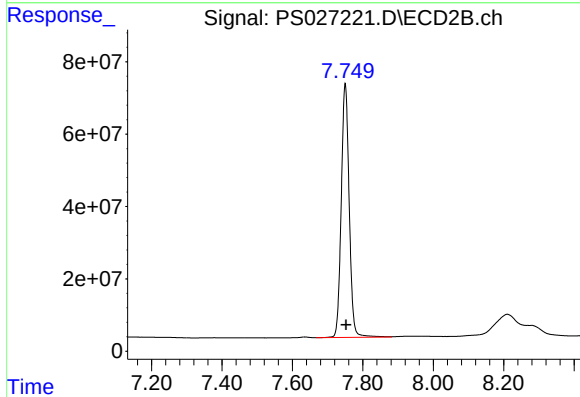


#4 2,4-DCAA

R.T.: 7.750 min
Delta R.T.: -0.002 min
Response: 1096303187
Conc: 472.80 ng/ml

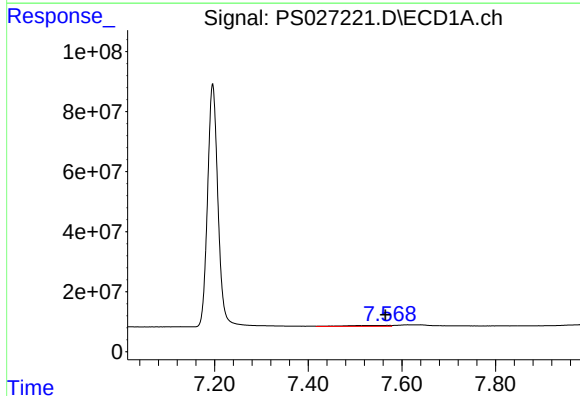


#6 MCP

R.T.: 7.569 min
Delta R.T.: 0.004 min
Response: 22540644
Conc: 2.94 ug/ml

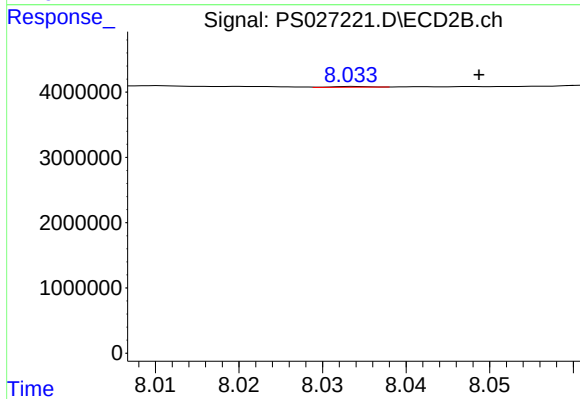

#6 MCP


R.T.: 8.034 min
Delta R.T.: -0.015 min
Response: 33885
Conc: N.D.

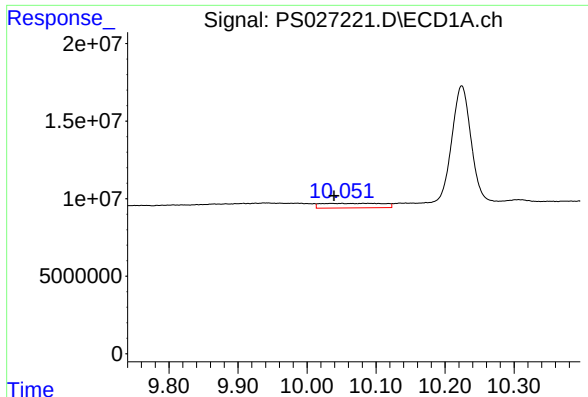

#13 2,4-DB


R.T.: 10.050 min
Delta R.T.: 0.011 min
Response: 18647388
Conc: 8.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

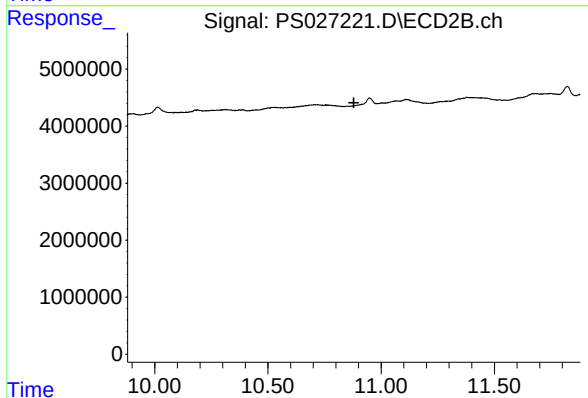


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.880 min
Response: 0
Conc: N.D.

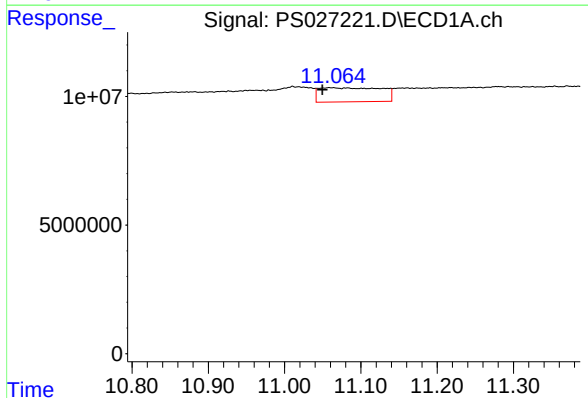

#15 Picloram

R.T.: 11.061 min
Delta R.T.: 0.011 min
Response: 30973537
Conc: 1.59 ng/ml

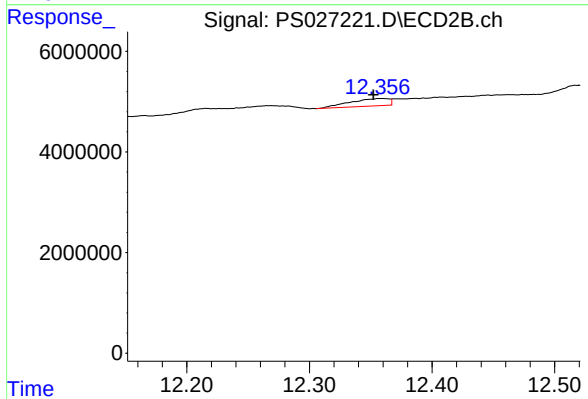

#15 Picloram

R.T.: 12.359 min
Delta R.T.: 0.007 min
Response: 3257702
Conc: N.D.