

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072719\
 Data File : PS005720.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2019 12:42
 Operator : SM\AJ
 Sample : K3614-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 BU-03-072419

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 00:52:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.556	5.275	264.6E6	199.4E6	182.363	200.509
Target Compounds							
2) T	3,5-DICHL...	0.000	4.594	0	52504406	N.D.	40.472
5) T	DICAMBA	5.776	0.000	21558547	0	3.610	N.D. #
7) T	MCPA	5.953	0.000	21195840	0	3.248	N.D. #
8) T	DICHLORPROP	0.000	5.965	0	15314567	N.D.	16.583
9) T	2,4-D	6.636	0.000	104.5E6	0	69.699	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072719\
Data File : PS005720.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2019 12:42
Operator : SM\AJ
Sample : K3614-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
BU-03-072419

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 00:52:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

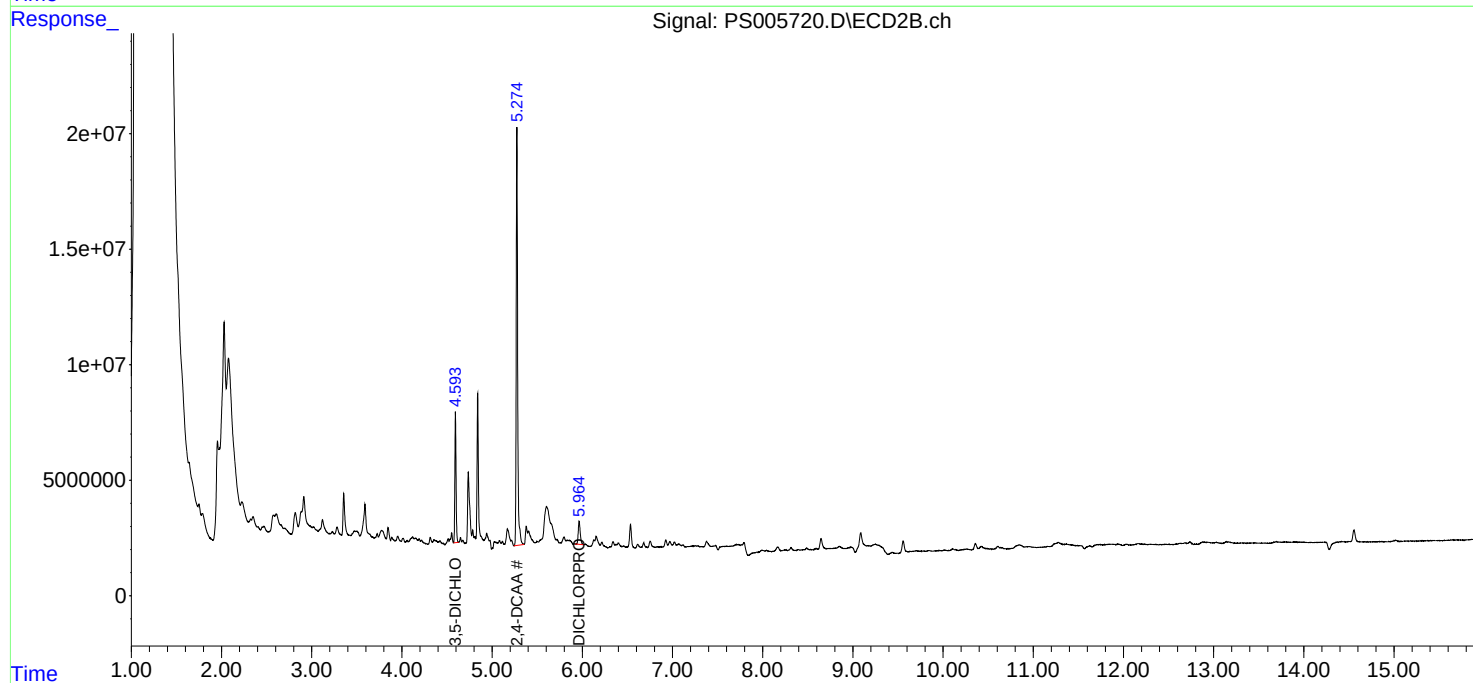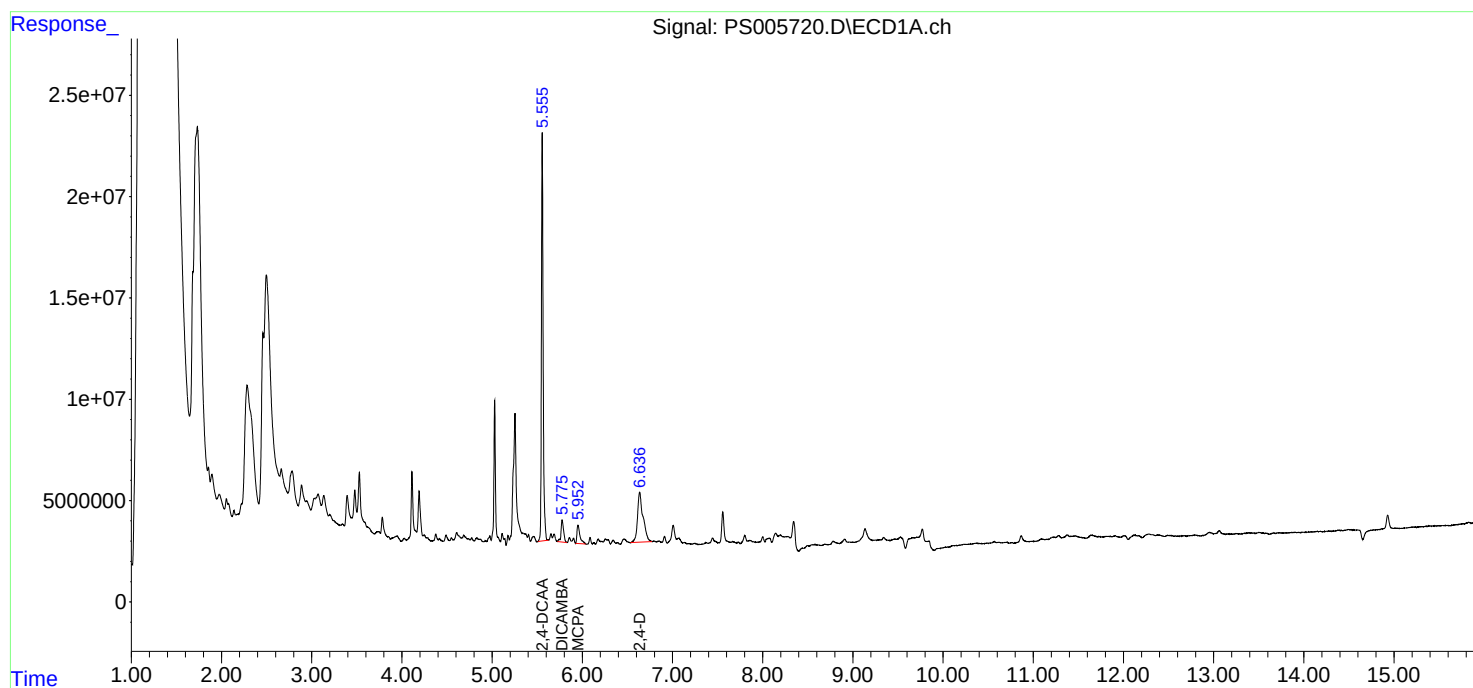


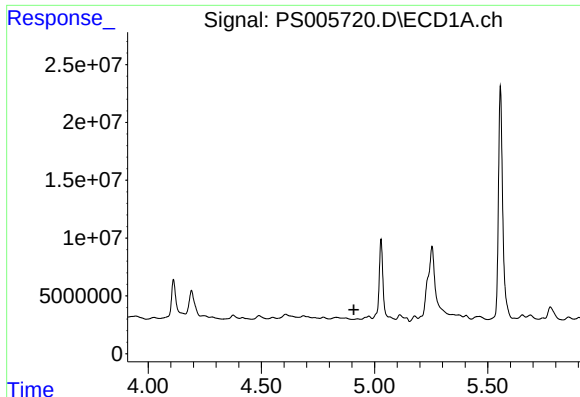

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BU-03-072419

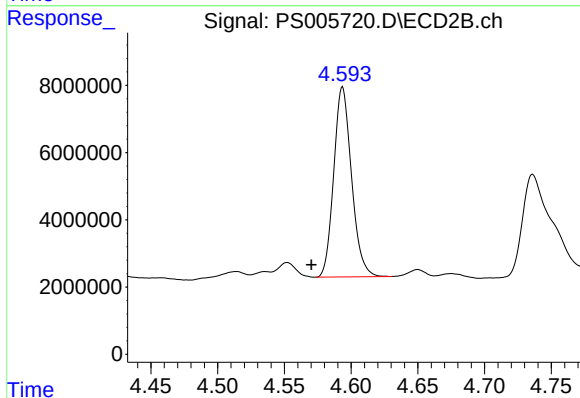


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.594 min
Delta R.T.: 0.023 min
Response: 52504406
Conc: 40.47 ng/ml

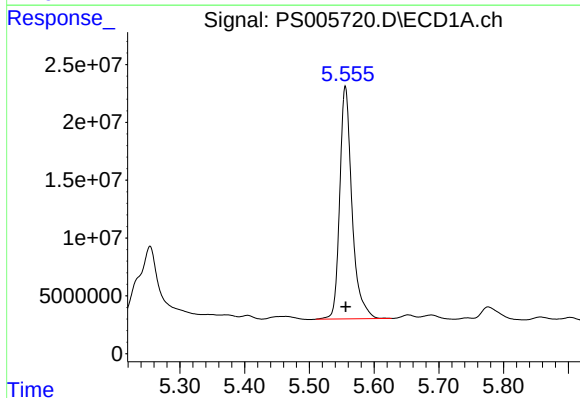


#4 2,4-DCAA

R.T.: 5.556 min
Delta R.T.: 0.000 min
Response: 264575081
Conc: 182.36 ng/ml

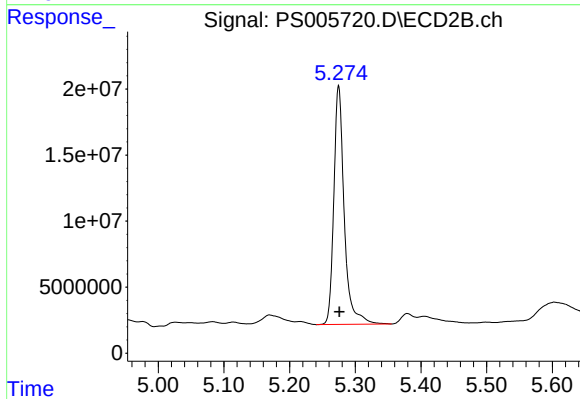

#4 2,4-DCAA


R.T.: 5.275 min
Delta R.T.: 0.000 min
Response: 199441854
Conc: 200.51 ng/ml

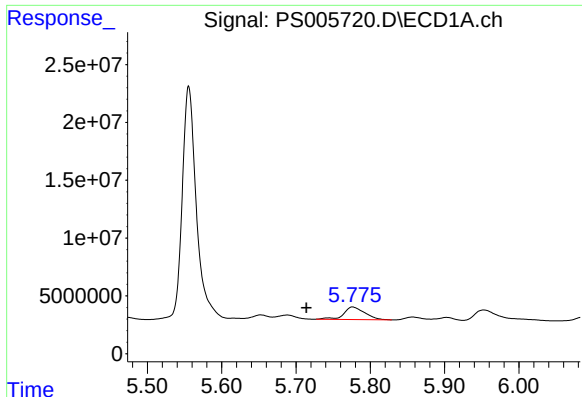

#5 DICAMBA


R.T.: 5.776 min
Delta R.T.: 0.062 min
Response: 21558547
Conc: 3.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
BU-03-072419

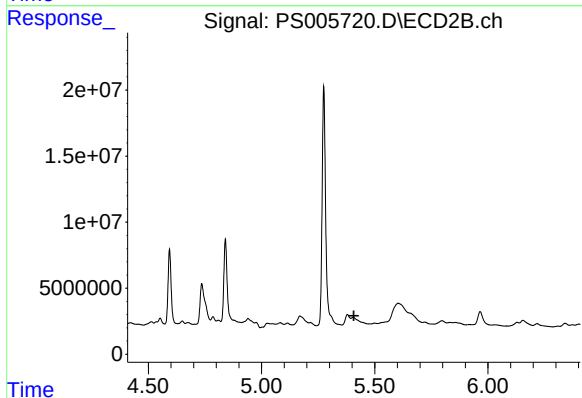


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.408 min
Response: 0
Conc: N.D.

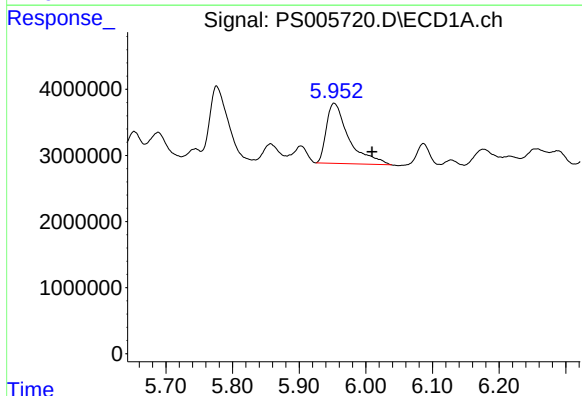


#7 MCPA

R.T.: 5.953 min
Delta R.T.: -0.057 min
Response: 21195840
Conc: 3.25 ug/ml

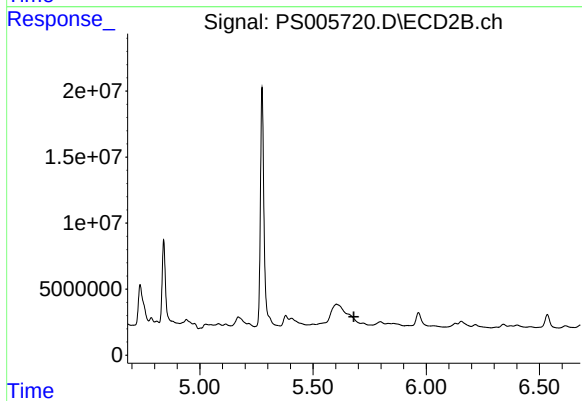

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 5.681 min
Response: 0
Conc: N.D.

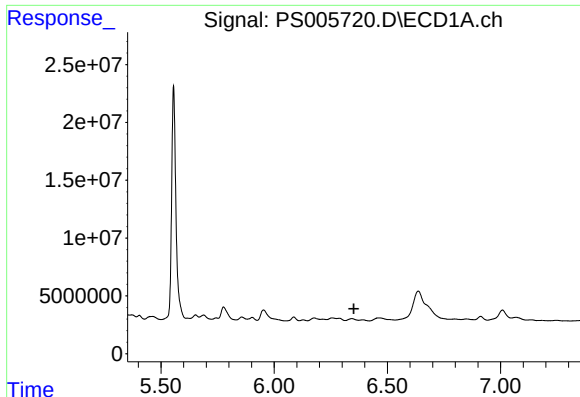

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BU-03-072419

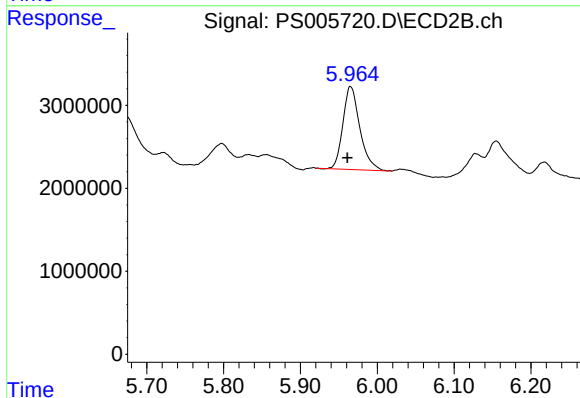


#8 DICHLORPROP

R.T.: 5.965 min
Delta R.T.: 0.004 min
Response: 15314567
Conc: 16.58 ng/ml

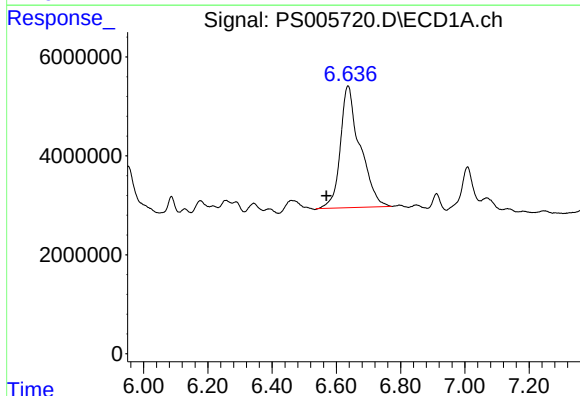

#9 2,4-D

R.T.: 6.636 min
Delta R.T.: 0.067 min
Response: 104455337
Conc: 69.70 ng/ml

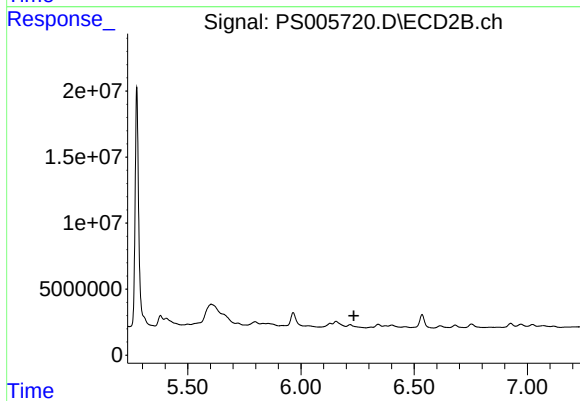

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.234 min
Response: 0
Conc: N.D.