

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072719\
 Data File : PS005723.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2019 13:48
 Operator : SM\AJ
 Sample : K3620-12
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-02-072519-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 00:54:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.593	5.313	274.8E6	195.9E6	189.402	196.915
Target Compounds							
2) T	3,5-DICHL...	0.000	4.632	0 68042473		N.D.	52.449
6) T	MCP	5.813	0.000	23613082	0	5.096	N.D. #
7) T	MCPA	0.000	5.642	0 112.9E6		N.D.	26.827
10) T	Pentachlo...	0.000	6.572	0 16516188		N.D.	1.272
11) T	2,4,5-TP ...	0.000	6.985	0 873.6E6		N.D.	168.404
12) T	2,4,5-T	7.595	0.000	31264607	0	3.746	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072719\
Data File : PS005723.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2019 13:48
Operator : SM\AJ
Sample : K3620-12
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-02-072519-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 00:54:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

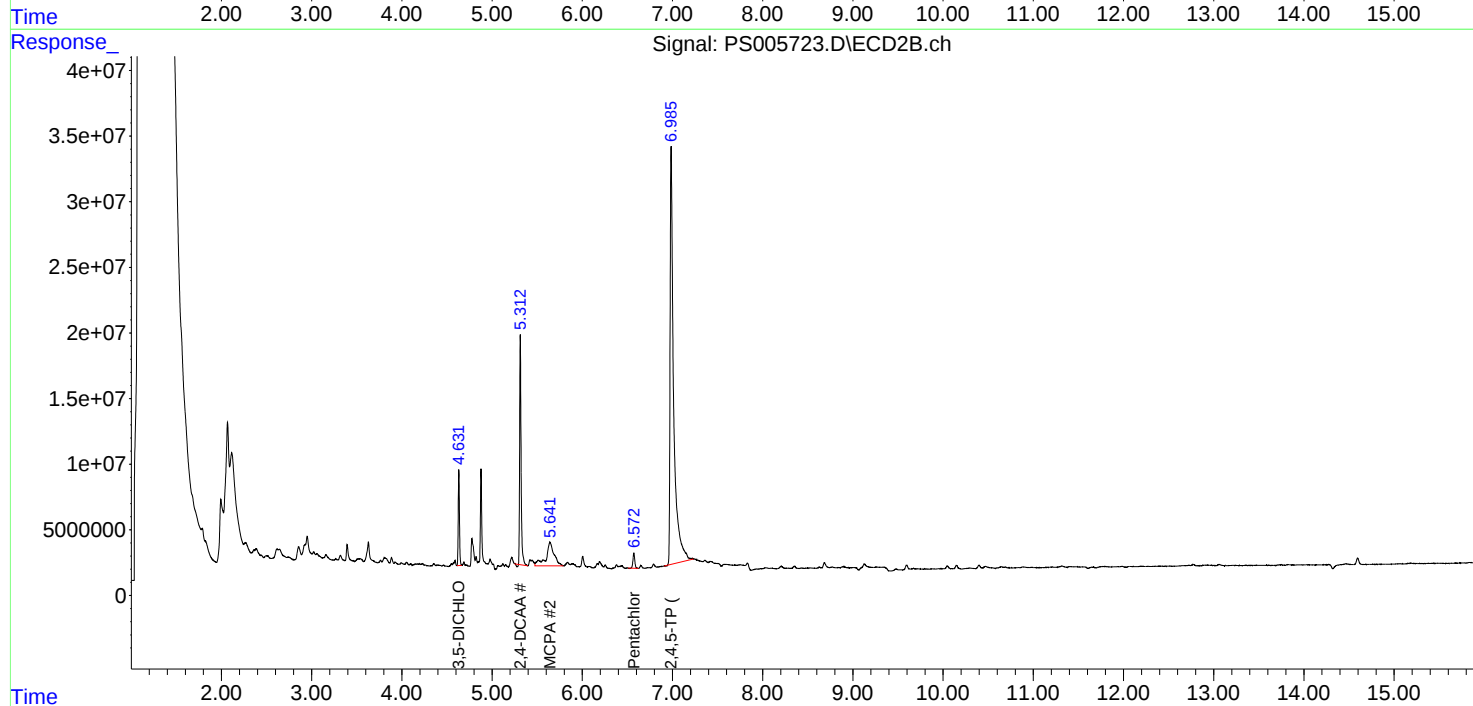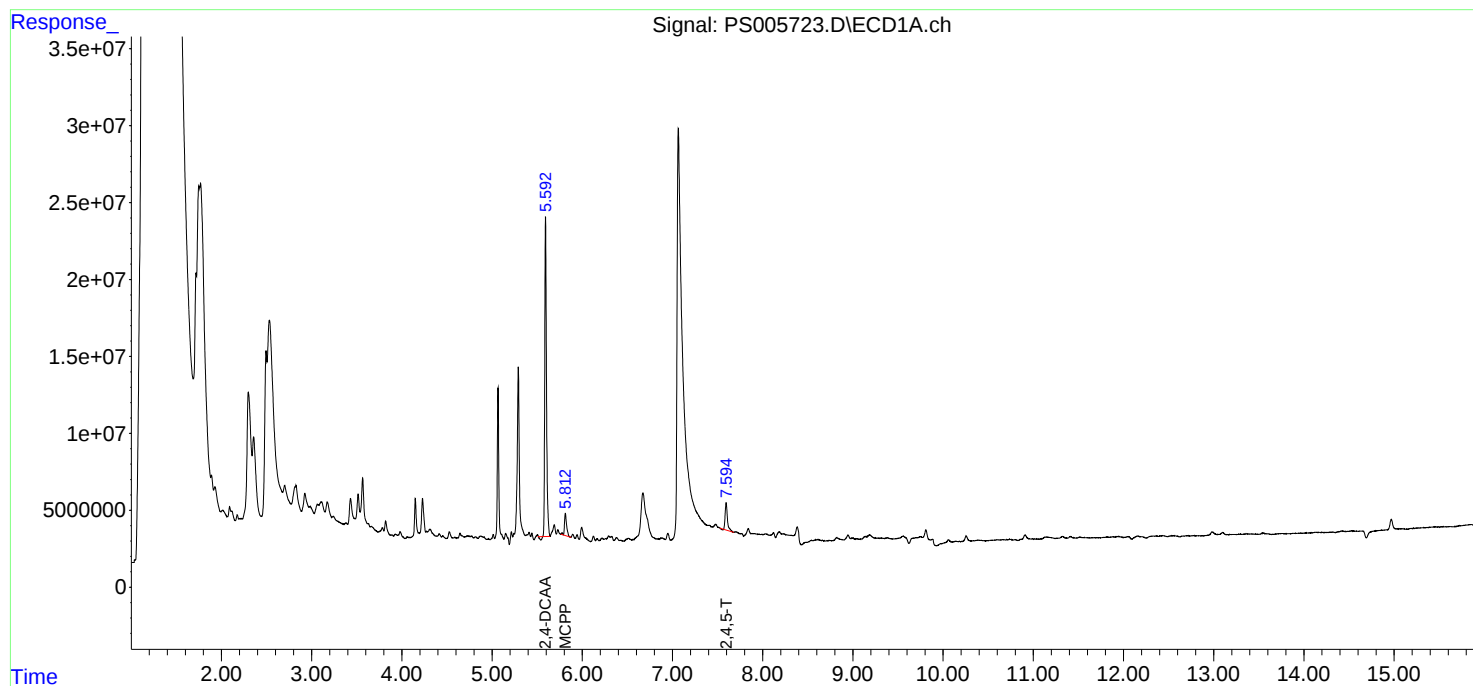


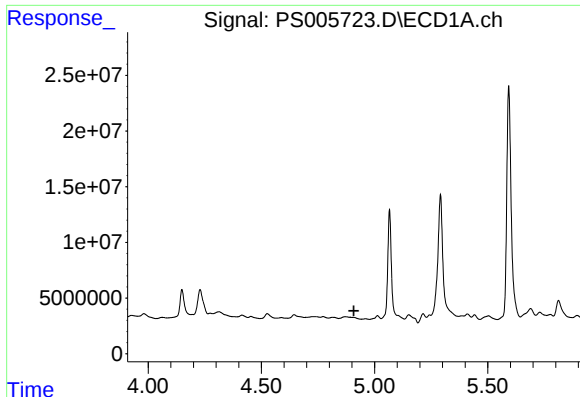

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-072519-A

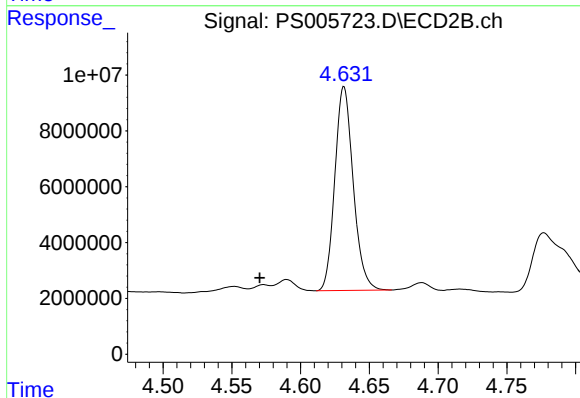


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.632 min
Delta R.T.: 0.061 min
Response: 68042473
Conc: 52.45 ng/ml

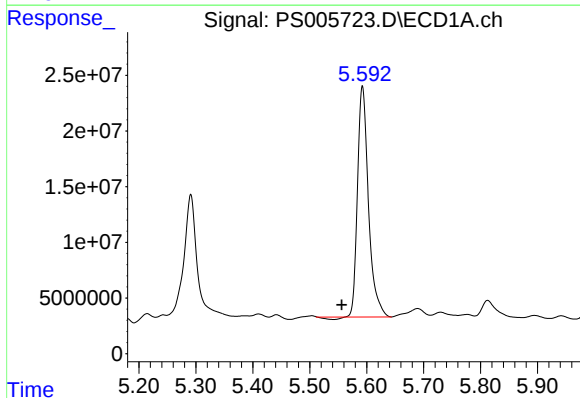


#4 2,4-DCAA

R.T.: 5.593 min
Delta R.T.: 0.037 min
Response: 274788203
Conc: 189.40 ng/ml

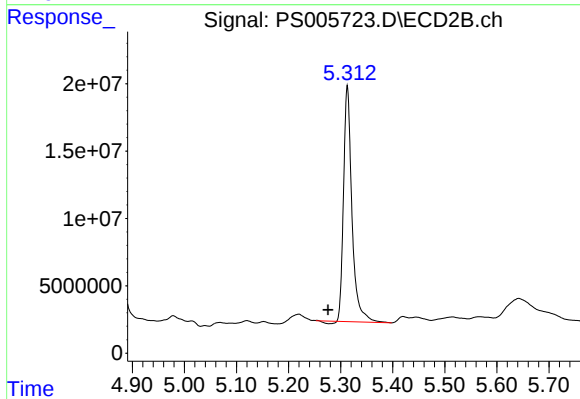

#4 2,4-DCAA


R.T.: 5.313 min
Delta R.T.: 0.037 min
Response: 195866745
Conc: 196.91 ng/ml

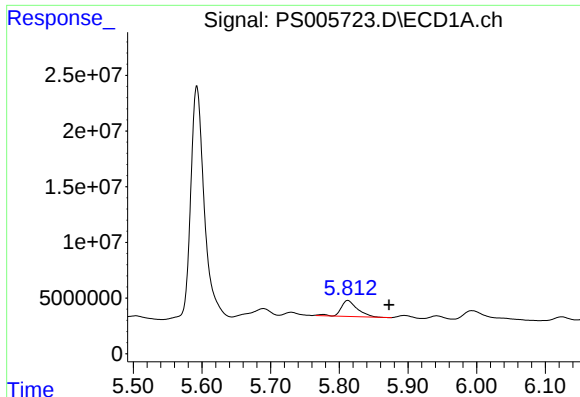

#6 MCPP


R.T.: 5.813 min
Delta R.T.: -0.060 min
Response: 23613082
Conc: 5.10 ug/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-072519-A

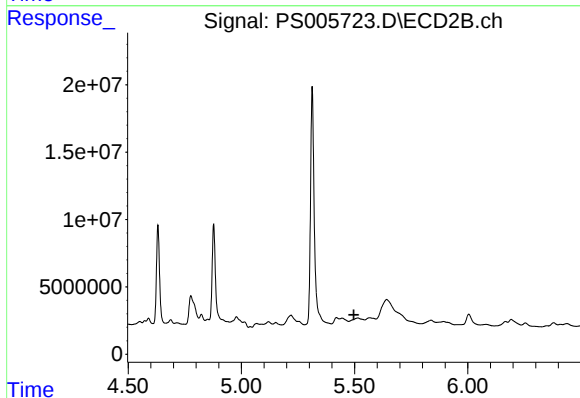


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.497 min
Response: 0
Conc: N.D.

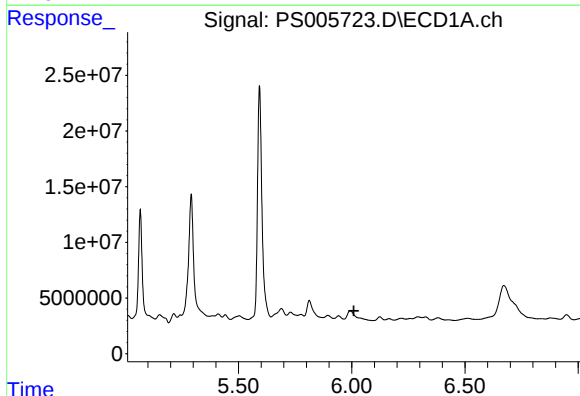


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.009 min
Response: 0
Conc: N.D.

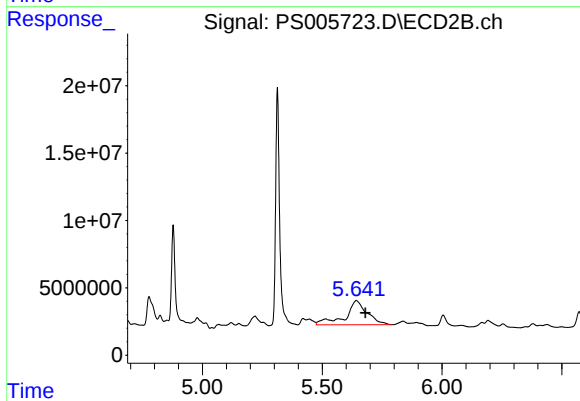

#7 MCPA


R.T.: 5.642 min
Delta R.T.: -0.039 min
Response: 112915162
Conc: 26.83 ug/ml

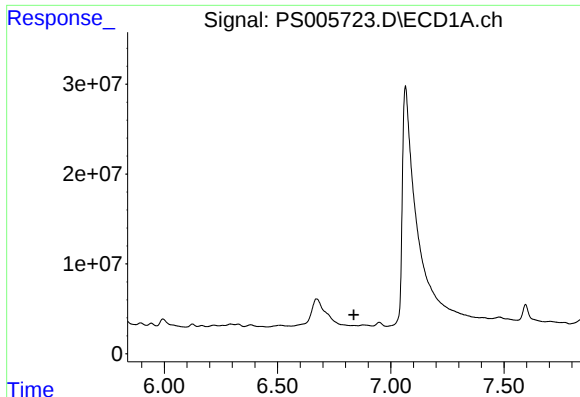

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-072519-A

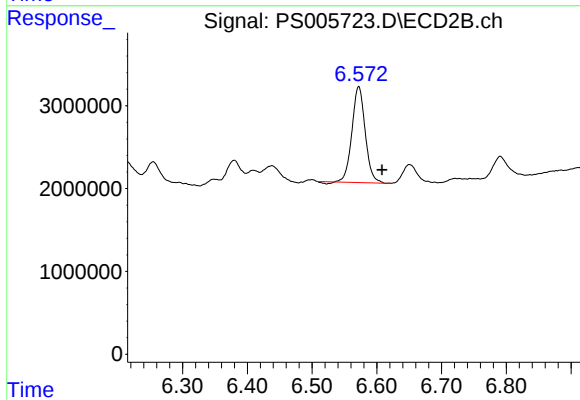


#10 Pentachlorophenol

R.T.: 6.572 min
Delta R.T.: -0.036 min
Response: 16516188
Conc: 1.27 ng/ml

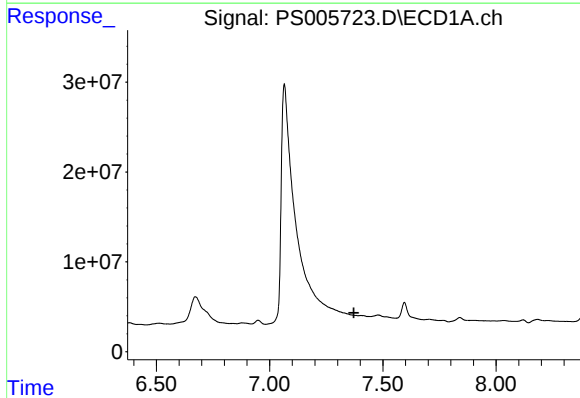


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

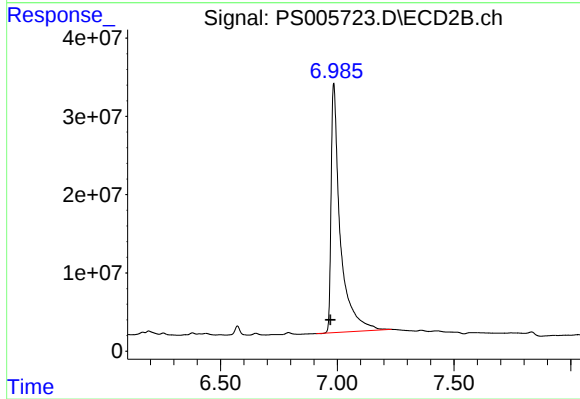

#11 2,4,5-TP (SILVEX)


R.T.: 6.985 min
Delta R.T.: 0.014 min
Response: 873561947
Conc: 168.40 ng/ml

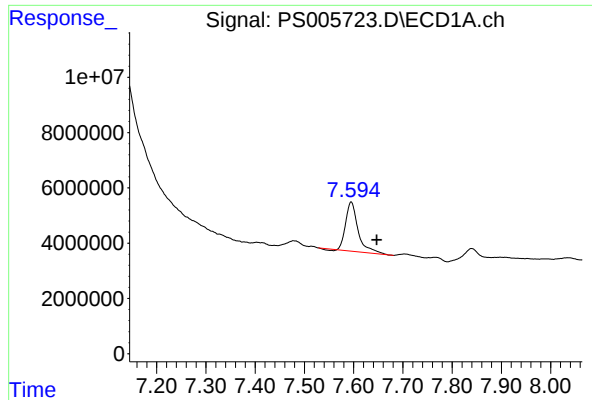

#12 2,4,5-T

R.T.: 7.595 min
Delta R.T.: -0.052 min
Response: 31264607
Conc: 3.75 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-072519-A

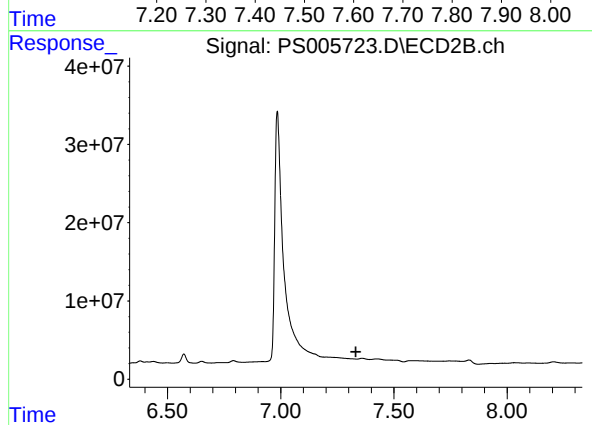

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.332 min
Response: 0
Conc: N.D.