

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072719\
 Data File : PS005724.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2019 14:10
 Operator : SM\AJ
 Sample : K3620-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-02-072519-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 00:54:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.581	5.301	293.1E6	200.8E6	202.039	201.825
Target Compounds							
2) T	3,5-DICHL...	0.000	4.619	0	55852348	N.D.	43.052
7) T	MCPA	0.000	5.630	0	81537728	N.D.	19.372
10) T	Pentachlo...	0.000	6.560	0	18188055	N.D.	1.401
11) T	2,4,5-TP ...	0.000	7.004	0	28002432	N.D.	5.398
12) T	2,4,5-T	7.584	0.000	33208040	0	3.979	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072719\
Data File : PS005724.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2019 14:10
Operator : SM\AJ
Sample : K3620-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-02-072519-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 00:54:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

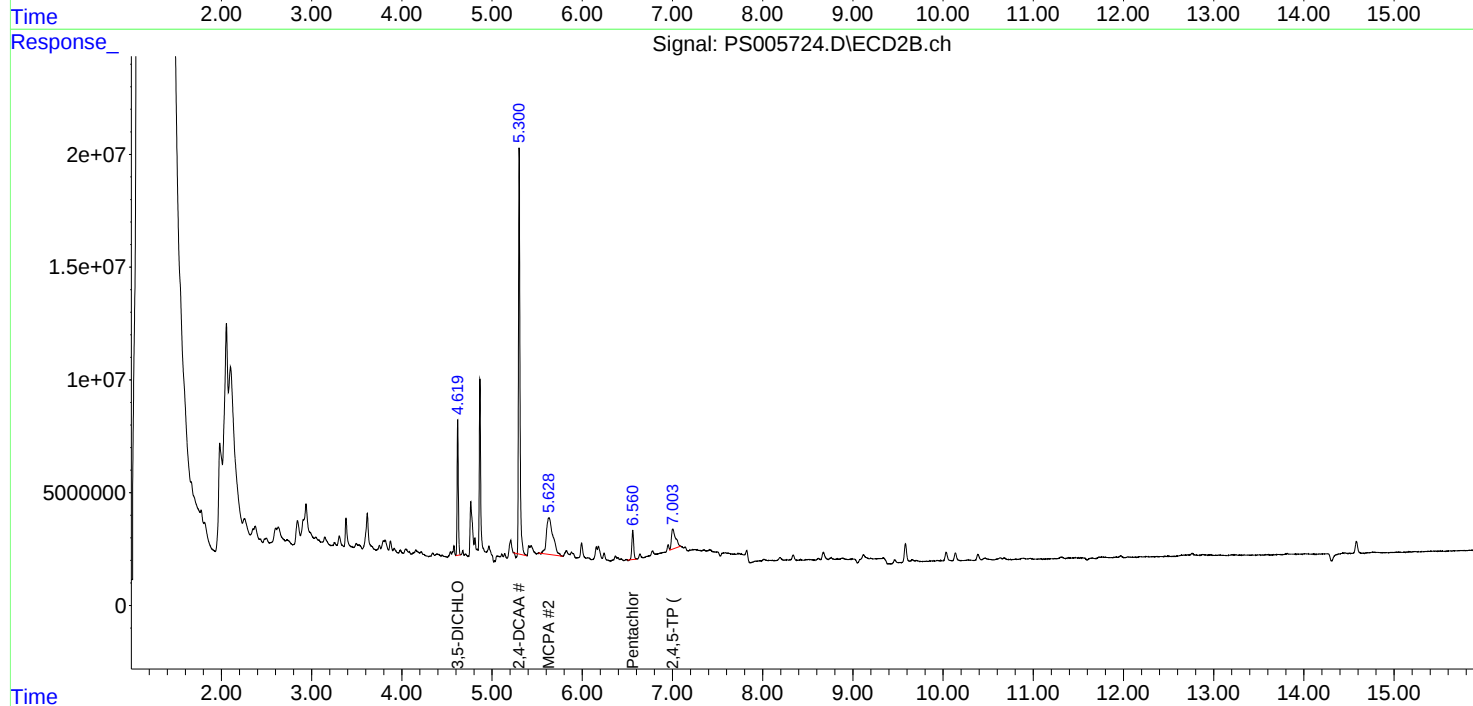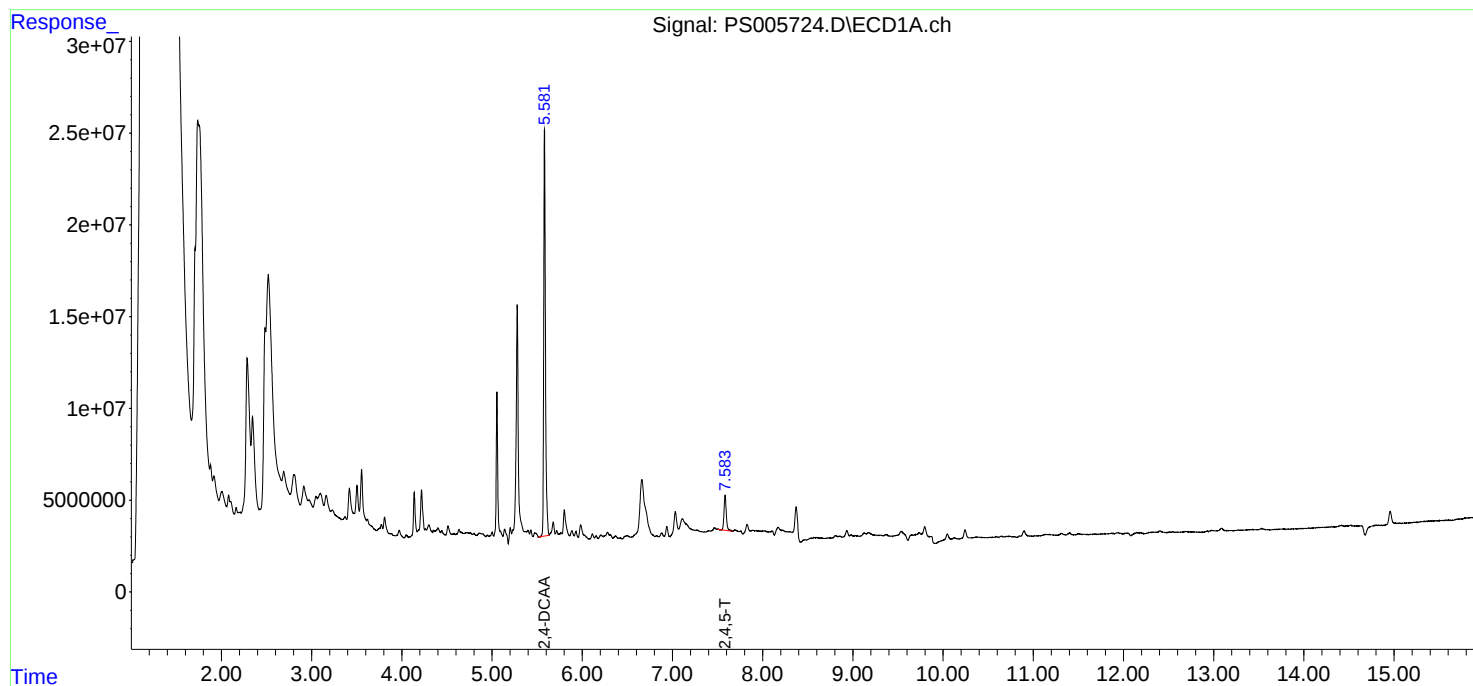


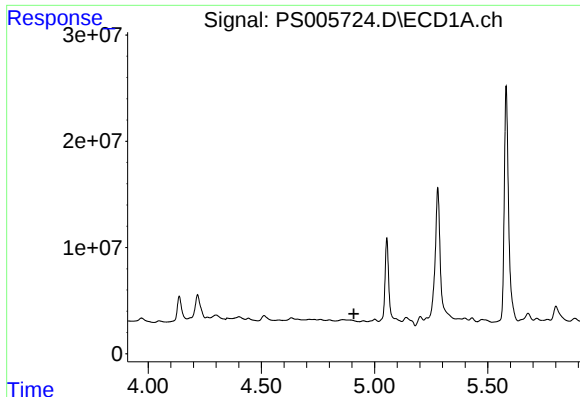

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-072519-B

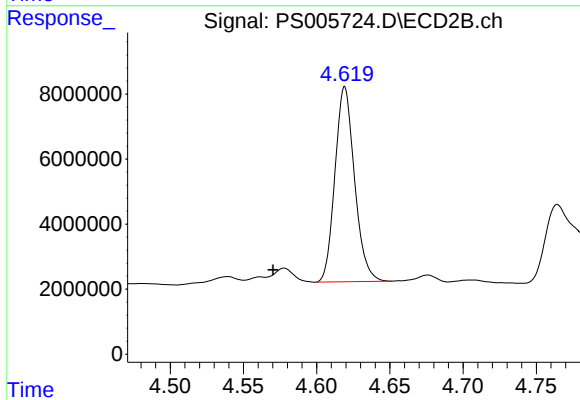


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.619 min
Delta R.T.: 0.049 min
Response: 55852348
Conc: 43.05 ng/ml

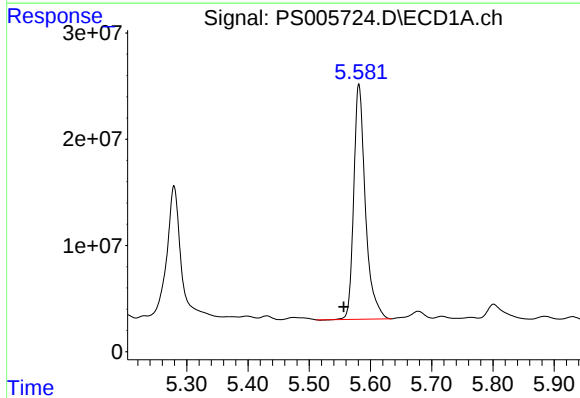


#4 2,4-DCAA

R.T.: 5.581 min
Delta R.T.: 0.025 min
Response: 293122454
Conc: 202.04 ng/ml

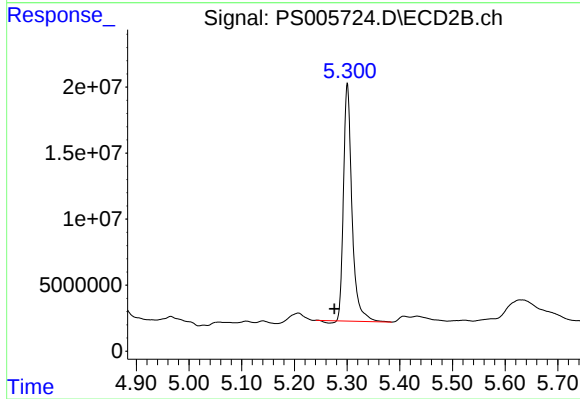

#4 2,4-DCAA


R.T.: 5.301 min
Delta R.T.: 0.025 min
Response: 200750690
Conc: 201.82 ng/ml

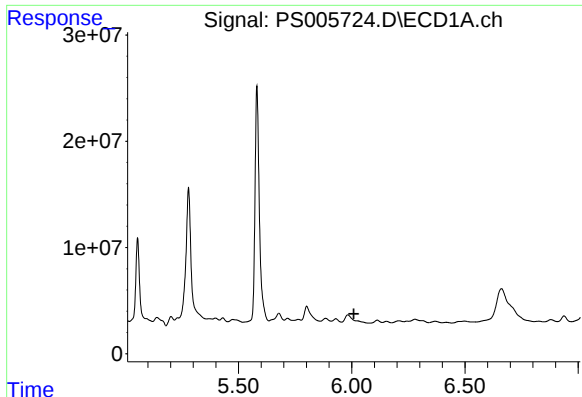

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-072519-B

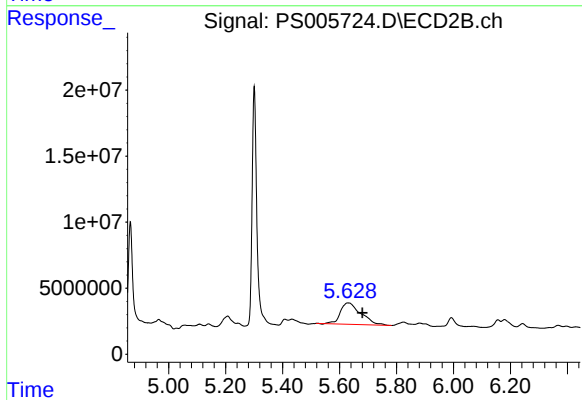


#7 MCPA

R.T.: 5.630 min
Delta R.T.: -0.051 min
Response: 81537728
Conc: 19.37 ug/ml

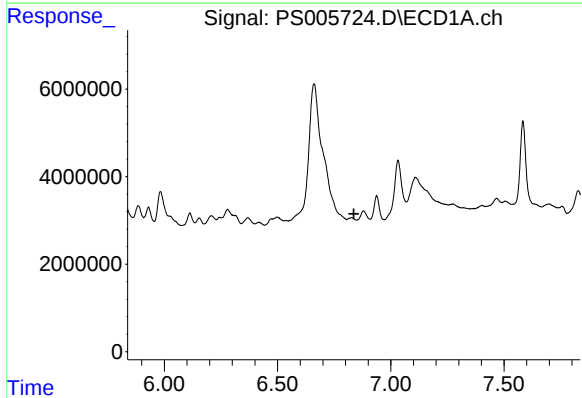


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

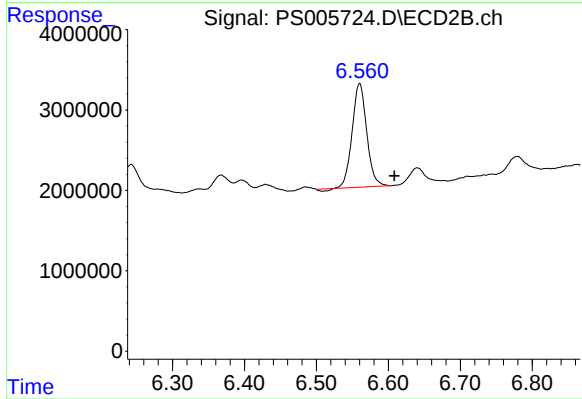

#10 Pentachlorophenol


R.T.: 6.560 min
Delta R.T.: -0.048 min
Response: 18188055
Conc: 1.40 ng/ml

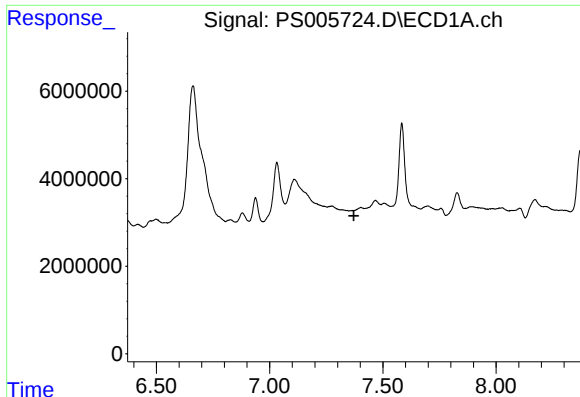

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-072519-B

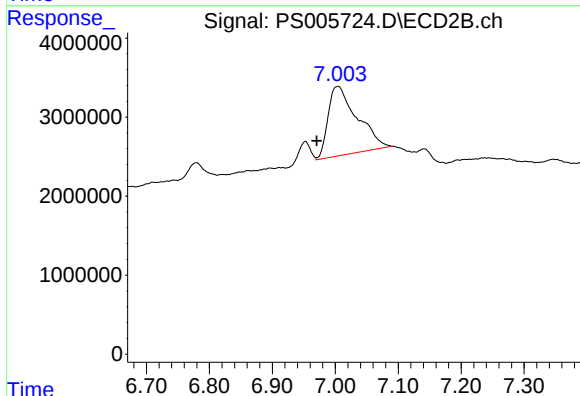


#11 2,4,5-TP (SILVEX)

R.T.: 7.004 min
Delta R.T.: 0.033 min
Response: 28002432
Conc: 5.40 ng/ml

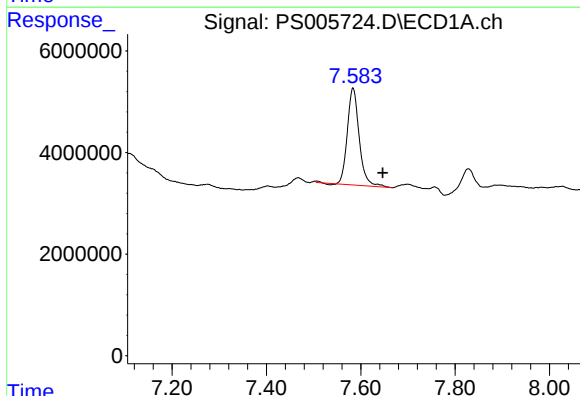

#12 2,4,5-T

R.T.: 7.584 min
Delta R.T.: -0.063 min
Response: 33208040
Conc: 3.98 ng/ml

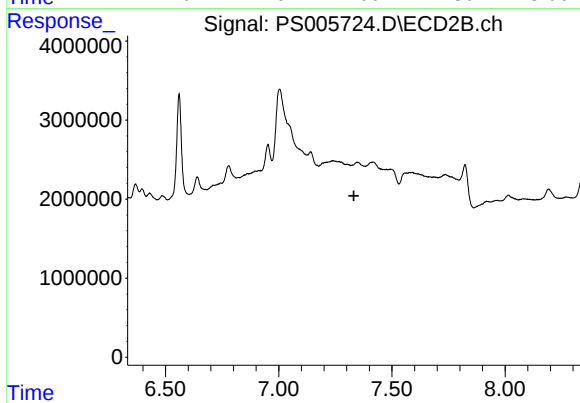

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.332 min
Response: 0
Conc: N.D.