

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072719\
 Data File : PS005729.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2019 16:00
 Operator : SM\AJ
 Sample : K3620-20
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-02-072519-E

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 00:56:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.561	5.280	270.2E6	194.3E6	186.210	195.299
Target Compounds							
2) T	3,5-DICHL...	0.000	4.599	0 65910637		N.D.	50.805
5) T	DICAMBA	5.780	0.000	29709885	0	4.974	N.D. #
10) T	Pentachlo...	0.000	6.540	0 18403750		N.D.	1.418
15) T	Picloram	9.142	9.093	60035871	44214329	5.129	5.886
16) T	DCPA	0.000	9.093	0 44214329		N.D.	6.705



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072719\
Data File : PS005729.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2019 16:00
Operator : SM\AJ
Sample : K3620-20
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-02-072519-E

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 00:56:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

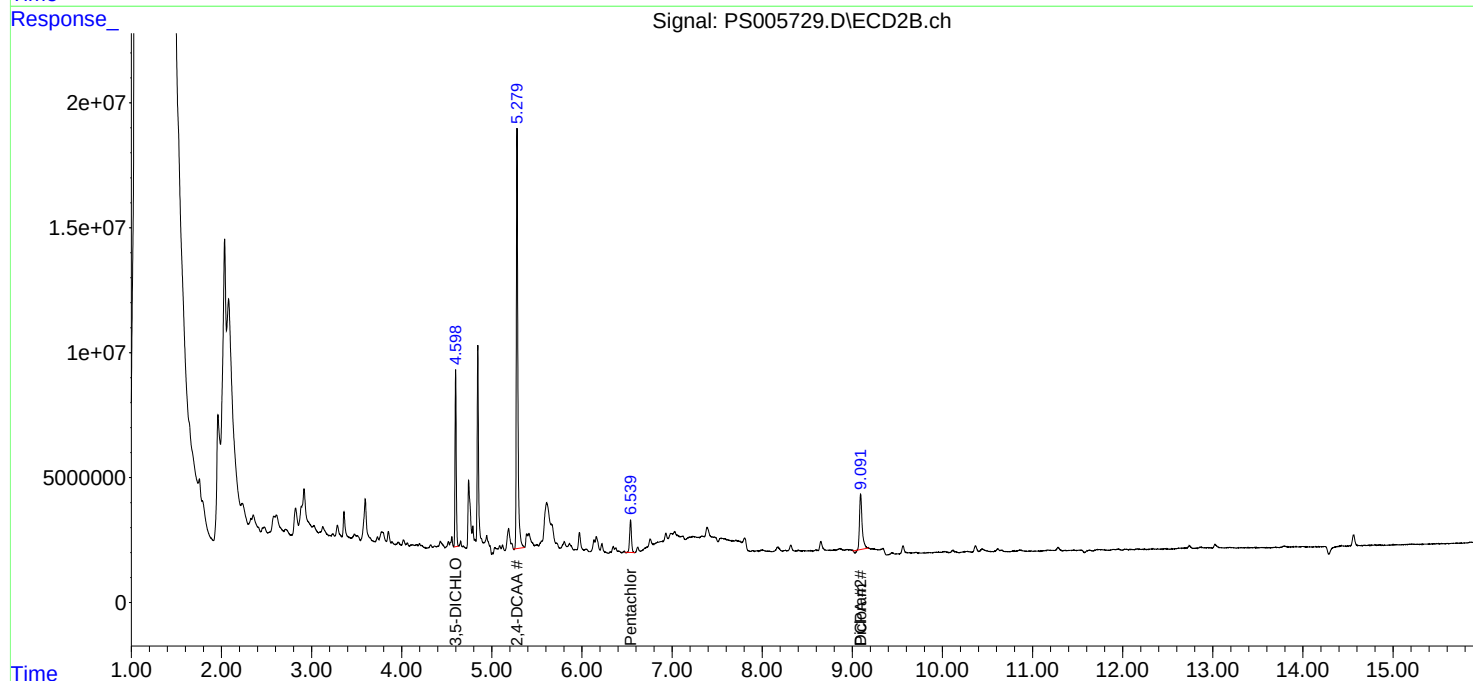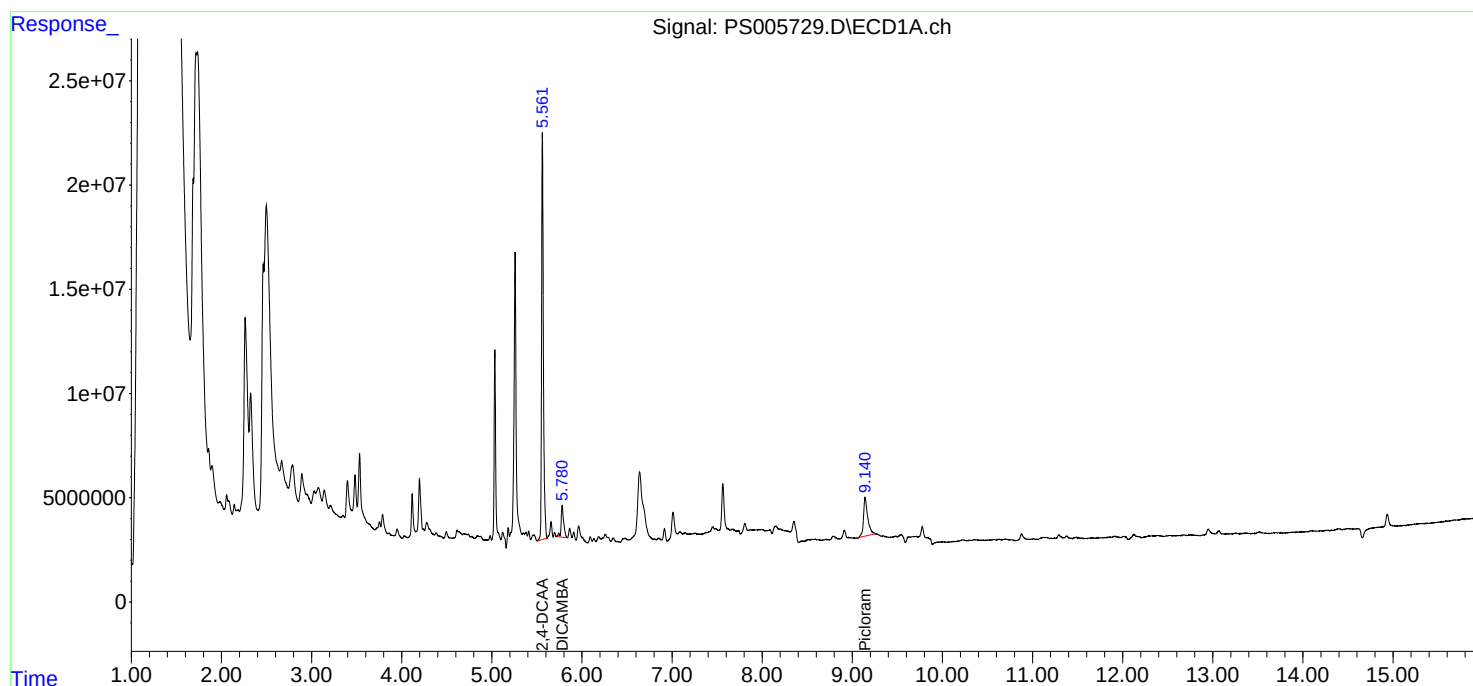


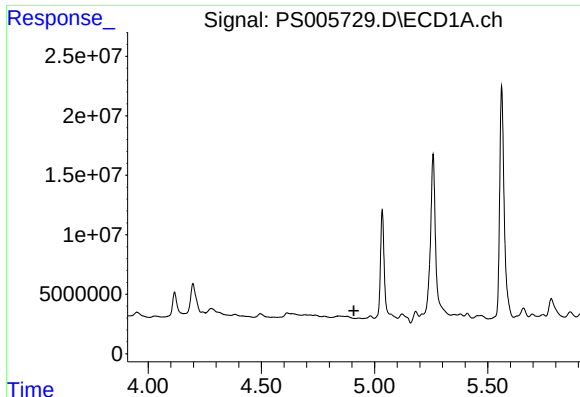

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-072519-E

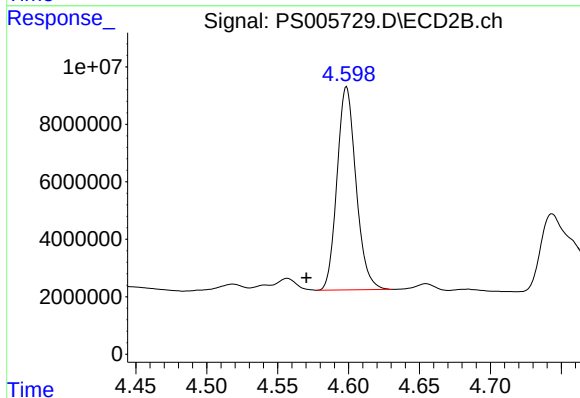


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.599 min
Delta R.T.: 0.028 min
Response: 65910637
Conc: 50.81 ng/ml

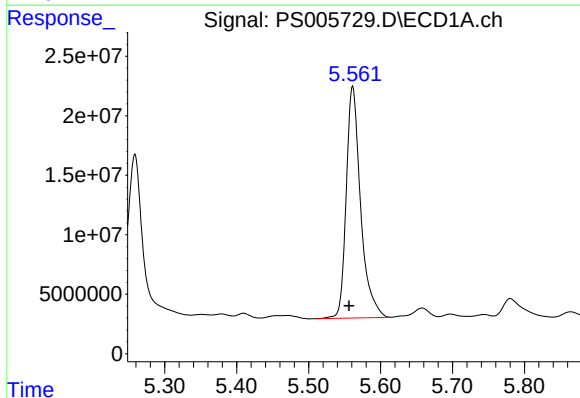


#4 2,4-DCAA

R.T.: 5.561 min
Delta R.T.: 0.005 min
Response: 270157201
Conc: 186.21 ng/ml

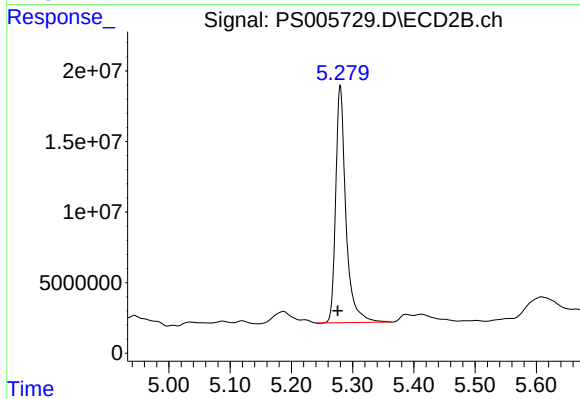

#4 2,4-DCAA


R.T.: 5.280 min
Delta R.T.: 0.004 min
Response: 194259865
Conc: 195.30 ng/ml

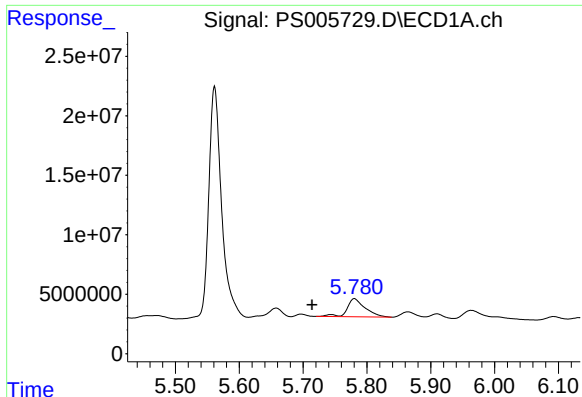

#5 DICAMBA


R.T.: 5.780 min
Delta R.T.: 0.066 min
Response: 29709885
Conc: 4.97 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-072519-E

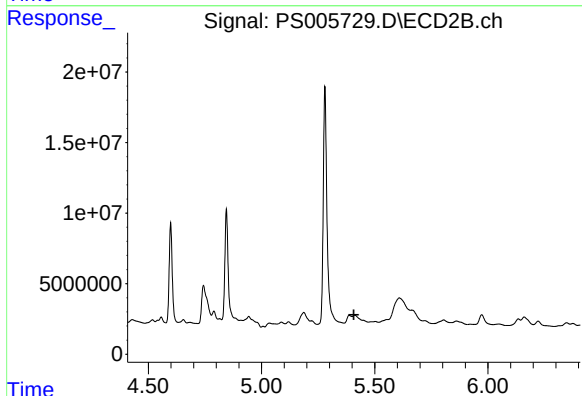


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.408 min
Response: 0
Conc: N.D.

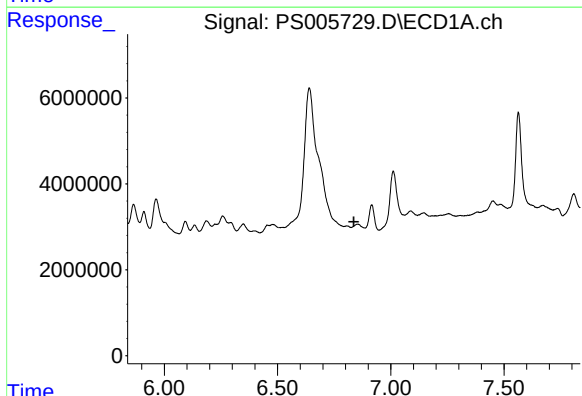


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.837 min
Response: 0
Conc: N.D.

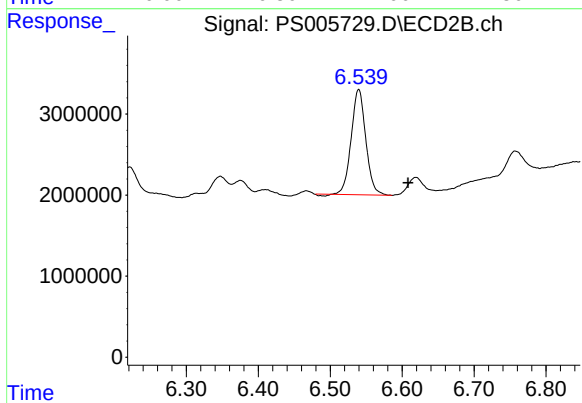

#10 Pentachlorophenol


R.T.: 6.540 min
Delta R.T.: -0.069 min
Response: 18403750
Conc: 1.42 ng/ml

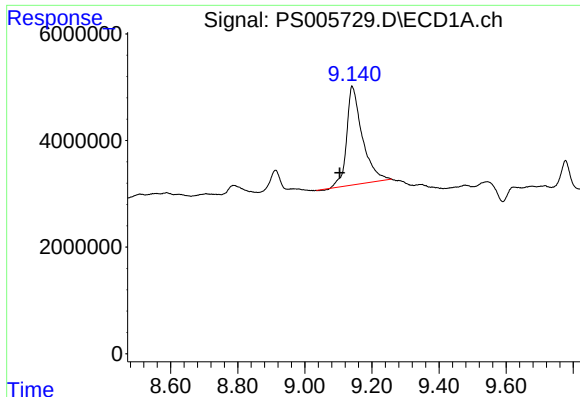

#15 Picloram


R.T.: 9.142 min
Delta R.T.: 0.038 min
Response: 60035871
Conc: 5.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-072519-E

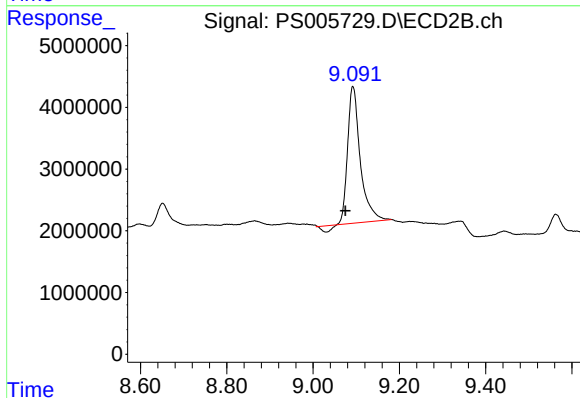


#15 Picloram

R.T.: 9.093 min
Delta R.T.: 0.017 min
Response: 44214329
Conc: 5.89 ng/ml

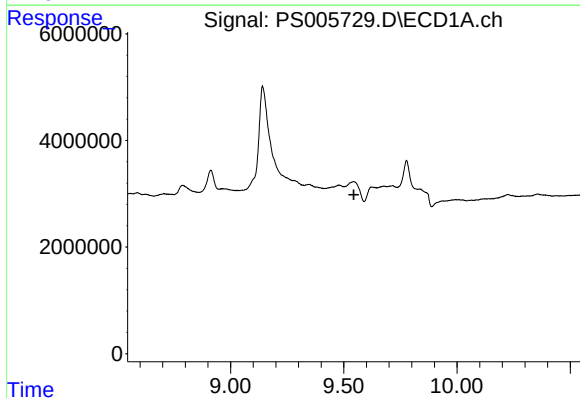

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.545 min
Response: 0
Conc: N.D.

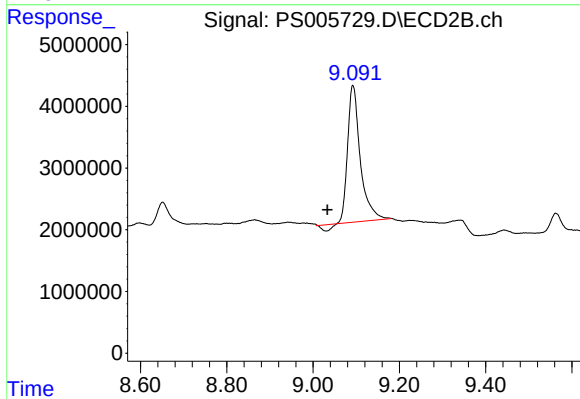

#16 DCPA

R.T.: 9.093 min
Delta R.T.: 0.060 min
Response: 44214329
Conc: 6.71 ng/ml