

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072719\
 Data File : PS005734.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2019 17:51
 Operator : SM\AJ
 Sample : K3961-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-10-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 00:58:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.583	5.302	292.8E6	199.7E6	201.818	200.732
Target Compounds							
2) T	3,5-DICHL...	0.000	4.621	0	50648978	N.D.	39.041
6) T	MCP	5.805	0.000	23943684	0	5.168	N.D. #
7) T	MCPA	0.000	5.631	0	88332376	N.D.	20.986
10) T	Pentachlo...	0.000	6.562	0	24901114	N.D.	1.918
12) T	2,4,5-T	7.585	0.000	38099365	0	4.565	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072719\
Data File : PS005734.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2019 17:51
Operator : SM\AJ
Sample : K3961-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-10-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 00:58:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

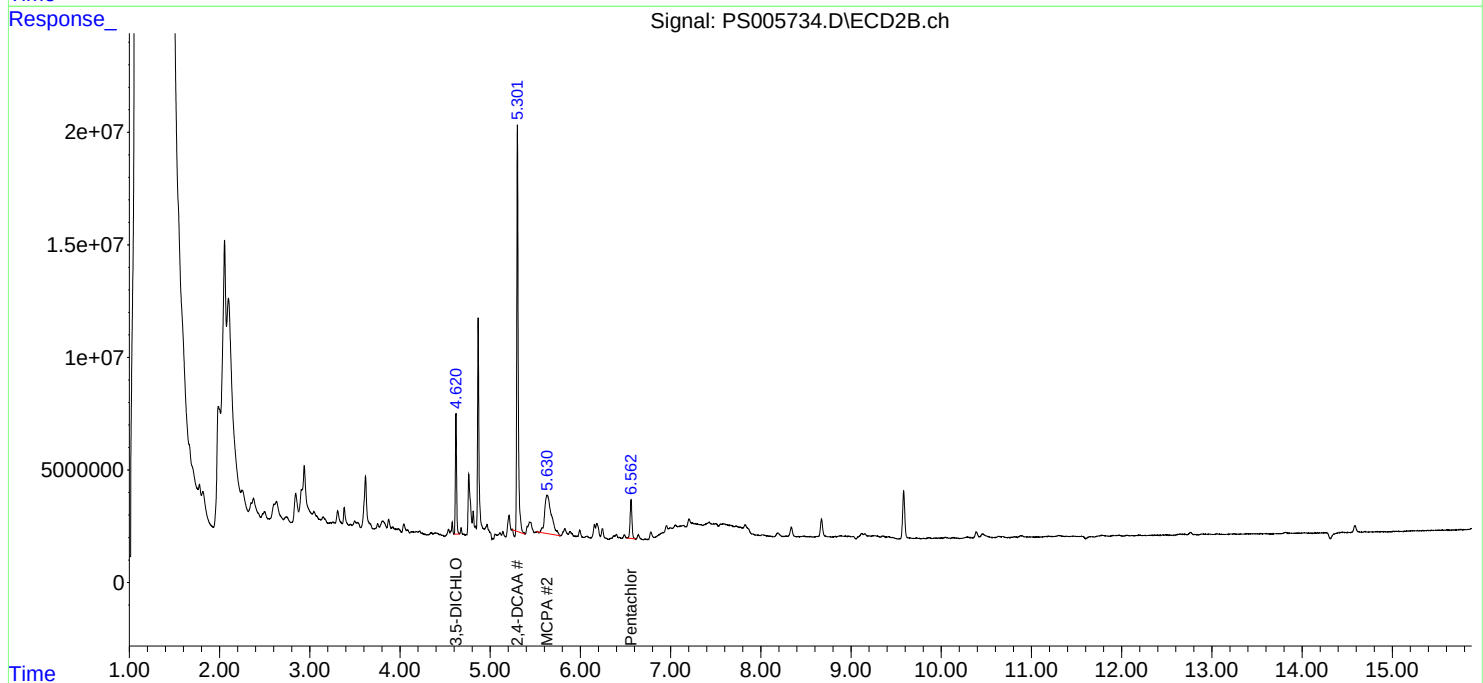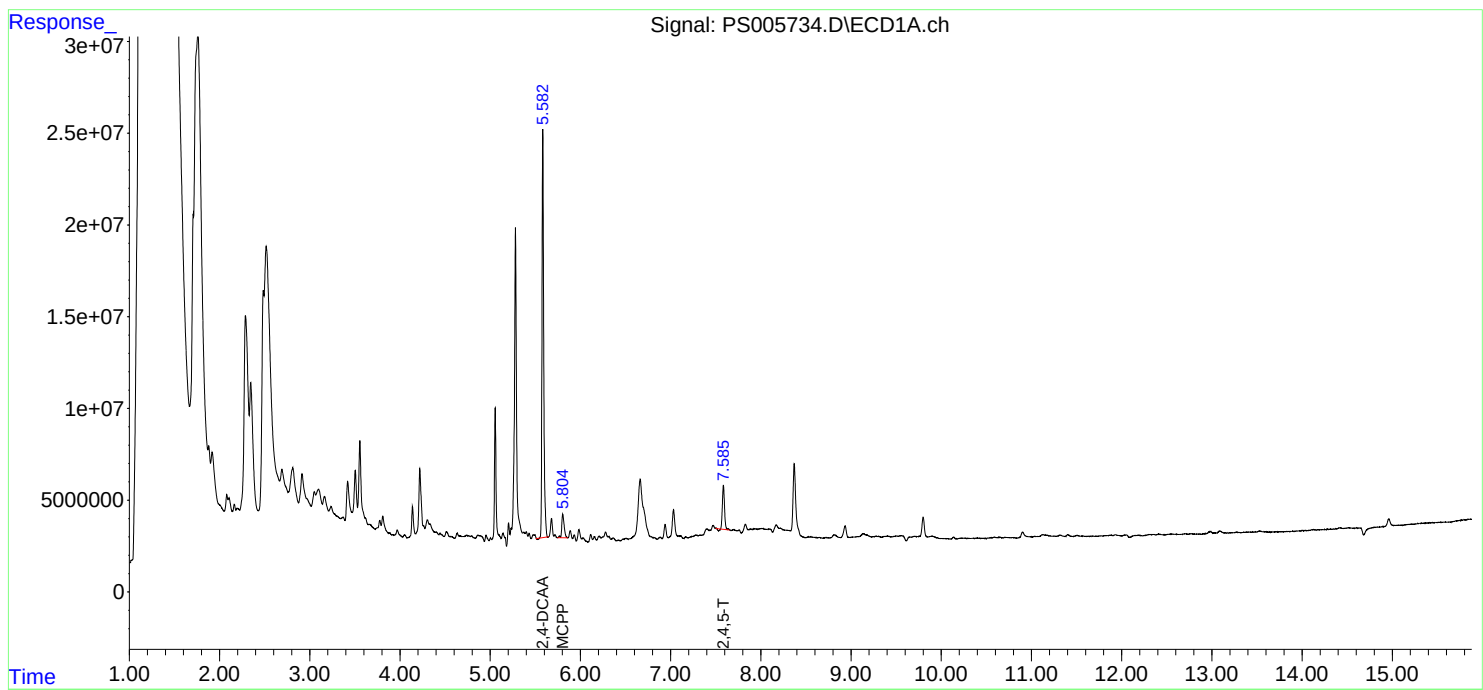


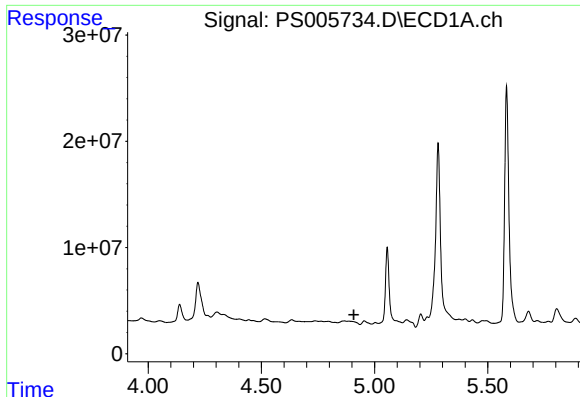

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-10-A

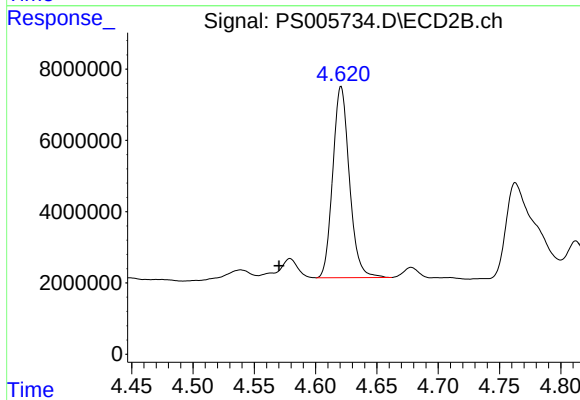


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.621 min
Delta R.T.: 0.051 min
Response: 50648978
Conc: 39.04 ng/ml

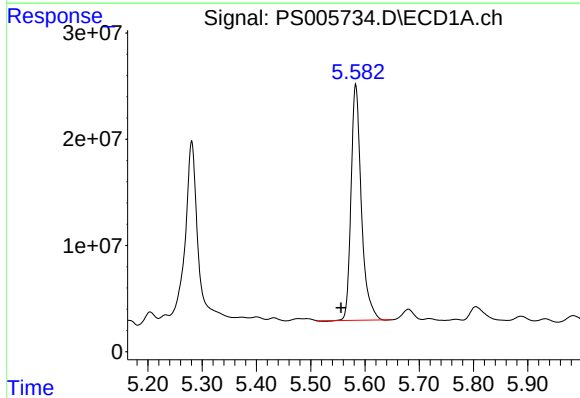


#4 2,4-DCAA

R.T.: 5.583 min
Delta R.T.: 0.027 min
Response: 292801534
Conc: 201.82 ng/ml

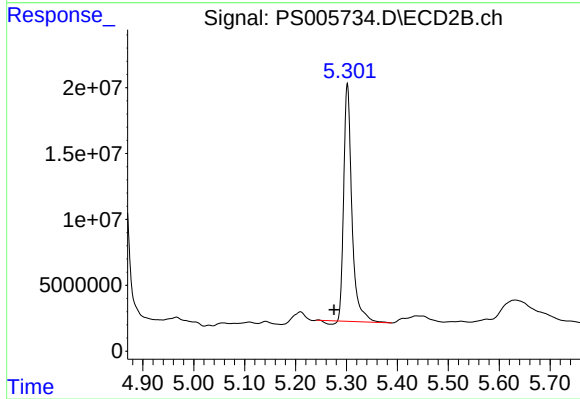

#4 2,4-DCAA


R.T.: 5.302 min
Delta R.T.: 0.026 min
Response: 199664158
Conc: 200.73 ng/ml

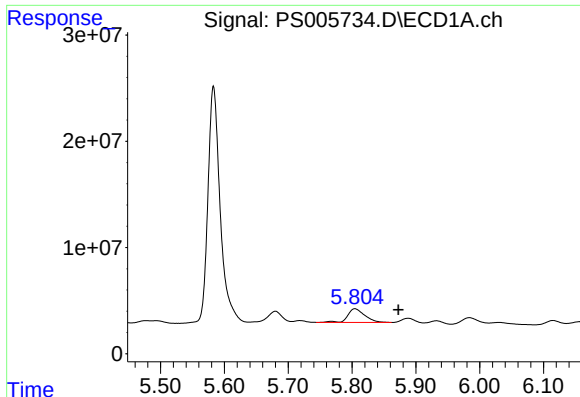

#6 MCPP


R.T.: 5.805 min
Delta R.T.: -0.068 min
Response: 23943684
Conc: 5.17 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-10-A

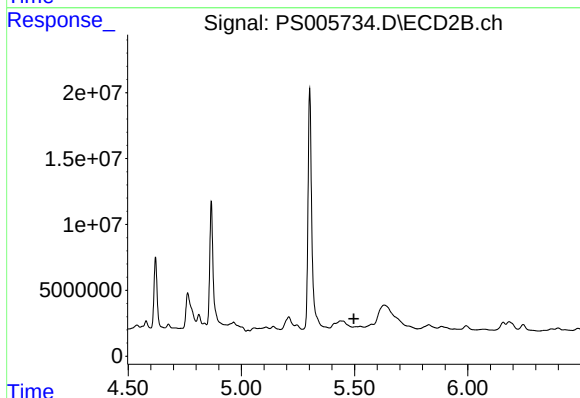


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.497 min
Response: 0
Conc: N.D.

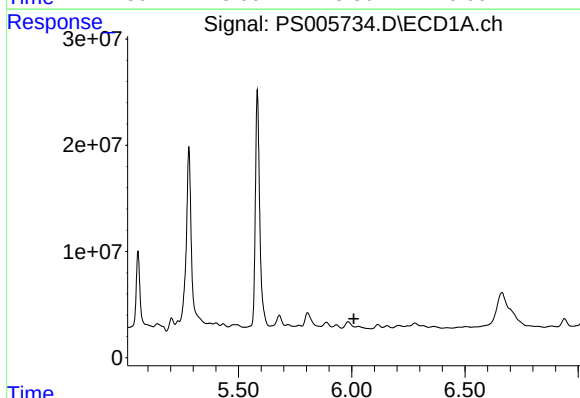


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.009 min
Response: 0
Conc: N.D.

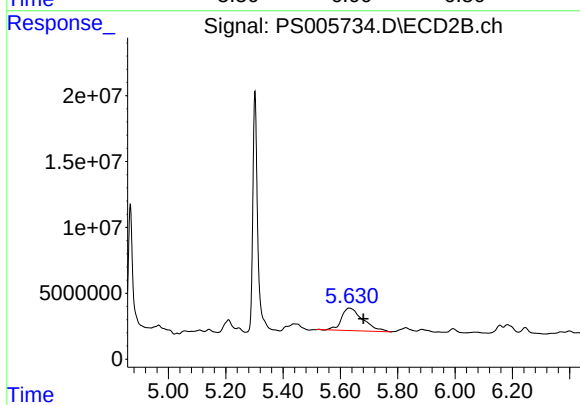

#7 MCPA


R.T.: 5.631 min
Delta R.T.: -0.050 min
Response: 88332376
Conc: 20.99 ug/ml

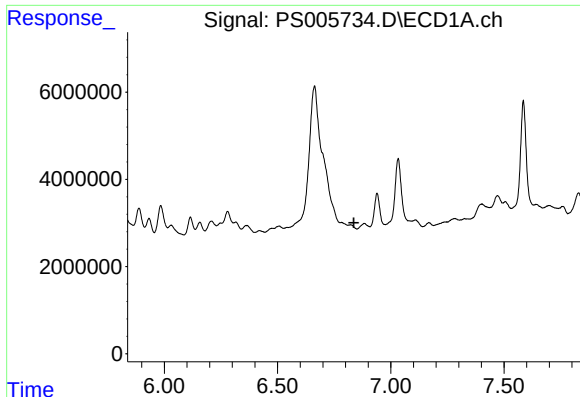

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-10-A

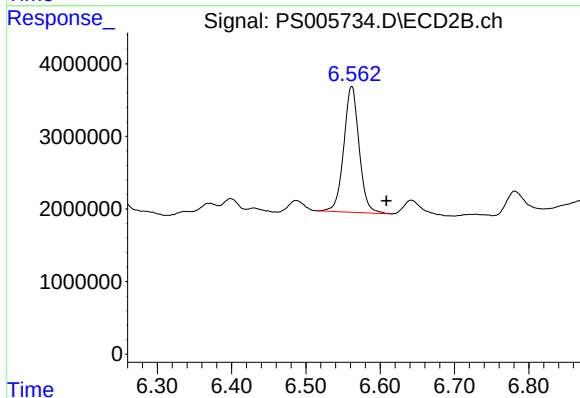


#10 Pentachlorophenol

R.T.: 6.562 min
Delta R.T.: -0.047 min
Response: 24901114
Conc: 1.92 ng/ml

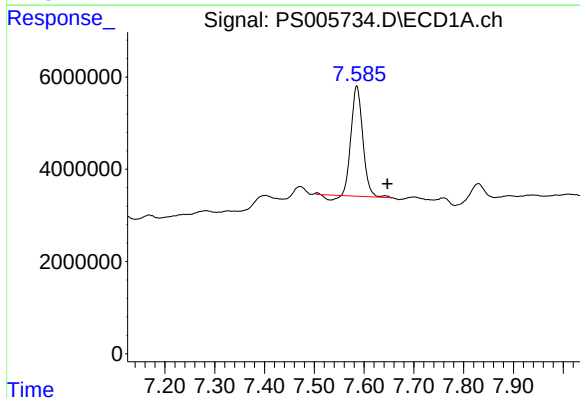

#12 2,4,5-T

R.T.: 7.585 min
Delta R.T.: -0.061 min
Response: 38099365
Conc: 4.56 ng/ml

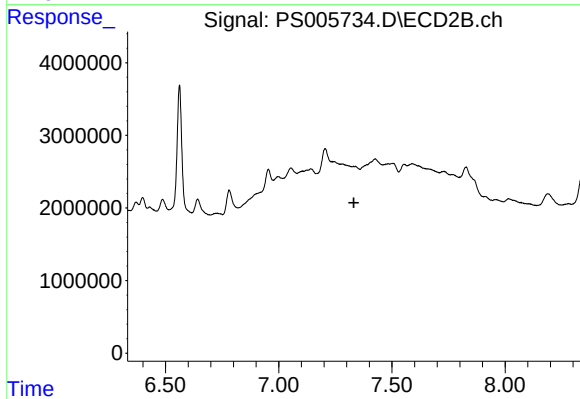

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.332 min
Response: 0
Conc: N.D.