

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072719\
 Data File : PS005737.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2019 18:57
 Operator : SM\AJ
 Sample : PB121733BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB121733BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 01:00:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.560	5.280	751.4E6	517.6E6	517.905	520.348
Target Compounds							
2) T	3,5-DICHL...	0.000	4.600	0	27103117	N.D.	20.892
6) T	MCP	5.868	0.000	15972681	0	3.447	N.D. #
7) T	MCPA	6.048	5.667	25189543	29852838	3.860	7.093 #
8) T	DICHLORPROP	0.000	5.980	0	20939374	N.D.	22.673
9) T	2,4-D	0.000	6.222	0	15764751	N.D.	14.674
10) T	Pentachlo...	0.000	6.540	0	19691585	N.D.	1.517
11) T	2,4,5-TP ...	0.000	6.939	0	21112343	N.D.	4.070
15) T	Picloram	0.000	9.111	0	51240670	N.D.	6.821



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072719\
Data File : PS005737.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2019 18:57
Operator : SM\AJ
Sample : PB121733BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB121733BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 01:00:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

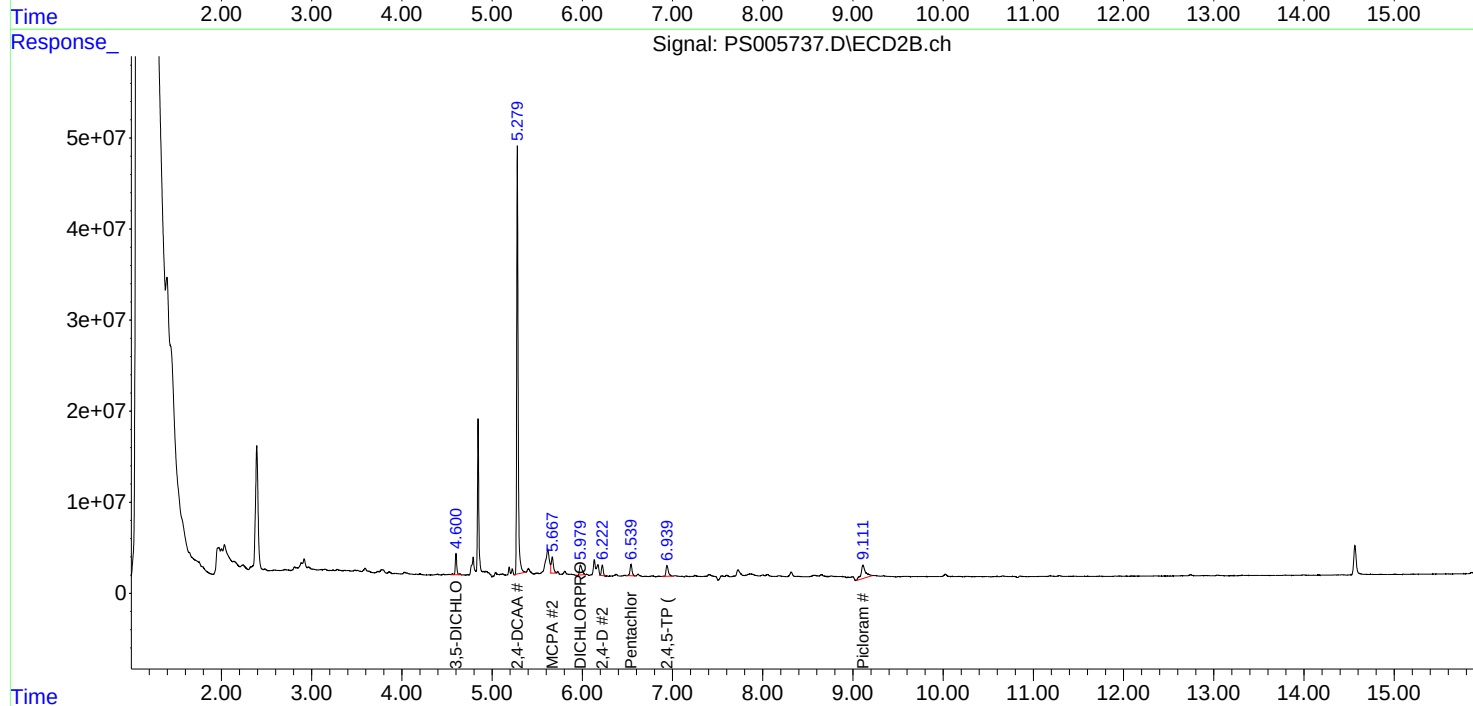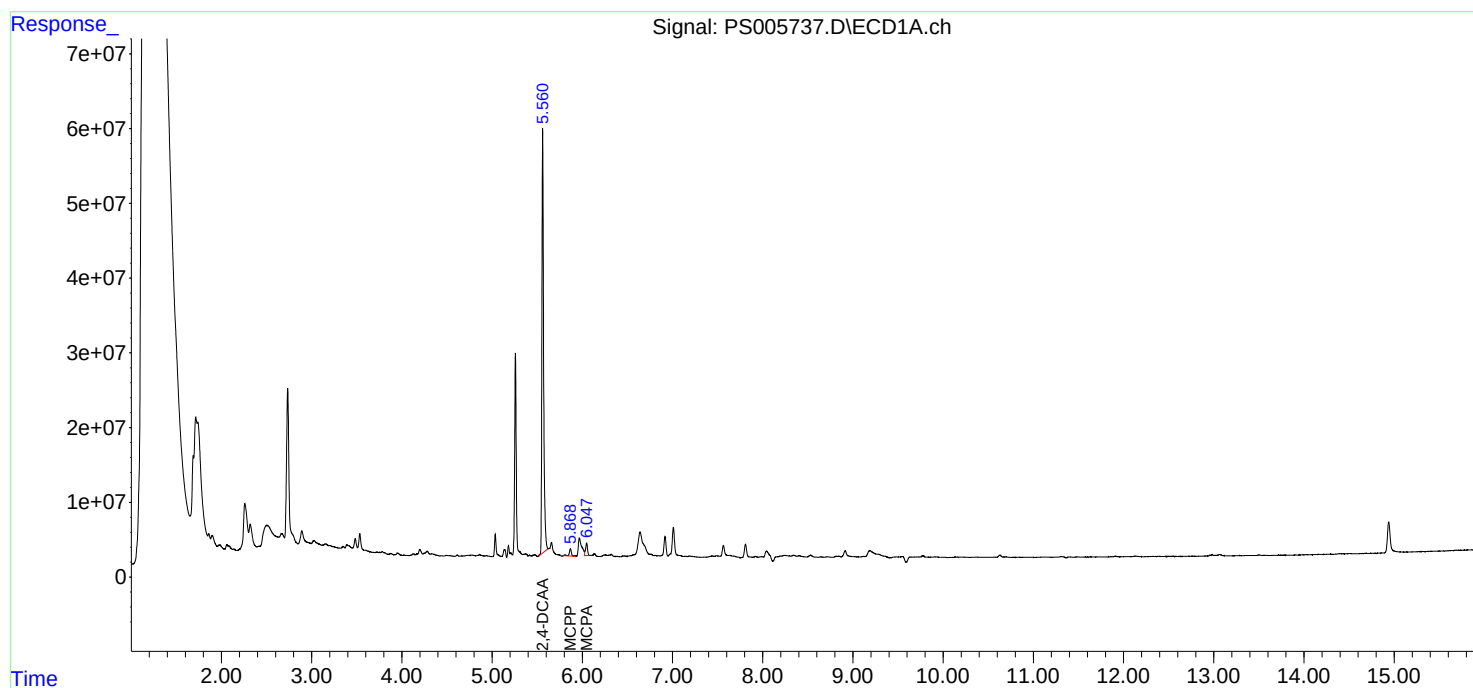


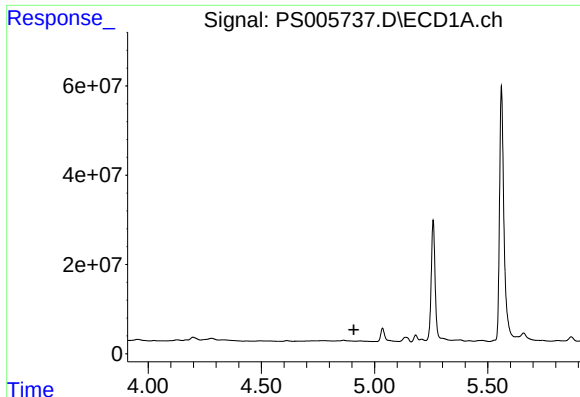

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB121733BL

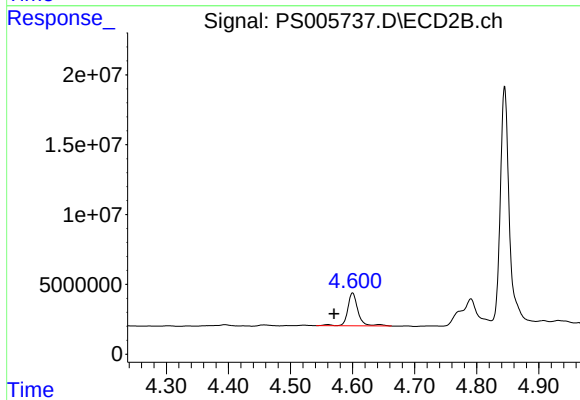


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.600 min
Delta R.T.: 0.030 min
Response: 27103117
Conc: 20.89 ng/ml

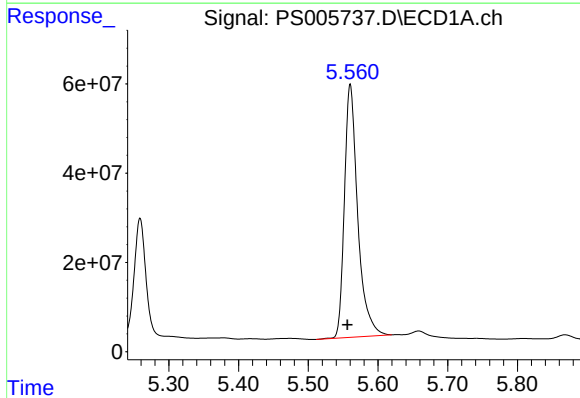


#4 2,4-DCAA

R.T.: 5.560 min
Delta R.T.: 0.004 min
Response: 751385720
Conc: 517.90 ng/ml

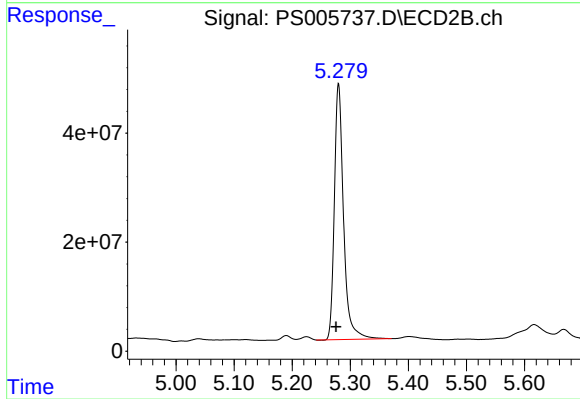

#4 2,4-DCAA


R.T.: 5.280 min
Delta R.T.: 0.004 min
Response: 517578780
Conc: 520.35 ng/ml

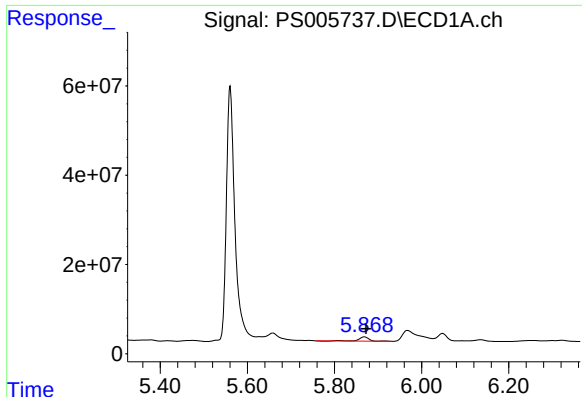

#6 MCPP


R.T.: 5.868 min
Delta R.T.: -0.004 min
Response: 15972681
Conc: 3.45 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB121733BL

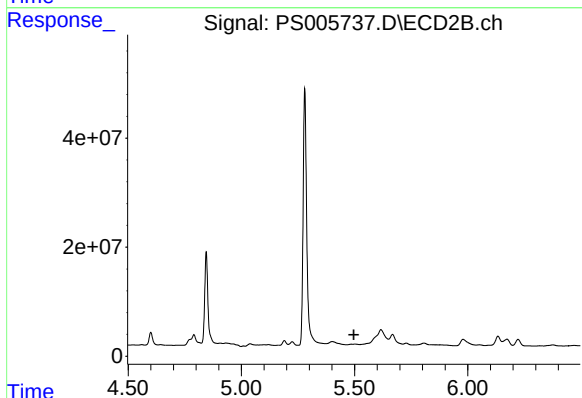


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

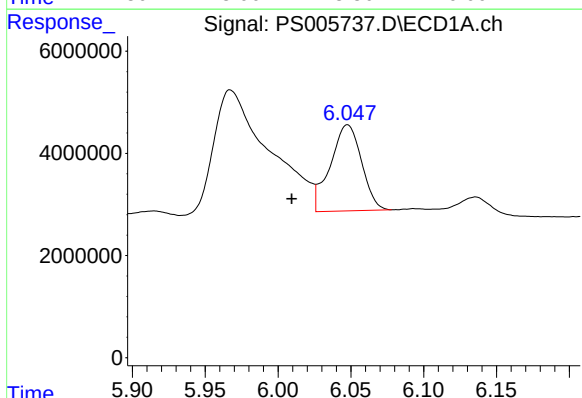


#7 MCPA

R.T.: 6.048 min
Delta R.T.: 0.038 min
Response: 25189543
Conc: 3.86 ug/ml

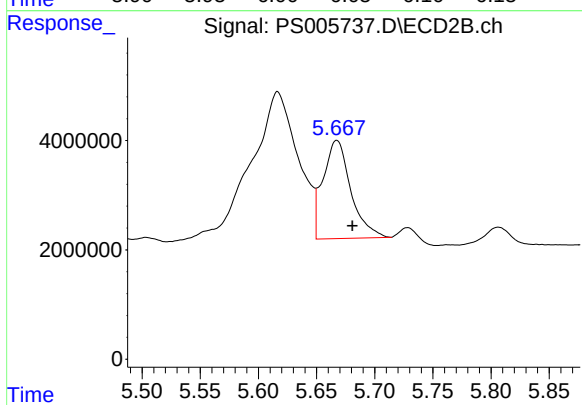

#7 MCPA


R.T.: 5.667 min
Delta R.T.: -0.013 min
Response: 29852838
Conc: 7.09 ug/ml

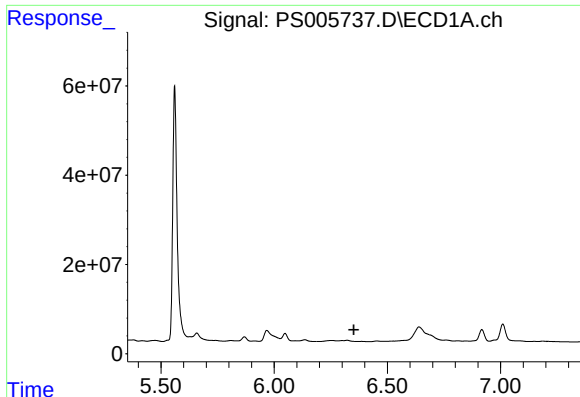

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB121733BL

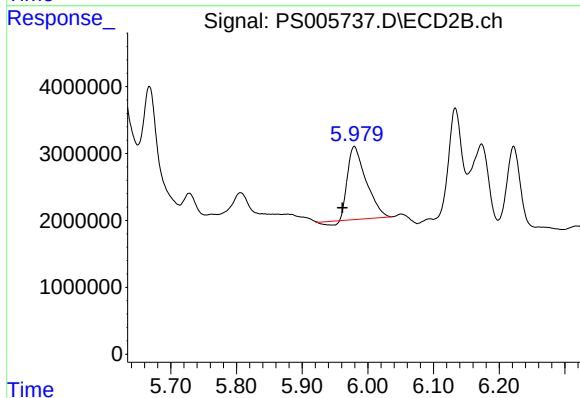


#8 DICHLORPROP

R.T.: 5.980 min
Delta R.T.: 0.018 min
Response: 20939374
Conc: 22.67 ng/ml

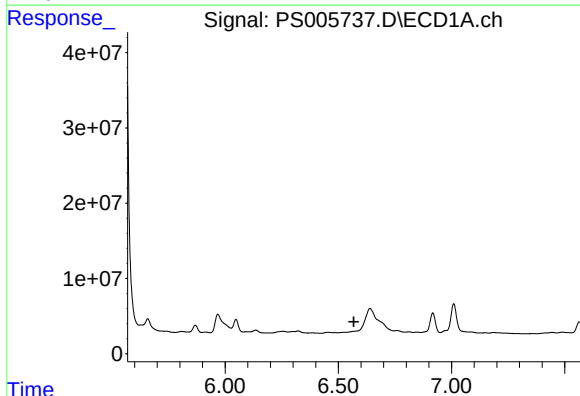


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.569 min
Response: 0
Conc: N.D.

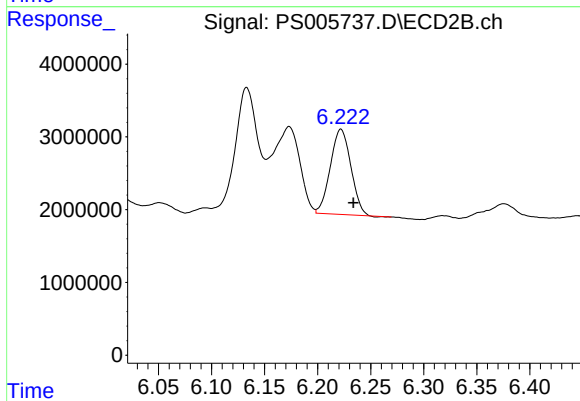

#9 2,4-D


R.T.: 6.222 min
Delta R.T.: -0.012 min
Response: 15764751
Conc: 14.67 ng/ml

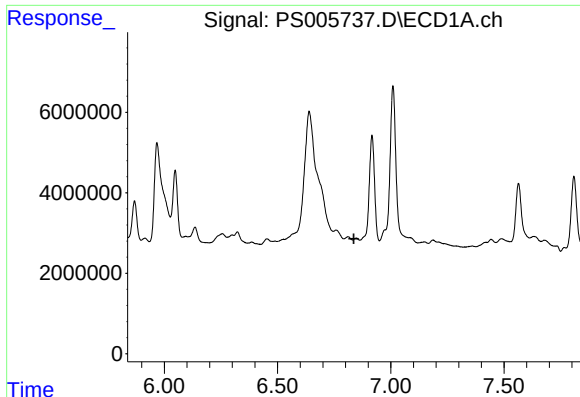

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB121733BL

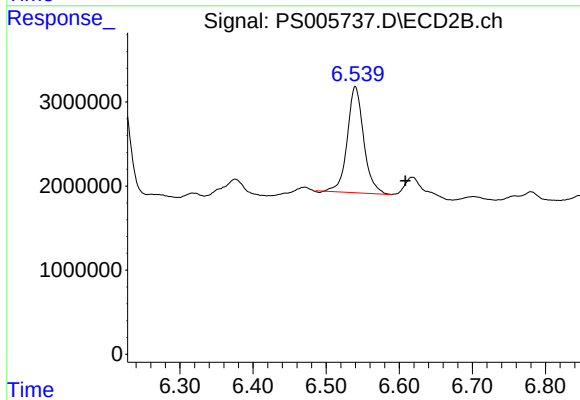


#10 Pentachlorophenol

R.T.: 6.540 min
Delta R.T.: -0.068 min
Response: 19691585
Conc: 1.52 ng/ml

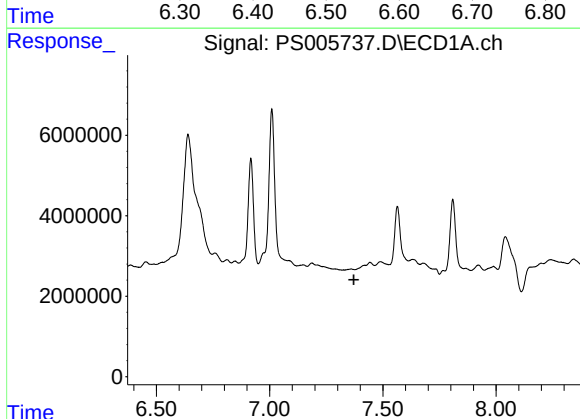


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

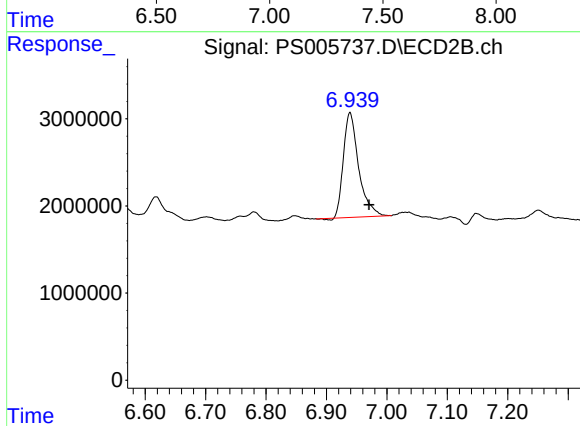

#11 2,4,5-TP (SILVEX)


R.T.: 6.939 min
Delta R.T.: -0.032 min
Response: 21112343
Conc: 4.07 ng/ml

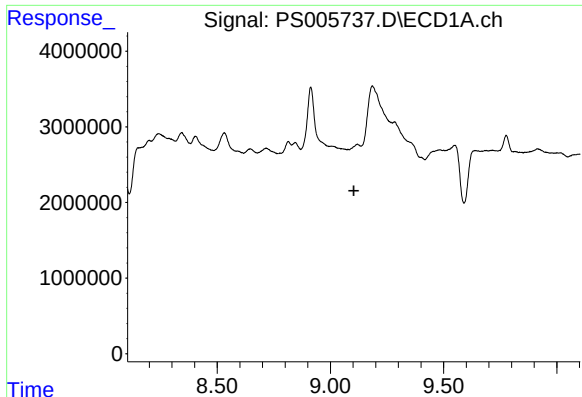

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 9.104 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB121733BL

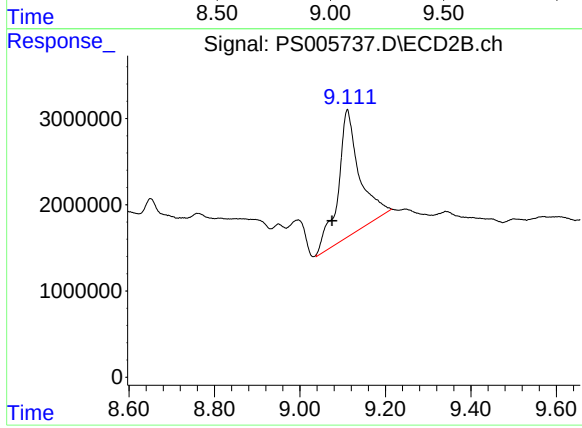

#15 Picloram

R.T.: 9.111 min
Delta R.T.: 0.036 min
Response: 51240670
Conc: 6.82 ng/ml