

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072719\
 Data File : PS005741.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2019 20:25
 Operator : SM\AJ
 Sample : K3990-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-2-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 01:02:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.562	5.282	442.1E6	207.6E6	304.735	208.728 #
Target Compounds							
1) T	Dalapon	0.000	1.732	0	1521.8E6	N.D.	1207.220
2) T	3,5-DICHL...	0.000	4.602	0	40283902	N.D.	31.052
5) T	DICAMBA	0.000	5.402	0	22374226	N.D.	5.994
6) T	MCP	5.872	0.000	16146854	0	3.485	N.D. #
7) T	MCPA	6.032	5.694	79508181	108.2E6	12.184	25.701 #
9) T	2,4-D	6.554	6.224	70426889	24403735	46.993	22.716 #
10) T	Pentachlo...	6.831	6.542	23080570	30918690	1.104	2.381 #
11) T	2,4,5-TP ...	0.000	6.936	0	42441104	N.D.	8.182
12) T	2,4,5-T	0.000	7.390	0	27803655	N.D.	5.849
13) T	2,4-DB	8.187	0.000	65735288	0	62.254	N.D. #
14) T	DINOSEB	0.000	8.168	0	26500218	N.D.	7.121
15) T	Picloram	9.050	9.111	11492533	32357037	<MDL	4.307 #
16) T	DCPA	9.490	8.993	84367833	30566883	8.297	4.636 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072719\
Data File : PS005741.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2019 20:25
Operator : SM\AJ
Sample : K3990-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-2-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 01:02:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

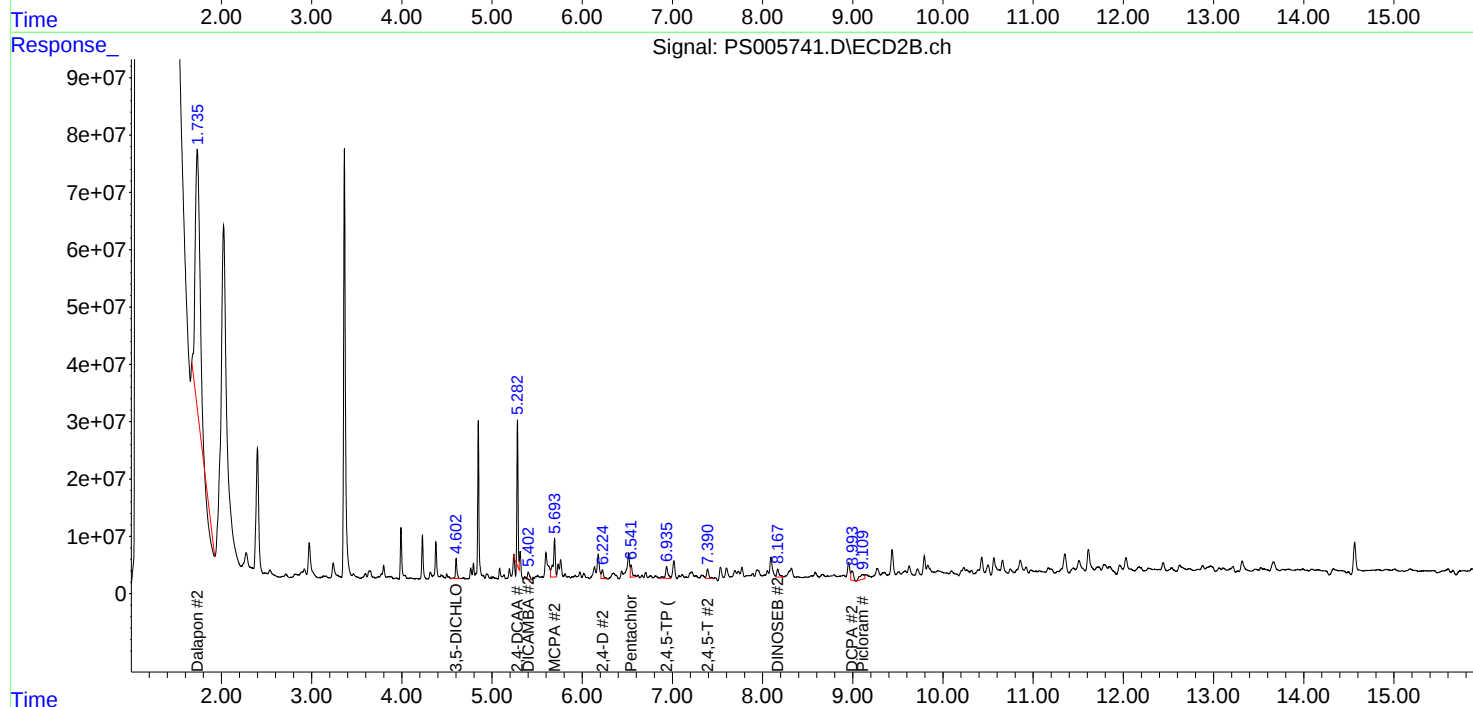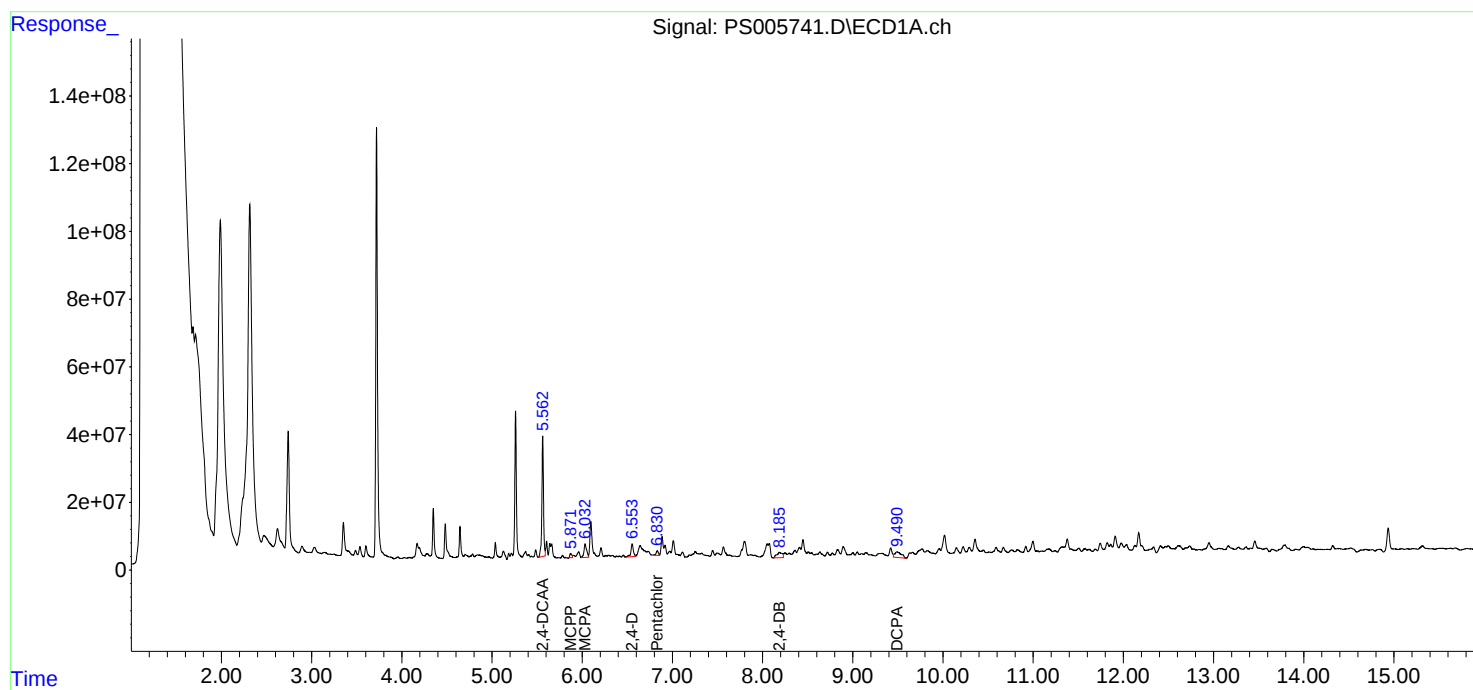


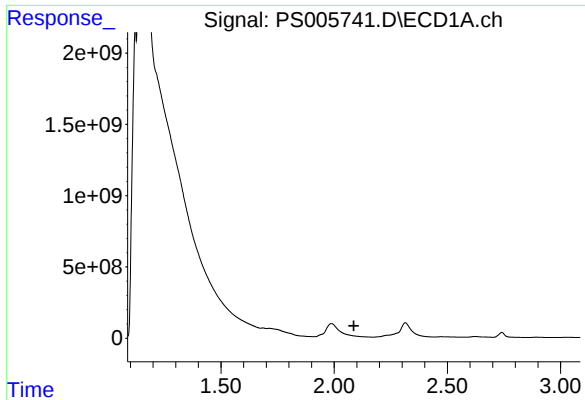

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.087 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-2-A

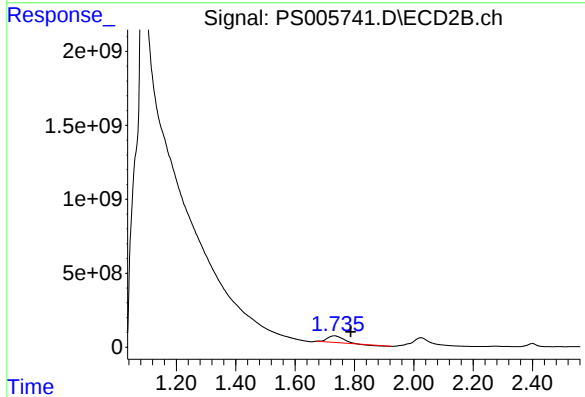


#1 Dalapon

R.T.: 1.732 min
Delta R.T.: -0.056 min
Response: 1521795192
Conc: 1207.22 ng/ml

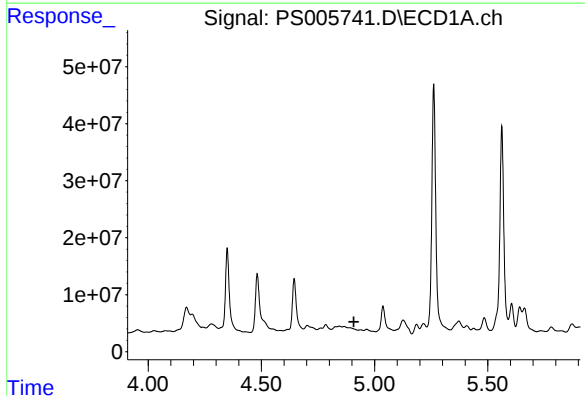


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

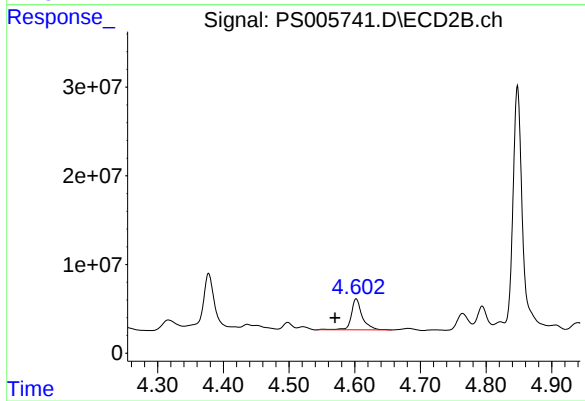

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.602 min
Delta R.T.: 0.032 min
Response: 40283902
Conc: 31.05 ng/ml

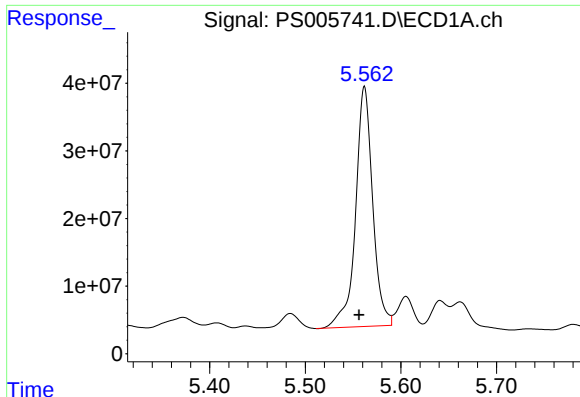

#4 2,4-DCAA


R.T.: 5.562 min
Delta R.T.: 0.006 min
Response: 442114399
Conc: 304.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-2-A

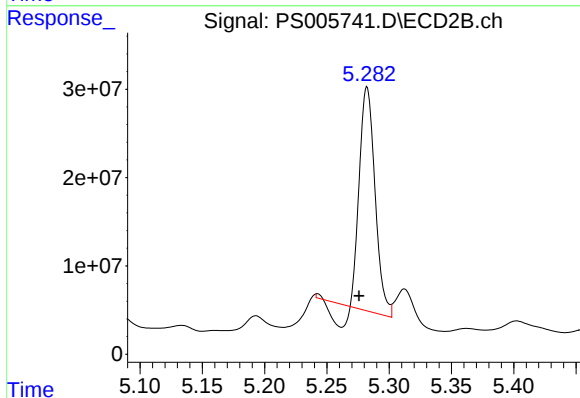


#4 2,4-DCAA

R.T.: 5.282 min
Delta R.T.: 0.007 min
Response: 207616878
Conc: 208.73 ng/ml

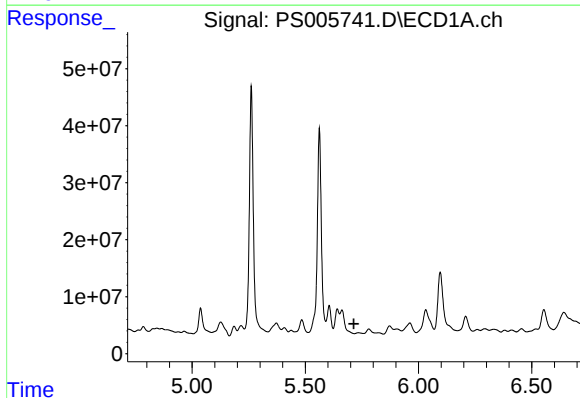


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.714 min
Response: 0
Conc: N.D.

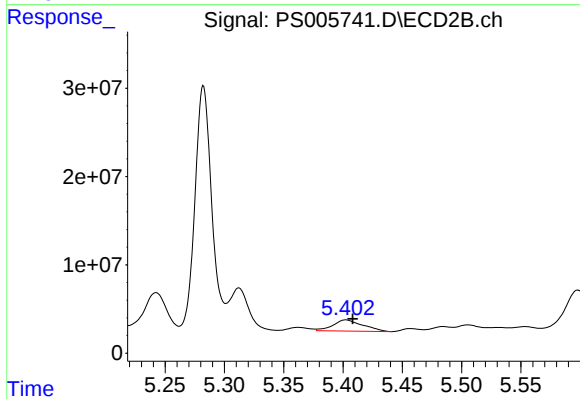

#5 DICAMBA


R.T.: 5.402 min
Delta R.T.: -0.006 min
Response: 22374226
Conc: 5.99 ng/ml

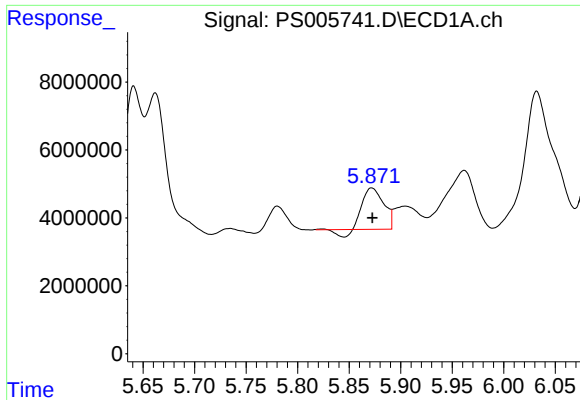

#6 MCPP


R.T.: 5.872 min
Delta R.T.: 0.000 min
Response: 16146854
Conc: 3.48 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-2-A

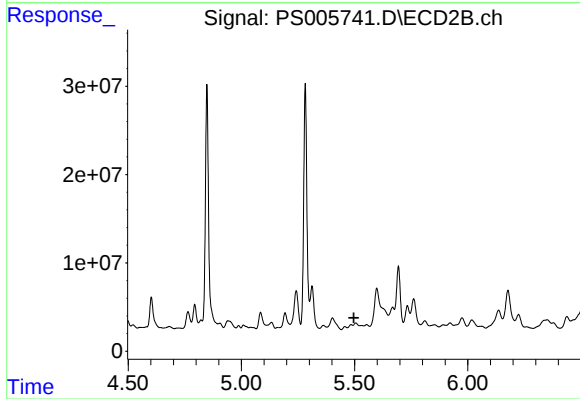


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.497 min
Response: 0
Conc: N.D.

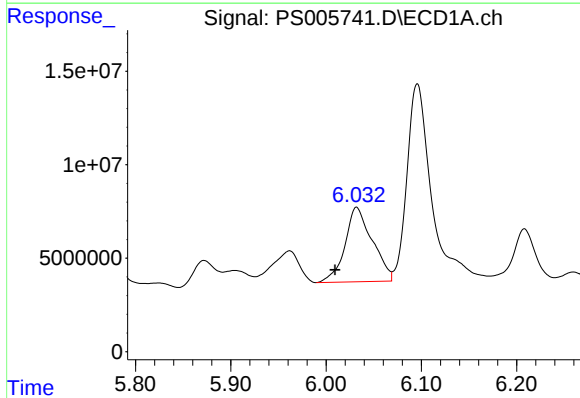


#7 MCPA

R.T.: 6.032 min
Delta R.T.: 0.023 min
Response: 79508181
Conc: 12.18 ug/ml

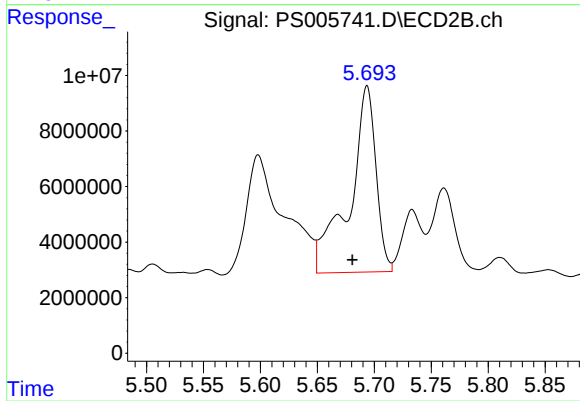

#7 MCPA


R.T.: 5.694 min
Delta R.T.: 0.013 min
Response: 108176081
Conc: 25.70 ug/ml

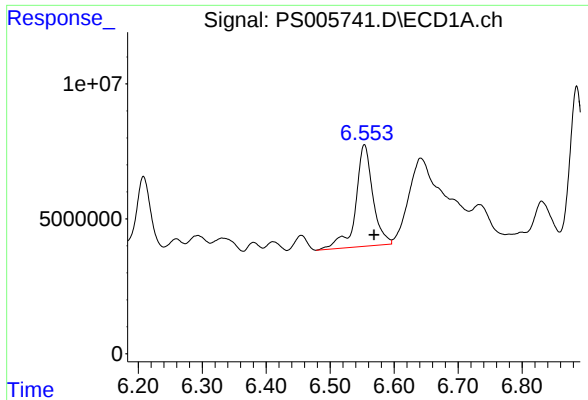

#9 2,4-D


R.T.: 6.554 min
Delta R.T.: -0.015 min
Response: 70426889
Conc: 46.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-2-A

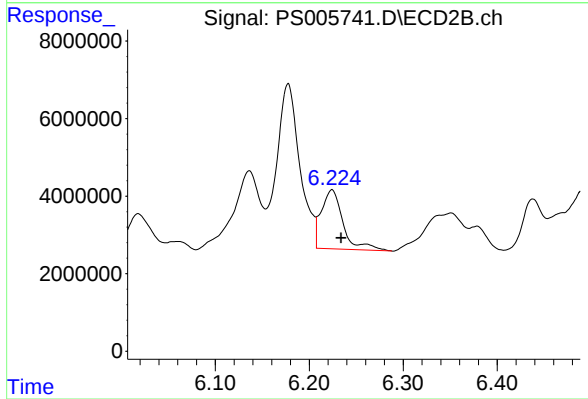


#9 2,4-D

R.T.: 6.224 min
Delta R.T.: -0.010 min
Response: 24403735
Conc: 22.72 ng/ml

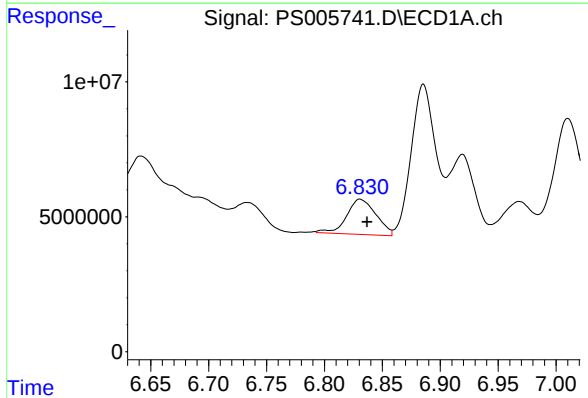


#10 Pentachlorophenol

R.T.: 6.831 min
Delta R.T.: -0.006 min
Response: 23080570
Conc: 1.10 ng/ml

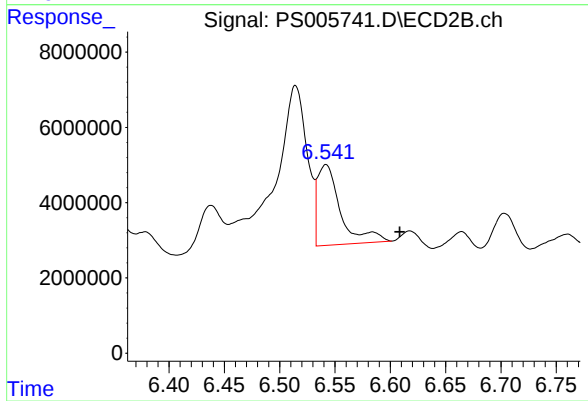

#10 Pentachlorophenol


R.T.: 6.542 min
Delta R.T.: -0.067 min
Response: 30918690
Conc: 2.38 ng/ml

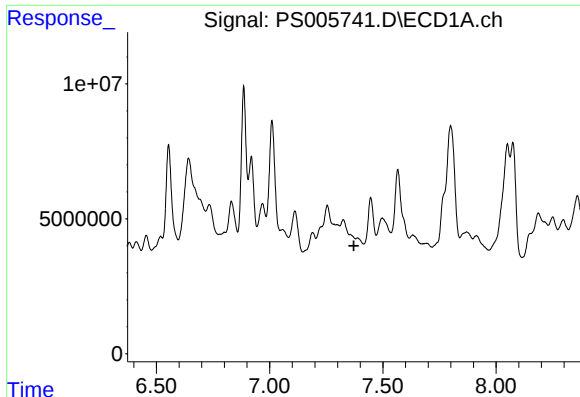

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-2-A

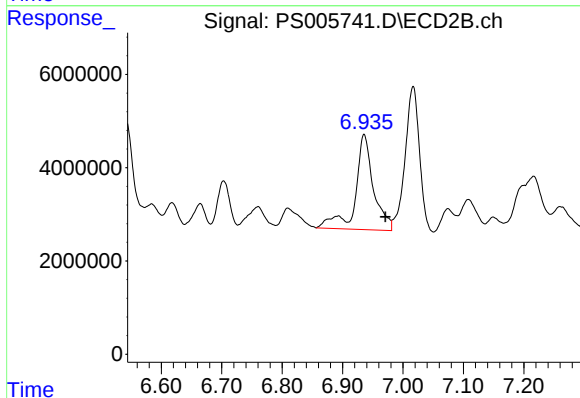


#11 2,4,5-TP (SILVEX)

R.T.: 6.936 min
Delta R.T.: -0.035 min
Response: 42441104
Conc: 8.18 ng/ml

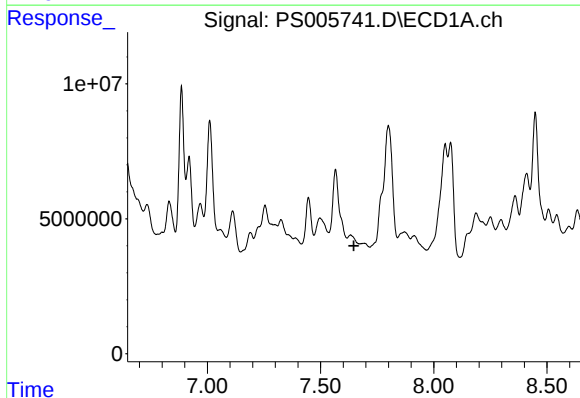


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.647 min
Response: 0
Conc: N.D.

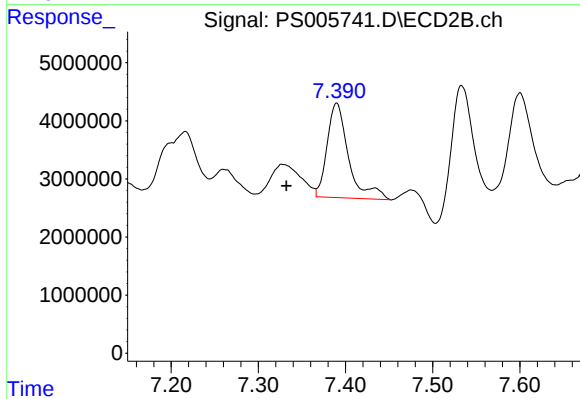

#12 2,4,5-T


R.T.: 7.390 min
Delta R.T.: 0.058 min
Response: 27803655
Conc: 5.85 ng/ml

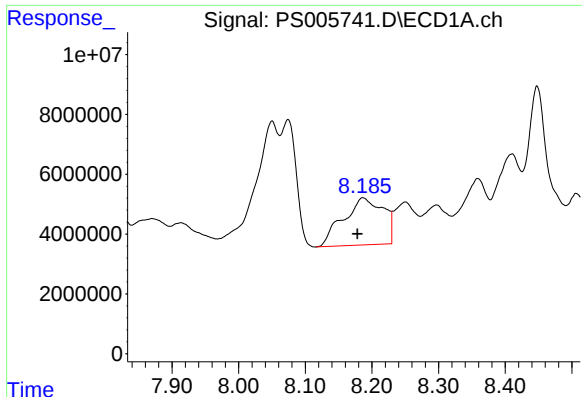

#13 2,4-DB


R.T.: 8.187 min
Delta R.T.: 0.008 min
Response: 65735288
Conc: 62.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-2-A

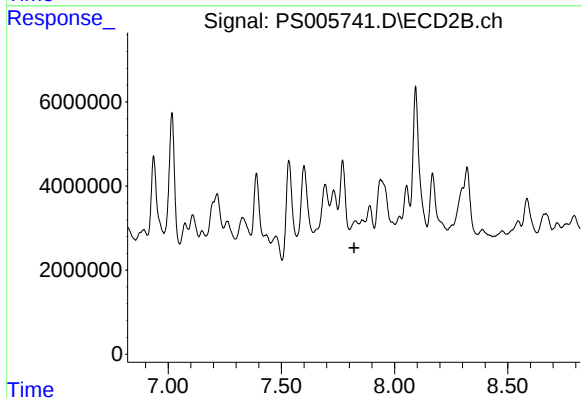


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.821 min
Response: 0
Conc: N.D.

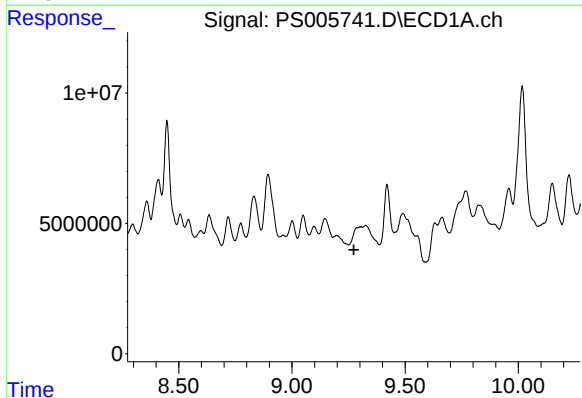


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.273 min
Response: 0
Conc: N.D.

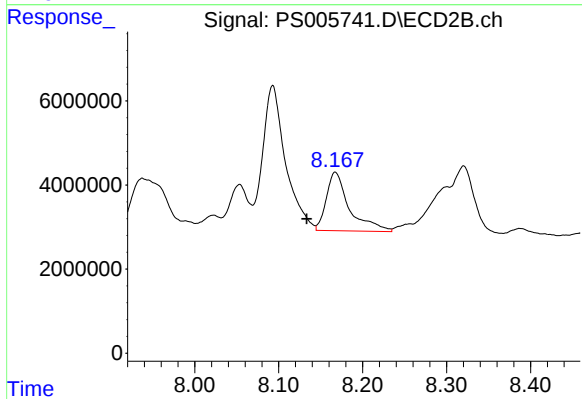

#14 DINOSEB


R.T.: 8.168 min
Delta R.T.: 0.034 min
Response: 26500218
Conc: 7.12 ng/ml

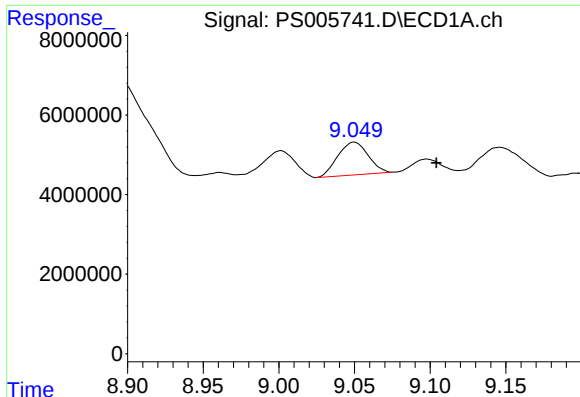

#15 Picloram


R.T.: 9.050 min
Delta R.T.: -0.054 min
Response: 11492533
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-2-A

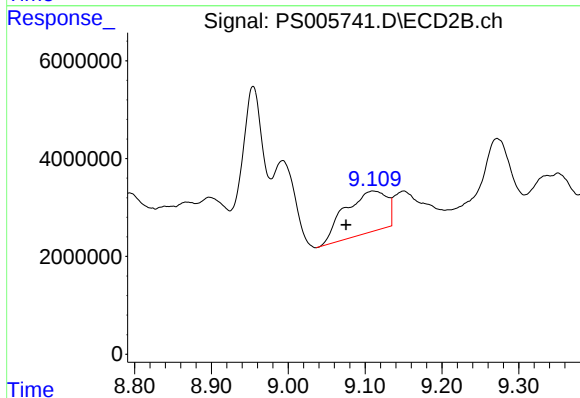


#15 Picloram

R.T.: 9.111 min
Delta R.T.: 0.036 min
Response: 32357037
Conc: 4.31 ng/ml

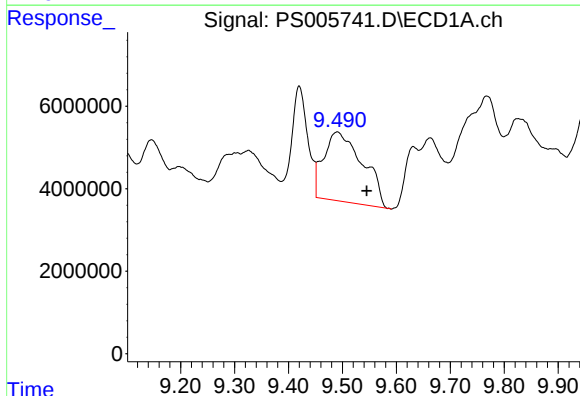

#16 DCPA

R.T.: 9.490 min
Delta R.T.: -0.055 min
Response: 84367833
Conc: 8.30 ng/ml

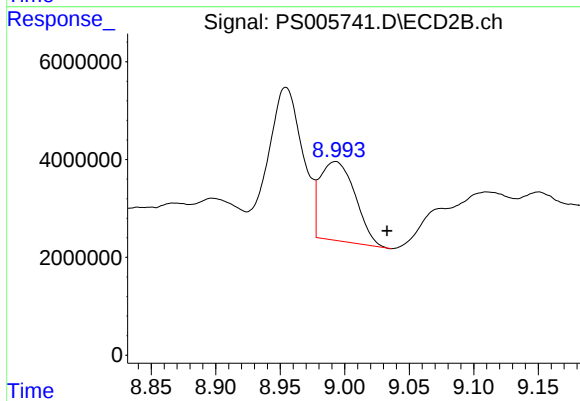

#16 DCPA

R.T.: 8.993 min
Delta R.T.: -0.040 min
Response: 30566883
Conc: 4.64 ng/ml