

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072719\
 Data File : PS005742.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2019 20:47
 Operator : SM\AJ
 Sample : K3990-04
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-2-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 01:02:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.558	5.277	407.5E6	237.5E6	280.893	238.820
Target Compounds							
2) T	3,5-DICHL...	0.000	4.597	0	11030704	N.D.	8.503
6) T	MCP	5.867	0.000	22799331	0	4.921	N.D. #
7) T	MCPA	5.979	5.687	52571779	14936684	8.056	3.549 #
8) T	DICHLORPROP	0.000	5.899	0	12415323	N.D.	13.443
9) T	2,4-D	6.639	6.220	125.2E6	18571040	83.519	17.287 #
11) T	2,4,5-TP ...	0.000	6.932	0	31377729	N.D.	6.049
13) T	2,4-DB	8.208	0.000	45027145	0	42.643	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072719\
Data File : PS005742.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2019 20:47
Operator : SM\AJ
Sample : K3990-04
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-2-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 01:02:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

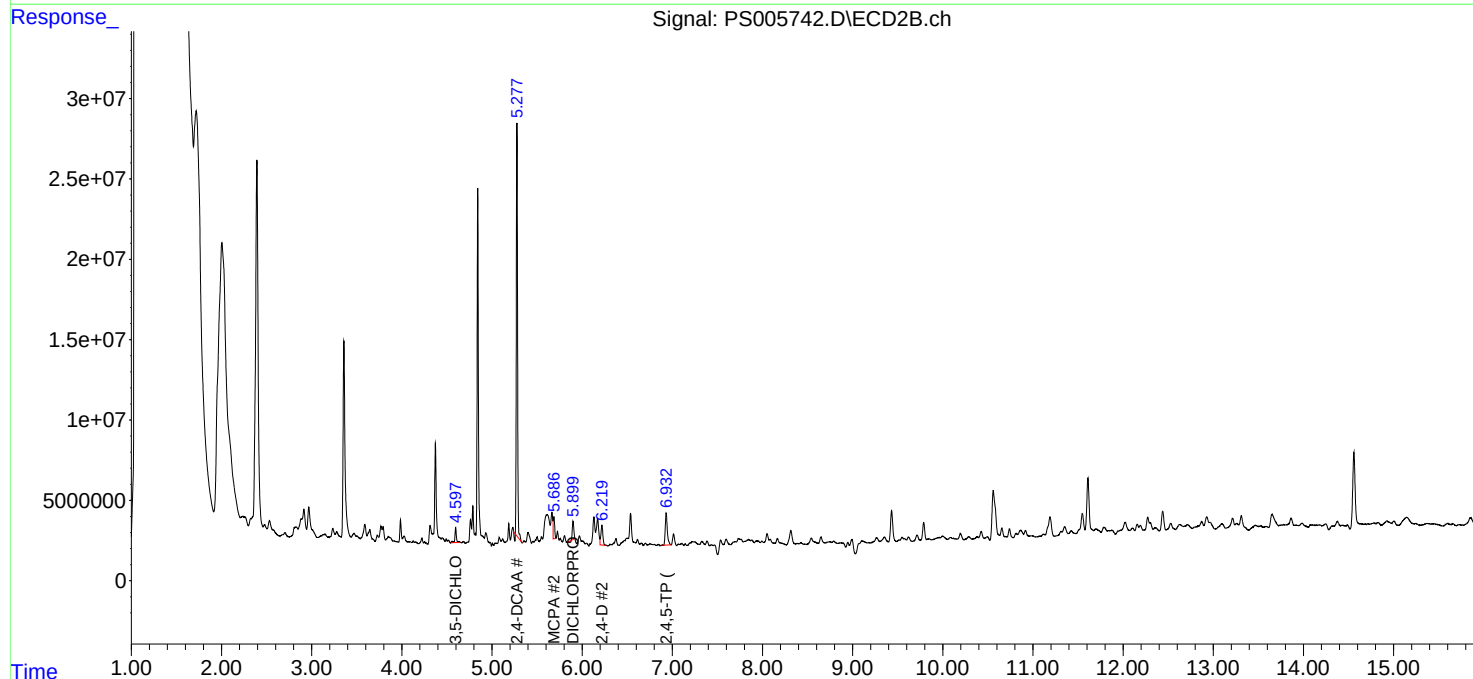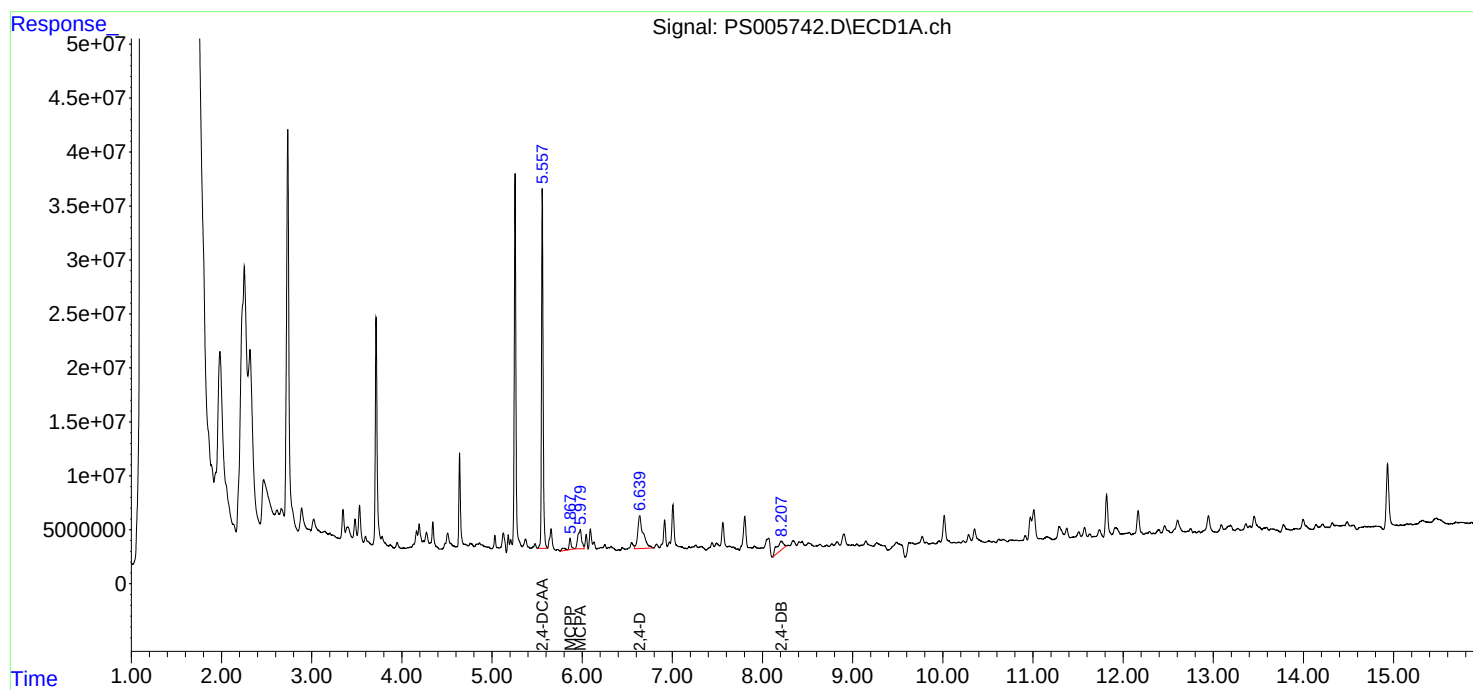


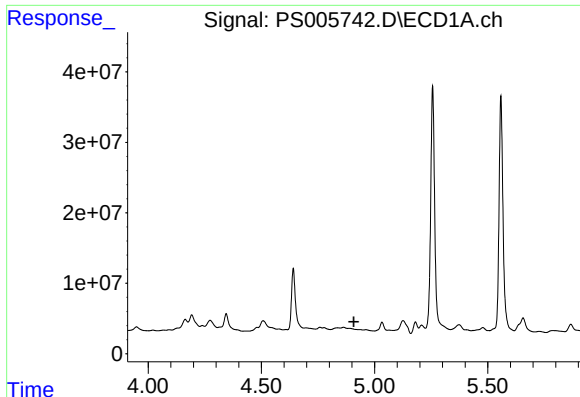

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-2-B

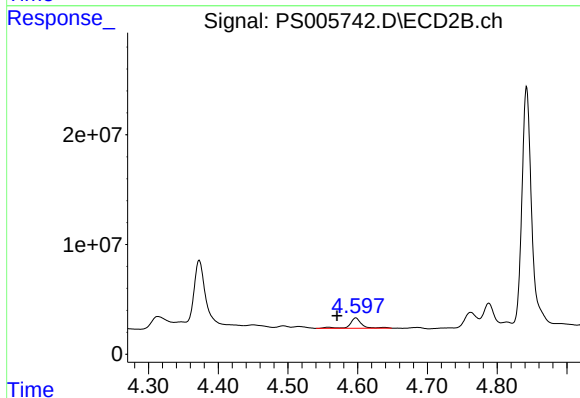


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.597 min
Delta R.T.: 0.027 min
Response: 11030704
Conc: 8.50 ng/ml

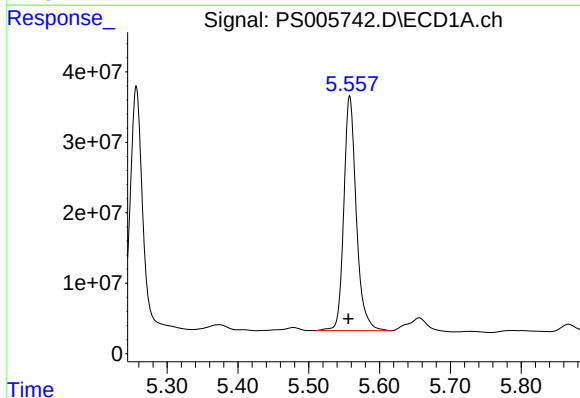


#4 2,4-DCAA

R.T.: 5.558 min
Delta R.T.: 0.002 min
Response: 407524103
Conc: 280.89 ng/ml

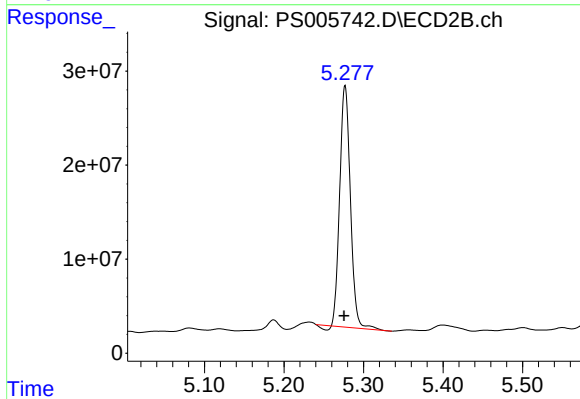

#4 2,4-DCAA


R.T.: 5.277 min
Delta R.T.: 0.001 min
Response: 237549318
Conc: 238.82 ng/ml

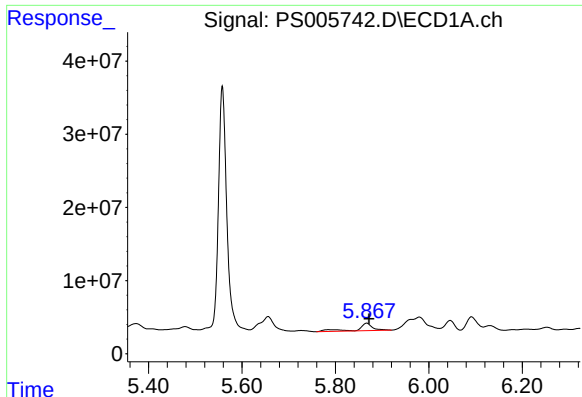

#6 MCPP


R.T.: 5.867 min
Delta R.T.: -0.006 min
Response: 22799331
Conc: 4.92 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-2-B

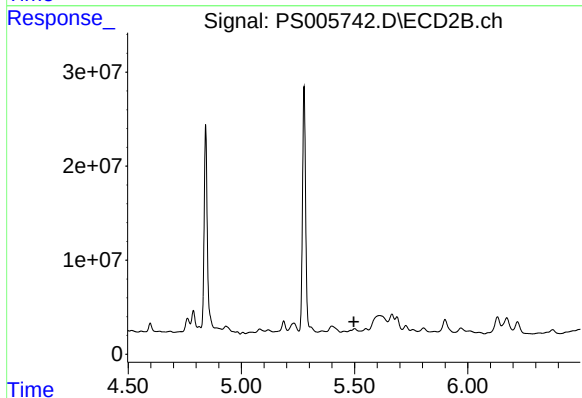


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

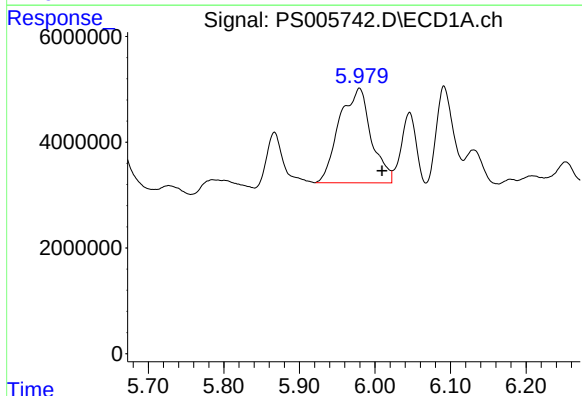


#7 MCPA

R.T.: 5.979 min
Delta R.T.: -0.030 min
Response: 52571779
Conc: 8.06 ug/ml

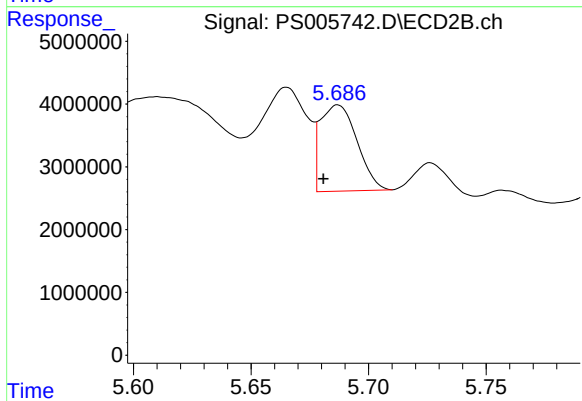

#7 MCPA


R.T.: 5.687 min
Delta R.T.: 0.006 min
Response: 14936684
Conc: 3.55 ug/ml

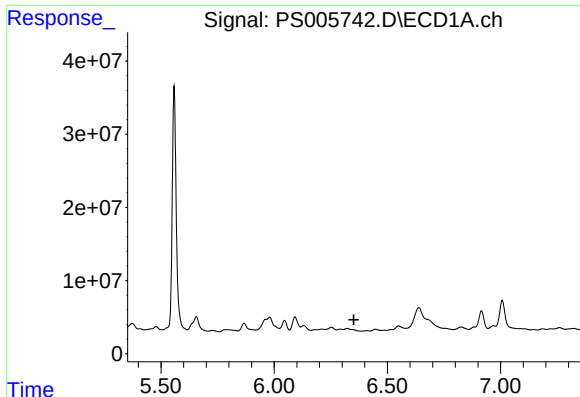

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-2-B

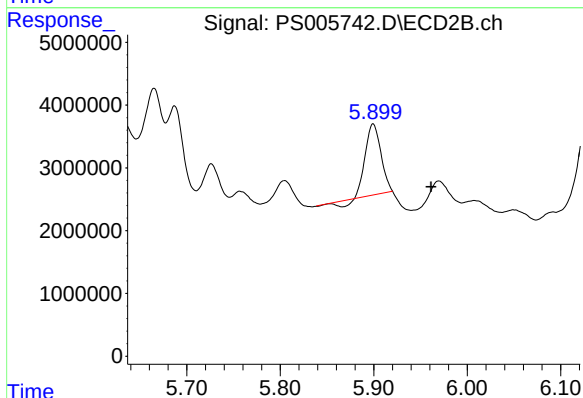


#8 DICHLORPROP

R.T.: 5.899 min
Delta R.T.: -0.062 min
Response: 12415323
Conc: 13.44 ng/ml

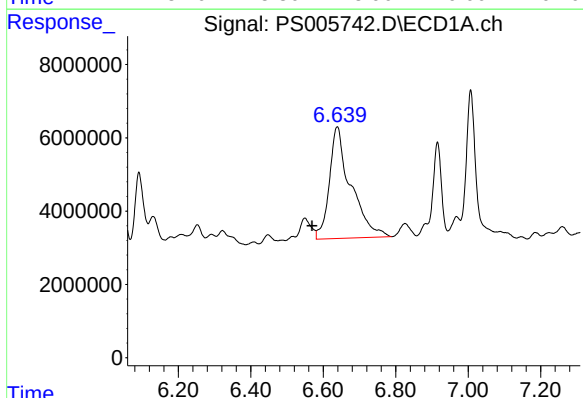


#9 2,4-D

R.T.: 6.639 min
Delta R.T.: 0.070 min
Response: 125167063
Conc: 83.52 ng/ml

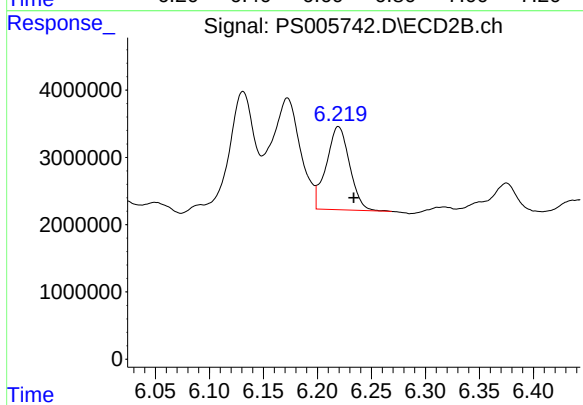

#9 2,4-D


R.T.: 6.220 min
Delta R.T.: -0.014 min
Response: 18571040
Conc: 17.29 ng/ml

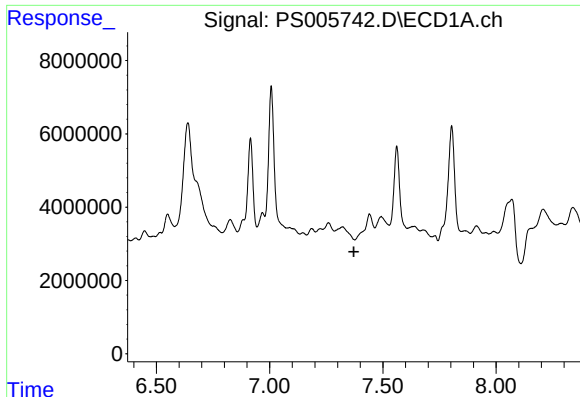

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-2-B

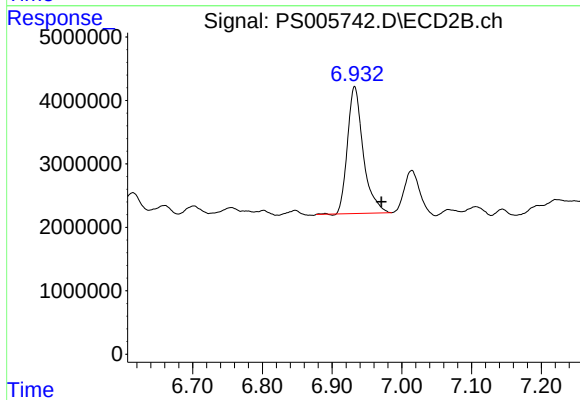


#11 2,4,5-TP (SILVEX)

R.T.: 6.932 min
Delta R.T.: -0.038 min
Response: 31377729
Conc: 6.05 ng/ml

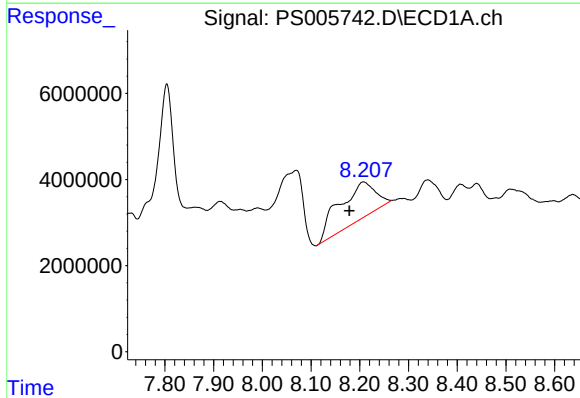

#13 2,4-DB

R.T.: 8.208 min
Delta R.T.: 0.029 min
Response: 45027145
Conc: 42.64 ng/ml

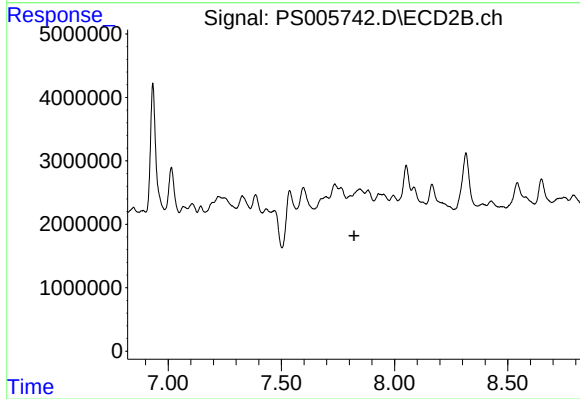

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 7.821 min
Response: 0
Conc: N.D.