

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072719\
 Data File : PS005743.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2019 21:09
 Operator : SM\AJ
 Sample : K3990-05
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-3-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 01:03:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.562	5.280	218.9E6	129.3E6	150.851	130.025
Target Compounds							
2) T	3,5-DICHL...	0.000	4.599	0	36356197	N.D.	28.024
6) T	MCP	5.868	0.000	11753086	0	2.537	N.D. #
7) T	MCPA	6.048	5.668	18393204	27595646	2.819	6.556 #
8) T	DICHLORPROP	0.000	5.902	0	5820288	N.D.	6.302
9) T	2,4-D	0.000	6.172	0	16322505	N.D.	15.194
10) T	Pentachlo...	0.000	6.540	0	30844074	N.D.	2.376
11) T	2,4,5-TP ...	0.000	6.936	0	30887303	N.D.	5.954
13) T	2,4-DB	8.215	0.000	42678860	0	40.419	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072719\
Data File : PS005743.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2019 21:09
Operator : SM\AJ
Sample : K3990-05
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-3-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 01:03:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

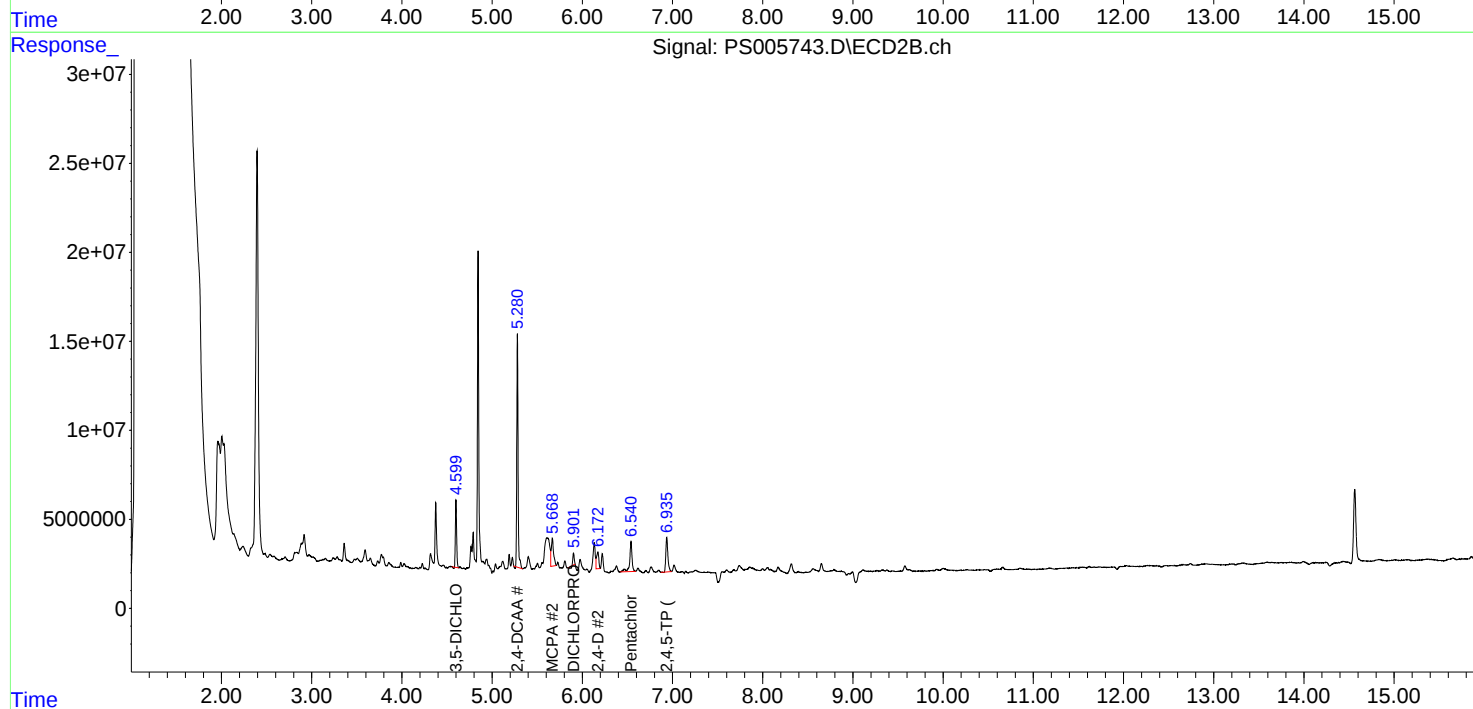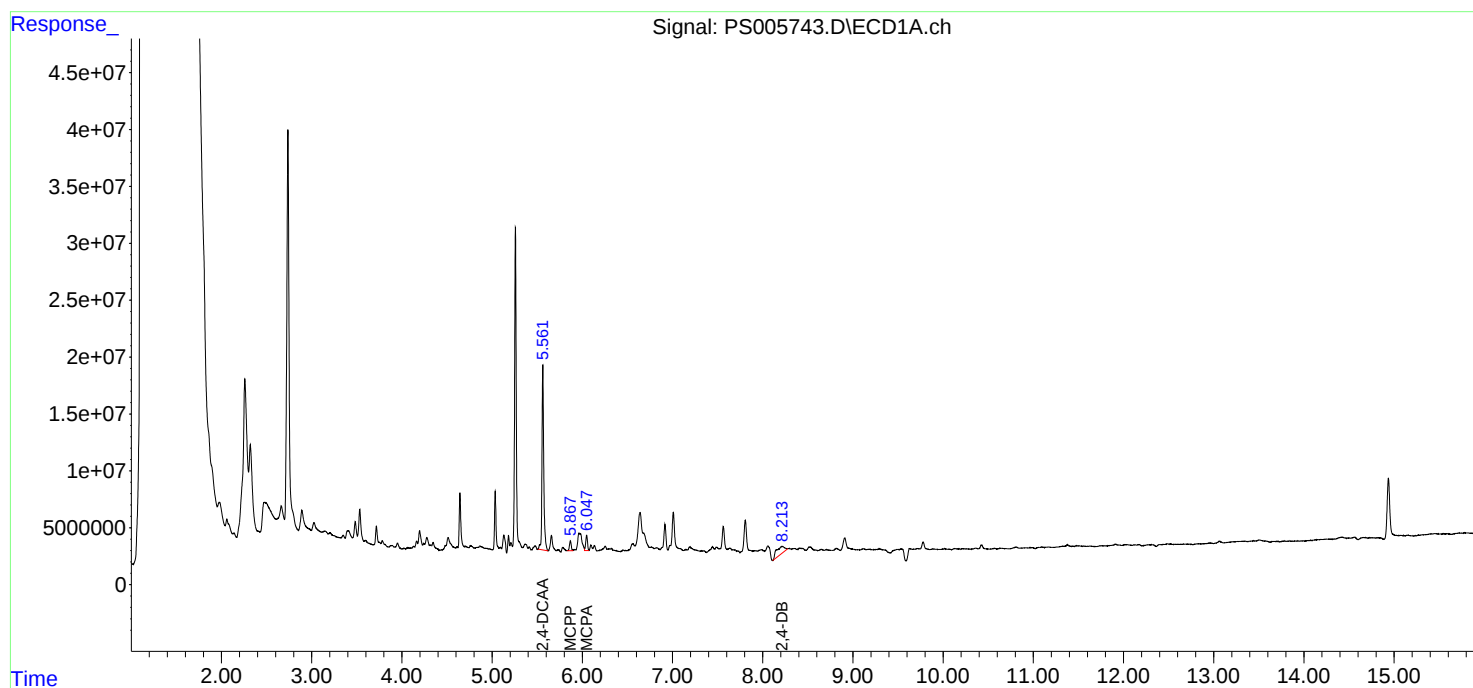


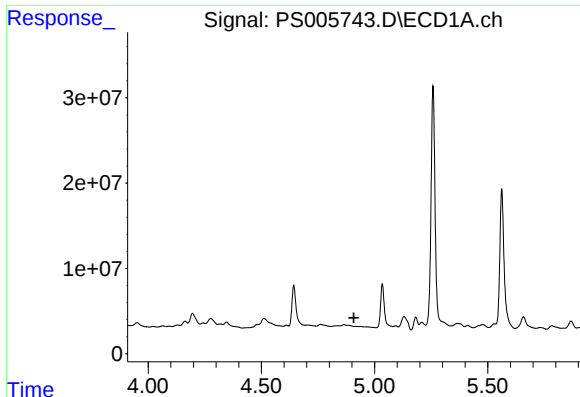

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3-A

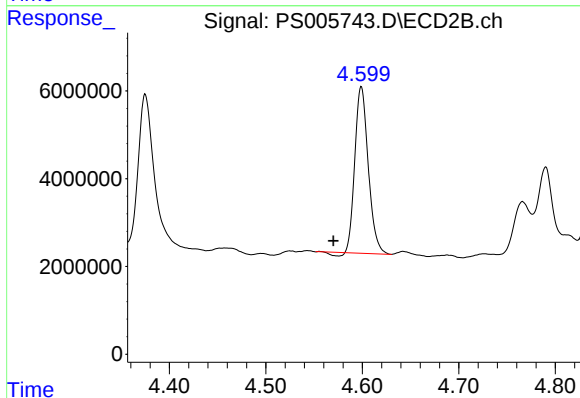


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.599 min
Delta R.T.: 0.029 min
Response: 36356197
Conc: 28.02 ng/ml

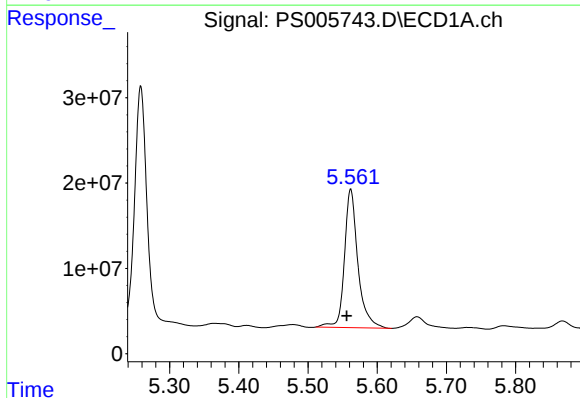


#4 2,4-DCAA

R.T.: 5.562 min
Delta R.T.: 0.006 min
Response: 218856594
Conc: 150.85 ng/ml

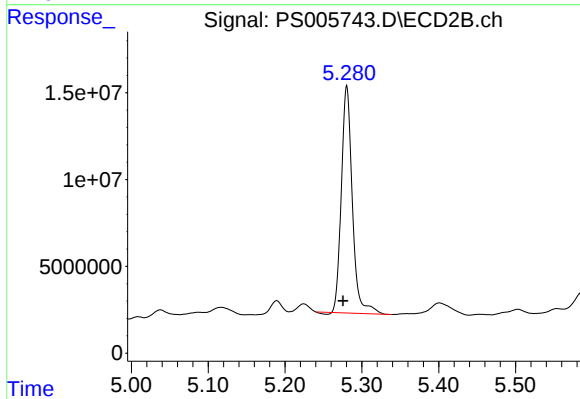

#4 2,4-DCAA


R.T.: 5.280 min
Delta R.T.: 0.005 min
Response: 129333421
Conc: 130.03 ng/ml

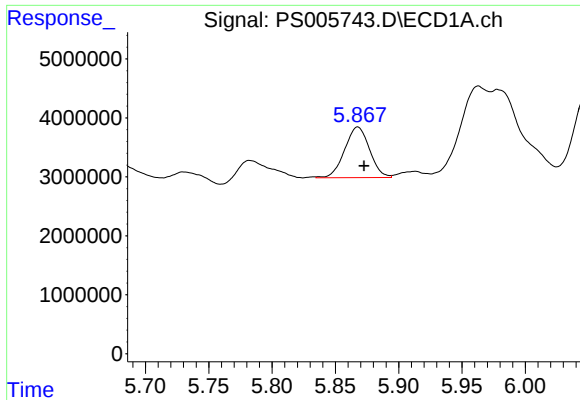

#6 MCPP


R.T.: 5.868 min
Delta R.T.: -0.005 min
Response: 11753086
Conc: 2.54 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-3-A

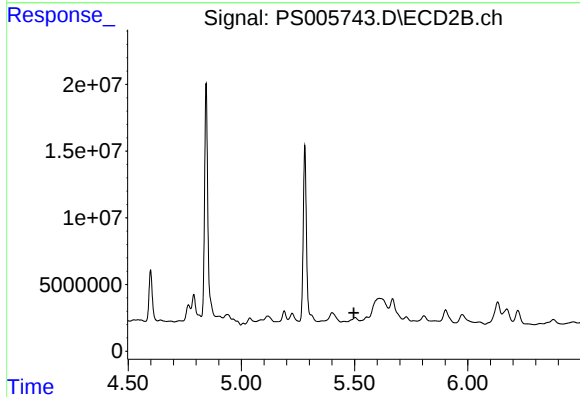


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

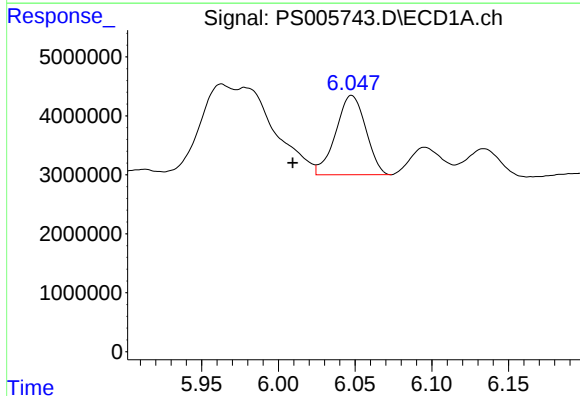


#7 MCPA

R.T.: 6.048 min
Delta R.T.: 0.038 min
Response: 18393204
Conc: 2.82 ug/ml

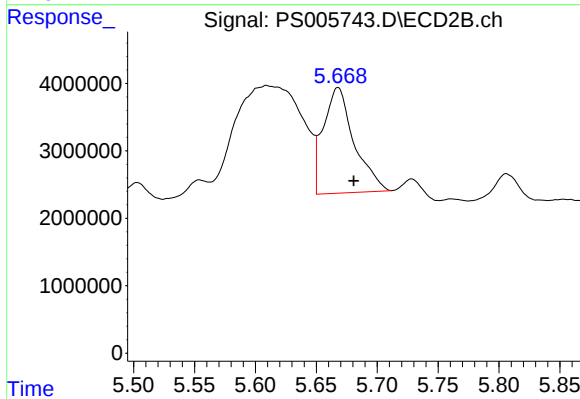

#7 MCPA


R.T.: 5.668 min
Delta R.T.: -0.013 min
Response: 27595646
Conc: 6.56 ug/ml

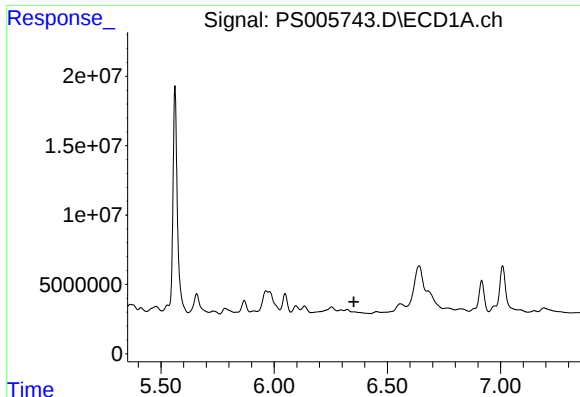

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3-A

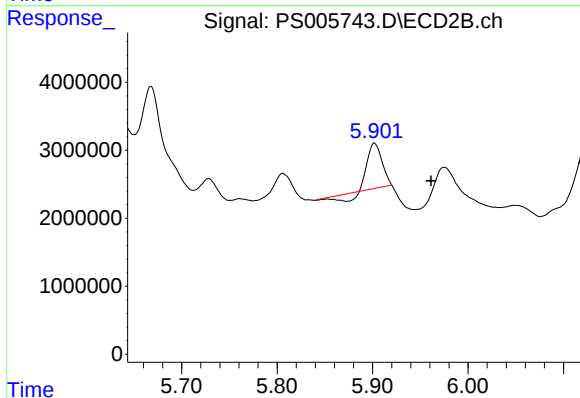


#8 DICHLORPROP

R.T.: 5.902 min
Delta R.T.: -0.059 min
Response: 5820288
Conc: 6.30 ng/ml

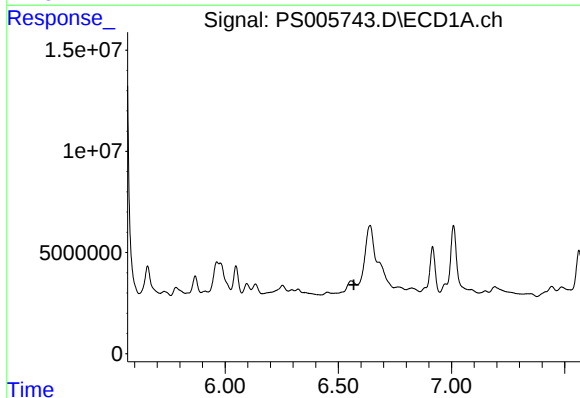


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.569 min
Response: 0
Conc: N.D.

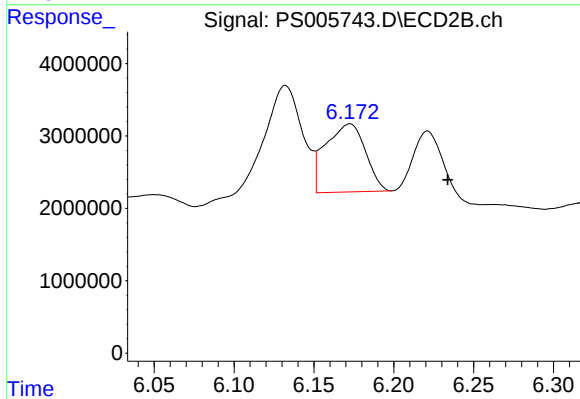

#9 2,4-D


R.T.: 6.172 min
Delta R.T.: -0.062 min
Response: 16322505
Conc: 15.19 ng/ml

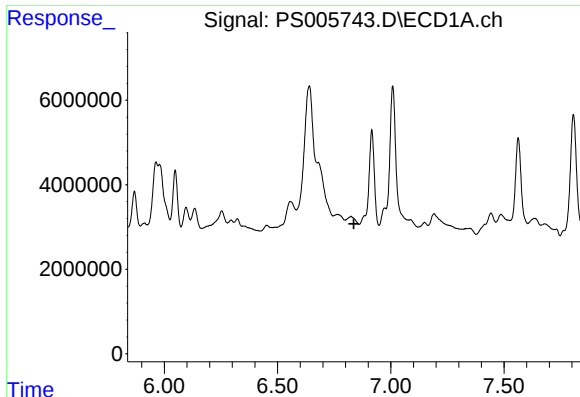

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3-A

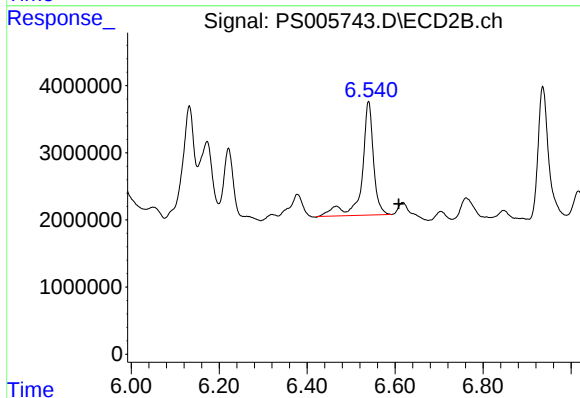


#10 Pentachlorophenol

R.T.: 6.540 min
Delta R.T.: -0.069 min
Response: 30844074
Conc: 2.38 ng/ml

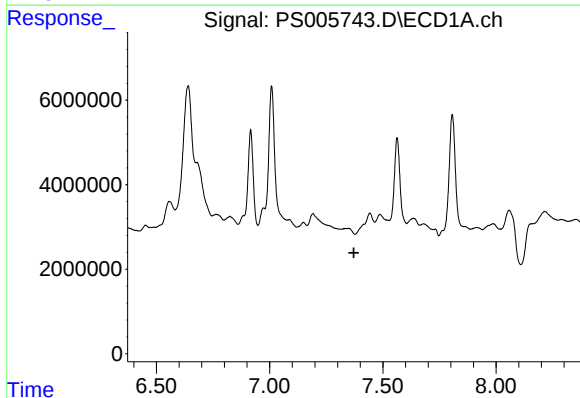


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

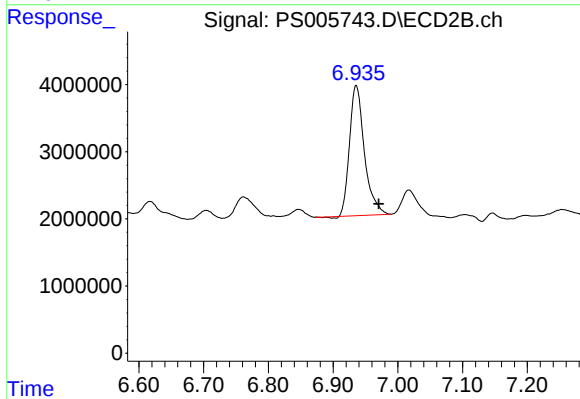

#11 2,4,5-TP (SILVEX)


R.T.: 6.936 min
Delta R.T.: -0.035 min
Response: 30887303
Conc: 5.95 ng/ml

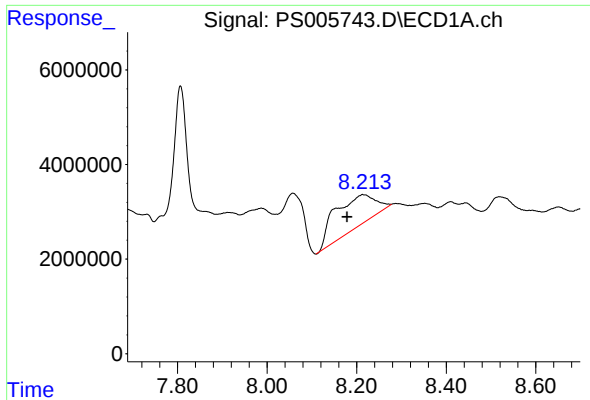

#13 2,4-DB

R.T.: 8.215 min
Delta R.T.: 0.036 min
Response: 42678860
Conc: 40.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3-A

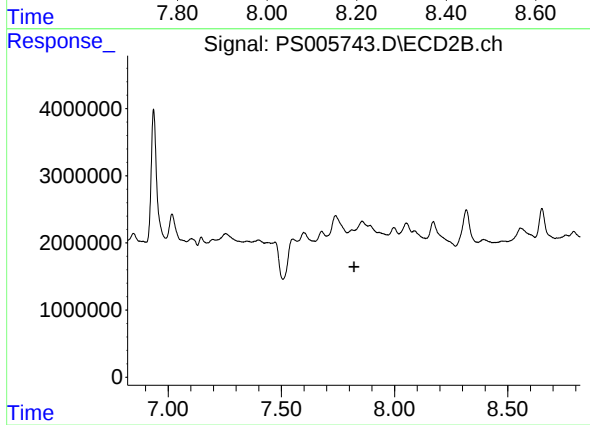

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.821 min
Response: 0
Conc: N.D.