

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072719\
 Data File : PS005747.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2019 22:38
 Operator : SM\AJ
 Sample : K3990-09
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-5-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 01:05:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.581	5.259	341.8E6	20918067	235.624	21.030 #
Target Compounds							
1) T	Dalapon	0.000	1.749	0	734.6E6	N.D.	582.738
2) T	3,5-DICHL...	0.000	4.621	0	73337881	N.D.	56.531
6) T	MCP	5.891	5.523	18563333	22801356	4.006	8.005 #
7) T	MCPA	5.976	5.711	46421944	78682981	7.114	18.694 #
8) T	DICHLORPROP	0.000	5.992	0	20236970	N.D.	21.913
9) T	2,4-D	6.572	6.242	19723815	22139694	13.161	20.609 #
10) T	Pentachlo...	6.904	6.561	40068084	41576247	1.917	3.202 #
11) T	2,4,5-TP ...	0.000	6.954	0	33554446	N.D.	6.469
12) T	2,4,5-T	7.584	0.000	66764271	0	7.999	N.D. #
13) T	2,4-DB	8.206	0.000	58465139	0	55.369	N.D. #
14) T	DINOSEB	0.000	8.111	0	41076885	N.D.	11.038
15) T	Picloram	0.000	9.121	0	24294346	N.D.	3.234
16) T	DCPA	0.000	8.973	0	21039320	N.D.	3.191



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072719\
Data File : PS005747.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2019 22:38
Operator : SM\AJ
Sample : K3990-09
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
TP-5-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 01:05:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

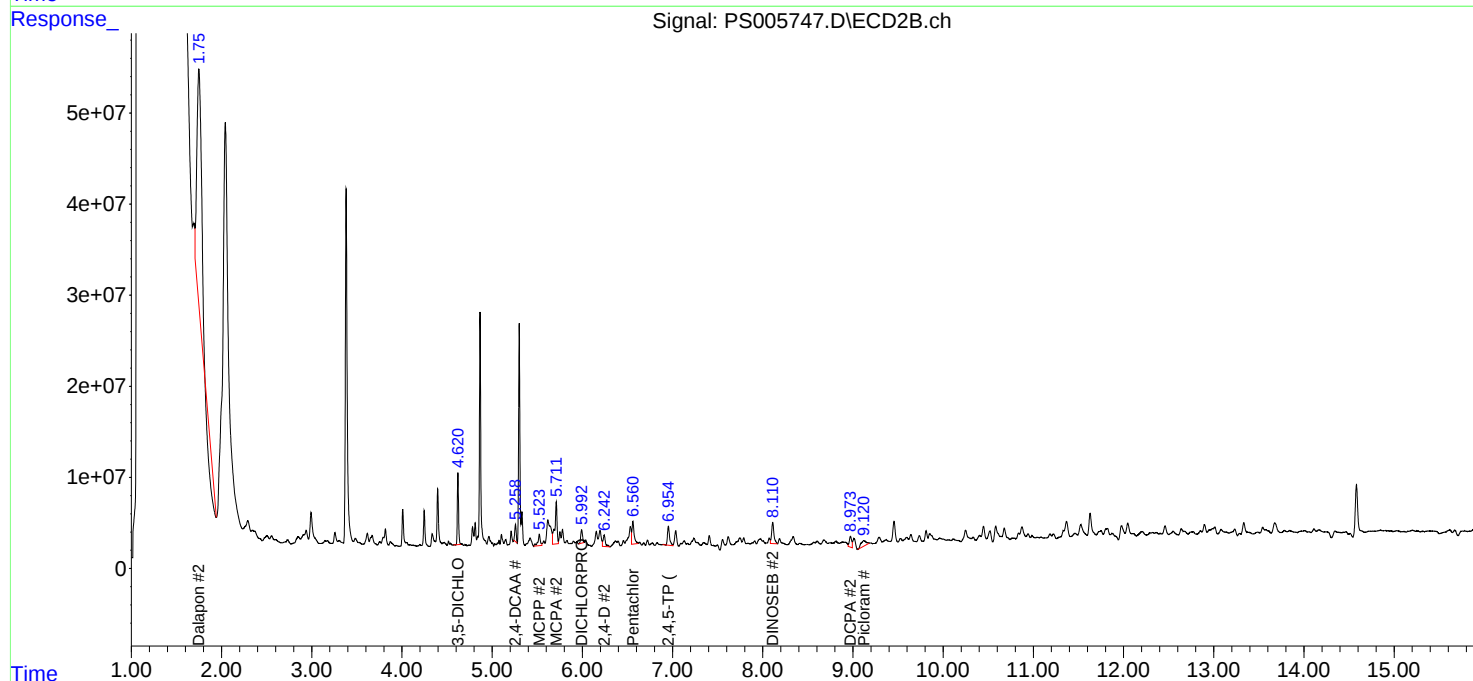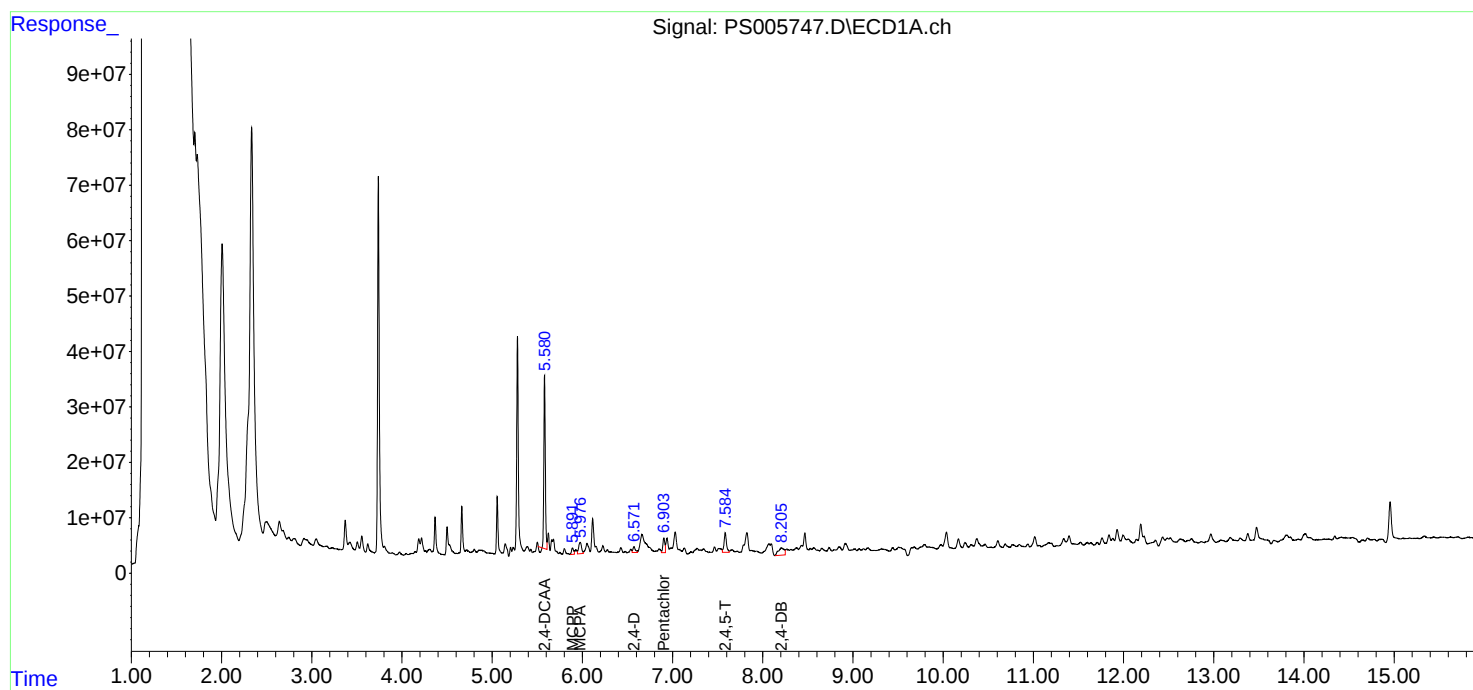


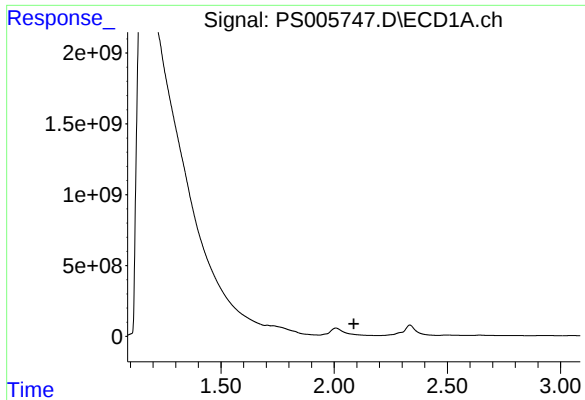

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.087 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-5-A

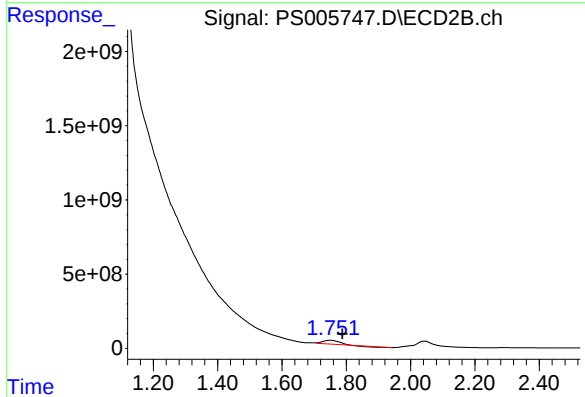


#1 Dalapon

R.T.: 1.749 min
Delta R.T.: -0.039 min
Response: 734586455
Conc: 582.74 ng/ml

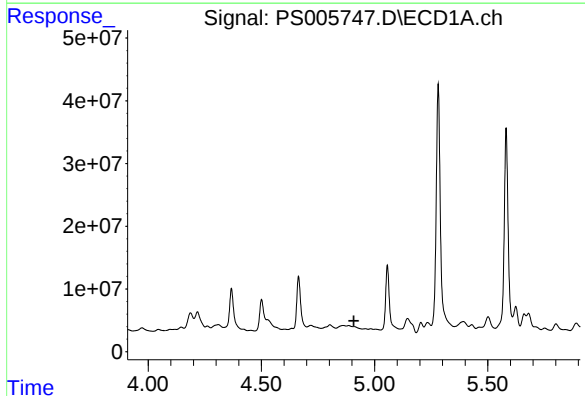


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

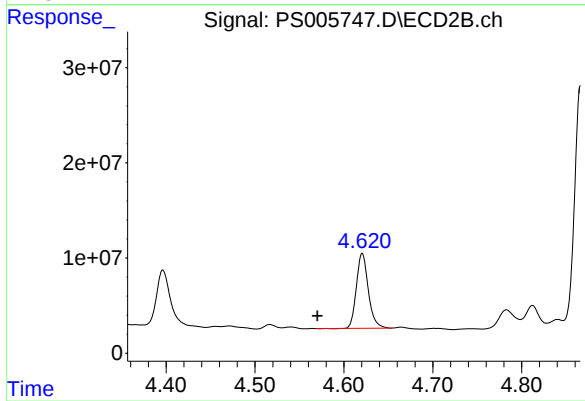

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.621 min
Delta R.T.: 0.051 min
Response: 73337881
Conc: 56.53 ng/ml

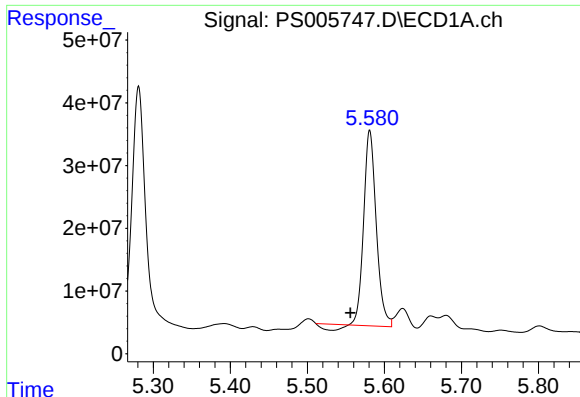

#4 2,4-DCAA


R.T.: 5.581 min
Delta R.T.: 0.025 min
Response: 341848009
Conc: 235.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-5-A

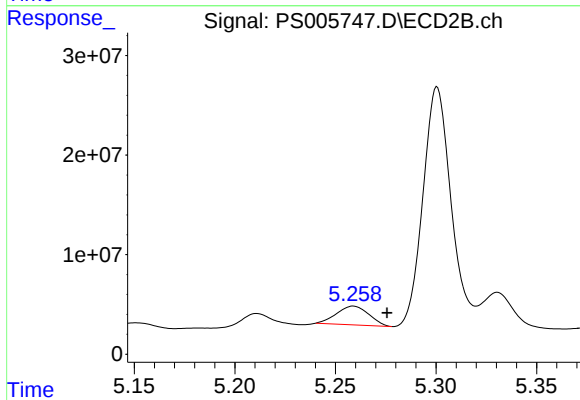


#4 2,4-DCAA

R.T.: 5.259 min
Delta R.T.: -0.017 min
Response: 20918067
Conc: 21.03 ng/ml

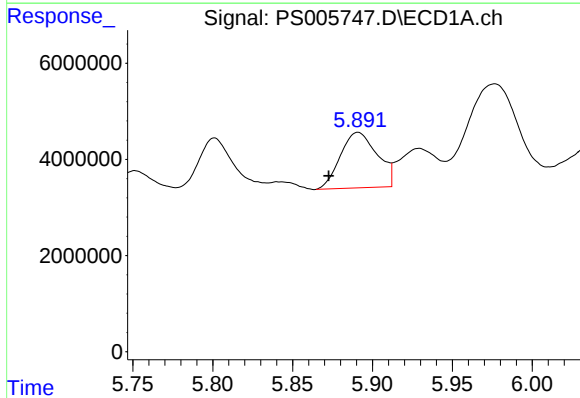


#6 MCPP

R.T.: 5.891 min
Delta R.T.: 0.018 min
Response: 18563333
Conc: 4.01 ug/ml

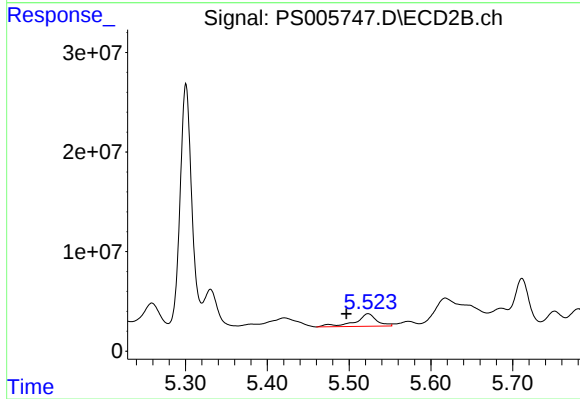

#6 MCPP


R.T.: 5.523 min
Delta R.T.: 0.026 min
Response: 22801356
Conc: 8.01 ug/ml

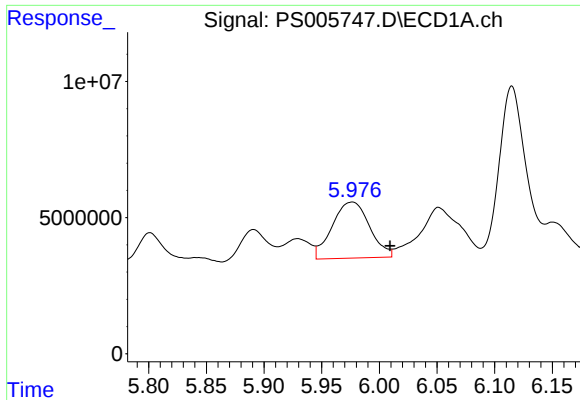

#7 MCPA


R.T.: 5.976 min
Delta R.T.: -0.033 min
Response: 46421944
Conc: 7.11 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-5-A

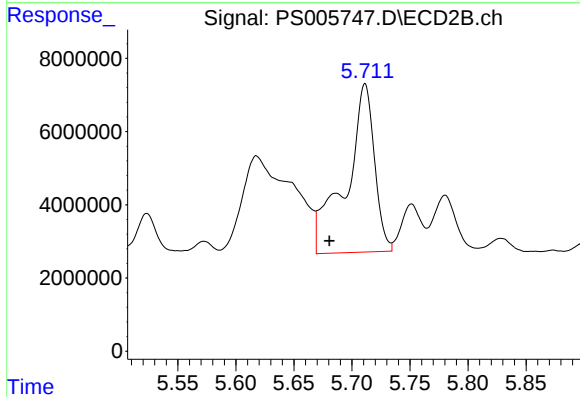


#7 MCPA

R.T.: 5.711 min
Delta R.T.: 0.030 min
Response: 78682981
Conc: 18.69 ug/ml

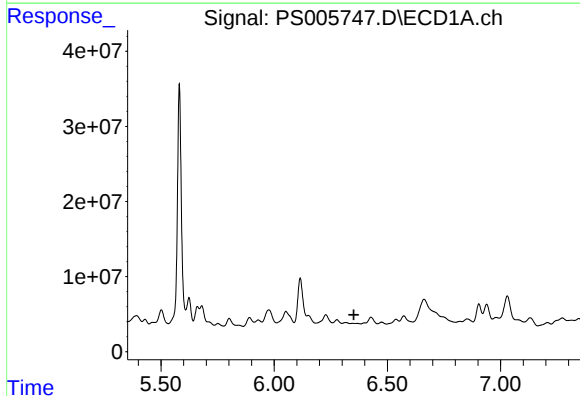


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.352 min
Response: 0
Conc: N.D.

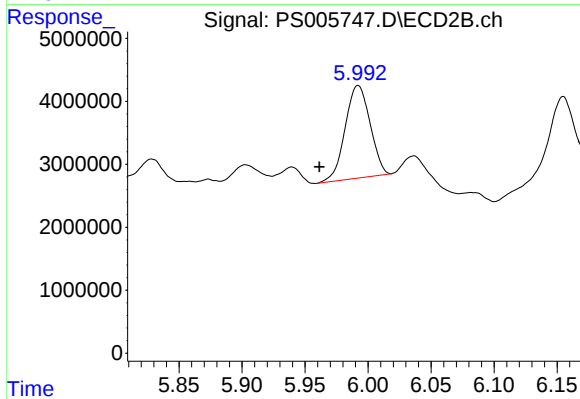

#8 DICHLORPROP


R.T.: 5.992 min
Delta R.T.: 0.031 min
Response: 20236970
Conc: 21.91 ng/ml

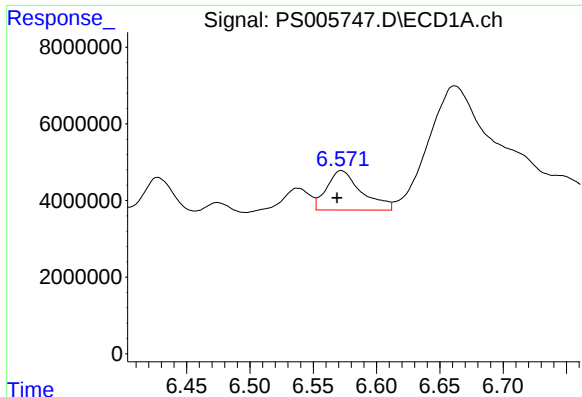

#9 2,4-D


R.T.: 6.572 min
Delta R.T.: 0.003 min
Response: 19723815
Conc: 13.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-5-A

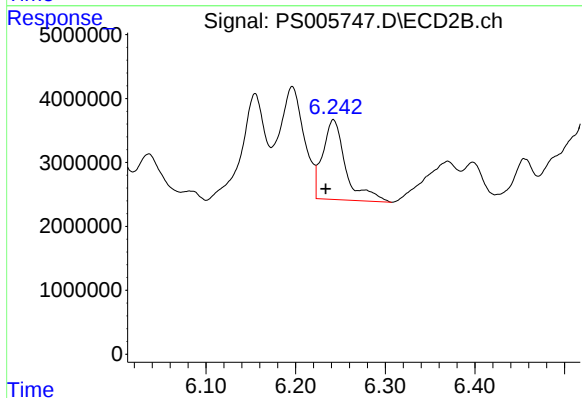


#9 2,4-D

R.T.: 6.242 min
Delta R.T.: 0.008 min
Response: 22139694
Conc: 20.61 ng/ml

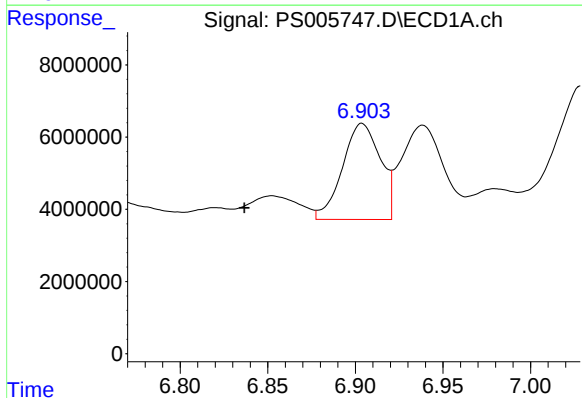


#10 Pentachlorophenol

R.T.: 6.904 min
Delta R.T.: 0.067 min
Response: 40068084
Conc: 1.92 ng/ml

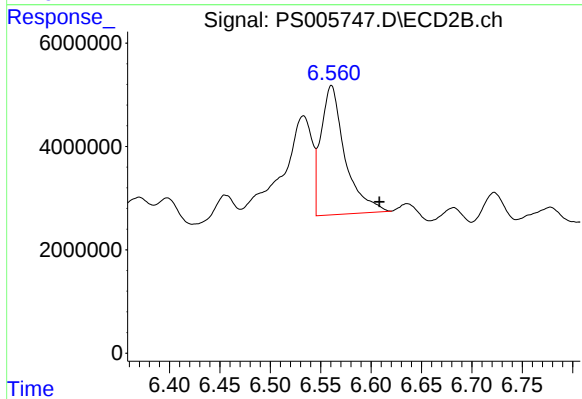

#10 Pentachlorophenol


R.T.: 6.561 min
Delta R.T.: -0.048 min
Response: 41576247
Conc: 3.20 ng/ml

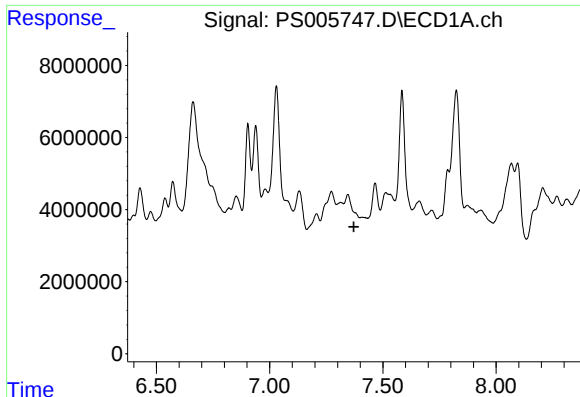

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-5-A

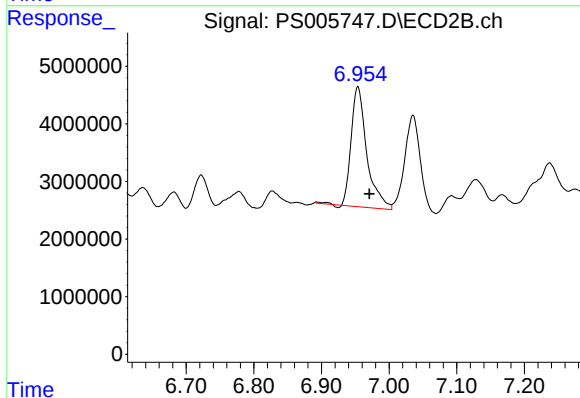


#11 2,4,5-TP (SILVEX)

R.T.: 6.954 min
Delta R.T.: -0.017 min
Response: 33554446
Conc: 6.47 ng/ml

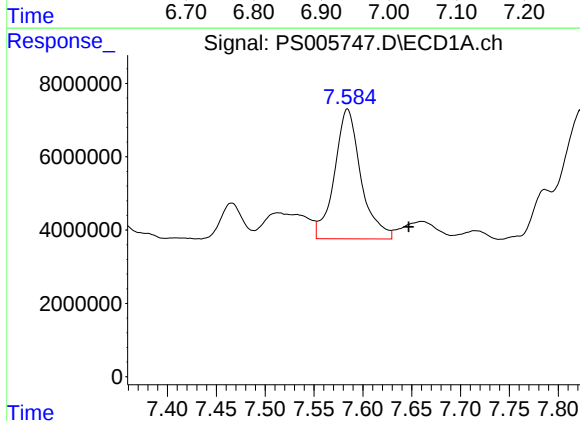


#12 2,4,5-T

R.T.: 7.584 min
Delta R.T.: -0.062 min
Response: 66764271
Conc: 8.00 ng/ml

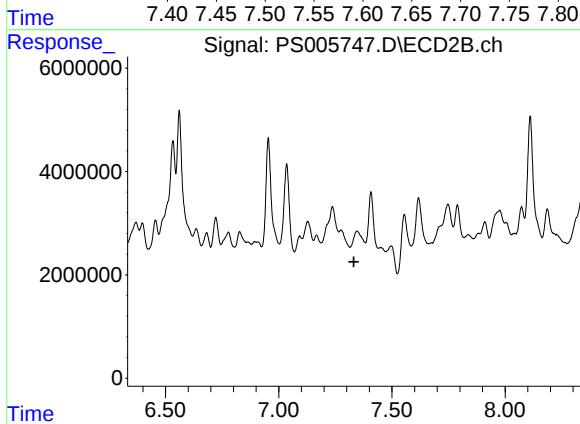

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.332 min
Response: 0
Conc: N.D.

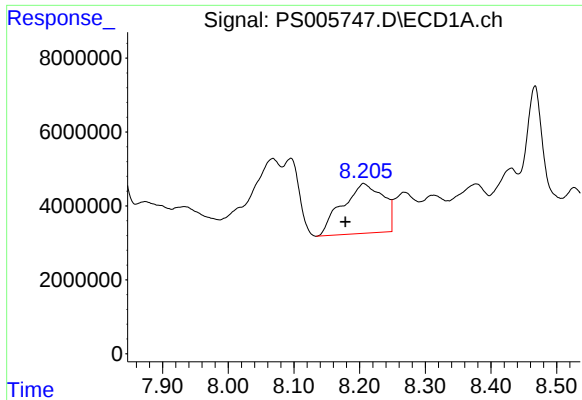

#13 2,4-DB


R.T.: 8.206 min
Delta R.T.: 0.028 min
Response: 58465139
Conc: 55.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-5-A

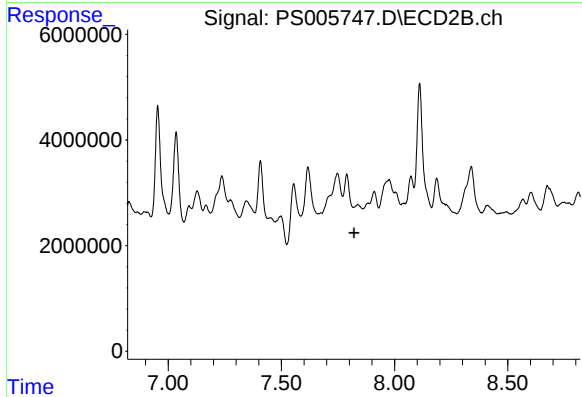


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.821 min
Response: 0
Conc: N.D.

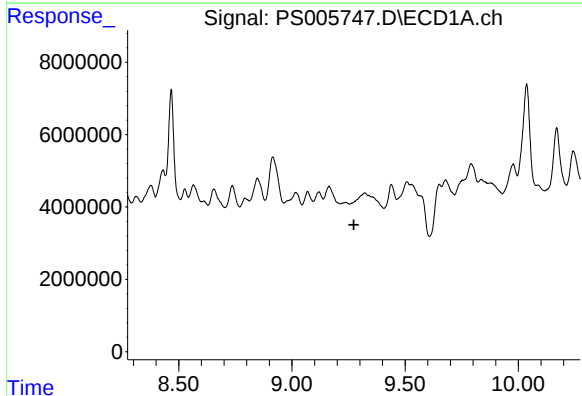


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.273 min
Response: 0
Conc: N.D.

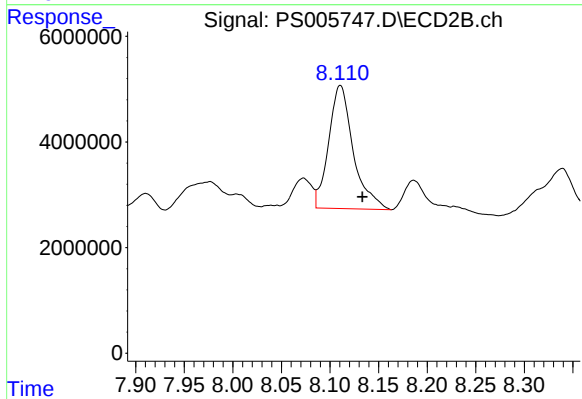

#14 DINOSEB


R.T.: 8.111 min
Delta R.T.: -0.023 min
Response: 41076885
Conc: 11.04 ng/ml

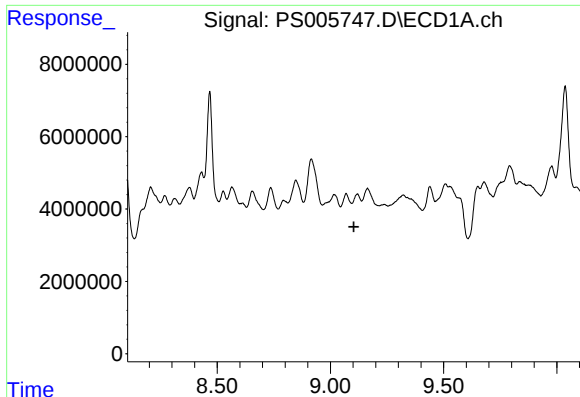

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 9.104 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-5-A

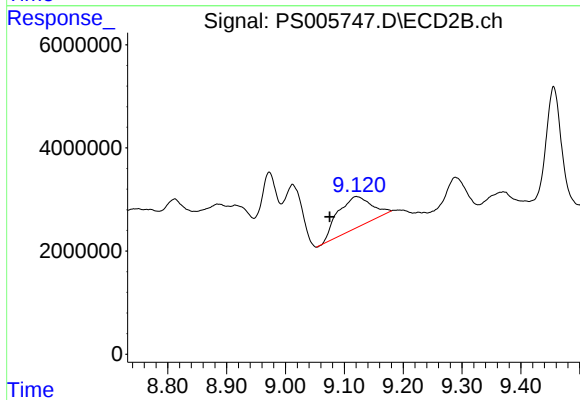


#15 Picloram

R.T.: 9.121 min
Delta R.T.: 0.046 min
Response: 24294346
Conc: 3.23 ng/ml

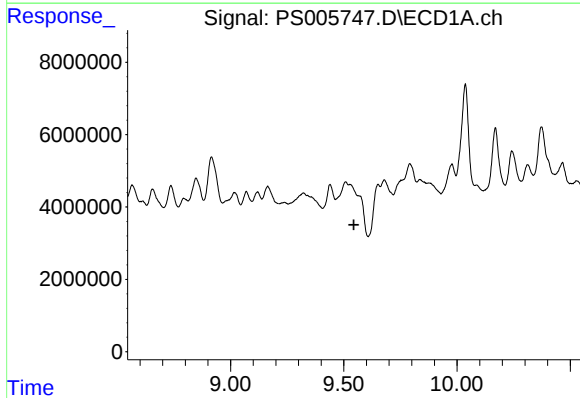

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.545 min
Response: 0
Conc: N.D.

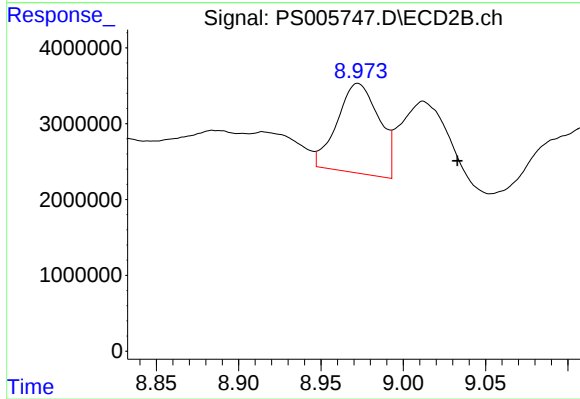

#16 DCPA

R.T.: 8.973 min
Delta R.T.: -0.060 min
Response: 21039320
Conc: 3.19 ng/ml