

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072722\
 Data File : PS020075.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2022 16:33
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 02:05:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072022.M
 Quant Title : 8080.M
 QLast Update : Wed Jul 20 17:52:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.192	6.777	1592.7E6	507.2E6	480.342	563.004
Target Compounds							
1) T	Dalapon	0.000	2.565f	0	80074	N.D.	<MDL
2) T	3,5-DICHL...	6.451f	0.000	4224586	0	<MDL	N.D. #
3) T	4-Nitroph...	6.980f	6.381	4525851	1221832	3.148	2.529
5) T	DICAMBA	0.000	7.002f	0	766193	N.D.	<MDL
6) T	MCP	7.563	7.002f	914363	766193	<MDL	<MDL #
7) T	MCPA	7.689	0.000	7029212	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.618f	0	3006968	N.D.	2.899
9) T	2,4-D	0.000	7.827	0	964077	N.D.	<MDL
10) T	Pentachlo...	8.613	8.278	3585538	1502278	<MDL	<MDL #
11) T	2,4,5-TP ...	9.169	8.643	3788288	516859	<MDL	<MDL #
12) T	2,4,5-T	9.389f	9.041	71224007	889924	3.296	<MDL #
13) T	2,4-DB	9.977	9.549	8681642	2760108	1.993	3.867 #
14) T	DINOSEB	0.000	9.847	0	987435	N.D.	<MDL
15) T	Picloram	10.948	10.858	199.6E6	61257151	5.730	7.971 #
16) T	DCPA	11.412	10.772	2211970	3589281	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072722\
Data File : PS020075.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2022 16:33
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 02:05:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072022.M
Quant Title : 8080.M
QLast Update : Wed Jul 20 17:52:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

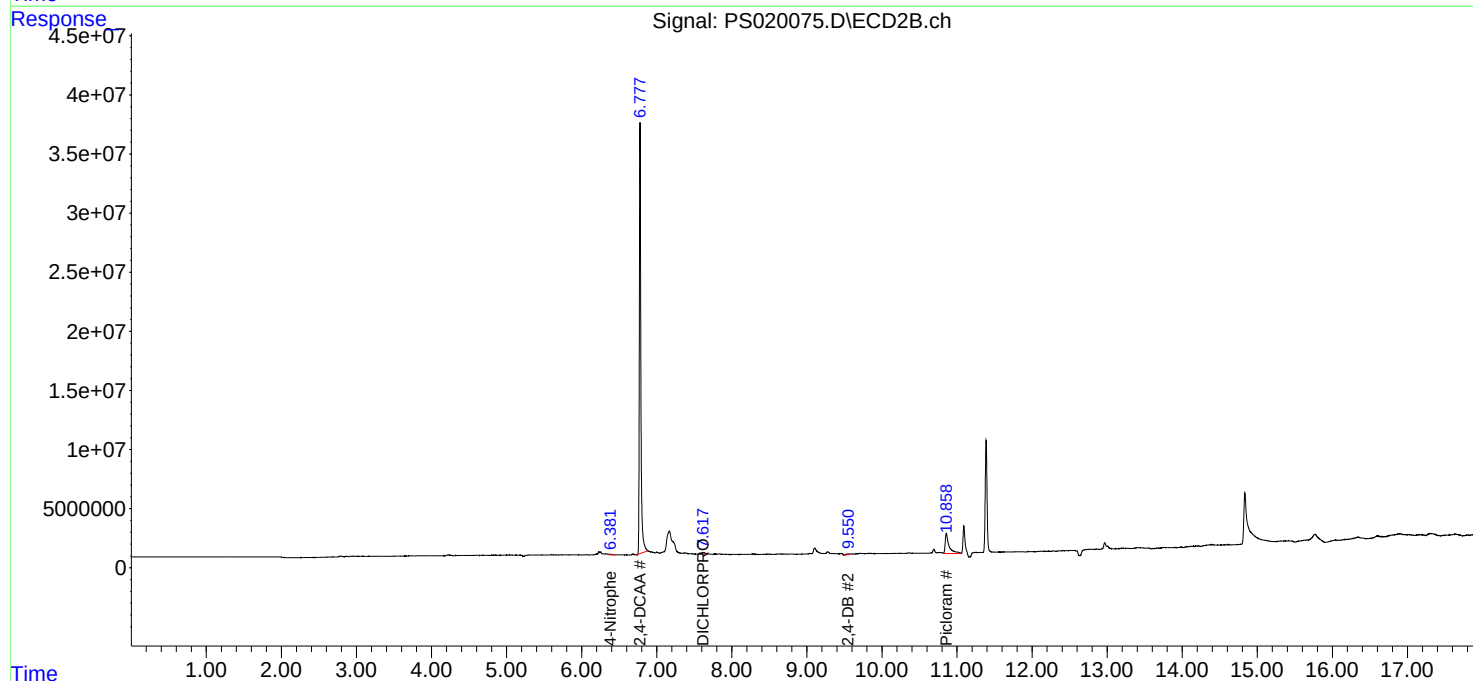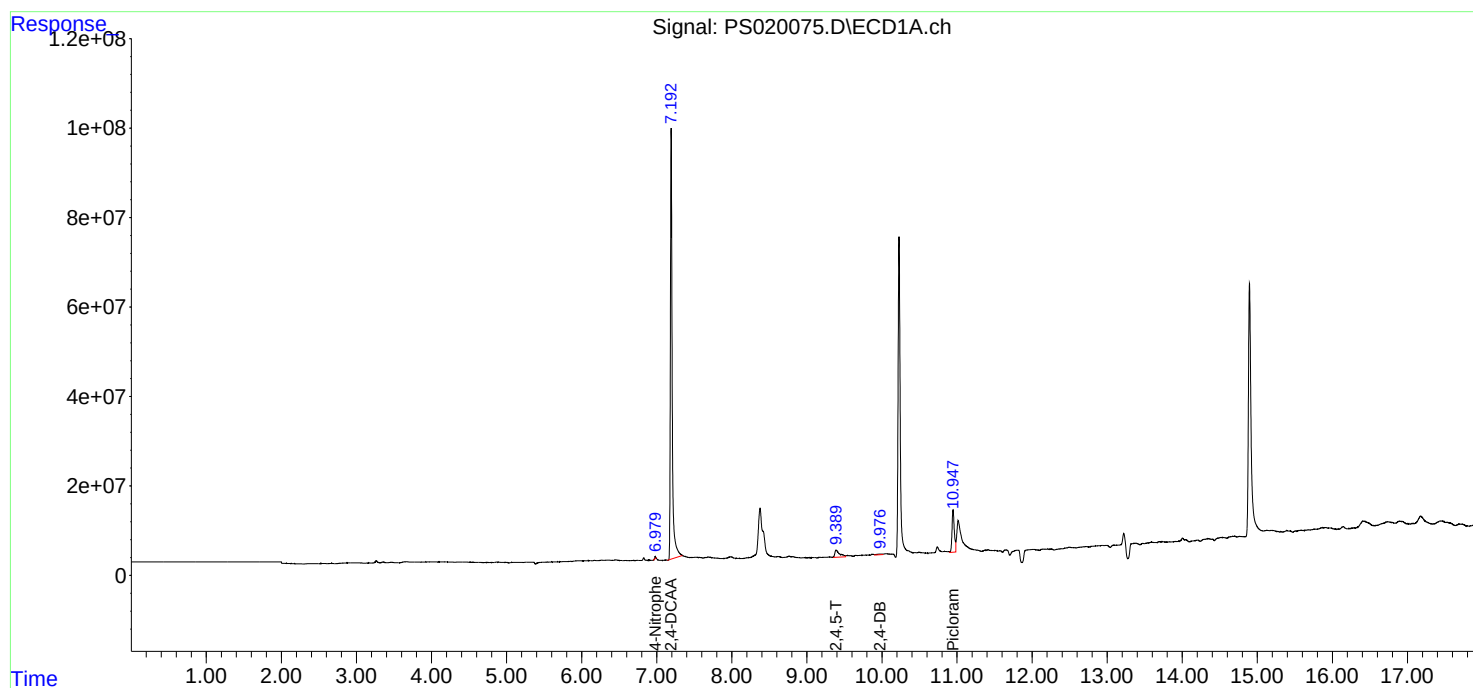


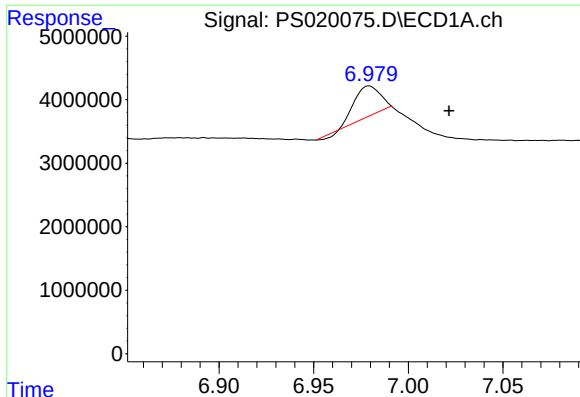

#3 4-Nitrophenol


R.T.: 6.980 min
Delta R.T.: -0.042 min
Response: 4525851
Conc: 3.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

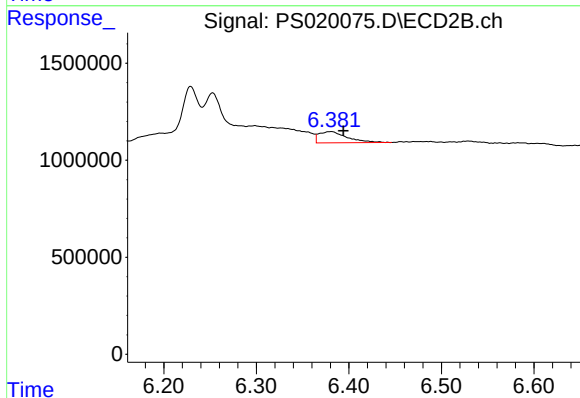


#3 4-Nitrophenol

R.T.: 6.381 min
Delta R.T.: -0.013 min
Response: 1221832
Conc: 2.53 ng/ml

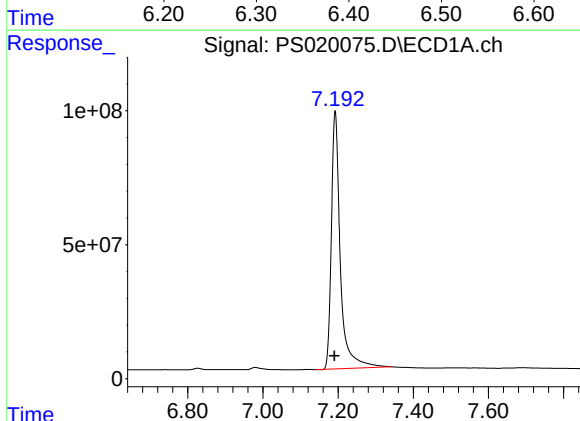


#4 2,4-DCAA

R.T.: 7.192 min
Delta R.T.: 0.002 min
Response: 1592741806
Conc: 480.34 ng/ml

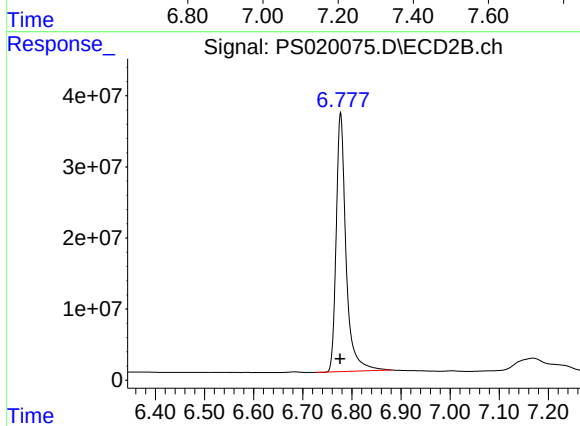

#4 2,4-DCAA


R.T.: 6.777 min
Delta R.T.: 0.001 min
Response: 507212206
Conc: 563.00 ng/ml

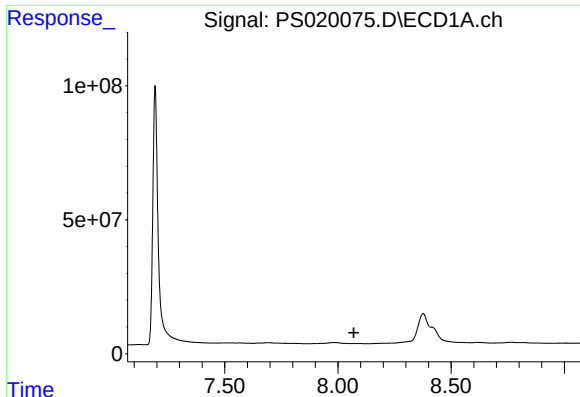

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

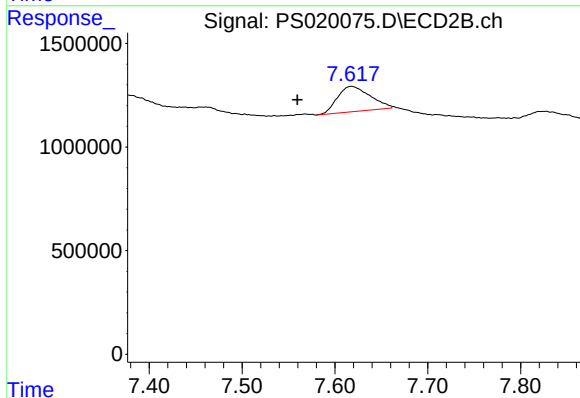


#8 DICHLORPROP

R.T.: 7.618 min
Delta R.T.: 0.058 min
Response: 3006968
Conc: 2.90 ng/ml

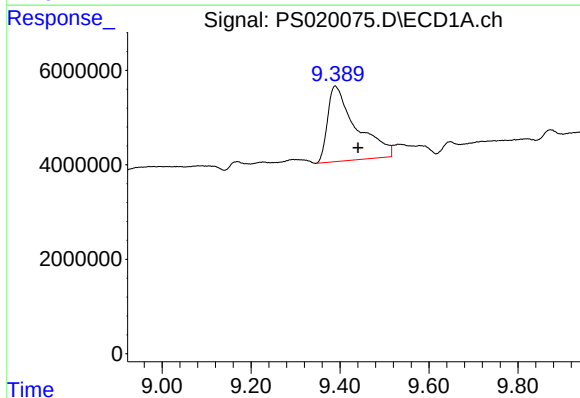


#12 2,4,5-T

R.T.: 9.389 min
Delta R.T.: -0.051 min
Response: 71224007
Conc: 3.30 ng/ml

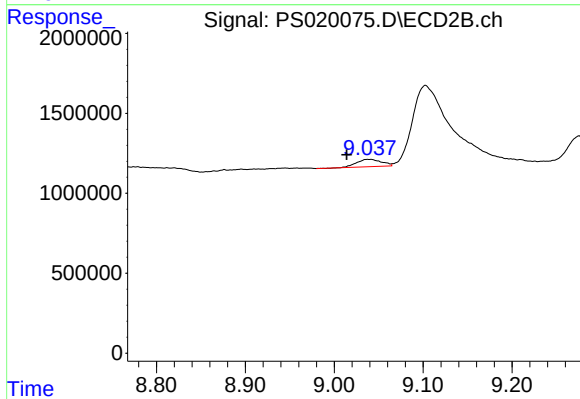

#12 2,4,5-T


R.T.: 9.041 min
Delta R.T.: 0.026 min
Response: 889924
Conc: N.D.

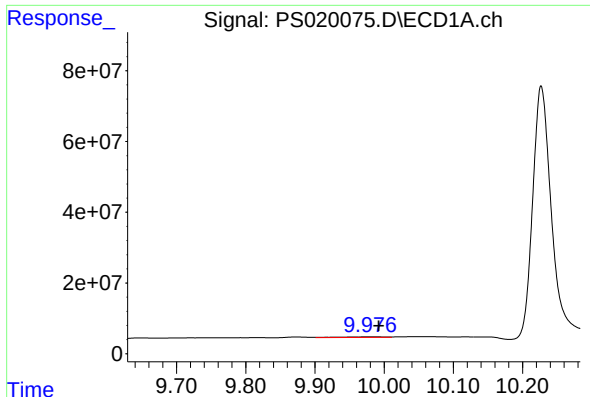

#13 2,4-DB


R.T.: 9.977 min
Delta R.T.: -0.015 min
Response: 8681642
Conc: 1.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

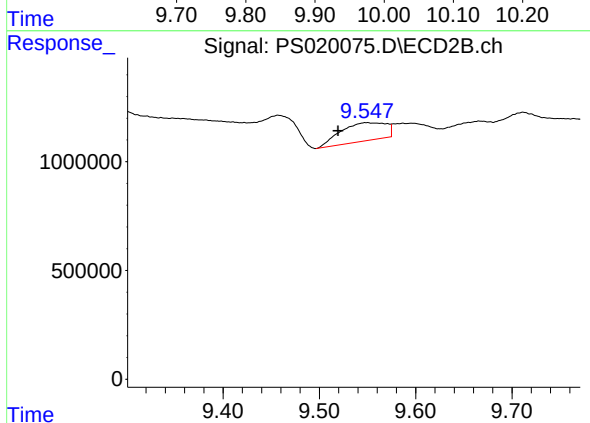


#13 2,4-DB

R.T.: 9.549 min
Delta R.T.: 0.030 min
Response: 2760108
Conc: 3.87 ng/ml

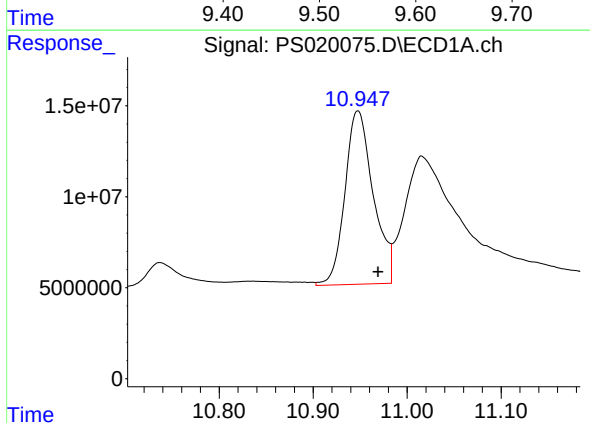

#15 Picloram

R.T.: 10.948 min
Delta R.T.: -0.021 min
Response: 199609597
Conc: 5.73 ng/ml

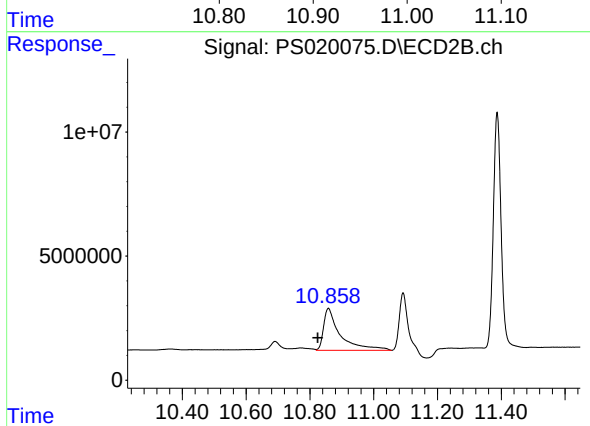

#15 Picloram

R.T.: 10.858 min
Delta R.T.: 0.034 min
Response: 61257151
Conc: 7.97 ng/ml