

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072722\
 Data File : PS020085.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2022 22:39
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 02:08:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072022.M
 Quant Title : 8080.M
 QLast Update : Wed Jul 20 17:52:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.192	6.776	1600.2E6	524.1E6	482.594	581.773
Target Compounds							
1) T	Dalapon	3.045	0.000	2991437	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.452f	5.910f	11131341	539250	2.562	<MDL #
3) T	4-Nitroph...	6.979f	6.378	4601377	1440527	3.201	2.982
5) T	DICAMBA	0.000	7.003f	0	1825170	N.D.	<MDL
6) T	MCP	0.000	7.003f	0	1825170	N.D.	<MDL
7) T	MCPA	7.683	0.000	9507520	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.613f	0	3444255	N.D.	3.320
9) T	2,4-D	0.000	7.822	0	985151	N.D.	<MDL
10) T	Pentachlo...	8.628	8.278	2613808	1904488	<MDL	<MDL #
11) T	2,4,5-TP ...	9.222f	8.605	10037561	1030801	<MDL	<MDL #
12) T	2,4,5-T	9.400f	9.035	8336184	2121476	<MDL	<MDL #
13) T	2,4-DB	9.985	9.552	14112222	3487340	3.240	4.886 #
14) T	DINOSEB	11.107	9.849	17997727	942421	1.001	<MDL #
15) T	Picloram	10.945	10.865f	280.2E6	19612895	8.044	2.552 #
16) T	DCPA	11.420	10.772	-169658	13244259	N.D.	1.833



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072722\
Data File : PS020085.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2022 22:39
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 02:08:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072022.M
Quant Title : 8080.M
QLast Update : Wed Jul 20 17:52:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

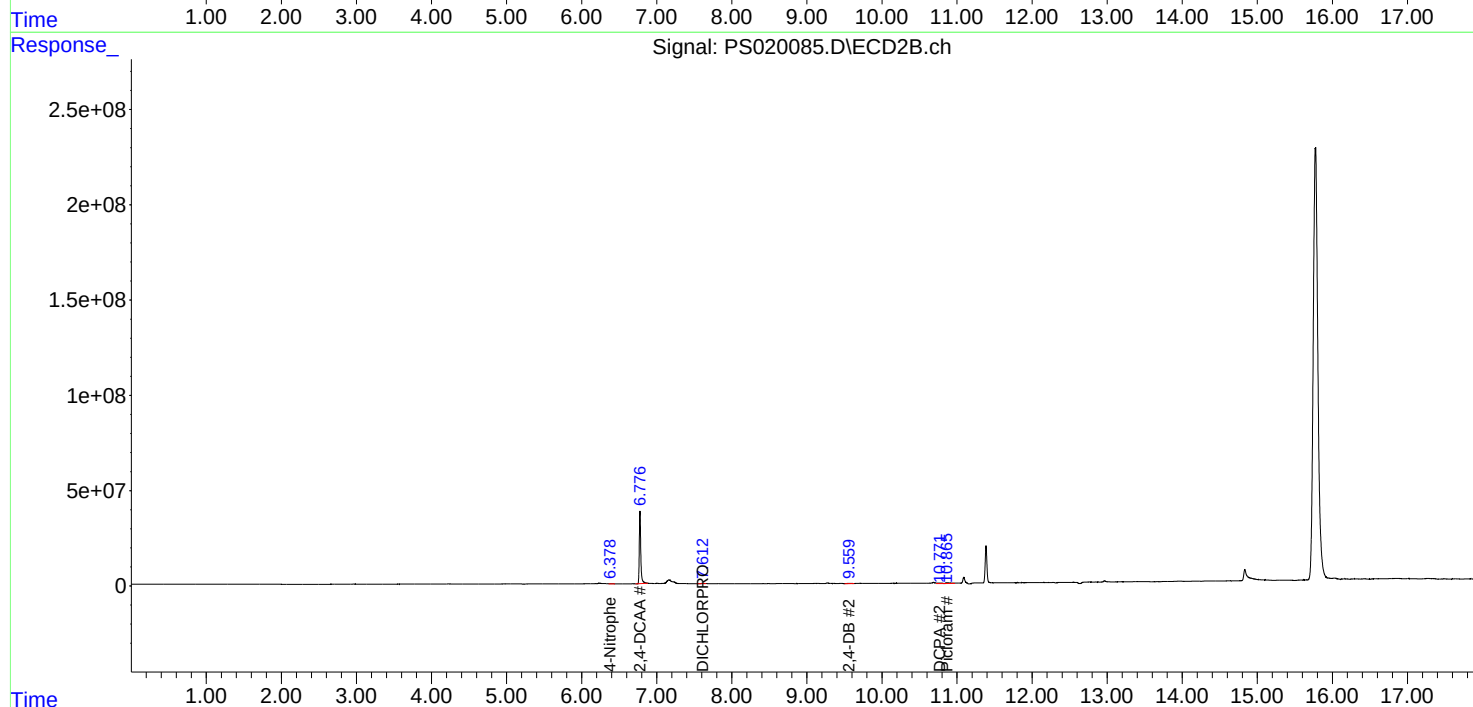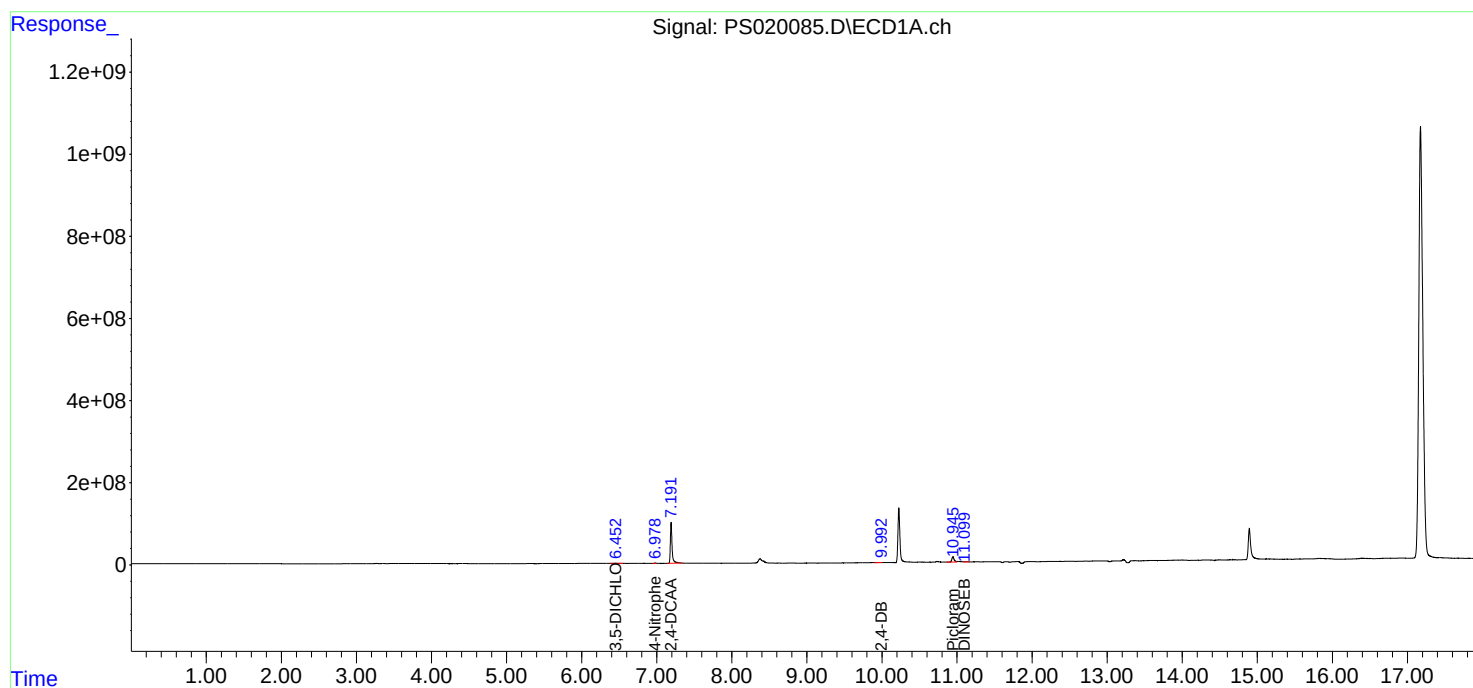


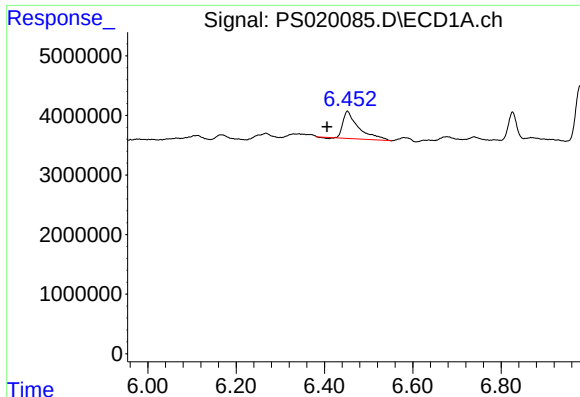

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.452 min
Delta R.T.: 0.046 min
Response: 11131341
Conc: 2.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

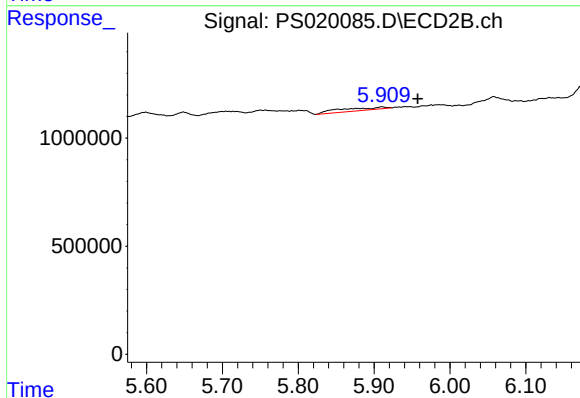


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.910 min
Delta R.T.: -0.047 min
Response: 539250
Conc: N.D.

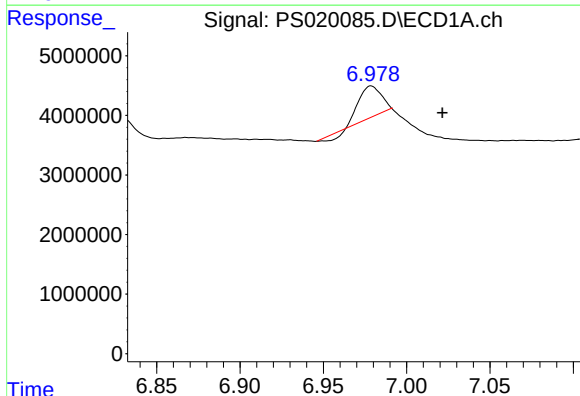


#3 4-Nitrophenol

R.T.: 6.979 min
Delta R.T.: -0.043 min
Response: 4601377
Conc: 3.20 ng/ml

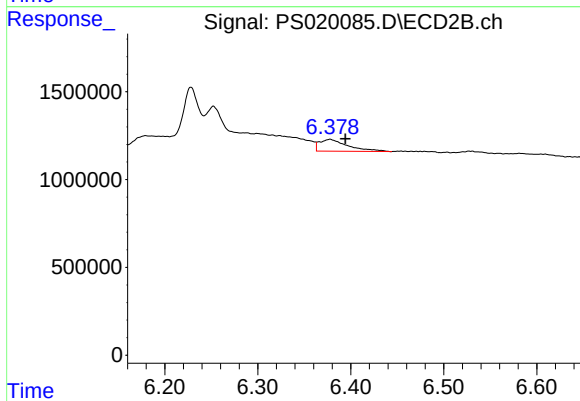

#3 4-Nitrophenol


R.T.: 6.378 min
Delta R.T.: -0.016 min
Response: 1440527
Conc: 2.98 ng/ml

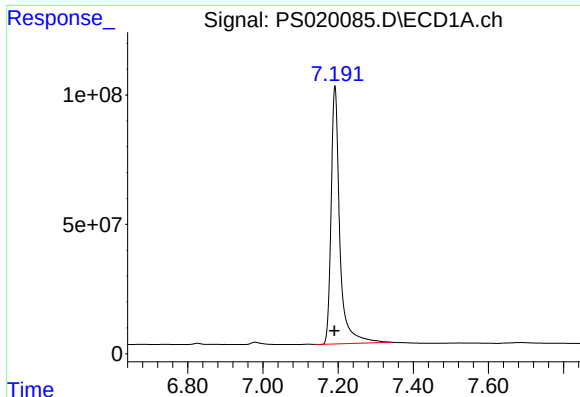

#4 2,4-DCAA


R.T.: 7.192 min
Delta R.T.: 0.001 min
Response: 1600207673
Conc: 482.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

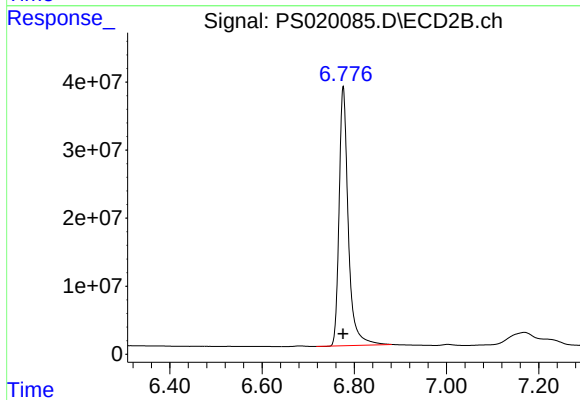


#4 2,4-DCAA

R.T.: 6.776 min
Delta R.T.: 0.000 min
Response: 524121563
Conc: 581.77 ng/ml

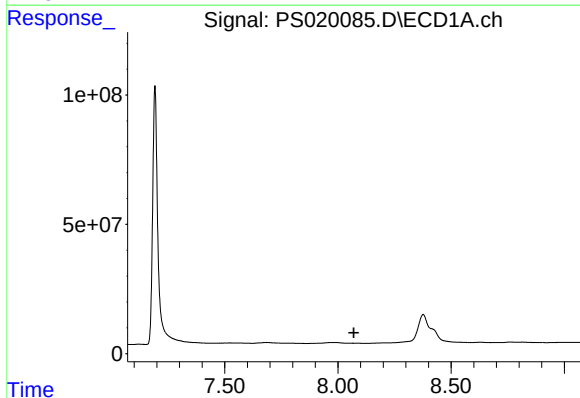


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.070 min
Response: 0
Conc: N.D.

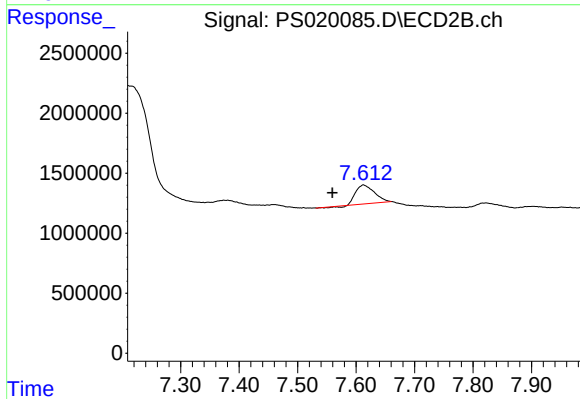

#8 DICHLORPROP


R.T.: 7.613 min
Delta R.T.: 0.053 min
Response: 3444255
Conc: 3.32 ng/ml

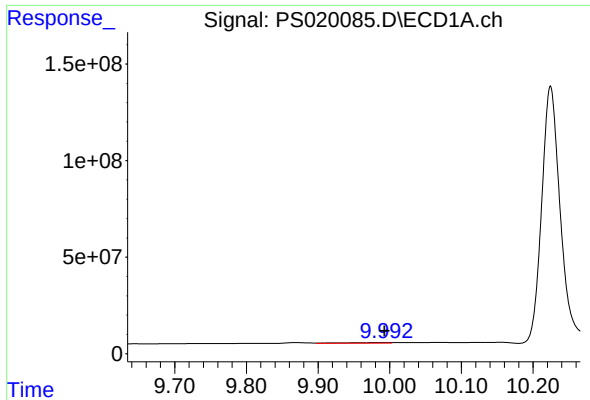

#13 2,4-DB


R.T.: 9.985 min
Delta R.T.: -0.007 min
Response: 14112222
Conc: 3.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

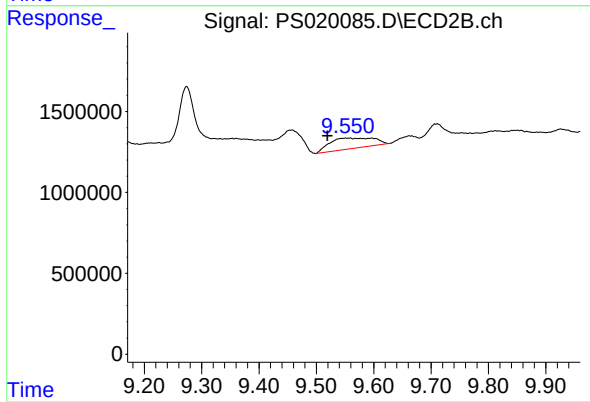


#13 2,4-DB

R.T.: 9.552 min
Delta R.T.: 0.032 min
Response: 3487340
Conc: 4.89 ng/ml

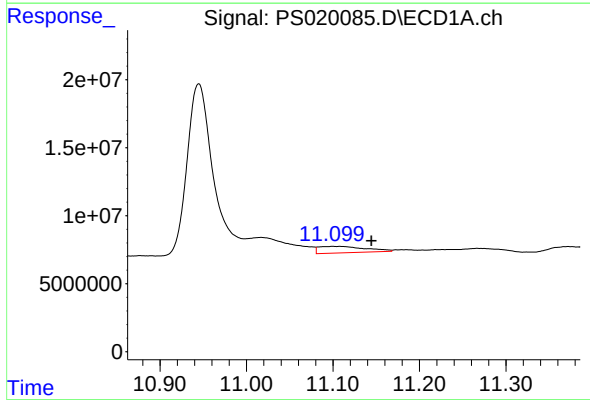


#14 DINOSEB

R.T.: 11.107 min
Delta R.T.: -0.037 min
Response: 17997727
Conc: 1.00 ng/ml

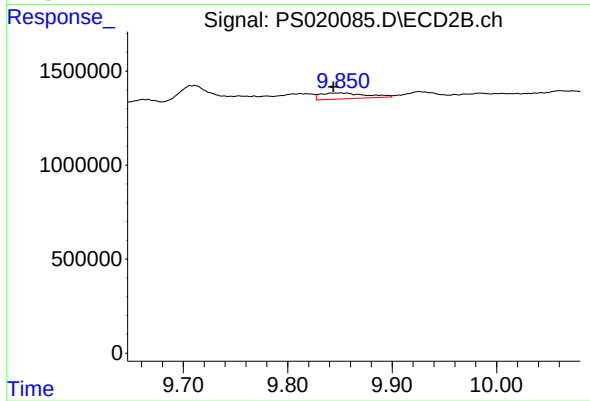

#14 DINOSEB


R.T.: 9.849 min
Delta R.T.: 0.005 min
Response: 942421
Conc: N.D.

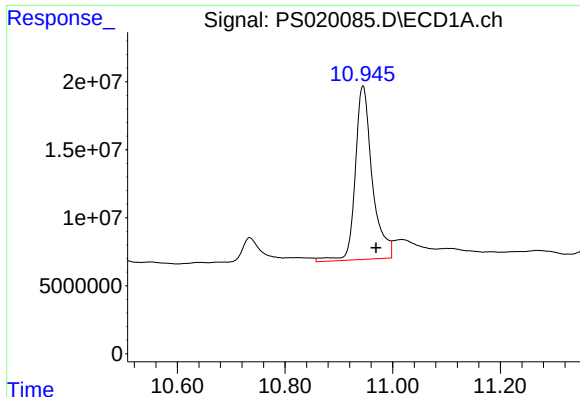

#15 Picloram


R.T.: 10.945 min
Delta R.T.: -0.024 min
Response: 280198955
Conc: 8.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

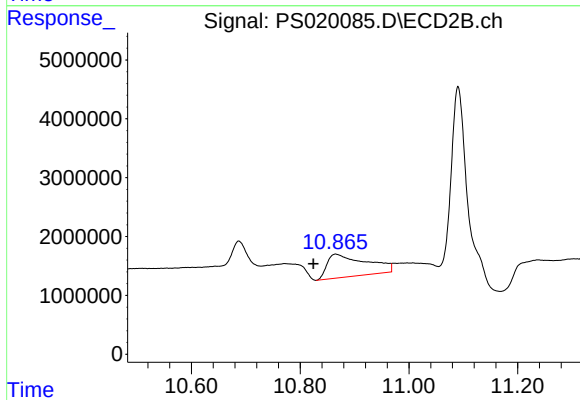


#15 Picloram

R.T.: 10.865 min
Delta R.T.: 0.041 min
Response: 19612895
Conc: 2.55 ng/ml

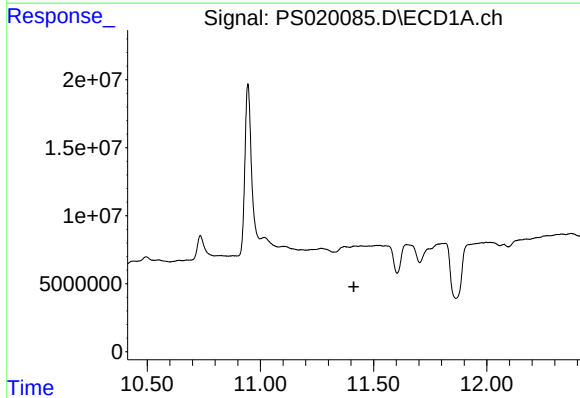

#16 DCPA

R.T.: 11.420 min
Delta R.T.: 0.007 min
Response: -169658
Conc: N.D.

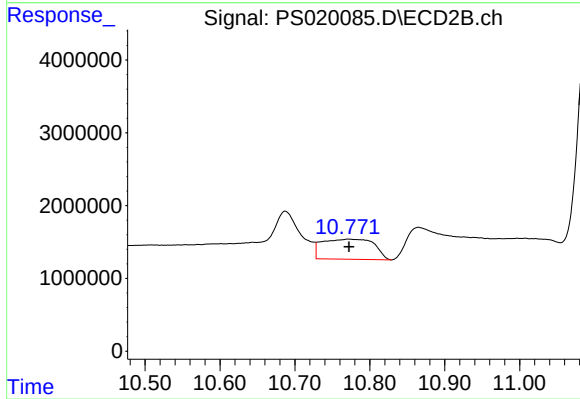

#16 DCPA

R.T.: 10.772 min
Delta R.T.: 0.000 min
Response: 13244259
Conc: 1.83 ng/ml