

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072822\
 Data File : PS020109.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2022 19:09
 Operator : AJ\MA
 Sample : N3839-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FIELD-DUPLICATE-01

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 08/02/2022
 Supervised By :mohammad ahmed 08/02/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 22:12:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072022.M
 Quant Title : 8080.M
 QLast Update : Wed Jul 20 17:52:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.189	6.774	548.4E6	196.1E6	165.392m	217.673 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072822\
Data File : PS020109.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2022 19:09
Operator : AJ\MA
Sample : N3839-04
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
FIELD-DUPLICATE-01


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 08/02/2022
Supervised By :mohammad ahmed 08/02/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 22:12:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072022.M
Quant Title : 8080.M
QLast Update : Wed Jul 20 17:52:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

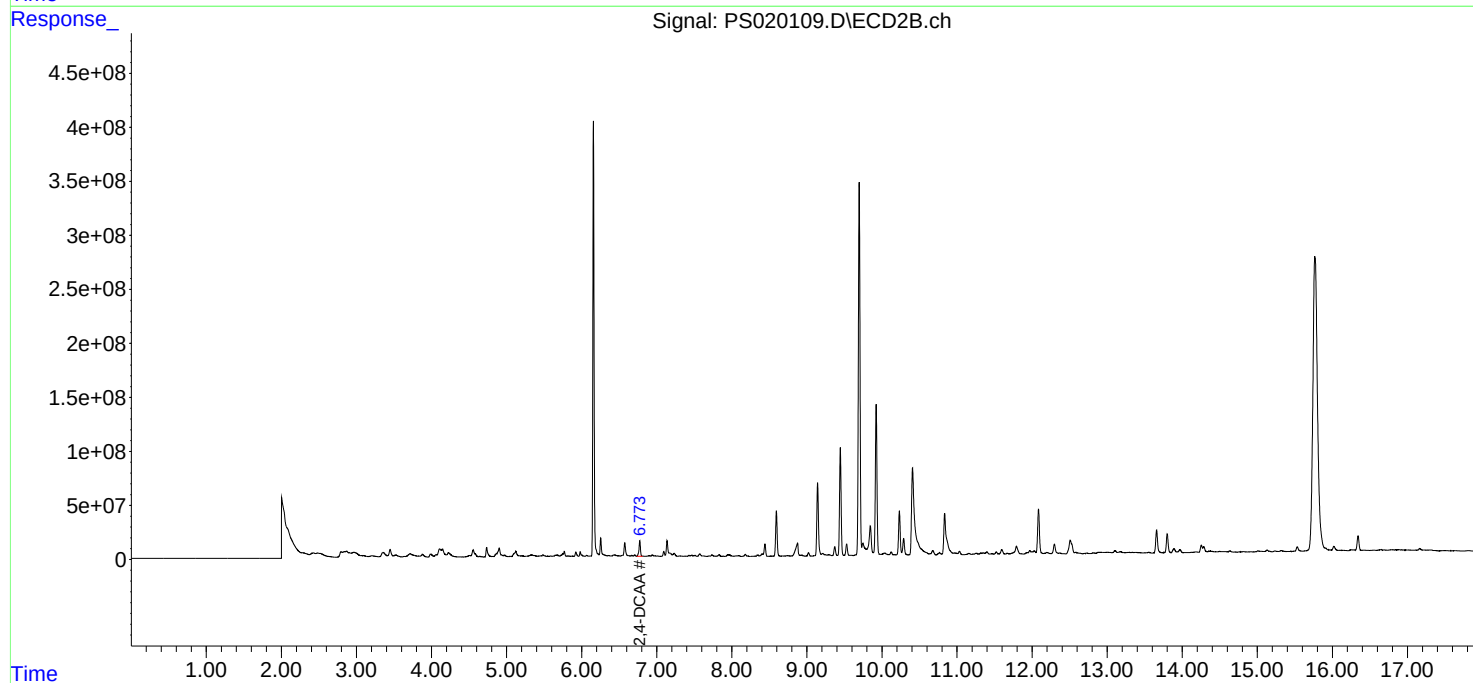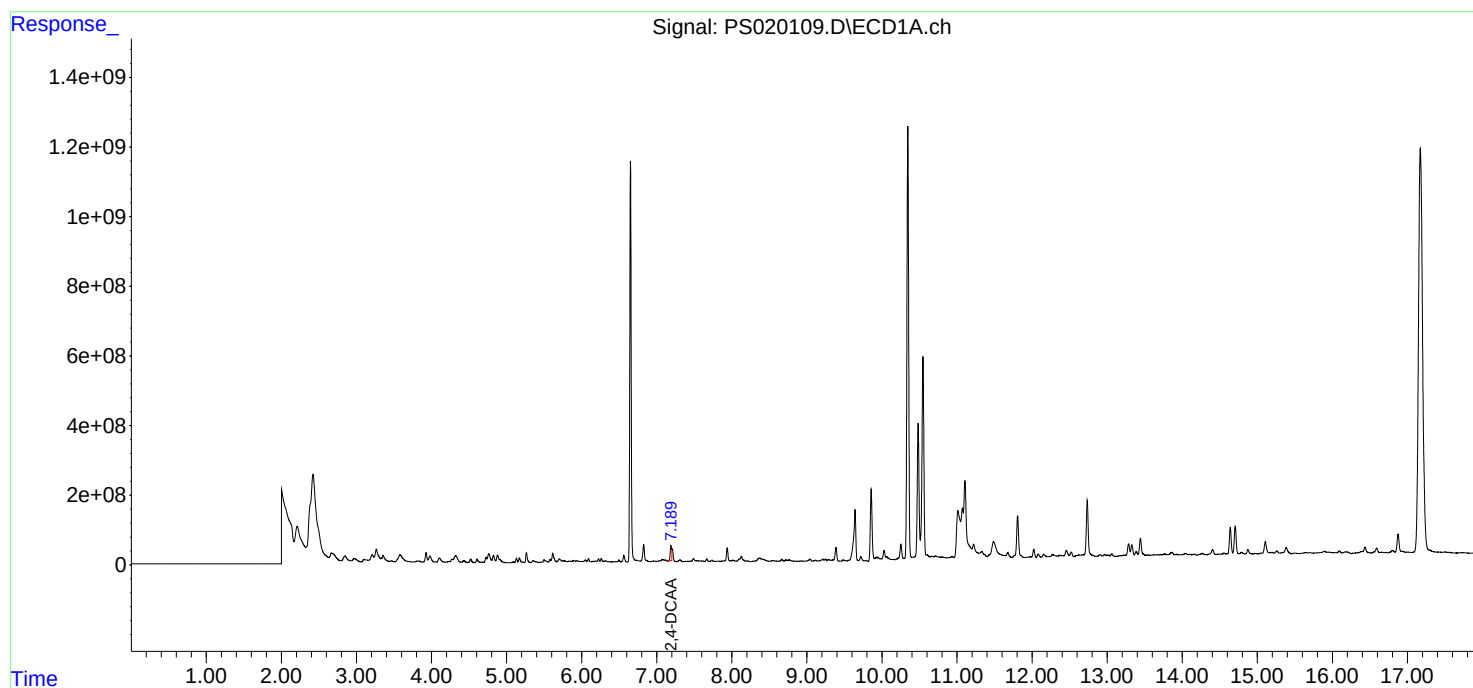

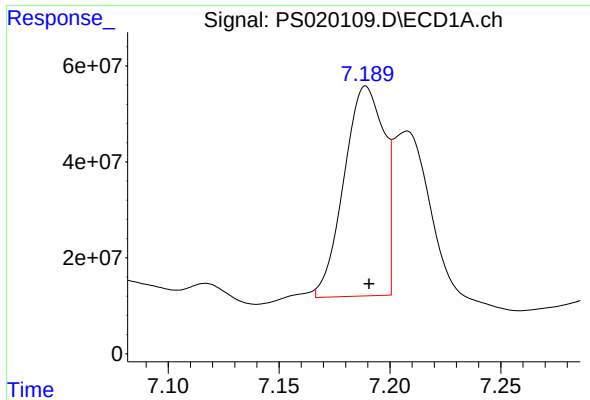


#4 2,4-DCAA

R.T.: 7.189 min
Delta R.T.: -0.002 min
Response: 548416130
Conc: 165.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
FIELD-DUPLICATE-01

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 08/02/2022
Supervised By :mohammad ahmed 08/02/2022

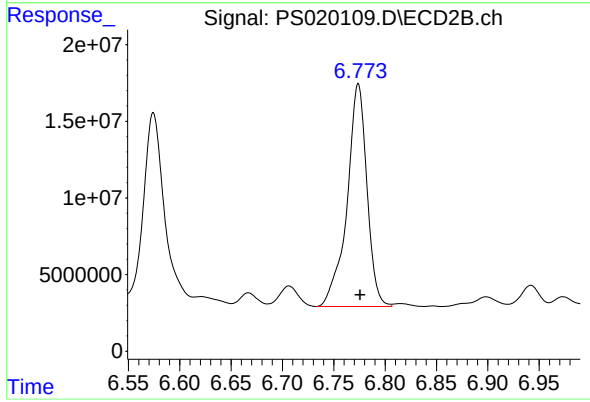

#4 2,4-DCAA

R.T.: 6.774 min
Delta R.T.: -0.002 min
Response: 196102458
Conc: 217.67 ng/ml