

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072920\
 Data File : PS011477.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2020 11:25
 Operator : DD\AJ
 Sample : L3434-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
ClientSampleId :
 11986

Manual Integrations
APPROVED
 Ankita
 7/30/2020 9:50:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 12:28:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.226	6.918	246.7E6	169.9E6	254.194m	301.709

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072920\
 Data File : PS011477.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2020 11:25
 Operator : DD\AJ
 Sample : L3434-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1



Instrument :
 ECD_S
 ClientSampleId :
 11986


Manual Integrations
 APPROVED

Ankita
 7/30/2020 9:50:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 12:28:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

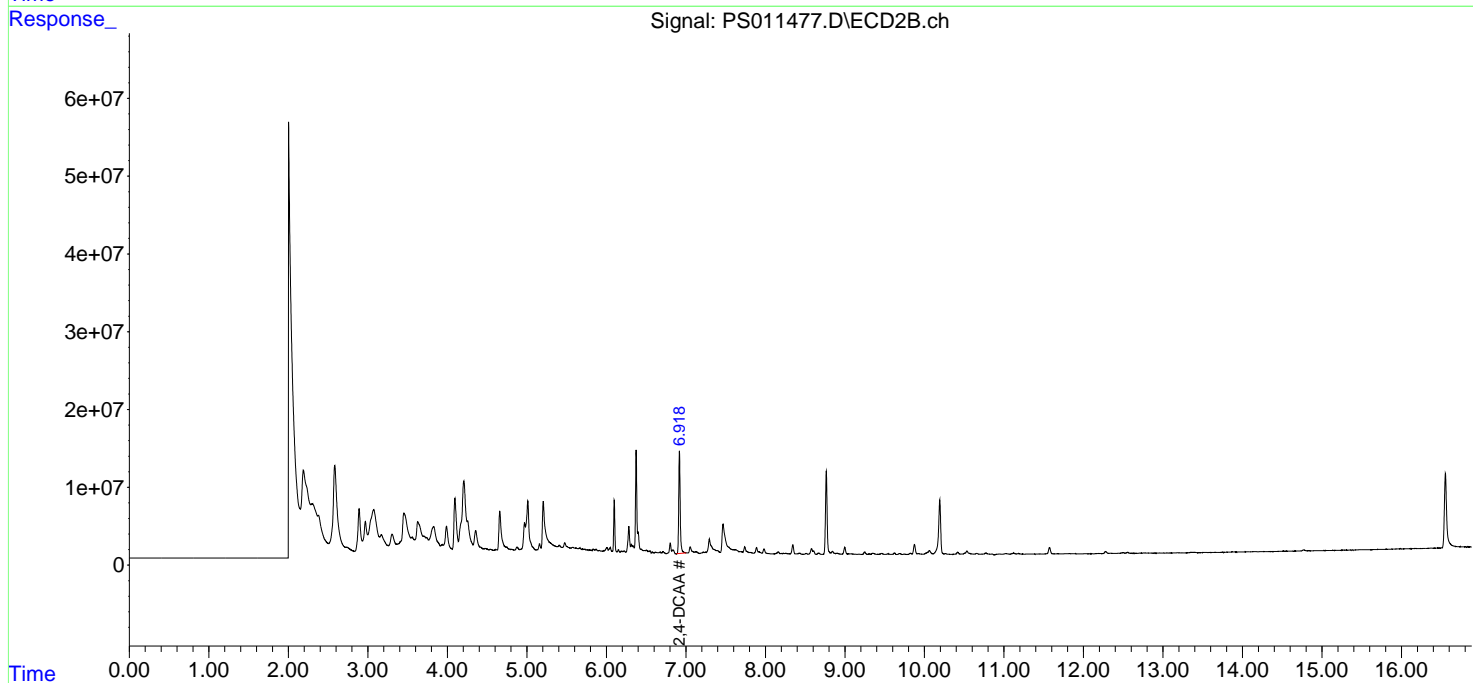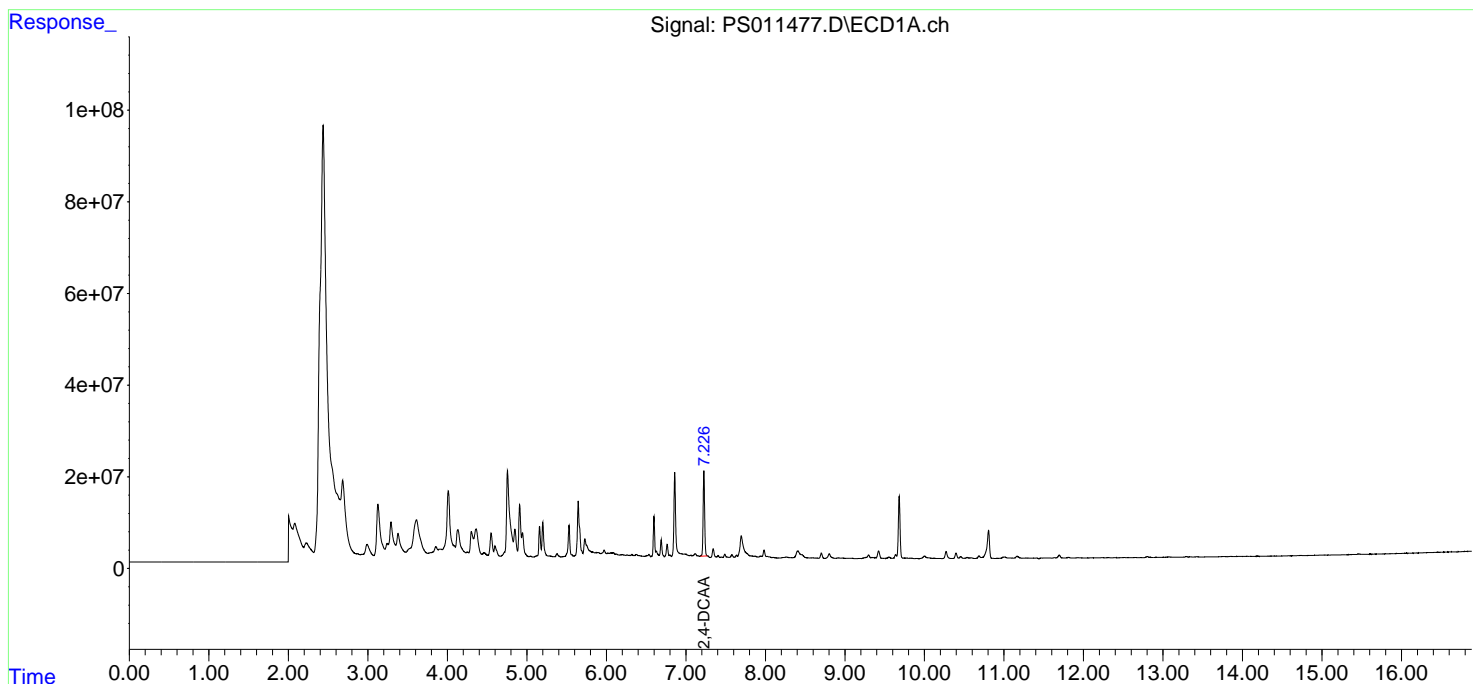

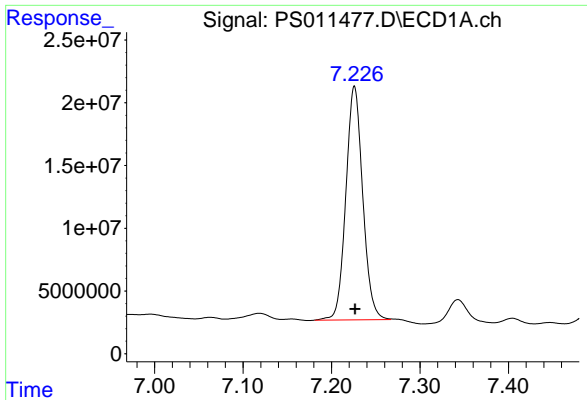


#4 2,4-DCAA

R.T.: 7.226 min
Delta R.T.: 0.000 min
Response: 246653738
Conc: 254.19 ng/ml m

Instrument :
ECD_S
ClientSampled :
11986

Manual Integrations
APPROVED
Ankita
7/30/2020 9:50:03 AM

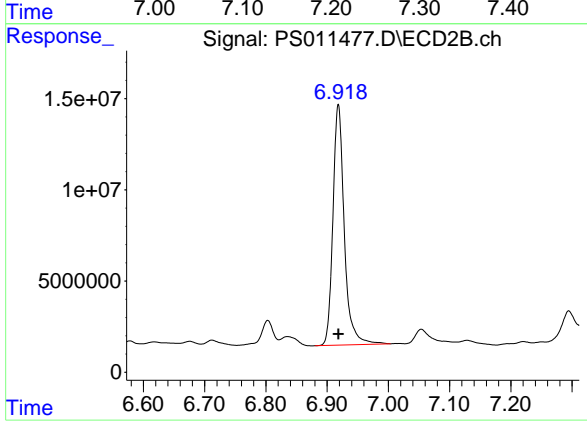

#4 2,4-DCAA

R.T.: 6.918 min
Delta R.T.: 0.000 min
Response: 169869067
Conc: 301.71 ng/ml