

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS072921\  
 Data File : PS016215.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 29 Jul 2021 09:45  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jul 30 02:22:12 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS063021.M  
 Quant Title : 8080.M  
 QLast Update : Wed Jun 30 00:31:48 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound | RT#1   | RT#2    | Resp#1     | Resp#2   | ng/ml   | ng/ml   |
|-----------------------------|----------|--------|---------|------------|----------|---------|---------|
| -----                       |          |        |         |            |          |         |         |
| System Monitoring Compounds |          |        |         |            |          |         |         |
| 4) S                        | 2,4-DCAA | 7.186  | 6.765   | 602.0E6    | 244.7E6  | 392.112 | 476.608 |
| Target Compounds            |          |        |         |            |          |         |         |
| 12) T                       | 2,4,5-T  | 0.000  | 9.068f  | 0 11315941 |          | N.D.    | 3.923   |
| 15) T                       | Picloram | 11.003 | 10.831  | 104.5E6    | 48229397 | 9.497   | 11.592  |
| 16) T                       | DCPA     | 0.000  | 10.831f | 0 48229397 |          | N.D.    | 11.215  |
| -----                       |          |        |         |            |          |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS072921\  
Data File : PS016215.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 29 Jul 2021 09:45  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jul 30 02:22:12 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS063021.M  
Quant Title : 8080.M  
QLast Update : Wed Jun 30 00:31:48 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

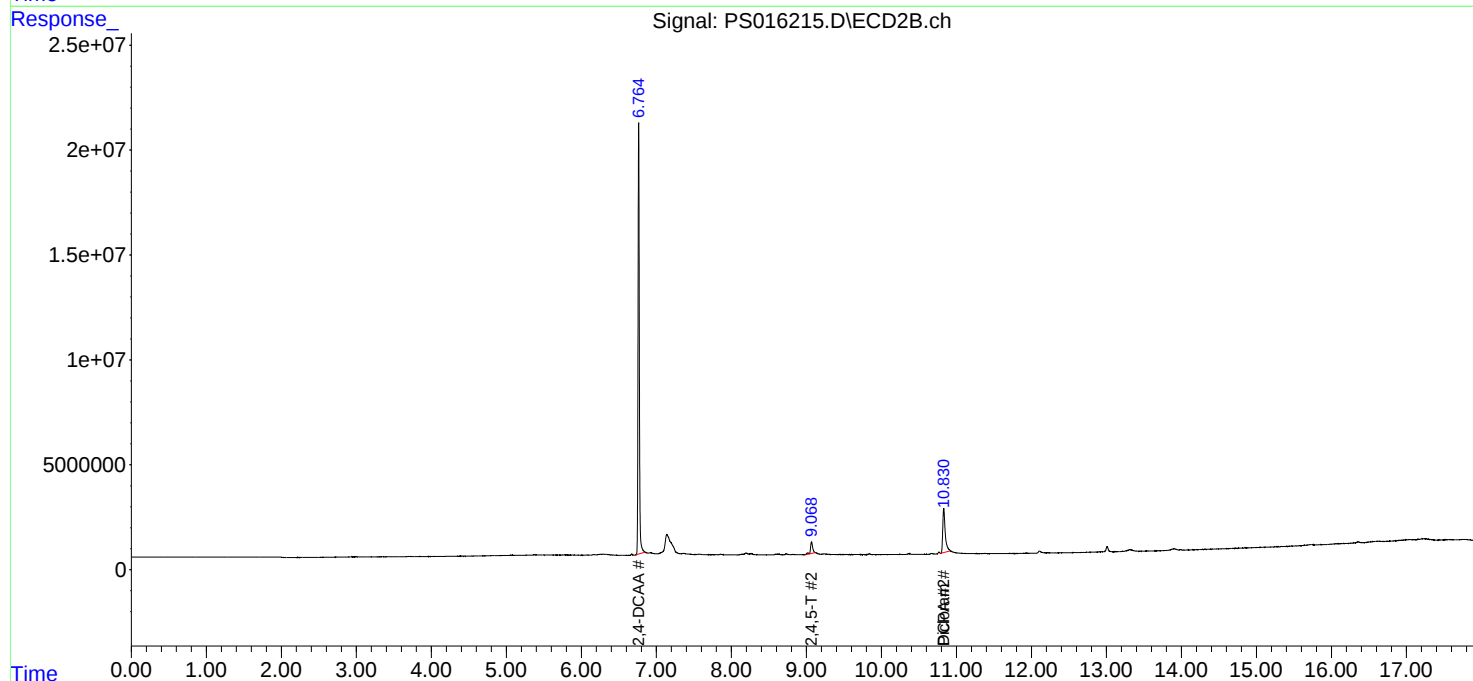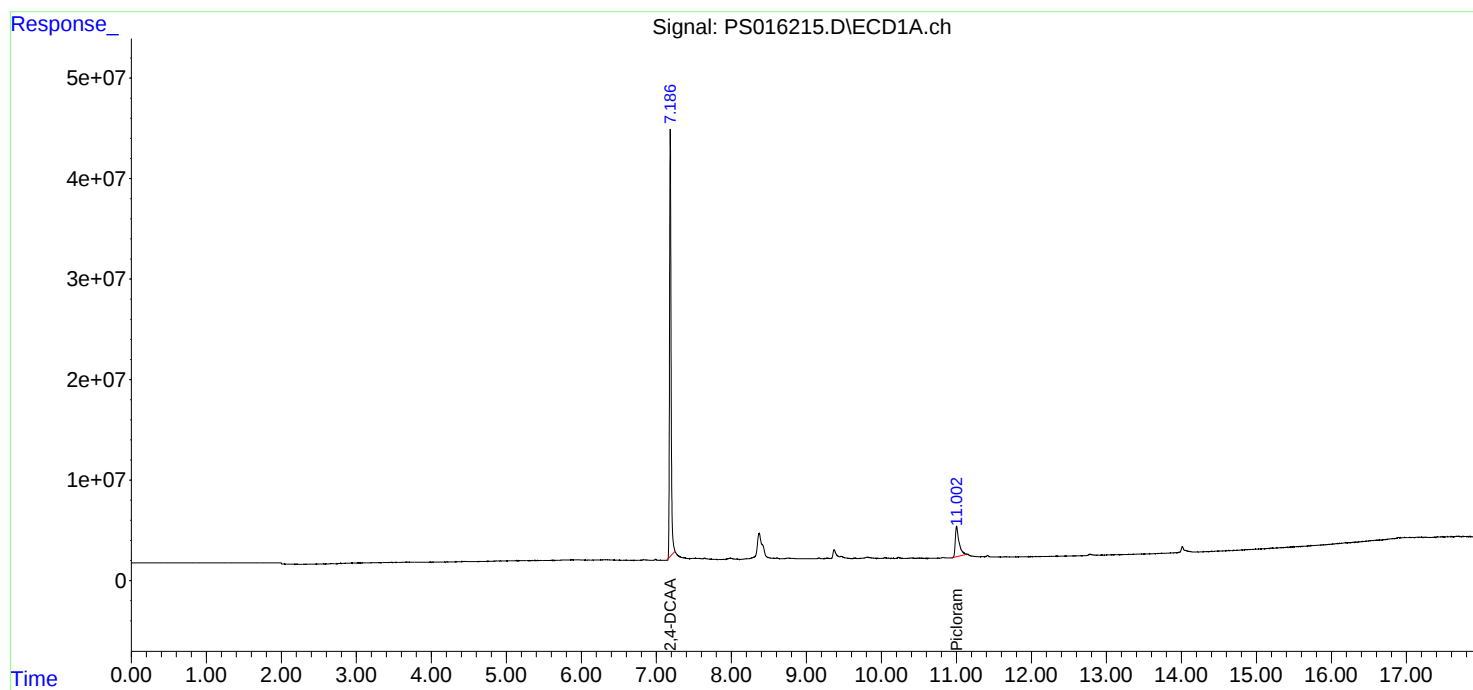


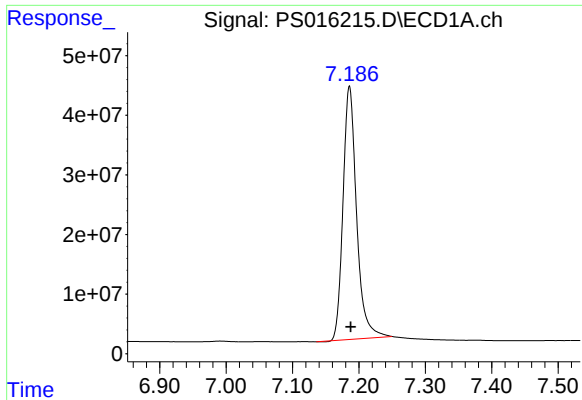

#4 2,4-DCAA


R.T.: 7.186 min  
Delta R.T.: -0.002 min  
Response: 601970789  
Conc: 392.11 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

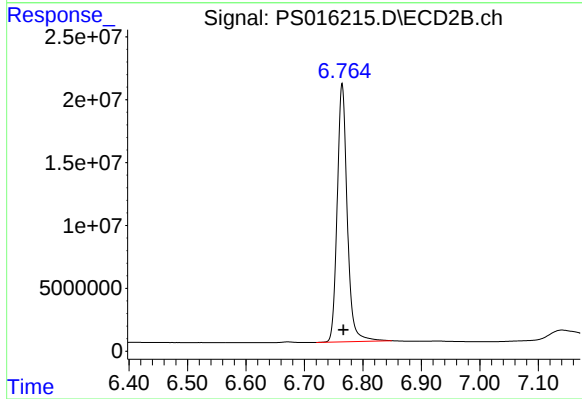


#4 2,4-DCAA

R.T.: 6.765 min  
Delta R.T.: -0.002 min  
Response: 244651275  
Conc: 476.61 ng/ml

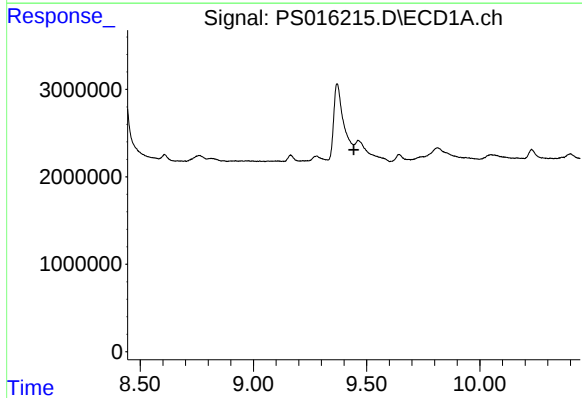


#12 2,4,5-T

R.T.: 0.000 min  
Exp R.T. : 9.443 min  
Response: 0  
Conc: N.D.

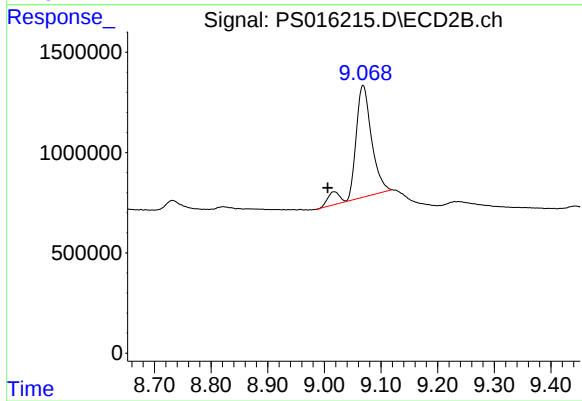

#12 2,4,5-T


R.T.: 9.068 min  
Delta R.T.: 0.062 min  
Response: 11315941  
Conc: 3.92 ng/ml

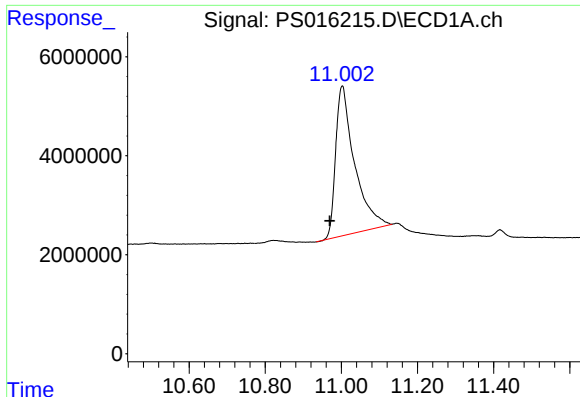

#15 Picloram


R.T.: 11.003 min  
Delta R.T.: 0.033 min  
Response: 104470256  
Conc: 9.50 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

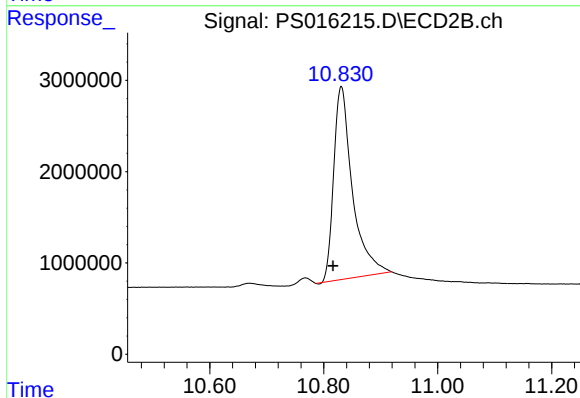


#15 Picloram

R.T.: 10.831 min  
Delta R.T.: 0.015 min  
Response: 48229397  
Conc: 11.59 ng/ml

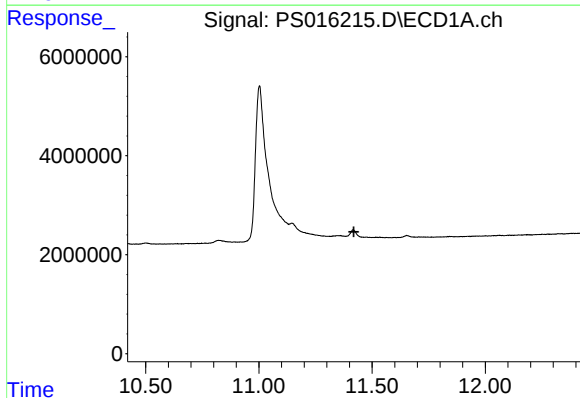

#16 DCPA

R.T.: 0.000 min  
Exp R.T. : 11.420 min  
Response: 0  
Conc: N.D.

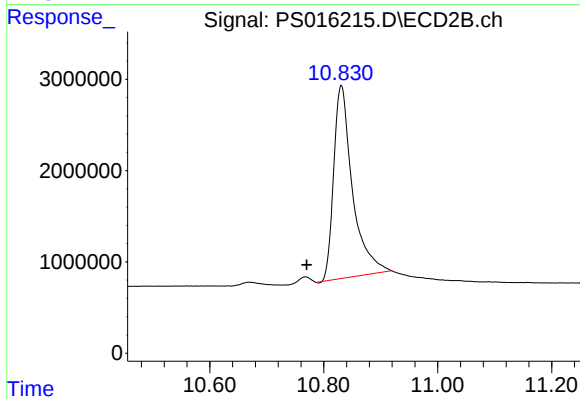

#16 DCPA

R.T.: 10.831 min  
Delta R.T.: 0.061 min  
Response: 48229397  
Conc: 11.22 ng/ml