

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072924\
 Data File : PS027247.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2024 02:17
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 06:56:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071224.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.194	7.751	1344.0E6	1184.5E6	531.498	510.823
Target Compounds							
1) T	Dalapon	0.000	2.705	0	426084	N.D.	<MDL
3) T	4-Nitroph...	6.992	0.000	5833232	0	3.639	N.D. #
5) T	DICAMBA	0.000	7.954	0	348241	N.D.	<MDL
6) T	MCP	7.613f	8.051	15208290	76769	1.981	<MDL #
8) T	DICHLORPROP	0.000	8.658	0	235016	N.D.	<MDL
9) T	2,4-D	0.000	9.037f	0	141115	N.D.	<MDL
10) T	Pentachlo...	8.622	0.000	2324534	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.152f	9.897	1592968	258376	<MDL	<MDL #
14) T	DINOSEB	11.219	11.259	2884411	3307852	<MDL	<MDL #
15) T	Picloram	11.075f	12.364	5510235	565893	<MDL	<MDL #
16) T	DCPA	11.534	12.288	1238036	2245083	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072924\
Data File : PS027247.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2024 02:17
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 06:56:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071224.M
Quant Title : 8080.M
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

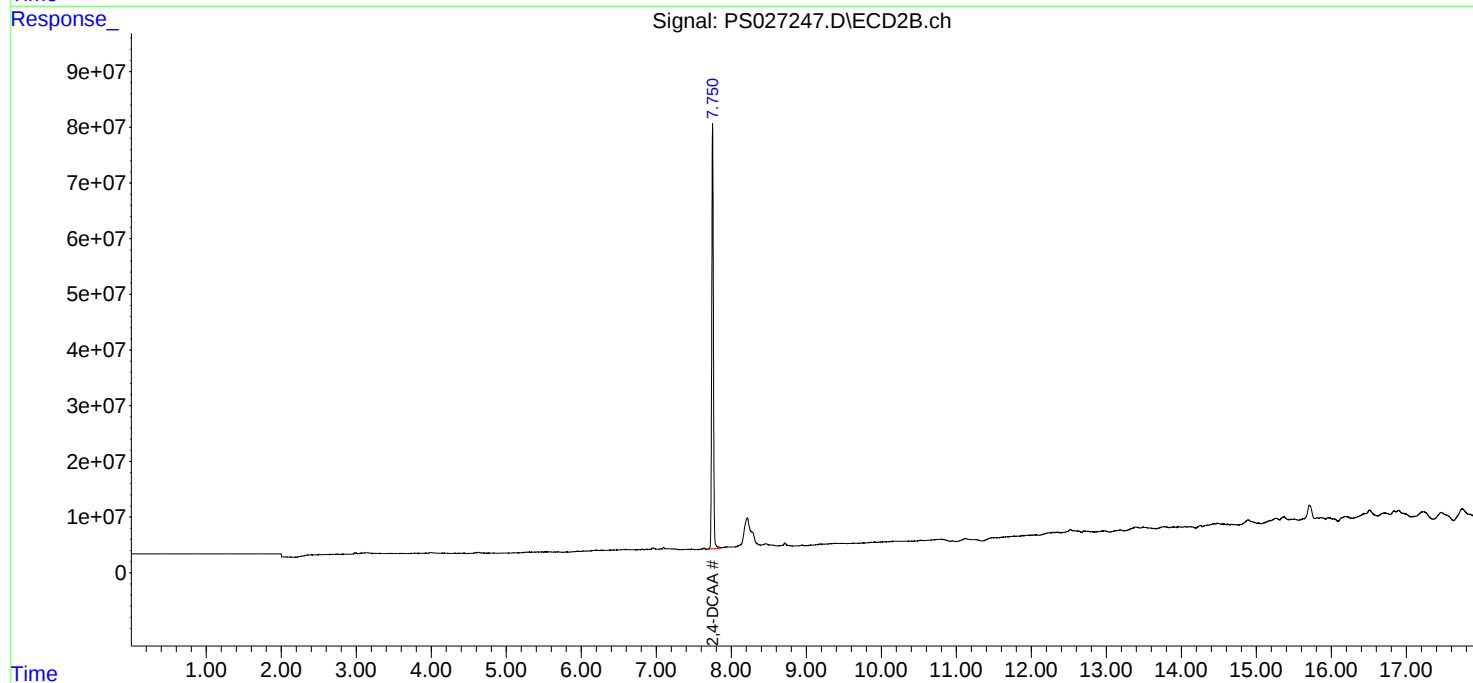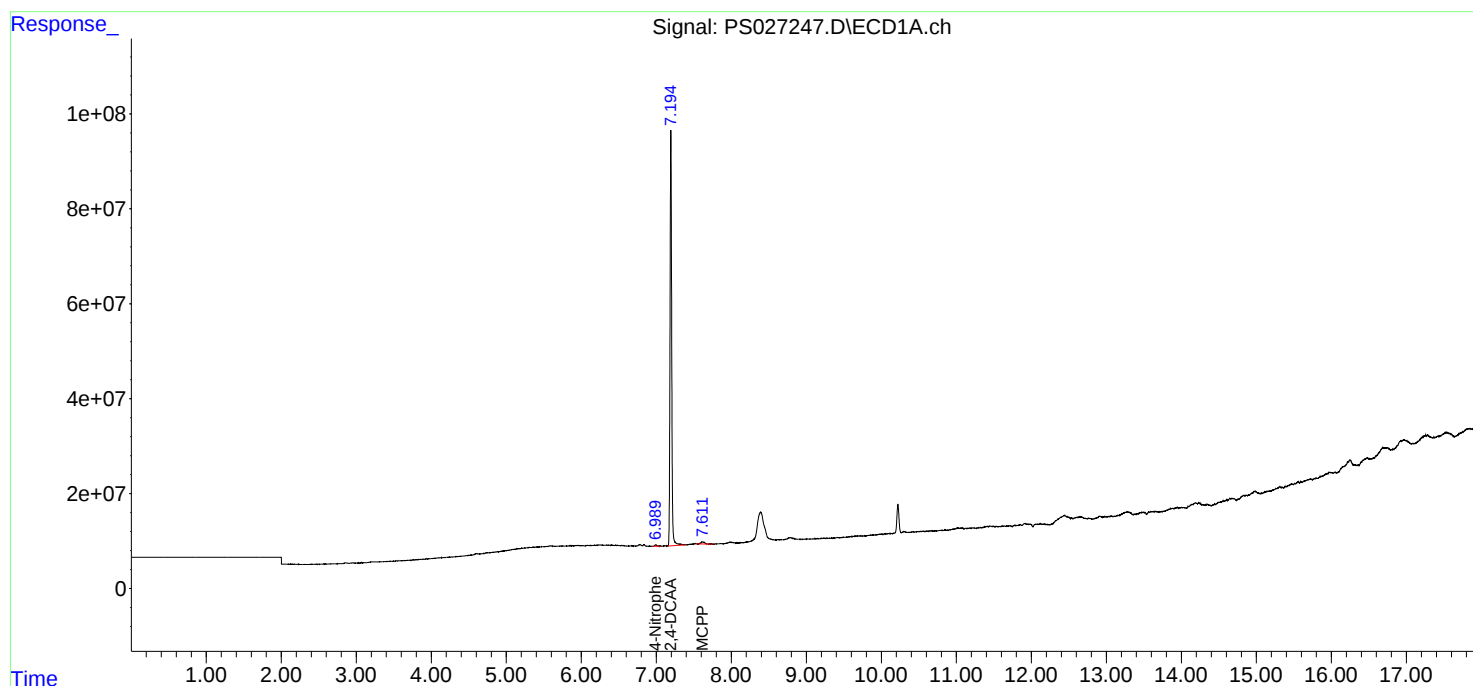


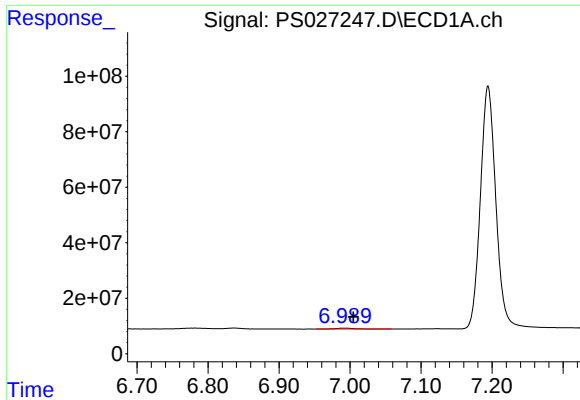

#3 4-Nitrophenol


R.T.: 6.992 min
Delta R.T.: -0.013 min
Response: 5833232
Conc: 3.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

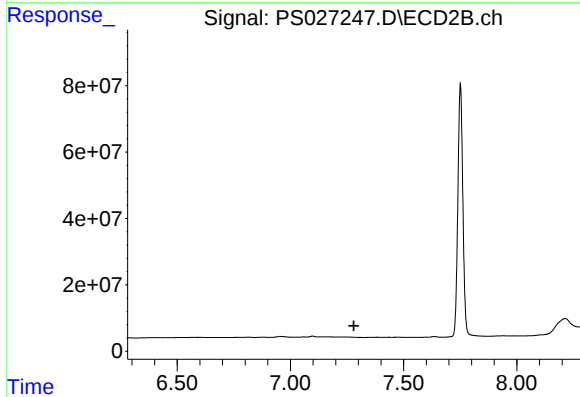


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 7.280 min
Response: 0
Conc: N.D.

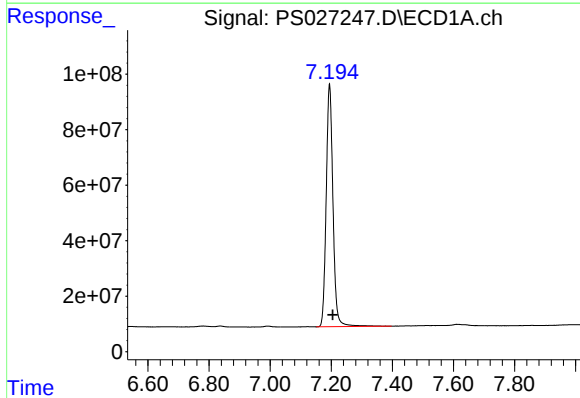


#4 2,4-DCAA

R.T.: 7.194 min
Delta R.T.: -0.011 min
Response: 1344033139
Conc: 531.50 ng/ml

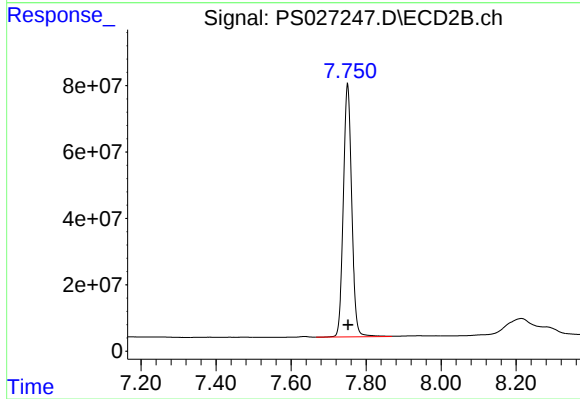

#4 2,4-DCAA


R.T.: 7.751 min
Delta R.T.: -0.002 min
Response: 1184457886
Conc: 510.82 ng/ml

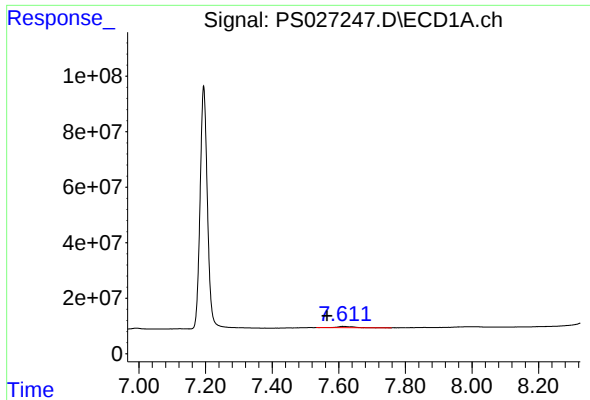

#6 MCPP

R.T.: 7.613 min
Delta R.T.: 0.049 min
Response: 15208290
Conc: 1.98 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

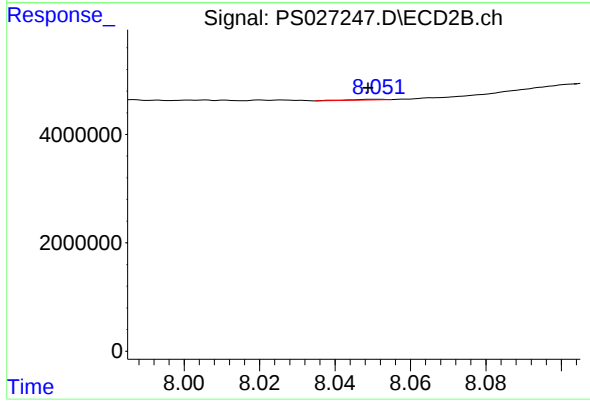

#6 MCPP

R.T.: 8.051 min
Delta R.T.: 0.003 min
Response: 76769
Conc: N.D.