

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073020\
 Data File : PS011496.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2020 08:10
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 13:49:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.482	0.000	102.6E6	0	76.685	N.D. #
5) T	DICAMBA	0.000	7.151	0	79882189	N.D.	34.884
6) T	MCPP	0.000	7.151	0	79882189	N.D.	41.865
8) T	DICHLORPROP	0.000	7.756	0	5912161	N.D.	9.822
12) T	2,4,5-T	9.417	0.000	11100390	0	2.200	N.D. #
15) T	Picloram	11.046	11.020	64243905	59011525	10.181	13.493 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073020\
Data File : PS011496.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2020 08:10
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 13:49:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
Quant Title : 8080.M
QLast Update : Mon Jul 13 16:10:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

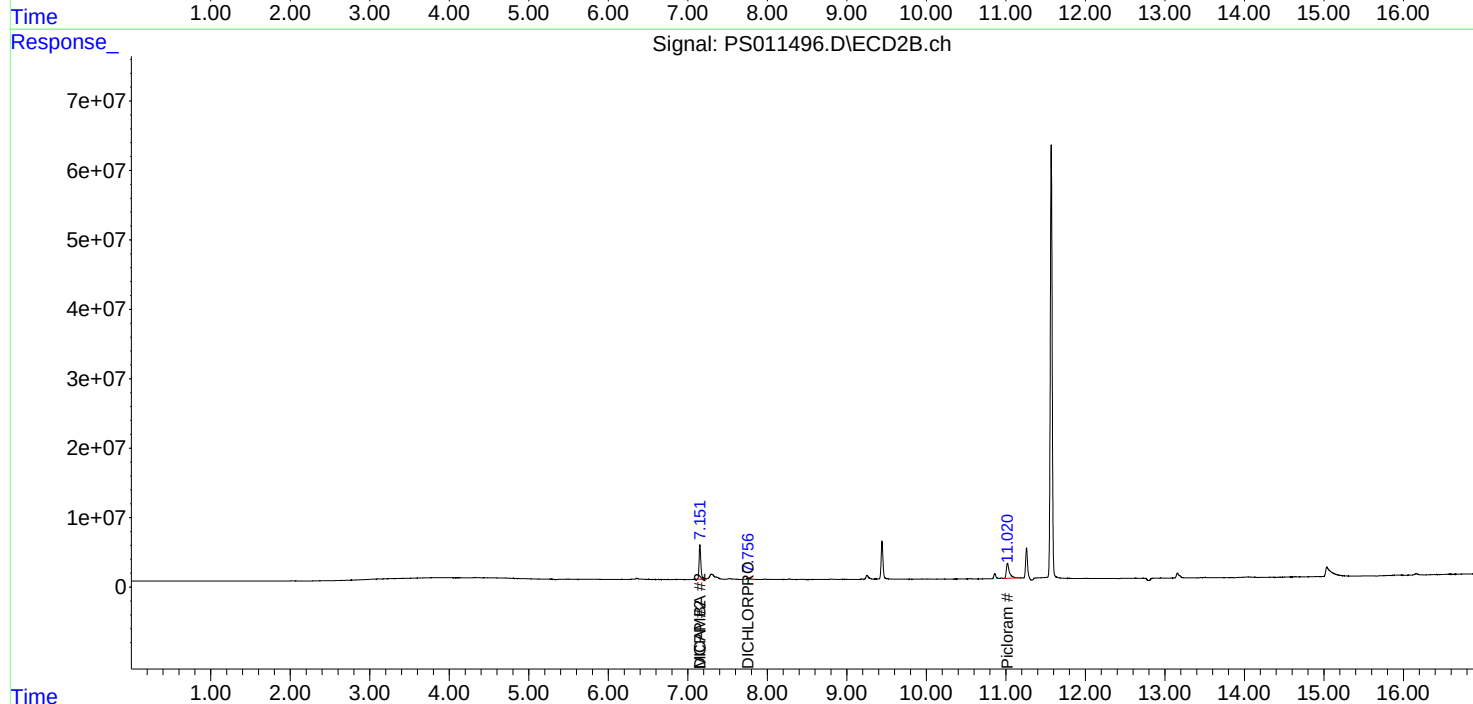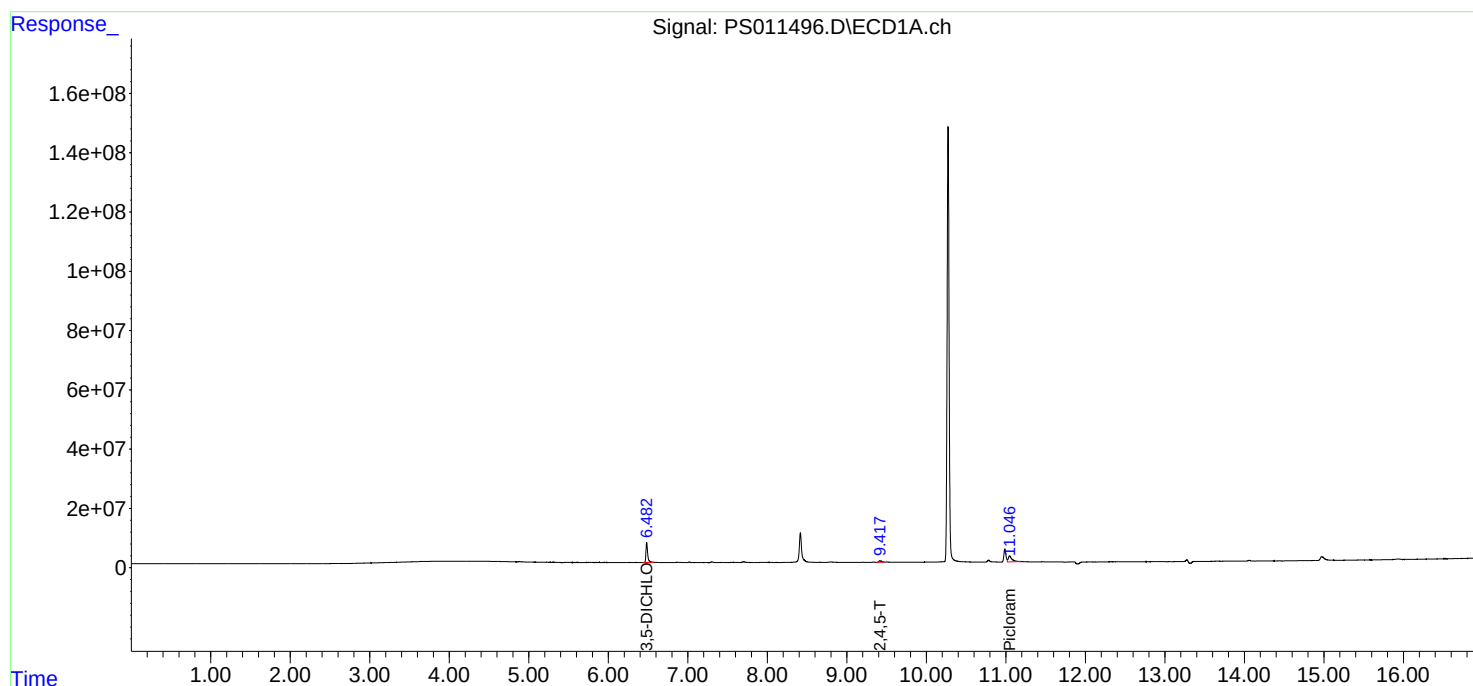


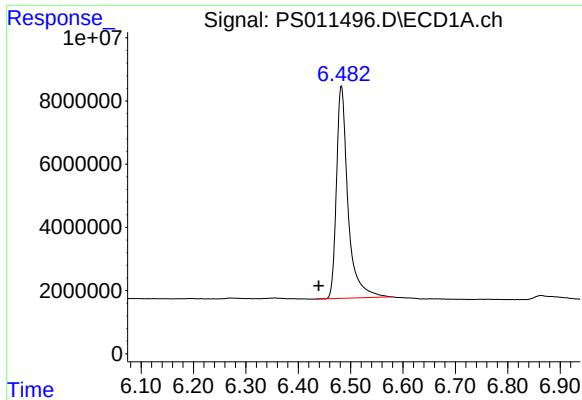

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.482 min
Delta R.T.: 0.043 min
Response: 102616494
Conc: 76.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

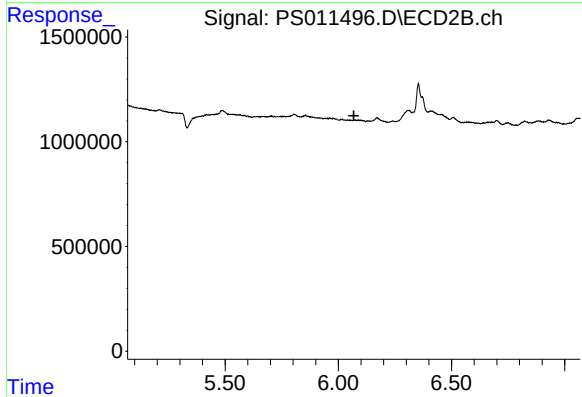


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.069 min
Response: 0
Conc: N.D.

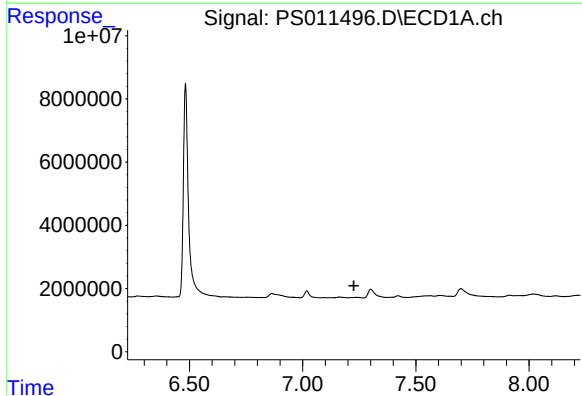


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.226 min
Response: 0
Conc: N.D.

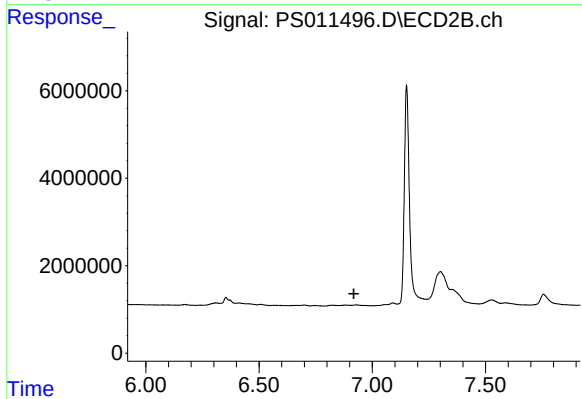

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.918 min
Response: 0
Conc: N.D.

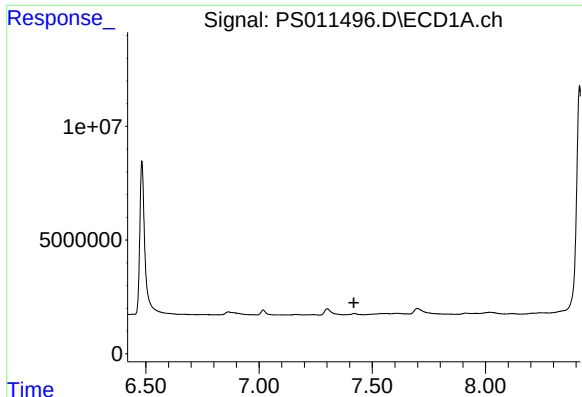

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

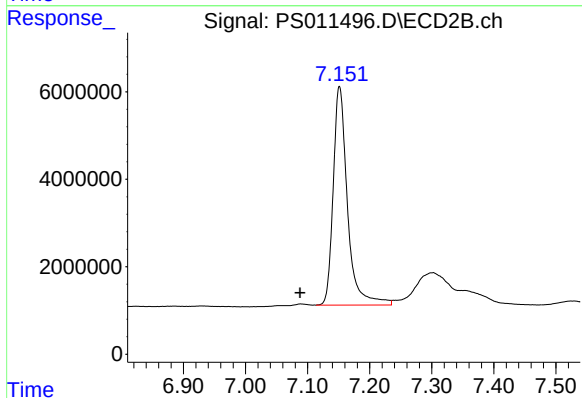


#5 DICAMBA

R.T.: 7.151 min
Delta R.T.: 0.063 min
Response: 79882189
Conc: 34.88 ng/ml

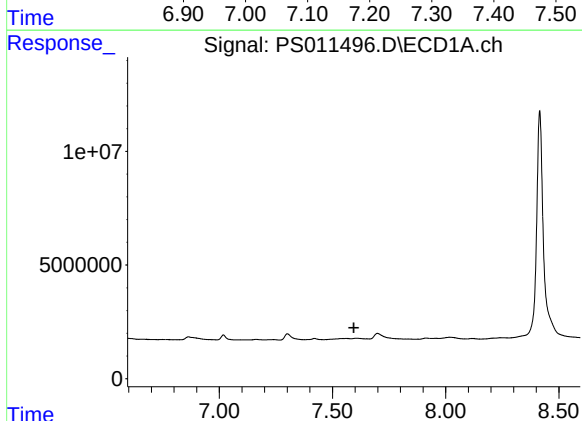


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.594 min
Response: 0
Conc: N.D.

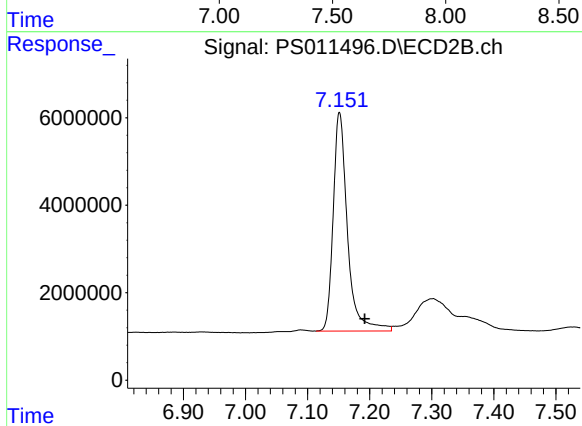

#6 MCP


R.T.: 7.151 min
Delta R.T.: -0.041 min
Response: 79882189
Conc: 41.87 ug/ml

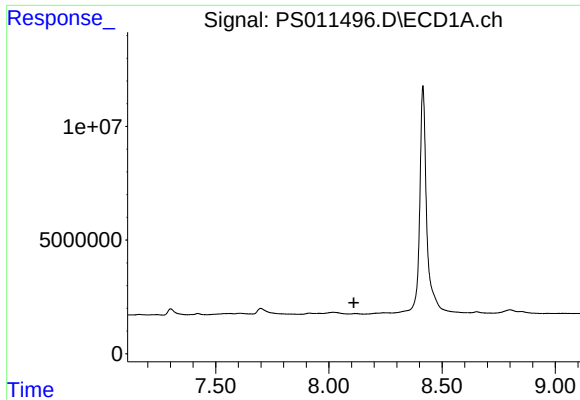

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.110 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

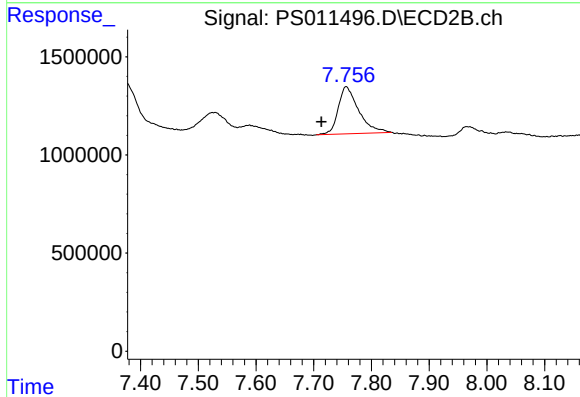


#8 DICHLORPROP

R.T.: 7.756 min
Delta R.T.: 0.043 min
Response: 5912161
Conc: 9.82 ng/ml

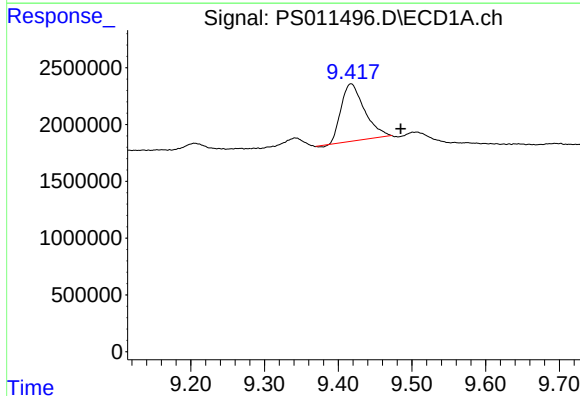


#12 2,4,5-T

R.T.: 9.417 min
Delta R.T.: -0.067 min
Response: 11100390
Conc: 2.20 ng/ml

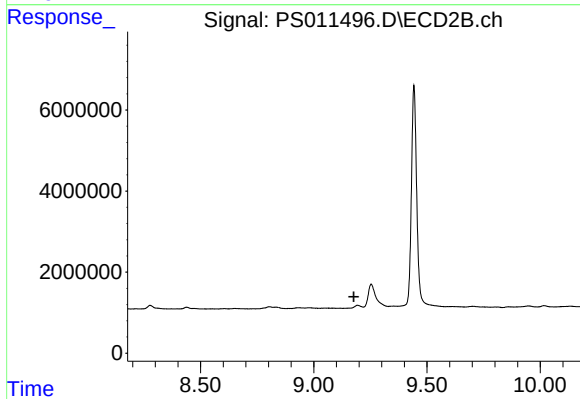

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.177 min
Response: 0
Conc: N.D.

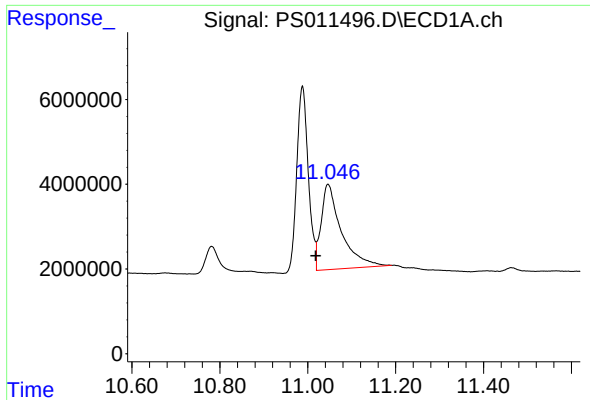

#15 Picloram

R.T.: 11.046 min
Delta R.T.: 0.028 min
Response: 64243905
Conc: 10.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

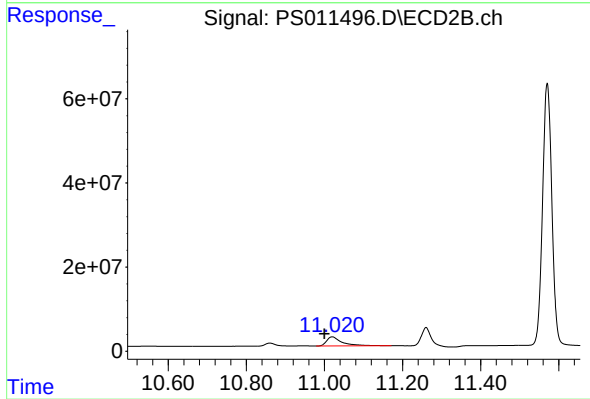

#15 Picloram

R.T.: 11.020 min
Delta R.T.: 0.021 min
Response: 59011525
Conc: 13.49 ng/ml