

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073020\
 Data File : PS011503.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2020 12:02
 Operator : DD\AJ
 Sample : L3435-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 13:51:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	6.917	8274067	4615635	8.527	8.198
Target Compounds							
2) T	3,5-DICHL...	0.000	6.099	0	34761787	N.D.	41.391
3) T	4-Nitroph...	6.999	6.548	6099635	2851072	13.836	8.696 #
5) T	DICAMBA	0.000	7.094	0	2210150	N.D.	<MDL
6) T	MCP	7.636	7.207	7776855	3329996	2.568	1.745 #
7) T	MCPA	7.773	7.406	21682519	7969089	5.084	2.765 #
8) T	DICHLORPROP	8.124	7.716	6948249	4960724	7.411	8.241
9) T	2,4-D	0.000	8.003	0	7108066	N.D.	9.482
10) T	Pentachlo...	8.703	8.436	16202359	6539798	1.226	<MDL #
11) T	2,4,5-TP ...	0.000	8.768	0	18733304	N.D.	6.127
12) T	2,4,5-T	9.503	9.176	14102961	11723321	2.795	3.865 #
13) T	2,4-DB	9.968	9.696	24515855	27724400	38.037	64.853 #
14) T	DINOSEB	0.000	10.038	0	27334537	N.D.	12.744
15) T	Picloram	0.000	11.020	0	12349797	N.D.	2.824
16) T	DCPA	0.000	10.938	0	10142981	N.D.	2.682



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073020\
Data File : PS011503.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2020 12:02
Operator : DD\AJ
Sample : L3435-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 13:51:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
Quant Title : 8080.M
QLast Update : Mon Jul 13 16:10:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

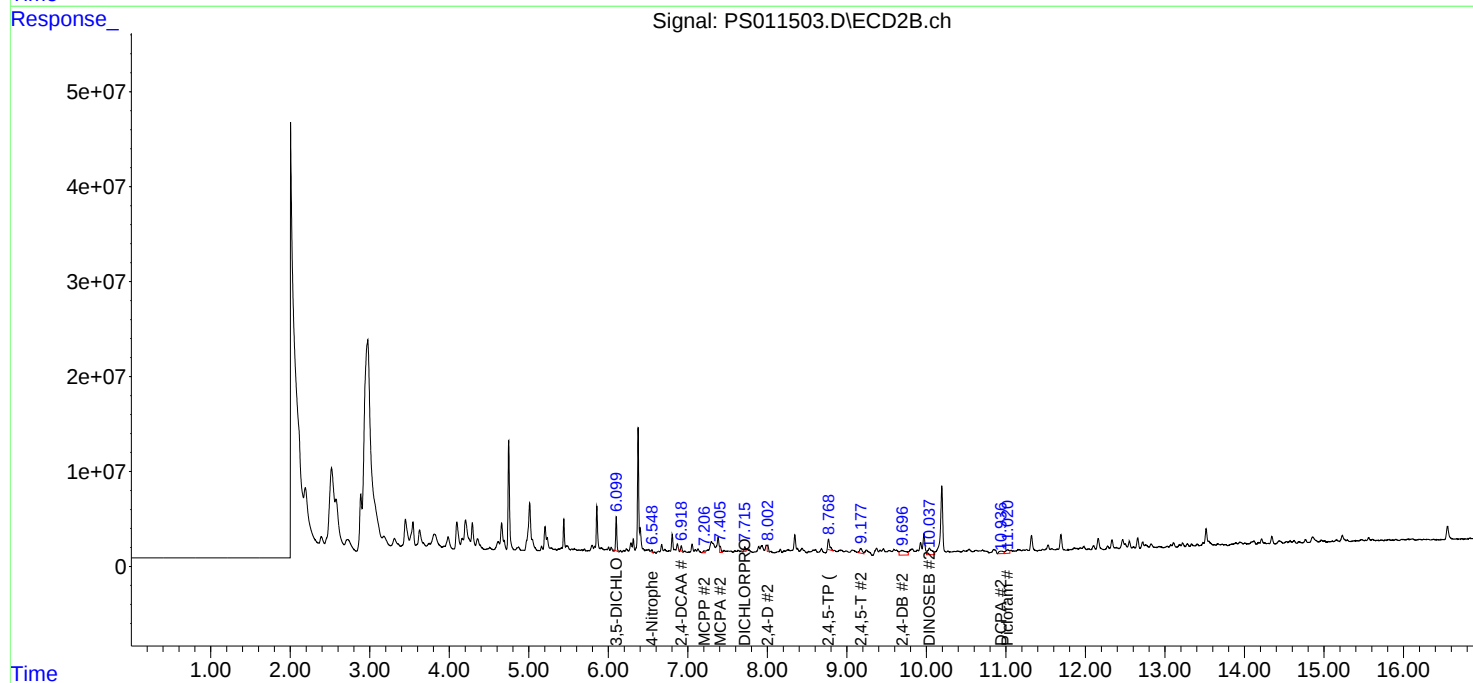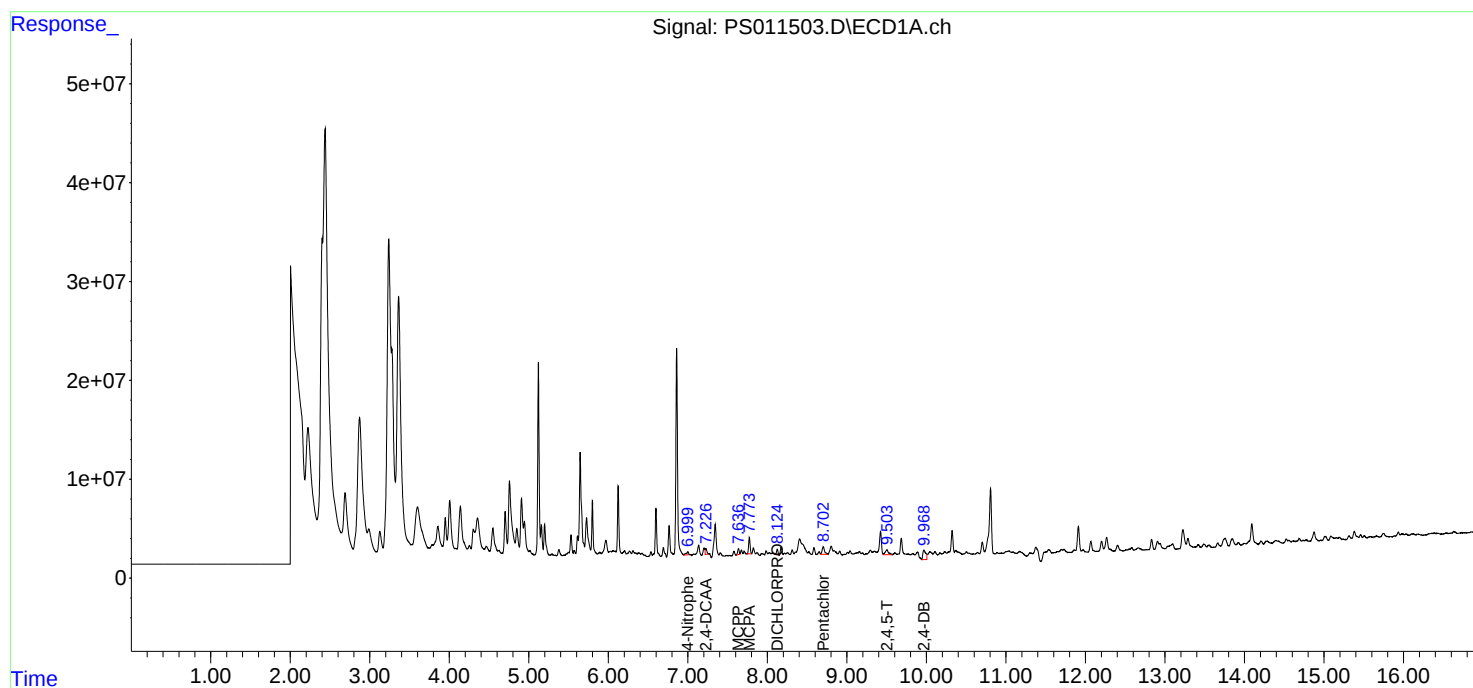


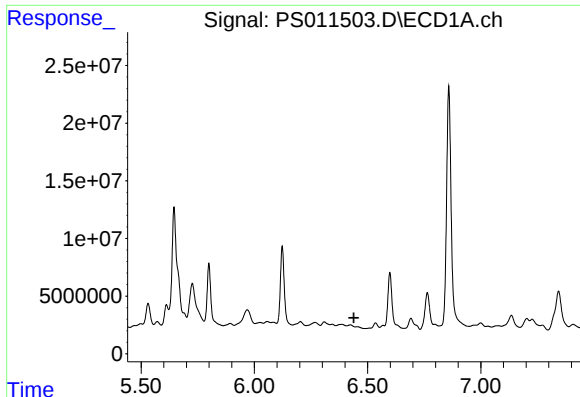

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.439 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

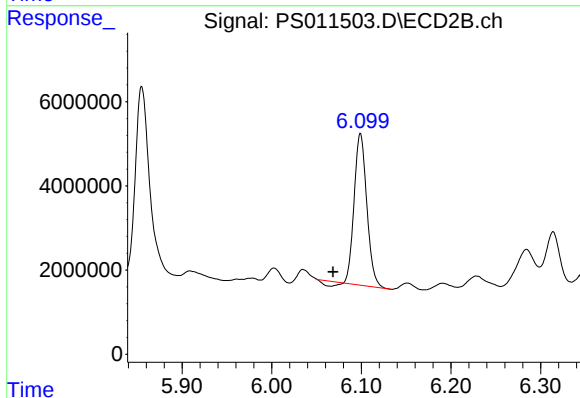


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.099 min
Delta R.T.: 0.030 min
Response: 34761787
Conc: 41.39 ng/ml

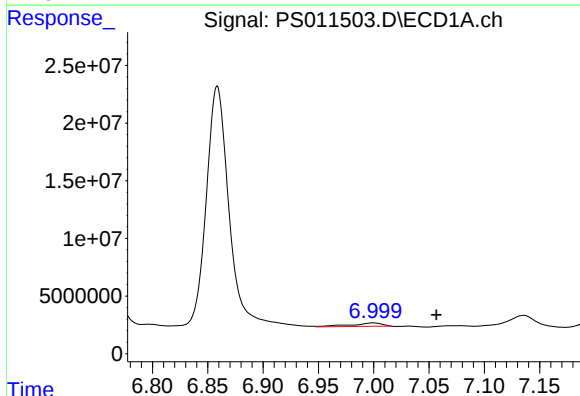


#3 4-Nitrophenol

R.T.: 6.999 min
Delta R.T.: -0.057 min
Response: 6099635
Conc: 13.84 ng/ml

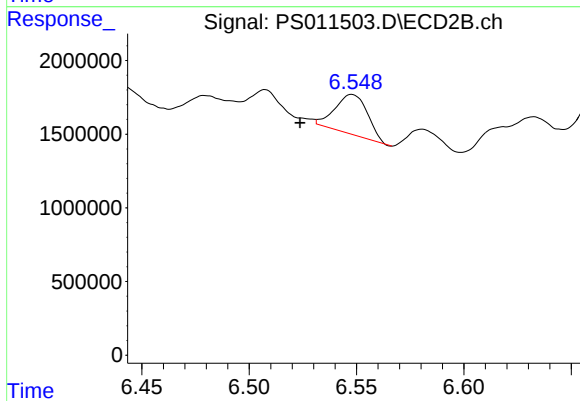

#3 4-Nitrophenol


R.T.: 6.548 min
Delta R.T.: 0.024 min
Response: 2851072
Conc: 8.70 ng/ml

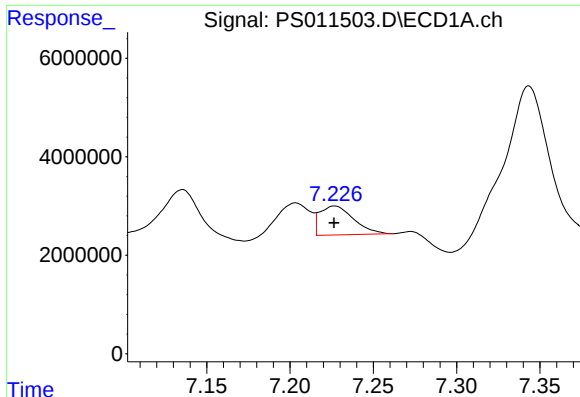

#4 2,4-DCAA


R.T.: 7.227 min
Delta R.T.: 0.000 min
Response: 8274067
Conc: 8.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

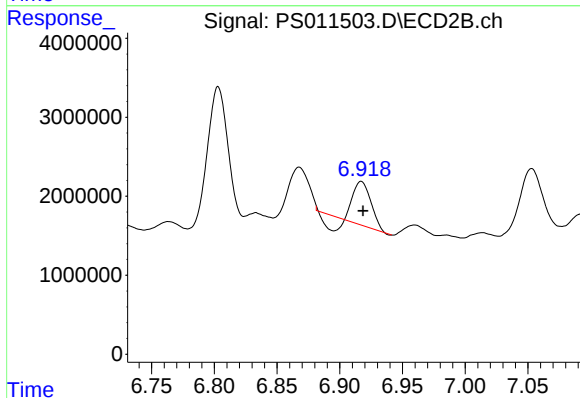


#4 2,4-DCAA

R.T.: 6.917 min
Delta R.T.: -0.001 min
Response: 4615635
Conc: 8.20 ng/ml

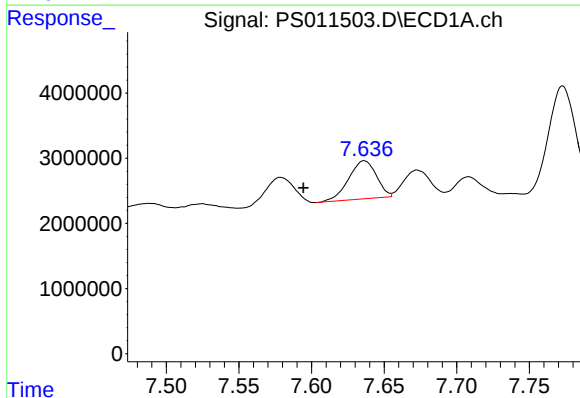


#6 MCP

R.T.: 7.636 min
Delta R.T.: 0.042 min
Response: 7776855
Conc: 2.57 ug/ml

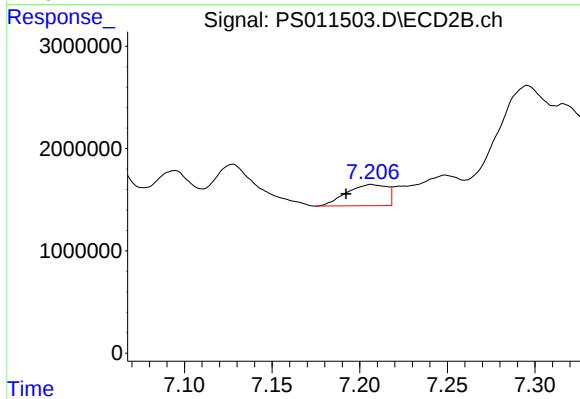

#6 MCP


R.T.: 7.207 min
Delta R.T.: 0.014 min
Response: 3329996
Conc: 1.75 ug/ml

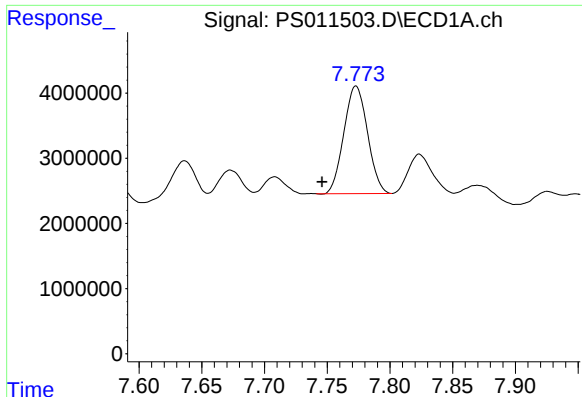

#7 MCPA


R.T.: 7.773 min
Delta R.T.: 0.027 min
Response: 21682519
Conc: 5.08 ug/ml

Instrument :
ECD_S
ClientSampleId :

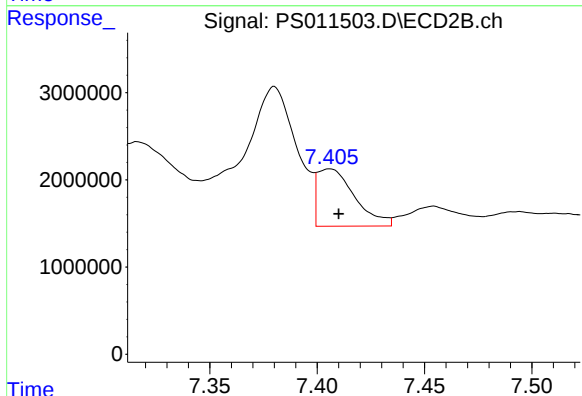


#7 MCPA

R.T.: 7.406 min
Delta R.T.: -0.004 min
Response: 7969089
Conc: 2.76 ug/ml

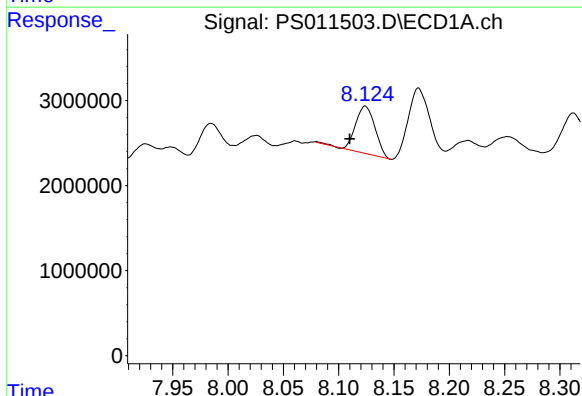


#8 DICHLORPROP

R.T.: 8.124 min
Delta R.T.: 0.014 min
Response: 6948249
Conc: 7.41 ng/ml

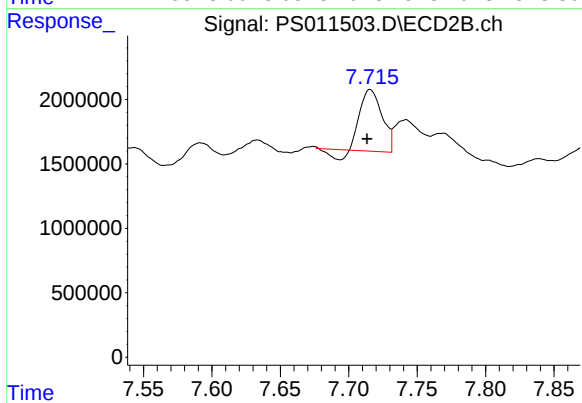

#8 DICHLORPROP


R.T.: 7.716 min
Delta R.T.: 0.002 min
Response: 4960724
Conc: 8.24 ng/ml

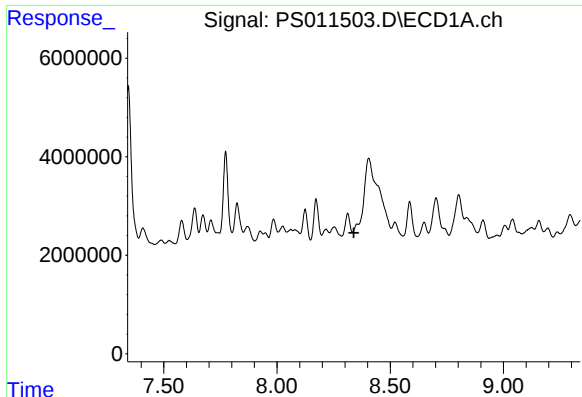

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.339 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

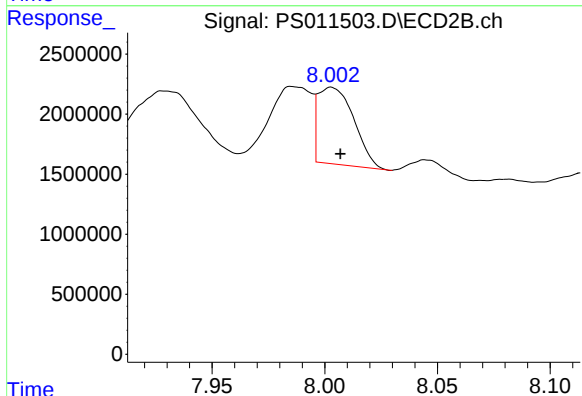


#9 2,4-D

R.T.: 8.003 min
Delta R.T.: -0.004 min
Response: 7108066
Conc: 9.48 ng/ml

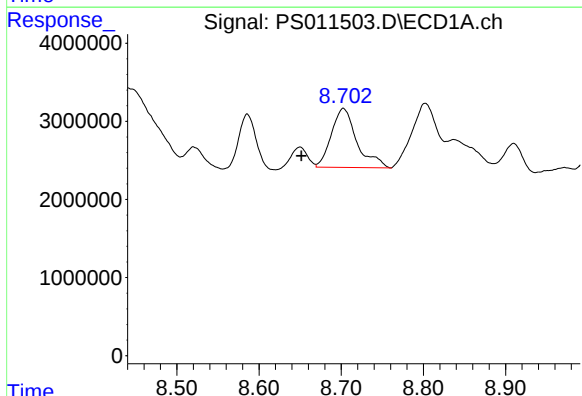


#10 Pentachlorophenol

R.T.: 8.703 min
Delta R.T.: 0.051 min
Response: 16202359
Conc: 1.23 ng/ml

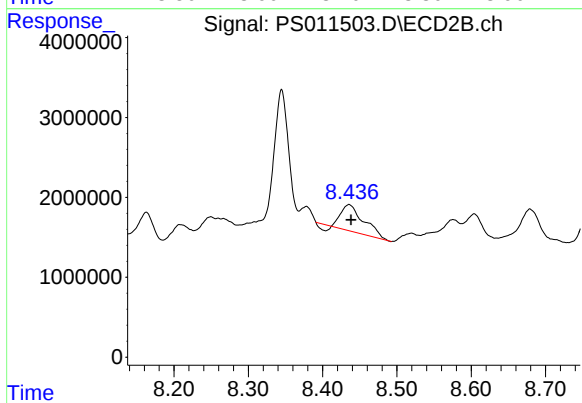

#10 Pentachlorophenol


R.T.: 8.436 min
Delta R.T.: -0.003 min
Response: 6539798
Conc: N.D.

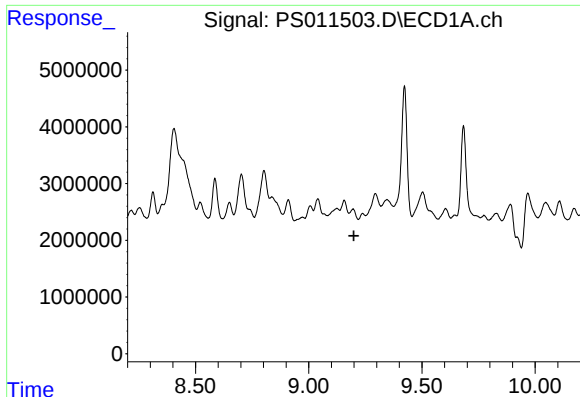

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.200 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

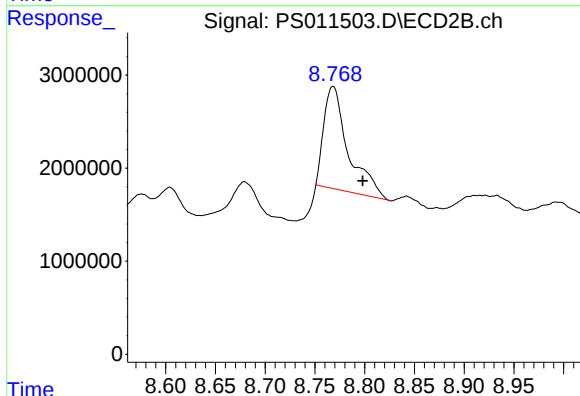


#11 2,4,5-TP (SILVEX)

R.T.: 8.768 min
Delta R.T.: -0.030 min
Response: 18733304
Conc: 6.13 ng/ml

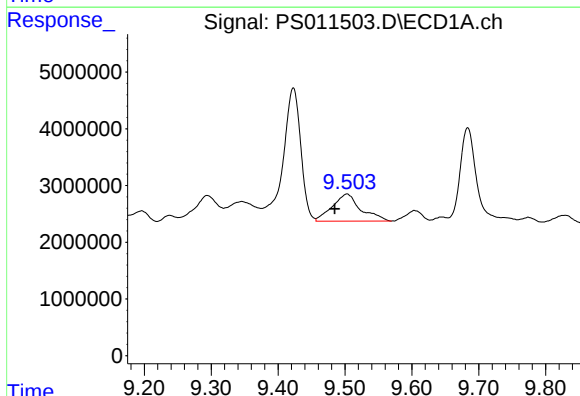


#12 2,4,5-T

R.T.: 9.503 min
Delta R.T.: 0.018 min
Response: 14102961
Conc: 2.79 ng/ml

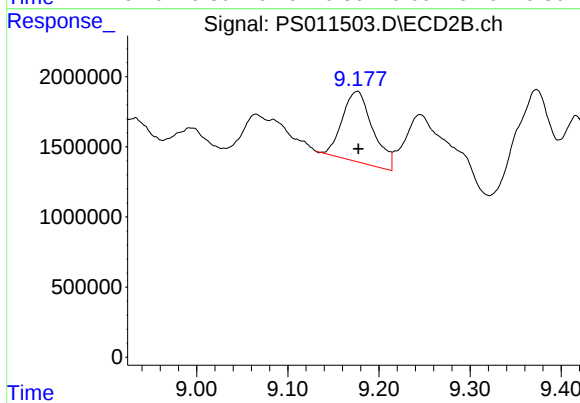

#12 2,4,5-T


R.T.: 9.176 min
Delta R.T.: -0.001 min
Response: 11723321
Conc: 3.87 ng/ml

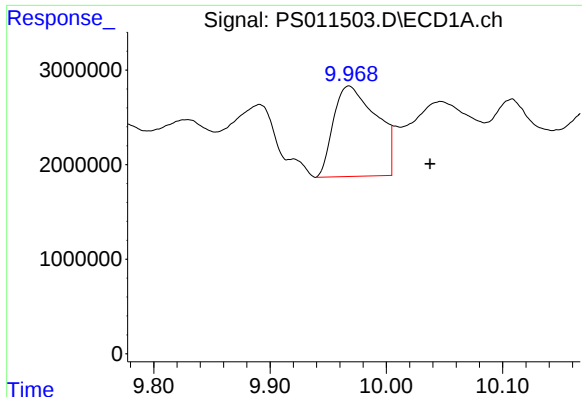

#13 2,4-DB


R.T.: 9.968 min
Delta R.T.: -0.070 min
Response: 24515855
Conc: 38.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

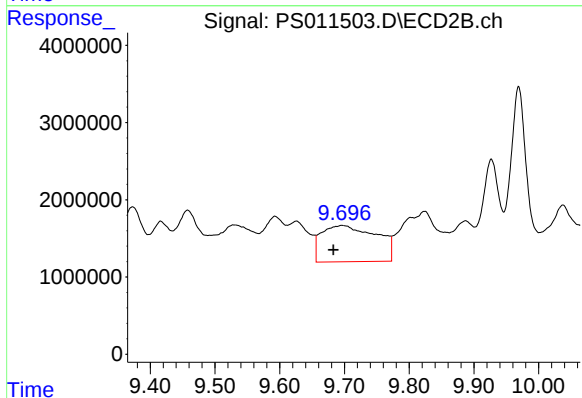


#13 2,4-DB

R.T.: 9.696 min
Delta R.T.: 0.013 min
Response: 27724400
Conc: 64.85 ng/ml

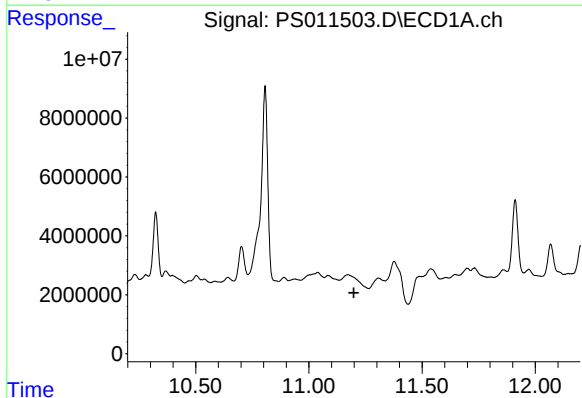


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.199 min
Response: 0
Conc: N.D.

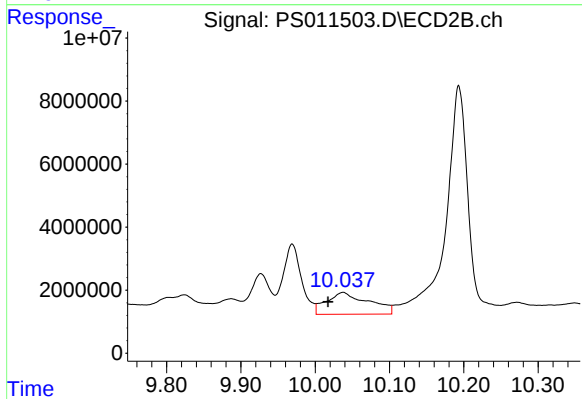

#14 DINOSEB


R.T.: 10.038 min
Delta R.T.: 0.020 min
Response: 27334537
Conc: 12.74 ng/ml

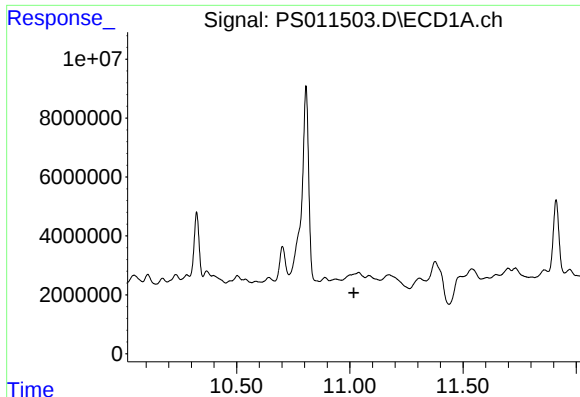

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 11.018 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

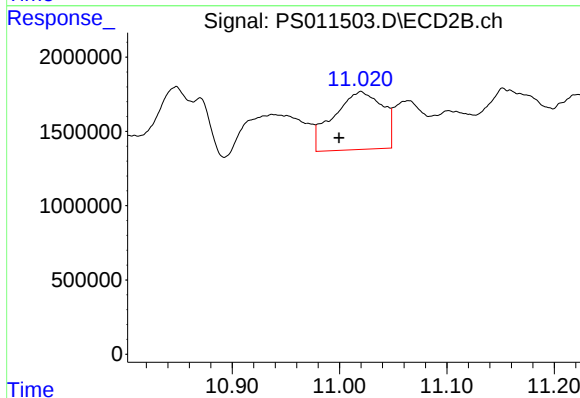


#15 Picloram

R.T.: 11.020 min
Delta R.T.: 0.021 min
Response: 12349797
Conc: 2.82 ng/ml

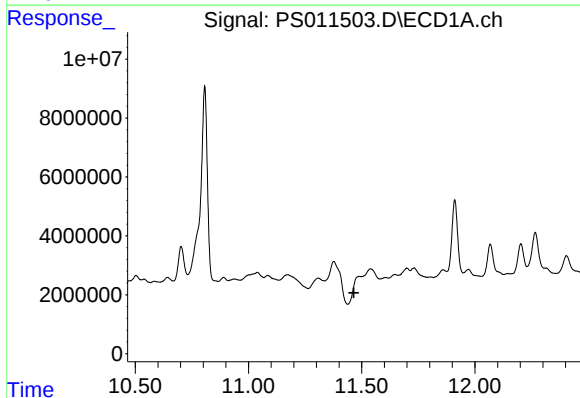

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.466 min
Response: 0
Conc: N.D.

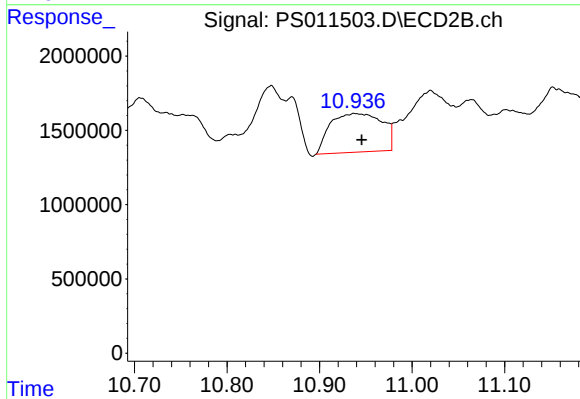

#16 DCPA

R.T.: 10.938 min
Delta R.T.: -0.008 min
Response: 10142981
Conc: 2.68 ng/ml