

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073021\
 Data File : PS016226.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2021 09:18
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 14:10:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
 Quant Title : 8080.M
 QLast Update : Wed Jun 30 00:31:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds									
10)	T	Pentachlo...	8.609	0.000	12692431	0	<MDL	N.D.	#
11)	T	2,4,5-TP ...	9.161	0.000	9144860	0	1.232	N.D.	#
12)	T	2,4,5-T	9.449	9.057f	17372895	18696722	2.225	6.481	#
14)	T	DINOSEB	11.152	0.000	11233488	0	2.049	N.D.	#
15)	T	Picloram	10.980	10.819	190.4E6	74860100	17.305	17.993	
16)	T	DCPA	11.420	10.766	15771426	6998341	1.462	1.627	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073021\
Data File : PS016226.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2021 09:18
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 14:10:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS063021.M
Quant Title : 8080.M
QLast Update : Wed Jun 30 00:31:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

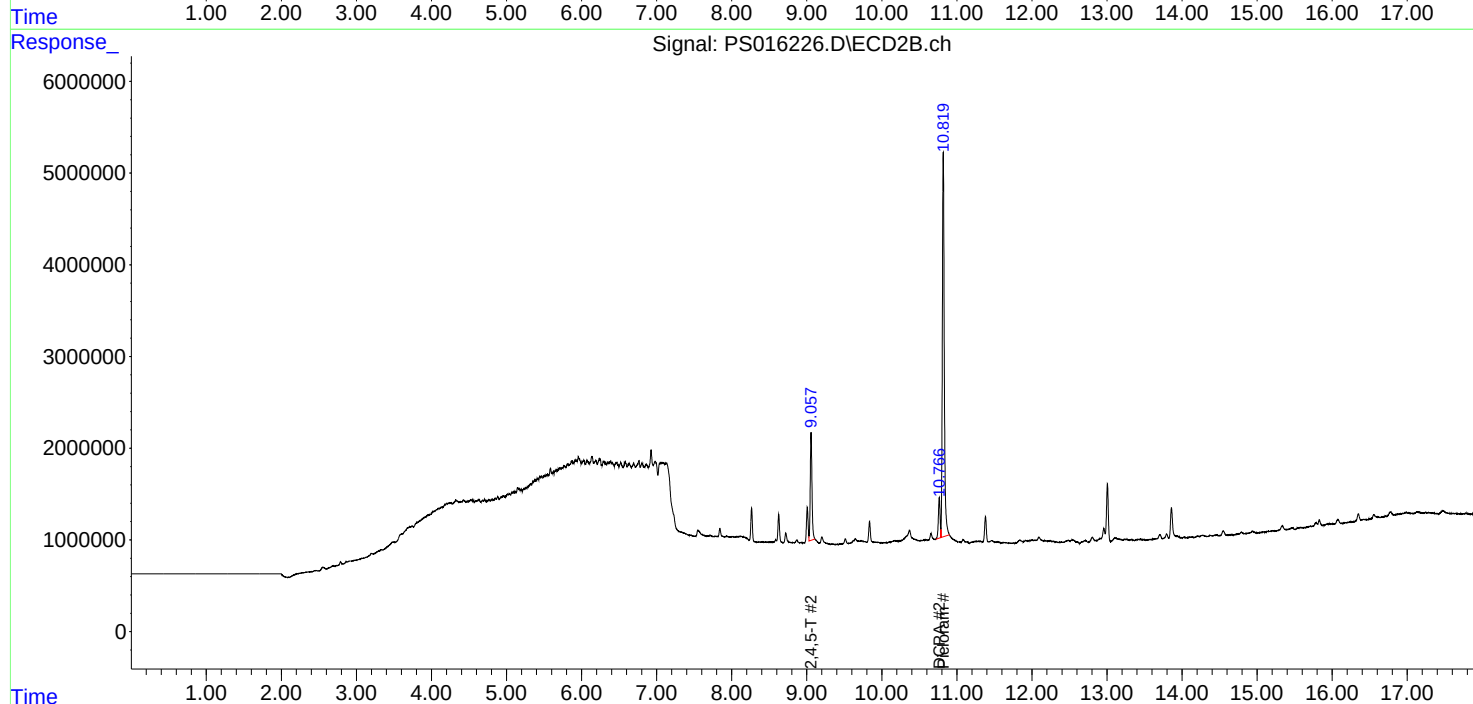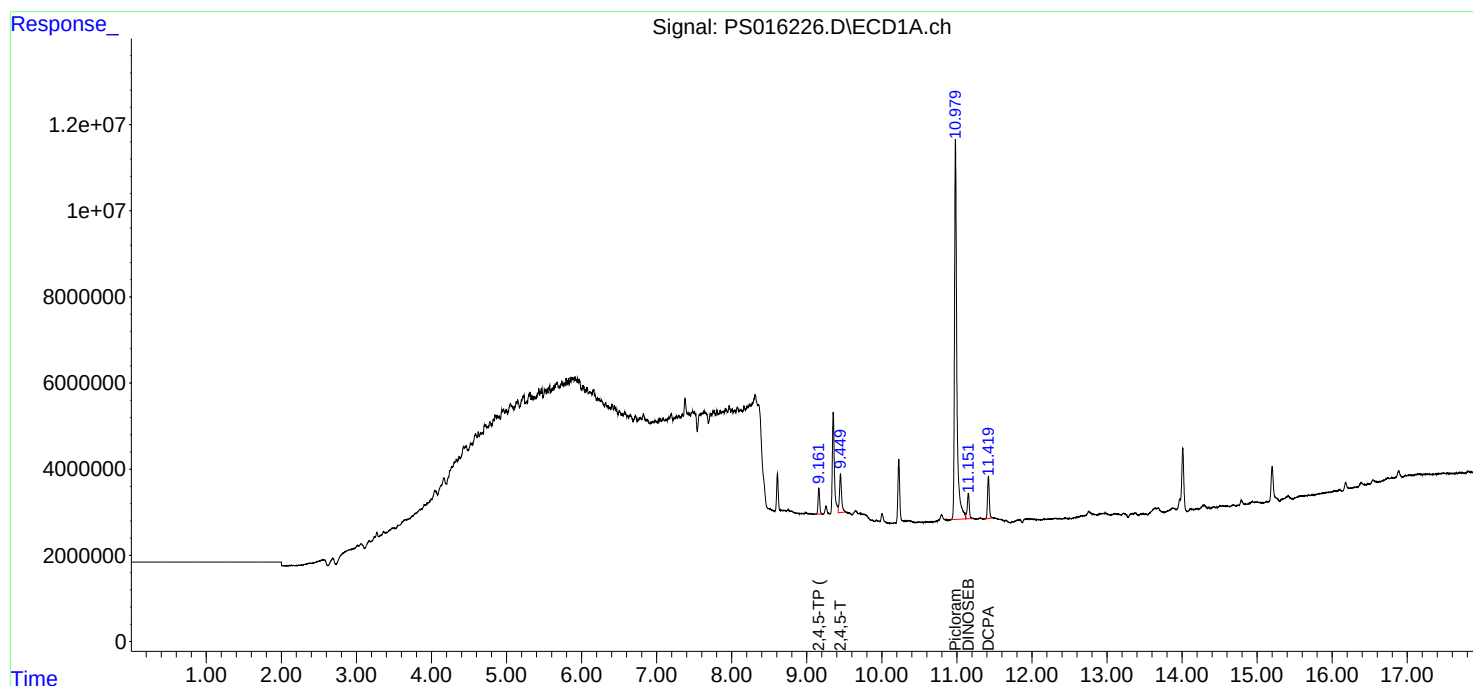


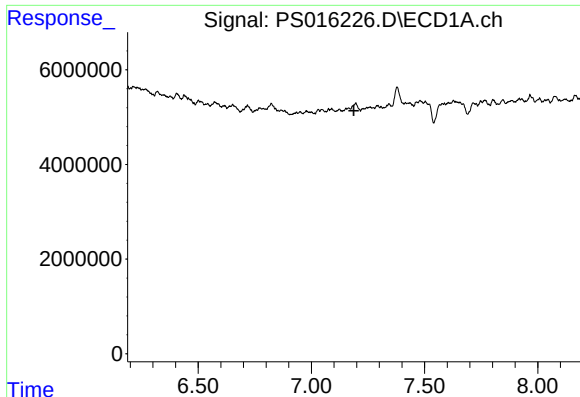

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

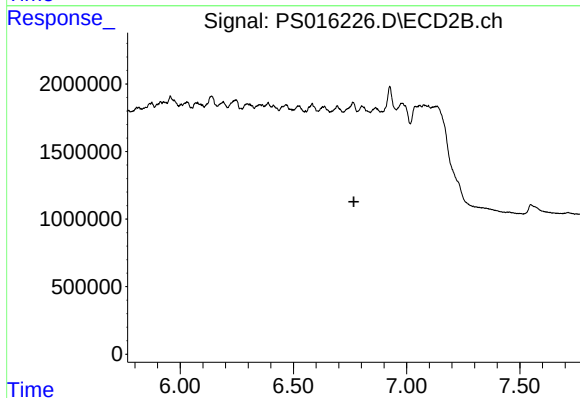


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.767 min
Response: 0
Conc: N.D.

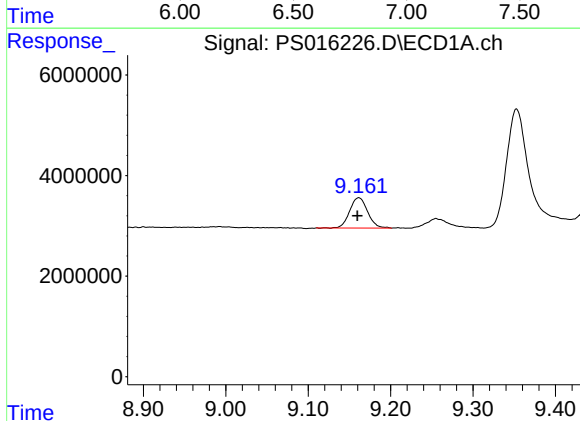


#11 2,4,5-TP (SILVEX)

R.T.: 9.161 min
Delta R.T.: 0.002 min
Response: 9144860
Conc: 1.23 ng/ml

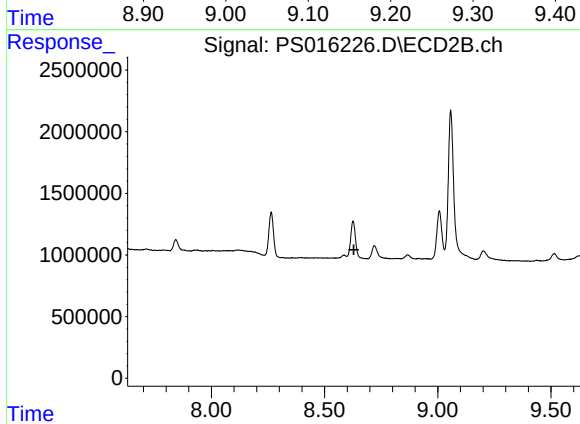

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 8.630 min
Response: 0
Conc: N.D.

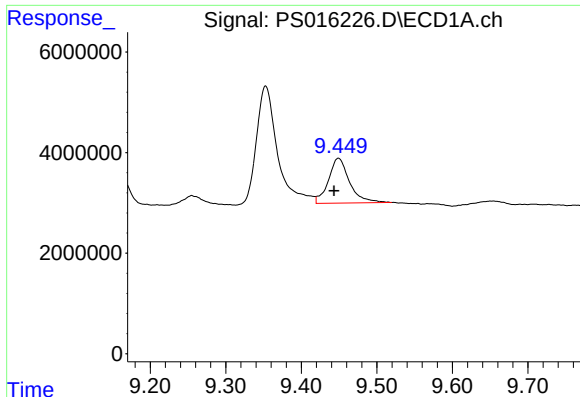

#12 2,4,5-T


R.T.: 9.449 min
Delta R.T.: 0.006 min
Response: 17372895
Conc: 2.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

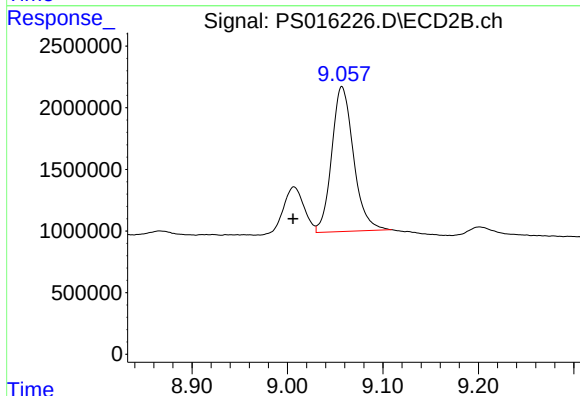


#12 2,4,5-T

R.T.: 9.057 min
Delta R.T.: 0.051 min
Response: 18696722
Conc: 6.48 ng/ml

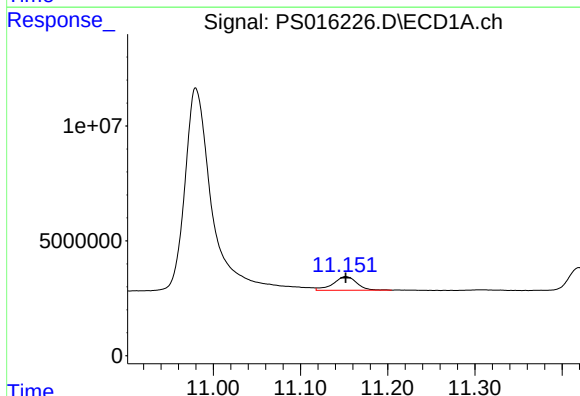


#14 DINOSEB

R.T.: 11.152 min
Delta R.T.: 0.000 min
Response: 11233488
Conc: 2.05 ng/ml

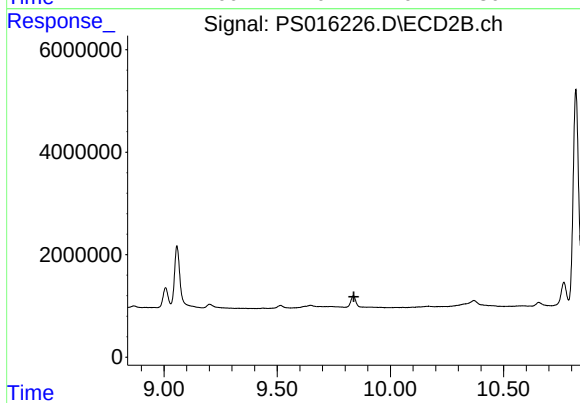

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.839 min
Response: 0
Conc: N.D.

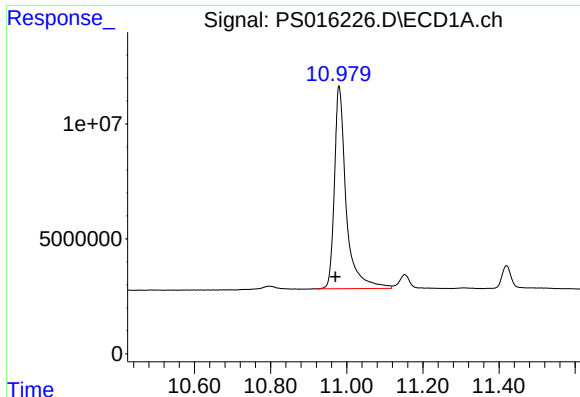

#15 Picloram


R.T.: 10.980 min
Delta R.T.: 0.010 min
Response: 190362597
Conc: 17.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

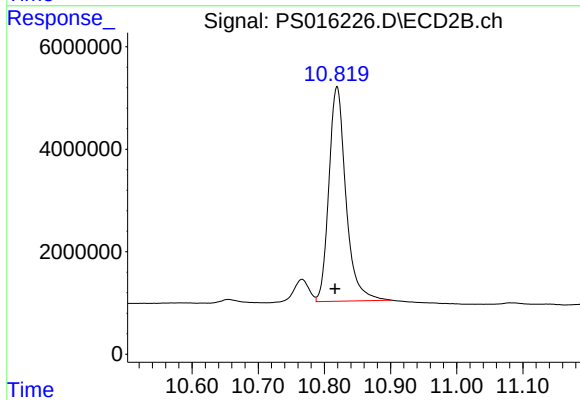


#15 Picloram

R.T.: 10.819 min
Delta R.T.: 0.003 min
Response: 74860100
Conc: 17.99 ng/ml

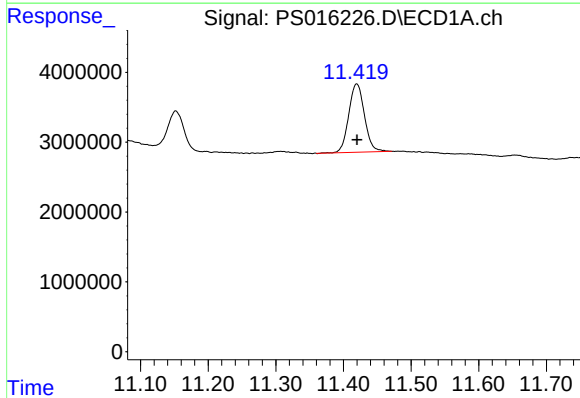

#16 DCPA

R.T.: 11.420 min
Delta R.T.: 0.000 min
Response: 15771426
Conc: 1.46 ng/ml

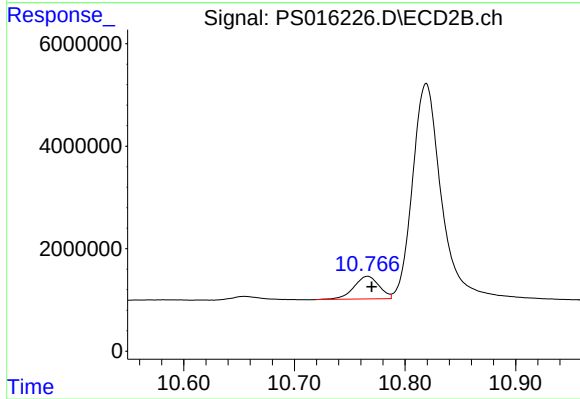

#16 DCPA

R.T.: 10.766 min
Delta R.T.: -0.004 min
Response: 6998341
Conc: 1.63 ng/ml