

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073118\
 Data File : PS001316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2018 12:27
 Operator : UA
 Sample : J4180-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 12:54:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.639	11.047	83749808	73053027	451.360	401.666
Target Compounds							
1) T	Dalapon	2.981	2.406	1216439	489426	5.130	2.148 #
5) T	DICAMBA	0.000	11.291	0	5150575	N.D.	7.515 #
6) T	MCPD	12.331	0.000	7530363	0	14.983	N.D. #
8) T	DICHLORPROP	0.000	12.418	0	717124	N.D.	4.048 #
10) T	Pentachlo...	0.000	13.409	0	3211689	N.D.	1.167 #
11) T	2,4,5-TP ...	0.000	14.027	0	10962507	N.D.	10.026 #
15) T	Picloram	17.170	16.941	5016242	6016478	3.174	4.364 #
16) T	DCPA	0.000	16.991	0	7995157	N.D.	5.536 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073118\
Data File : PS001316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2018 12:27
Operator : UA
Sample : J4180-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 12:54:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

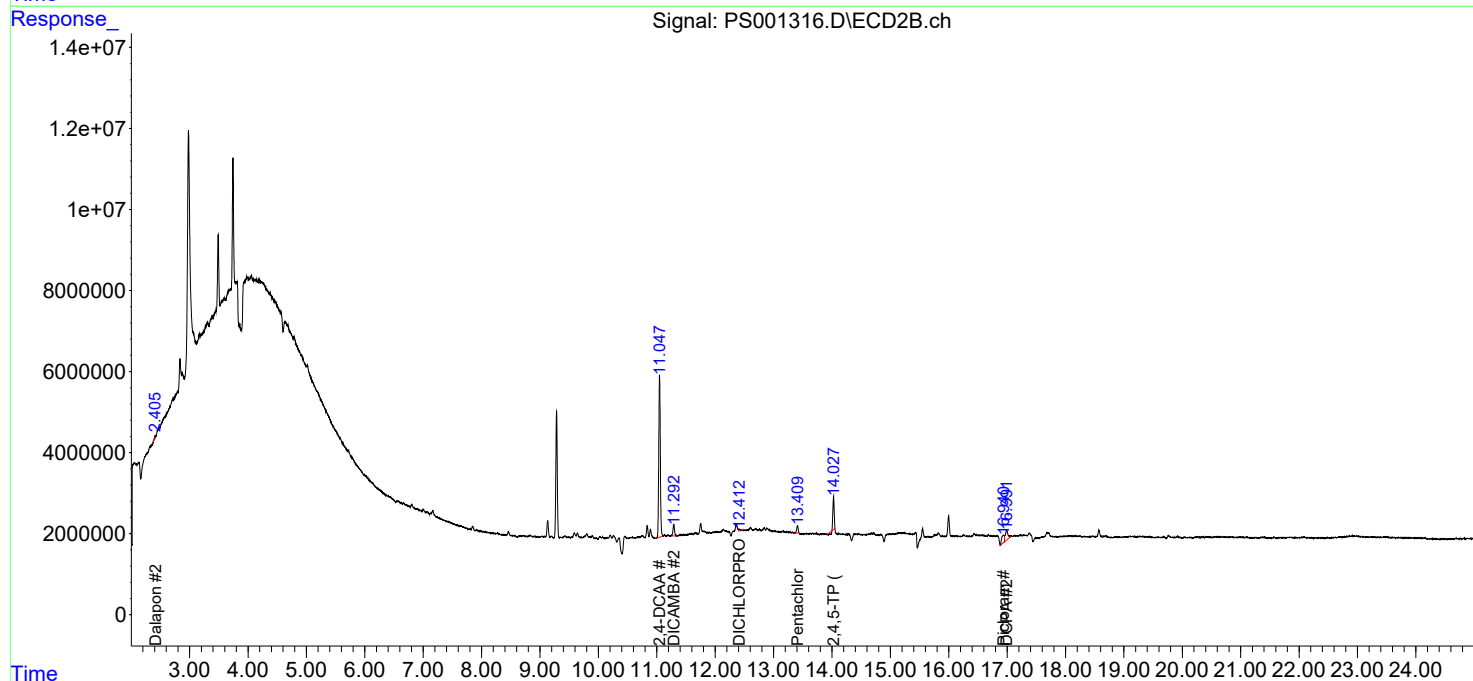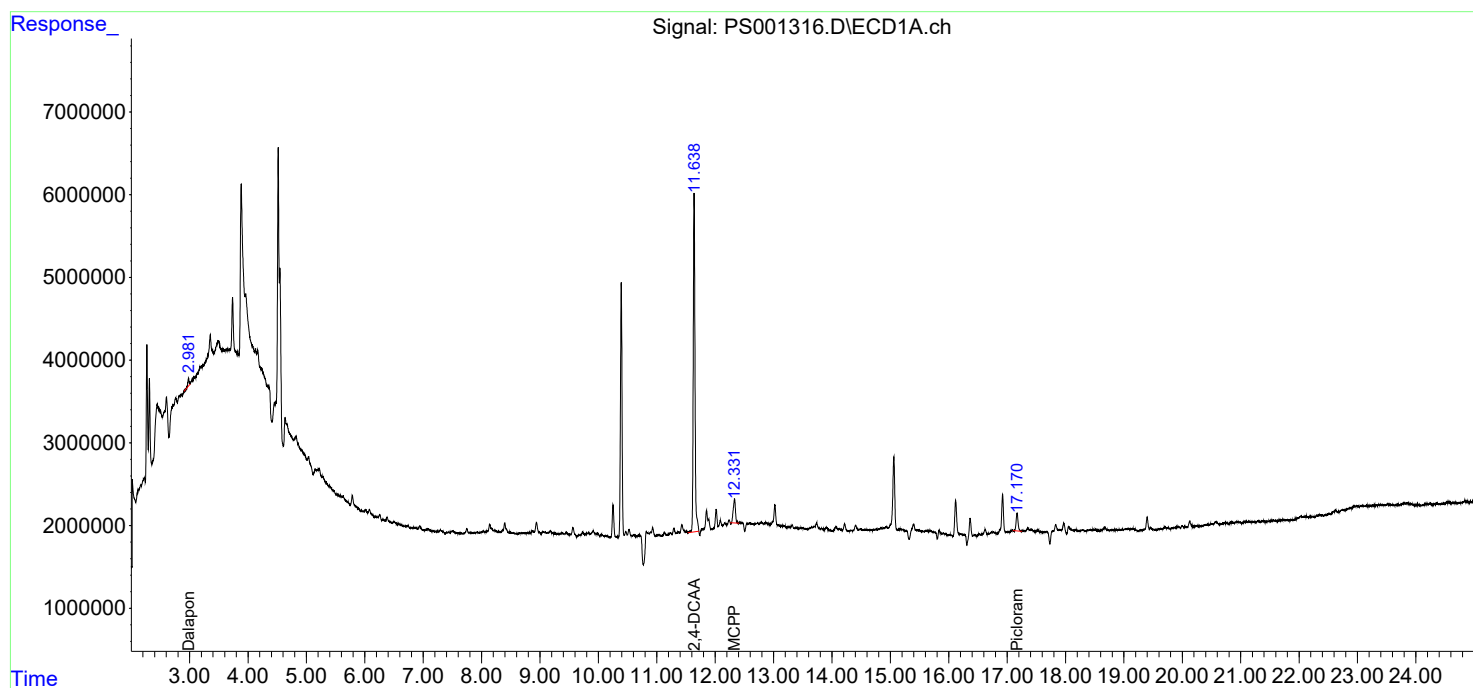


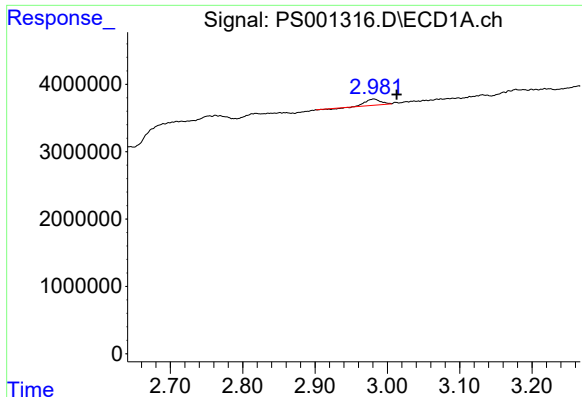

#1 Dalapon


R.T.: 2.981 min
Delta R.T.: -0.032 min
Response: 1216439
Conc: 5.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

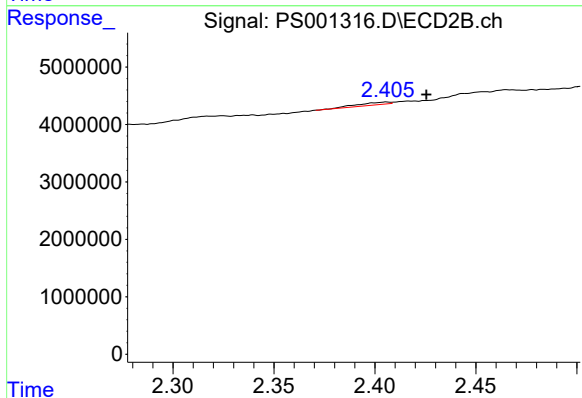


#1 Dalapon

R.T.: 2.406 min
Delta R.T.: -0.020 min
Response: 489426
Conc: 2.15 ng/ml

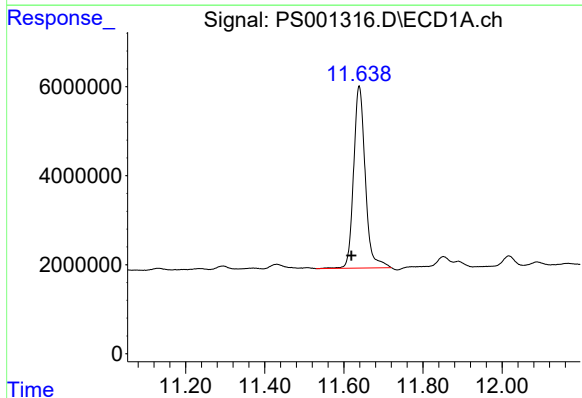


#4 2,4-DCAA

R.T.: 11.639 min
Delta R.T.: 0.019 min
Response: 83749808
Conc: 451.36 ng/ml

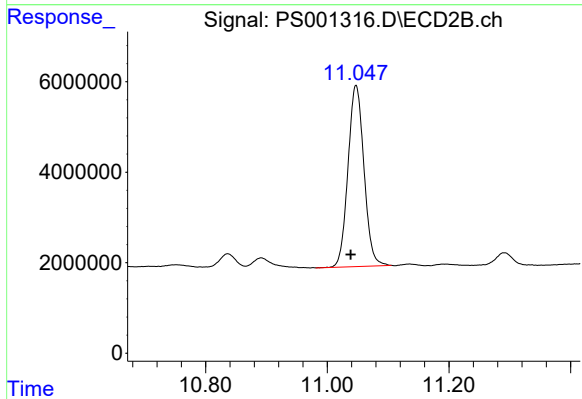

#4 2,4-DCAA


R.T.: 11.047 min
Delta R.T.: 0.009 min
Response: 73053027
Conc: 401.67 ng/ml

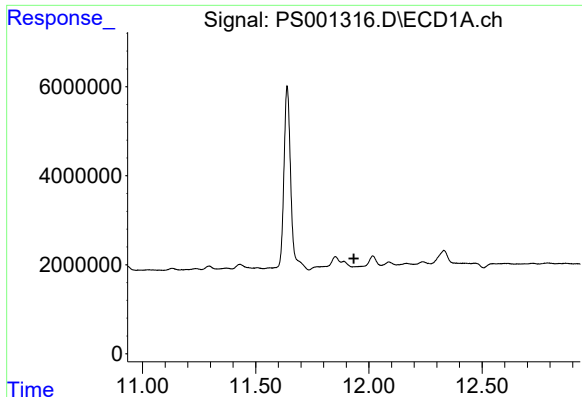

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.934 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

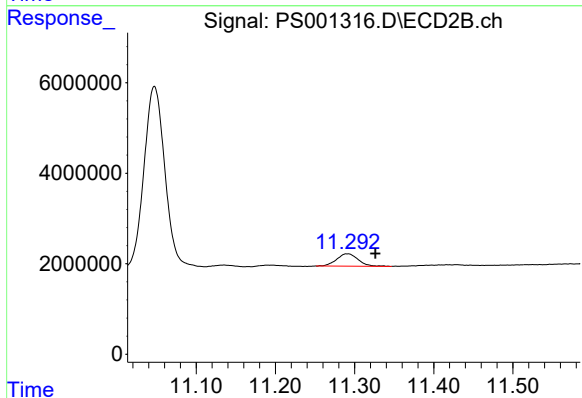


#5 DICAMBA

R.T.: 11.291 min
Delta R.T.: -0.036 min
Response: 5150575
Conc: 7.51 ng/ml

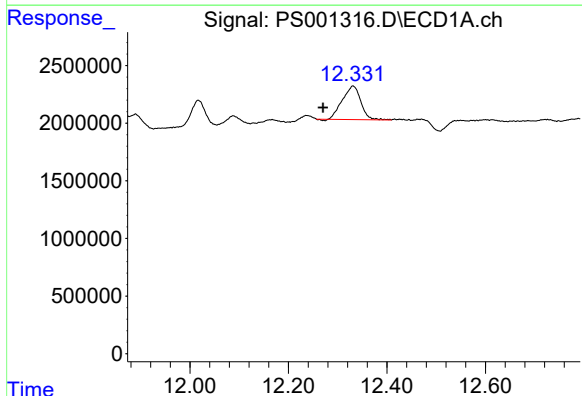


#6 MCP

R.T.: 12.331 min
Delta R.T.: 0.061 min
Response: 7530363
Conc: 14.98 ug/ml

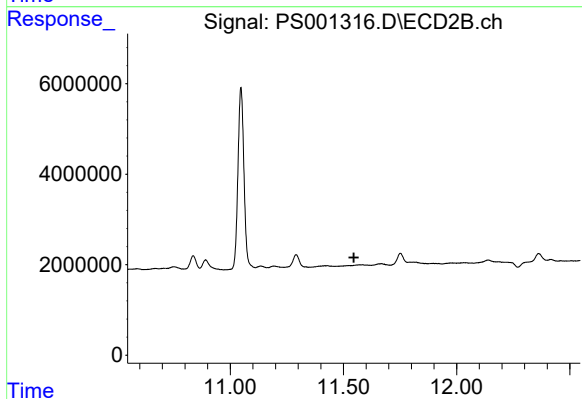

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.546 min
Response: 0
Conc: N.D.

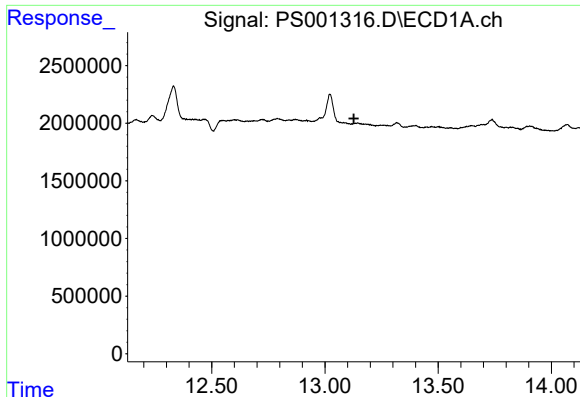

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.128 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

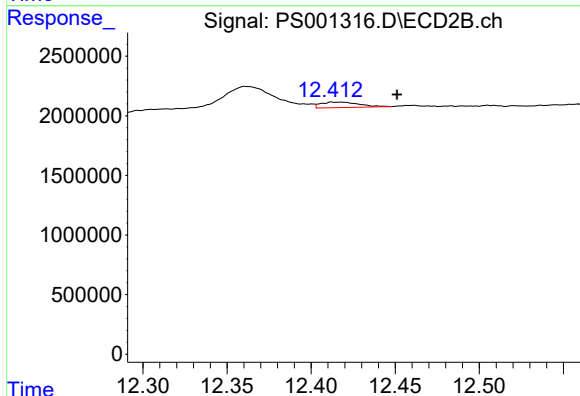


#8 DICHLORPROP

R.T.: 12.418 min
Delta R.T.: -0.033 min
Response: 717124
Conc: 4.05 ng/ml

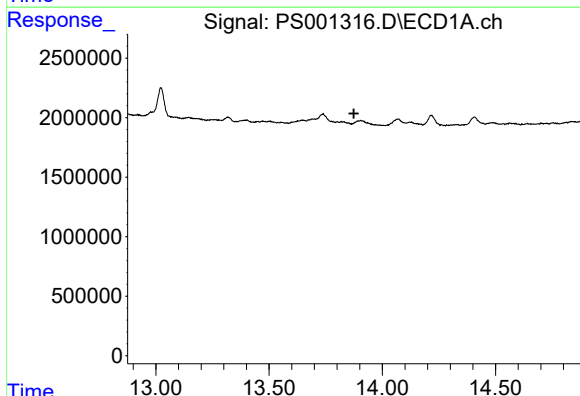


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.874 min
Response: 0
Conc: N.D.

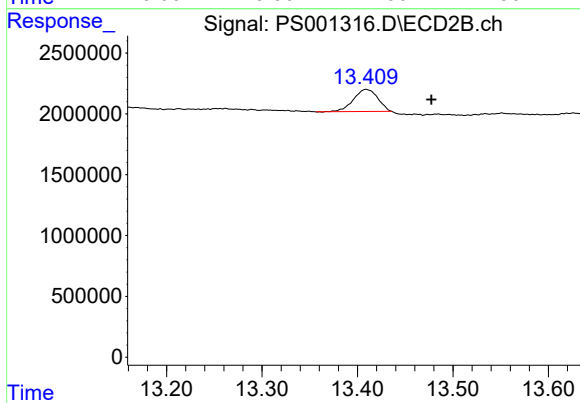

#10 Pentachlorophenol


R.T.: 13.409 min
Delta R.T.: -0.069 min
Response: 3211689
Conc: 1.17 ng/ml

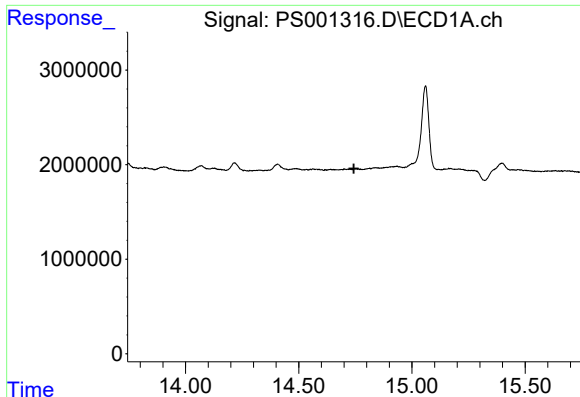

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.743 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

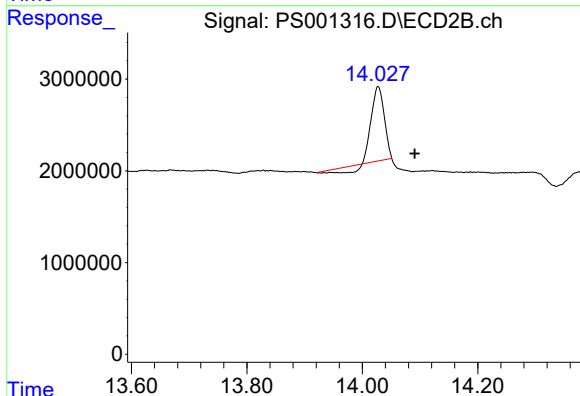


#11 2,4,5-TP (SILVEX)

R.T.: 14.027 min
Delta R.T.: -0.064 min
Response: 10962507
Conc: 10.03 ng/ml

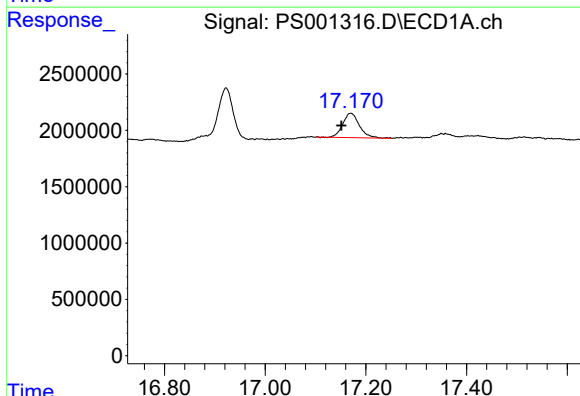


#15 Picloram

R.T.: 17.170 min
Delta R.T.: 0.018 min
Response: 5016242
Conc: 3.17 ng/ml

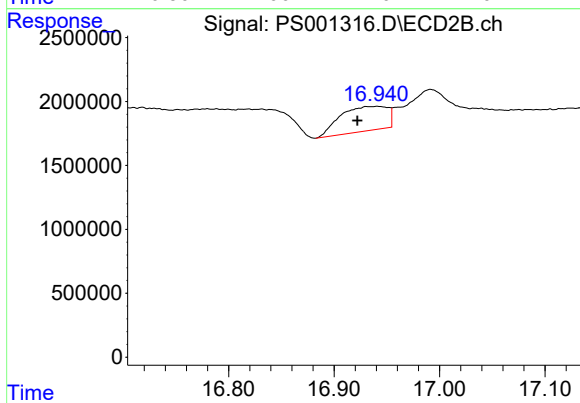

#15 Picloram


R.T.: 16.941 min
Delta R.T.: 0.019 min
Response: 6016478
Conc: 4.36 ng/ml

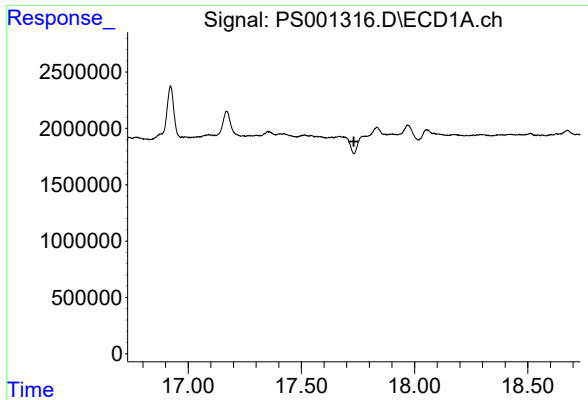

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.732 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

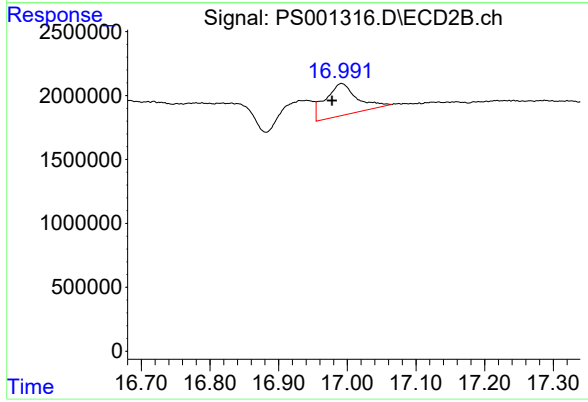

#16 DCPA

R.T.: 16.991 min
Delta R.T.: 0.014 min
Response: 7995157
Conc: 5.54 ng/ml