

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073118\
 Data File : PS001317.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2018 12:58
 Operator : UA
 Sample : J4218-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 13:41:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.616	11.035	68368413	59583739	368.464	327.608
Target Compounds							
2) T	3,5-DICHL...	0.000	9.121	0	122020	N.D.	0.479 #
5) T	DICAMBA	0.000	11.278	0	3677319	N.D.	5.365 #
6) T	MCP	12.306	0.000	7608778	0	15.139	N.D. #
8) T	DICHLORPROP	0.000	12.398	0	951939	N.D.	5.374 #
16) T	DCPA	17.798	17.011	5414830	9041270	4.011	6.260 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073118\
Data File : PS001317.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2018 12:58
Operator : UA
Sample : J4218-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 13:41:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

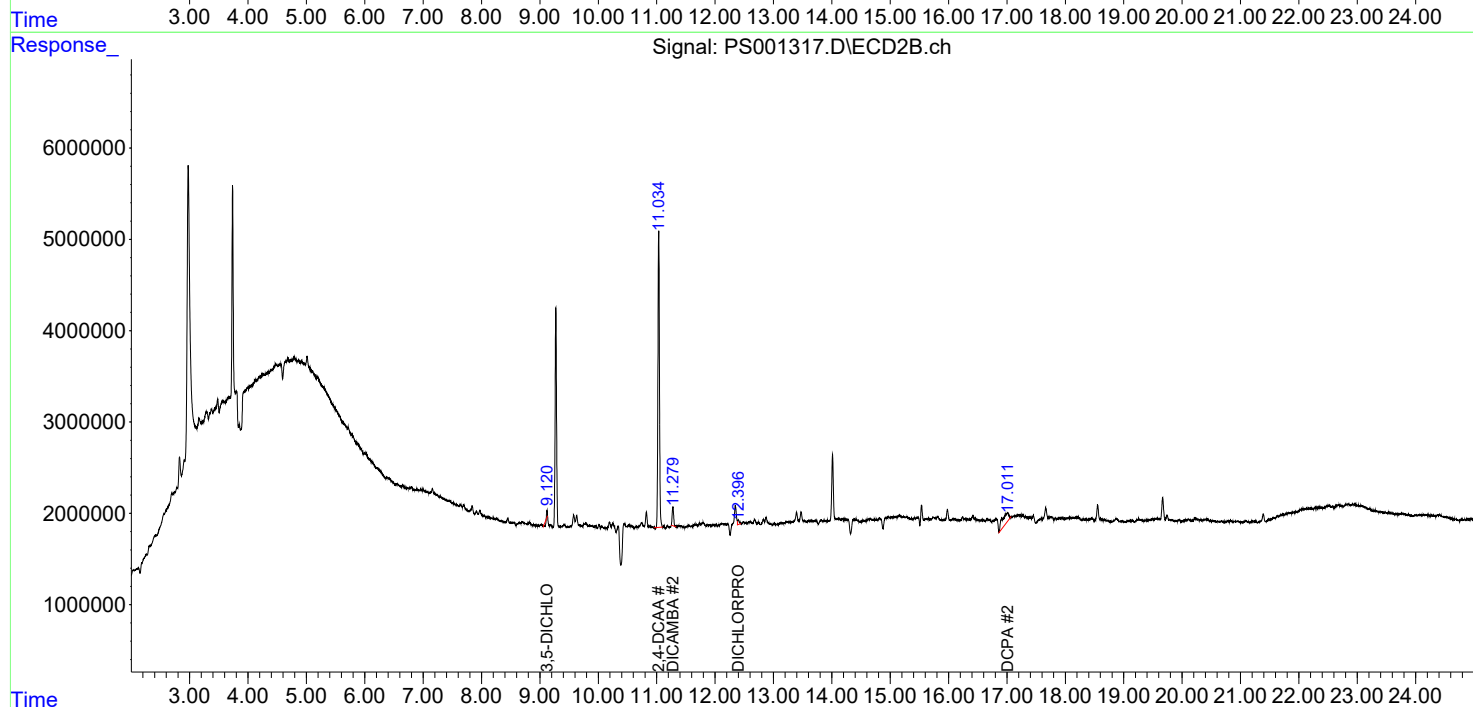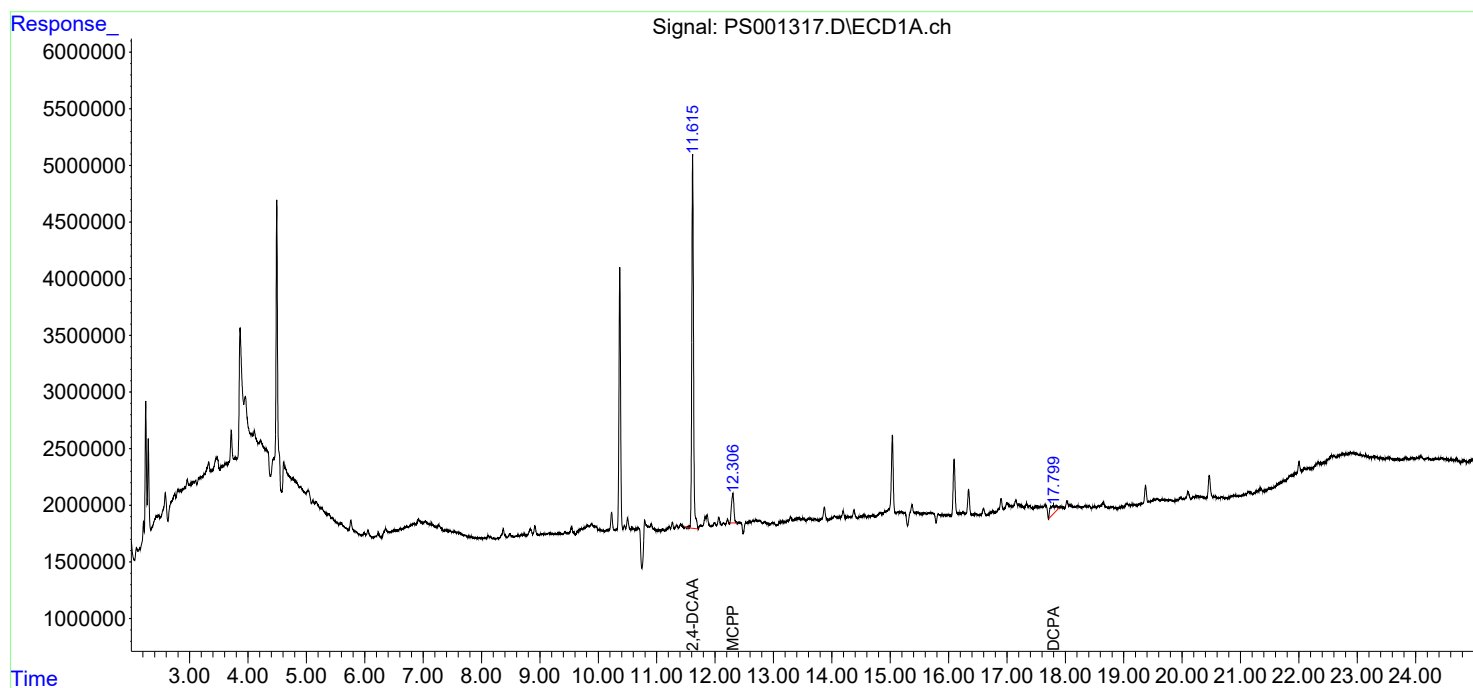


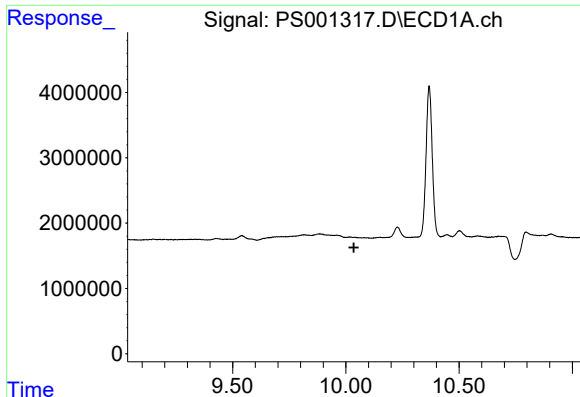

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

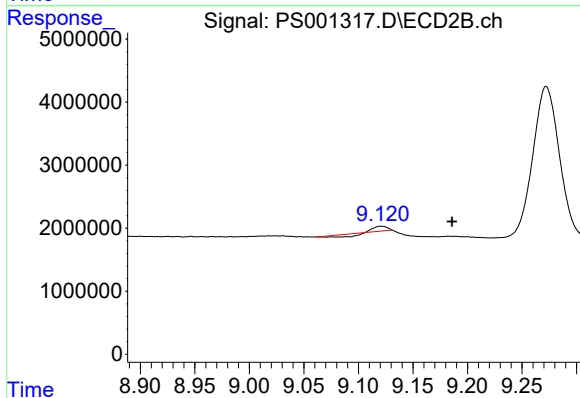


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.121 min
Delta R.T.: -0.065 min
Response: 122020
Conc: 0.48 ng/ml

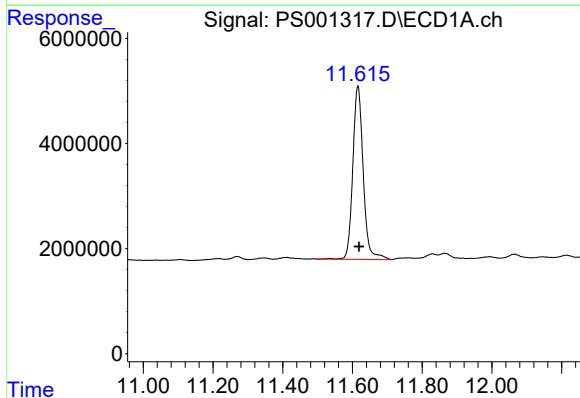


#4 2,4-DCAA

R.T.: 11.616 min
Delta R.T.: -0.004 min
Response: 68368413
Conc: 368.46 ng/ml

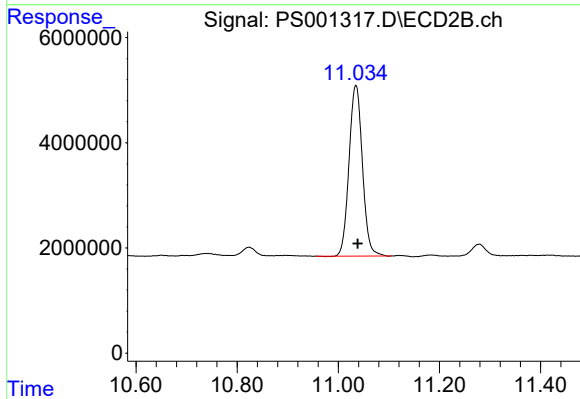

#4 2,4-DCAA


R.T.: 11.035 min
Delta R.T.: -0.004 min
Response: 59583739
Conc: 327.61 ng/ml

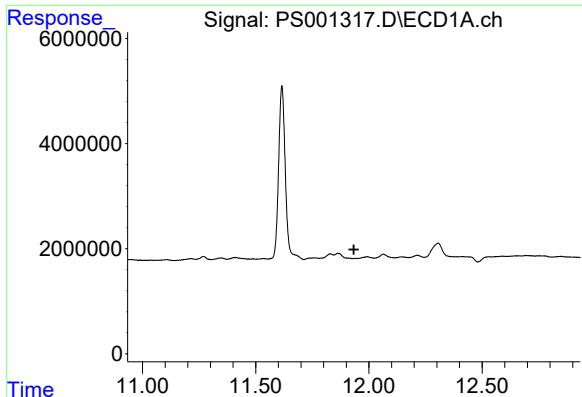

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.934 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

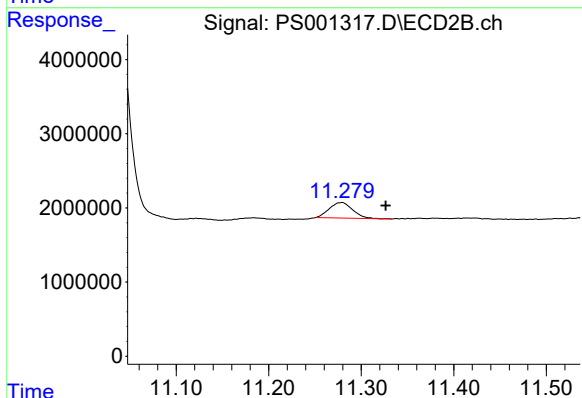


#5 DICAMBA

R.T.: 11.278 min
Delta R.T.: -0.048 min
Response: 3677319
Conc: 5.37 ng/ml

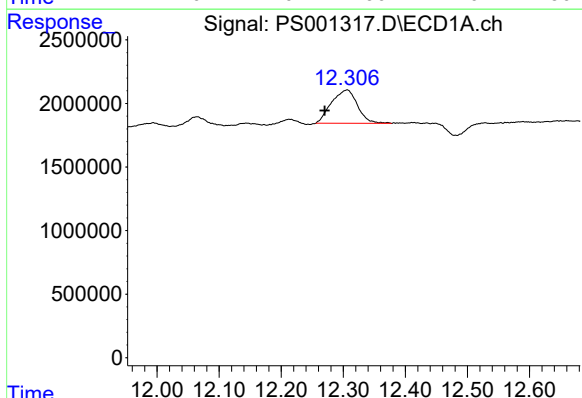


#6 MCP

R.T.: 12.306 min
Delta R.T.: 0.036 min
Response: 7608778
Conc: 15.14 ug/ml

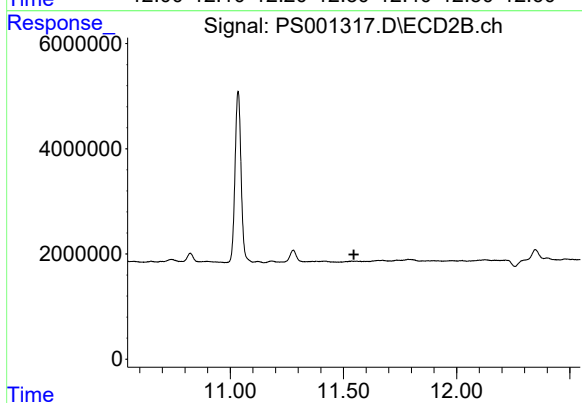

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.546 min
Response: 0
Conc: N.D.

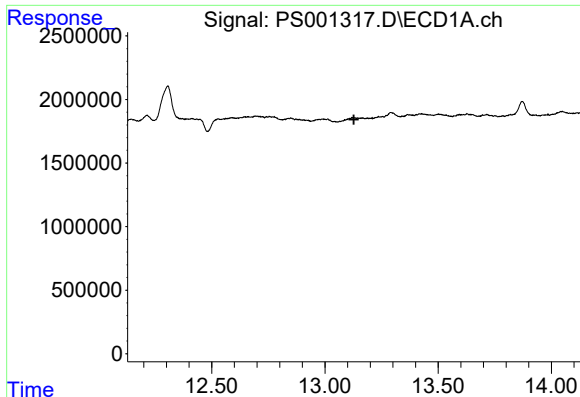

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.128 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

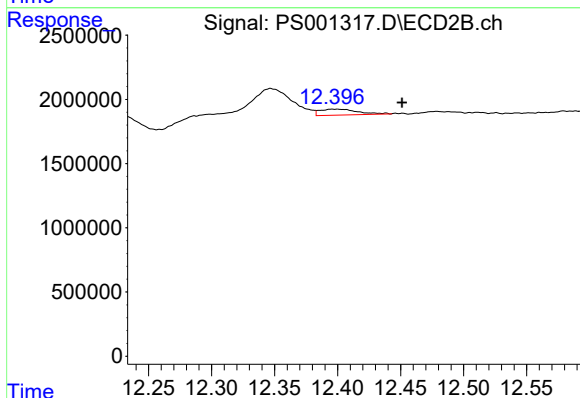


#8 DICHLORPROP

R.T.: 12.398 min
Delta R.T.: -0.053 min
Response: 951939
Conc: 5.37 ng/ml

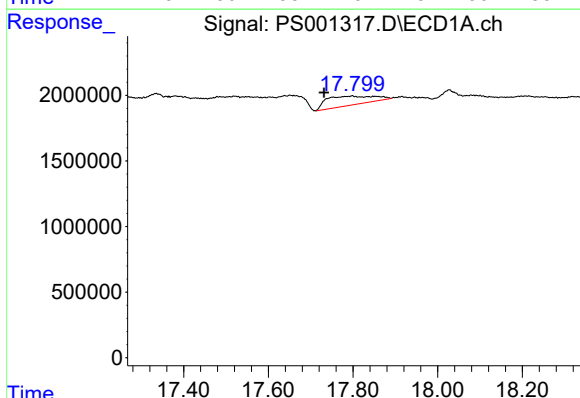

#16 DCPA

R.T.: 17.798 min
Delta R.T.: 0.066 min
Response: 5414830
Conc: 4.01 ng/ml

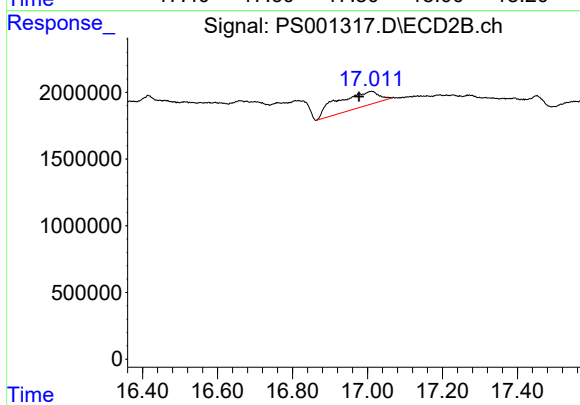

#16 DCPA

R.T.: 17.011 min
Delta R.T.: 0.033 min
Response: 9041270
Conc: 6.26 ng/ml