

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS073118\  
 Data File : PS001318.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 31 Jul 2018 13:29  
 Operator : UA  
 Sample : J4217-04  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jul 31 14:48:52 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS072118.M  
 Quant Title : 8080.M  
 QLast Update : Sat Jul 21 01:18:58 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1   | RT#2   | Resp#1   | Resp#2   | ng/ml   | ng/ml   |
|-----------------------------|--------------|--------|--------|----------|----------|---------|---------|
| -----                       |              |        |        |          |          |         |         |
| System Monitoring Compounds |              |        |        |          |          |         |         |
| 4) S                        | 2,4-DCAA     | 11.635 | 11.056 | 71939425 | 63784711 | 387.709 | 350.707 |
| Target Compounds            |              |        |        |          |          |         |         |
| 5) T                        | DICAMBA      | 0.000  | 11.299 | 0        | 4218228  | N.D.    | 6.155 # |
| 6) T                        | MCPP         | 12.323 | 0.000  | 8782179  | 0        | 17.473  | N.D. #  |
| 11) T                       | 2,4,5-TP ... | 0.000  | 14.033 | 0        | 6249271  | N.D.    | 5.715 # |
| 15) T                       | Picloram     | 0.000  | 16.935 | 0        | 2133172  | N.D.    | 1.547 # |
| 16) T                       | DCPA         | 0.000  | 16.935 | 0        | 2133172  | N.D.    | 1.477 # |
| -----                       |              |        |        |          |          |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS073118\  
Data File : PS001318.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 31 Jul 2018 13:29  
Operator : UA  
Sample : J4217-04  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jul 31 14:48:52 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS072118.M  
Quant Title : 8080.M  
QLast Update : Sat Jul 21 01:18:58 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

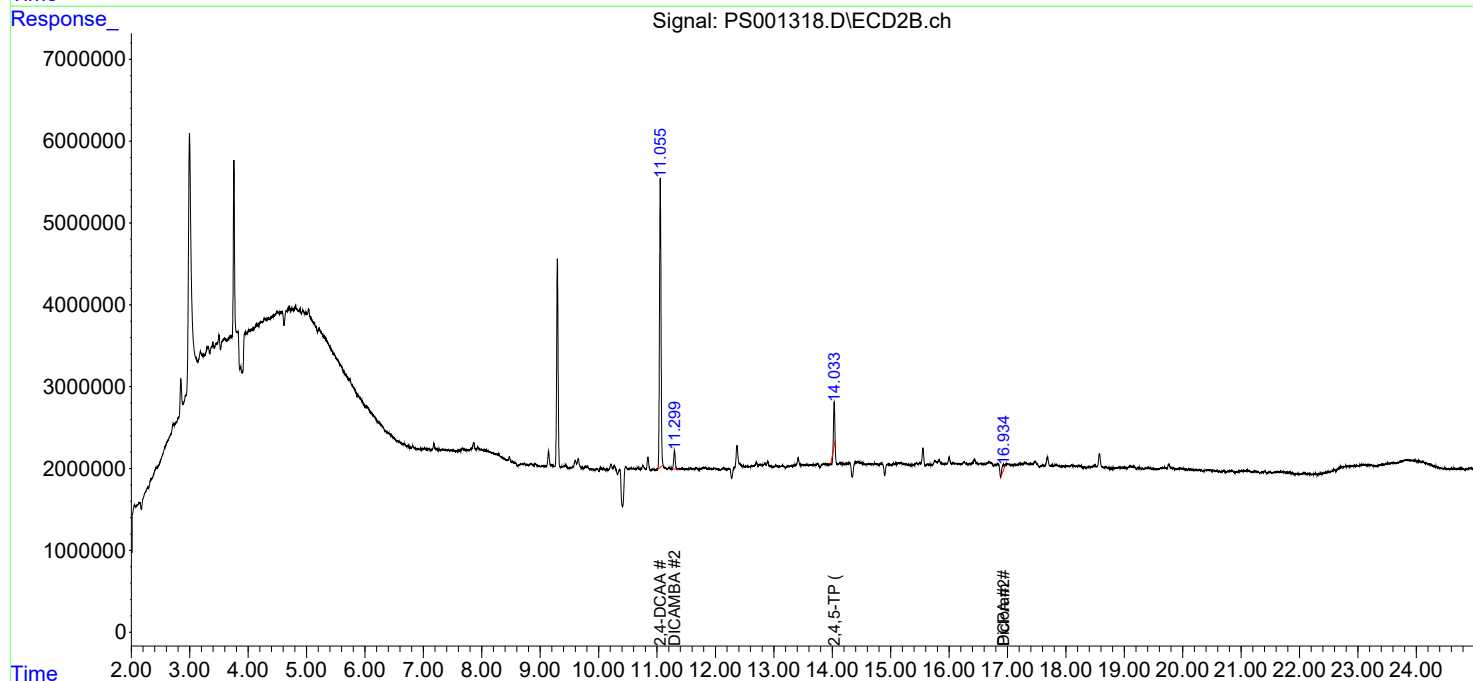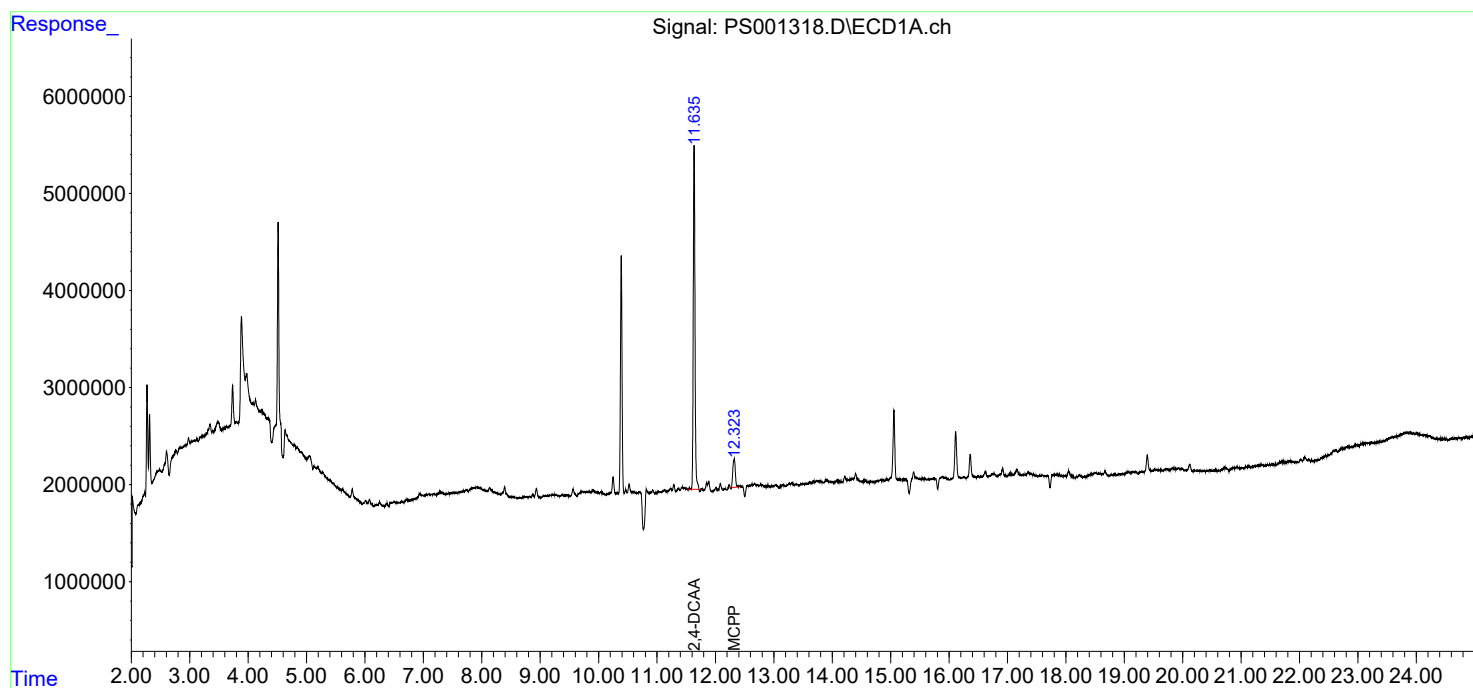


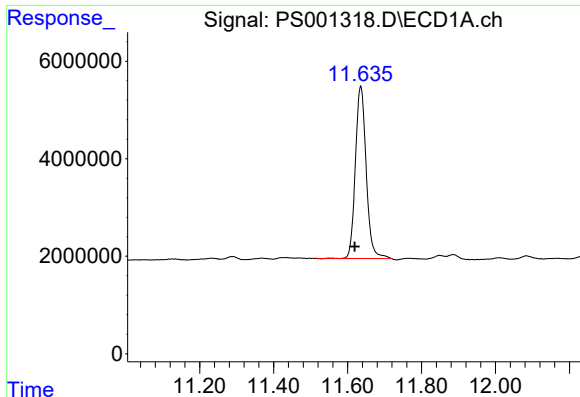

#4 2,4-DCAA


R.T.: 11.635 min  
Delta R.T.: 0.016 min  
Response: 71939425  
Conc: 387.71 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

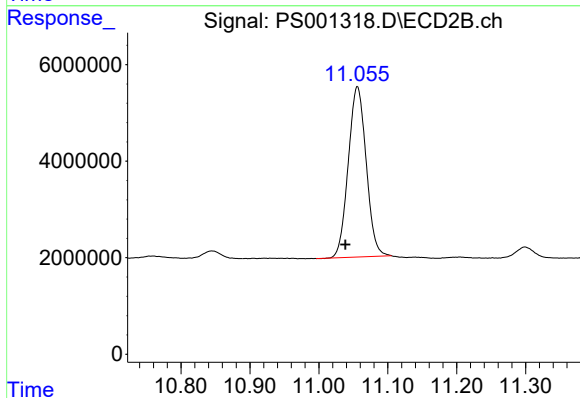


#4 2,4-DCAA

R.T.: 11.056 min  
Delta R.T.: 0.017 min  
Response: 63784711  
Conc: 350.71 ng/ml

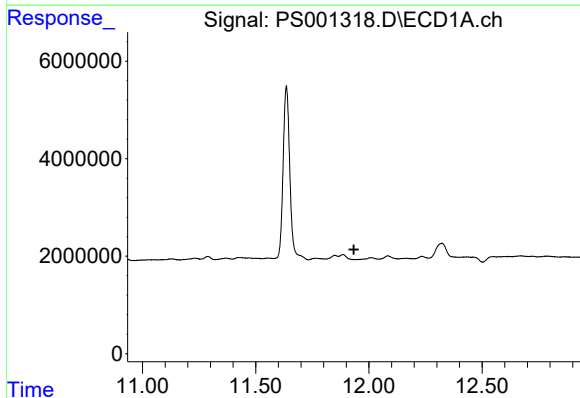


#5 DICAMBA

R.T.: 0.000 min  
Exp R.T. : 11.934 min  
Response: 0  
Conc: N.D.

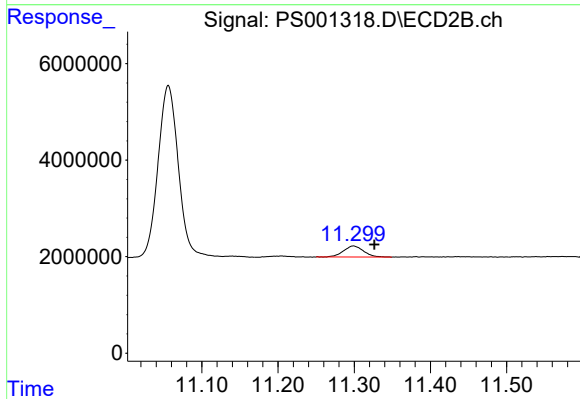

#5 DICAMBA


R.T.: 11.299 min  
Delta R.T.: -0.028 min  
Response: 4218228  
Conc: 6.15 ng/ml

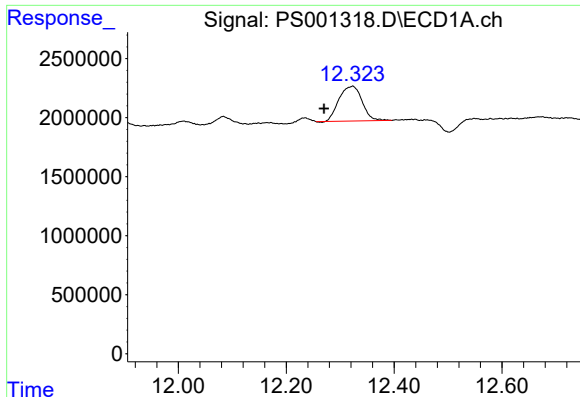

#6 MCPP


R.T.: 12.323 min  
Delta R.T.: 0.052 min  
Response: 8782179  
Conc: 17.47 ug/ml

Instrument :  
ECD\_S  
ClientSampleId :

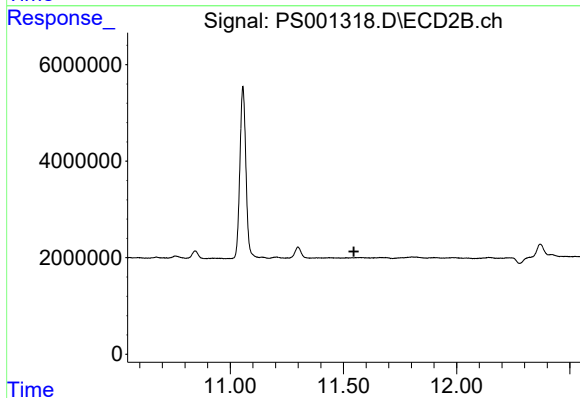


#6 MCPP

R.T.: 0.000 min  
Exp R.T. : 11.546 min  
Response: 0  
Conc: N.D.

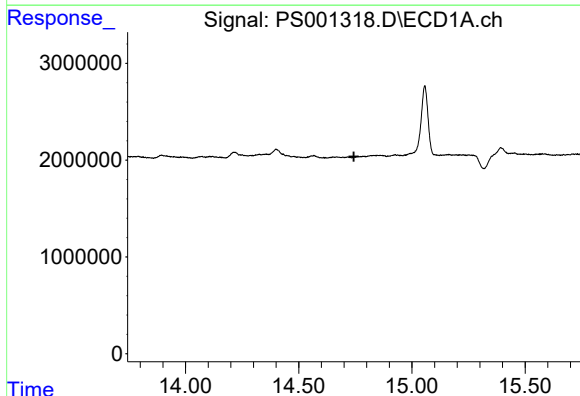


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min  
Exp R.T. : 14.743 min  
Response: 0  
Conc: N.D.

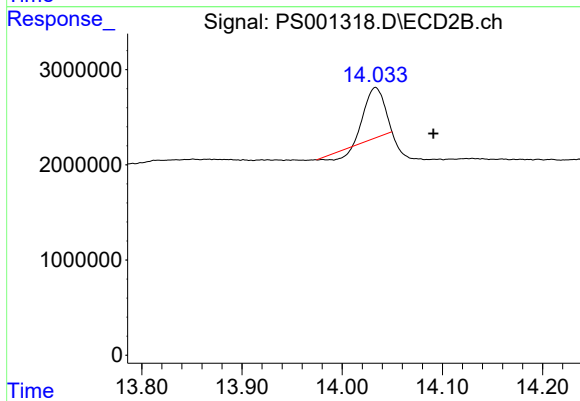

#11 2,4,5-TP (SILVEX)


R.T.: 14.033 min  
Delta R.T.: -0.058 min  
Response: 6249271  
Conc: 5.72 ng/ml

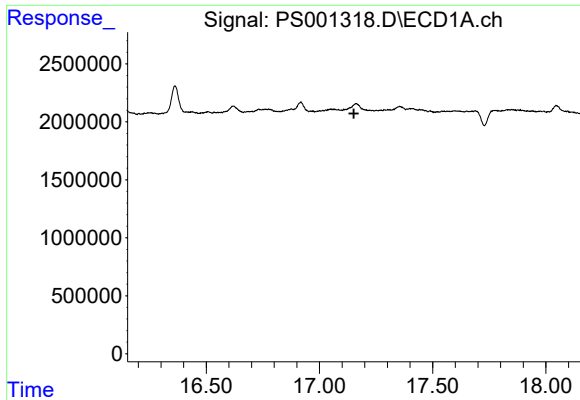

#15 Picloram


R.T.: 0.000 min  
Exp R.T.: 17.152 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

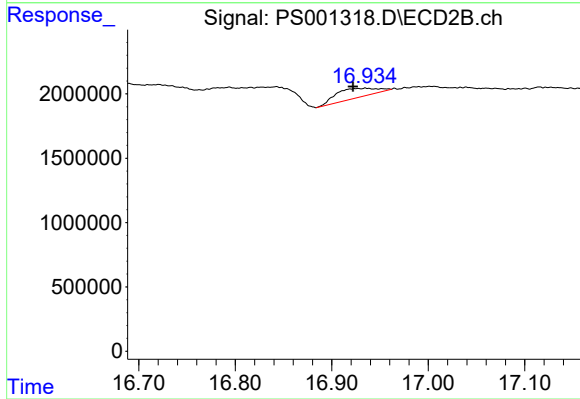


#15 Picloram

R.T.: 16.935 min  
Delta R.T.: 0.013 min  
Response: 2133172  
Conc: 1.55 ng/ml

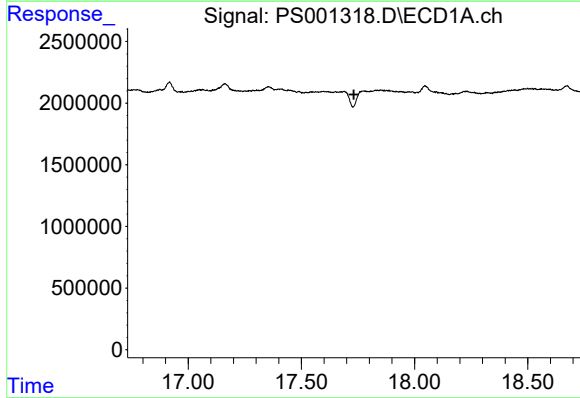

#16 DCPA

R.T.: 0.000 min  
Exp R.T.: 17.732 min  
Response: 0  
Conc: N.D.

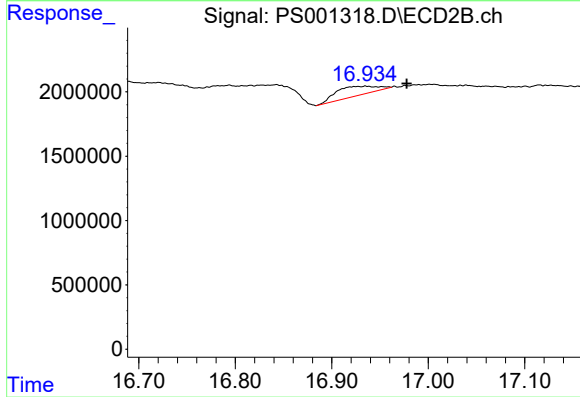

#16 DCPA

R.T.: 16.935 min  
Delta R.T.: -0.043 min  
Response: 2133172  
Conc: 1.48 ng/ml