

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073119\
 Data File : PS005775.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2019 10:30
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 14:25:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.565	5.280	489.0E6	351.7E6	337.076	353.549
Target Compounds							
6) T	MCP	0.000	5.478	0	160.7E6	N.D.	56.423
9) T	2,4-D	6.577	0.000	756.8E6	0	504.979	N.D. #
12) T	2,4,5-T	7.628	0.000	50672206	0	6.071	N.D. #
15) T	Picloram	0.000	9.116	0	82684846	N.D.	11.007



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073119\
Data File : PS005775.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2019 10:30
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 14:25:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

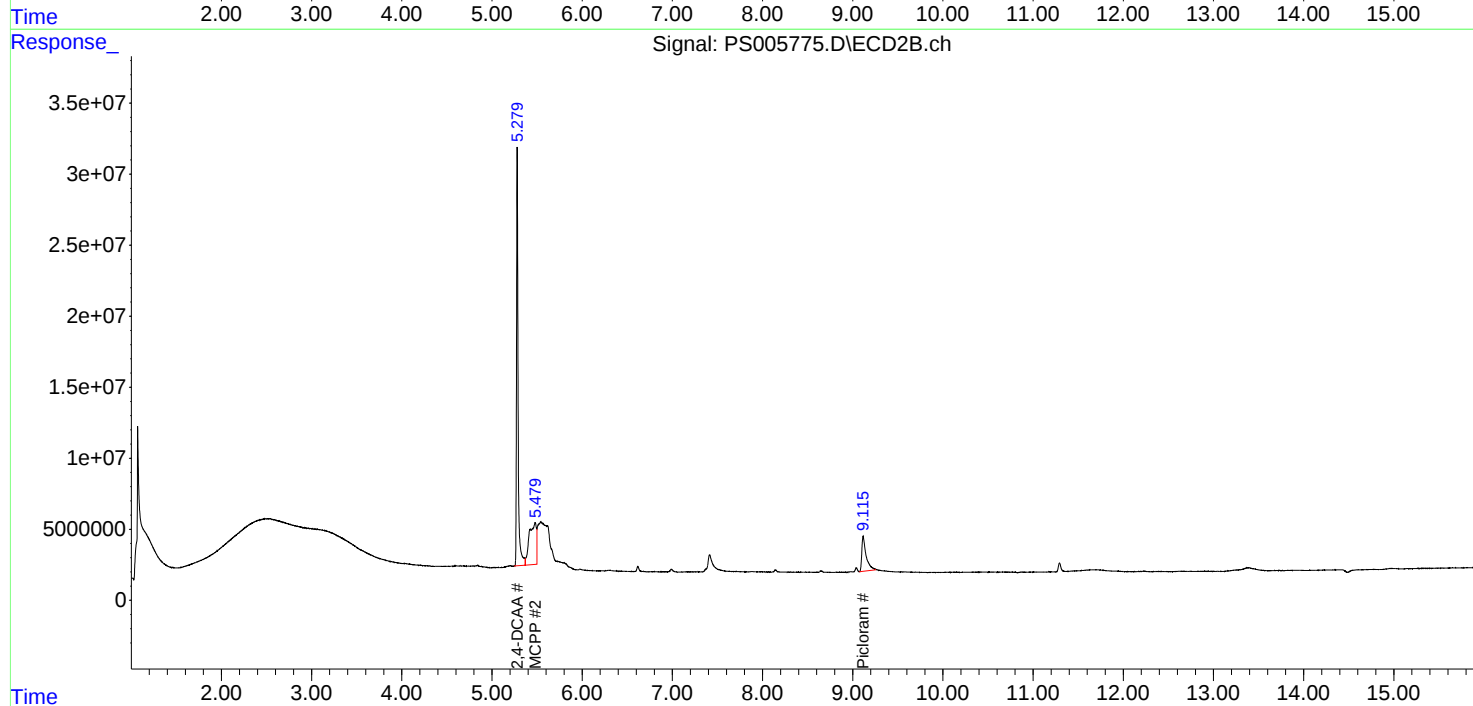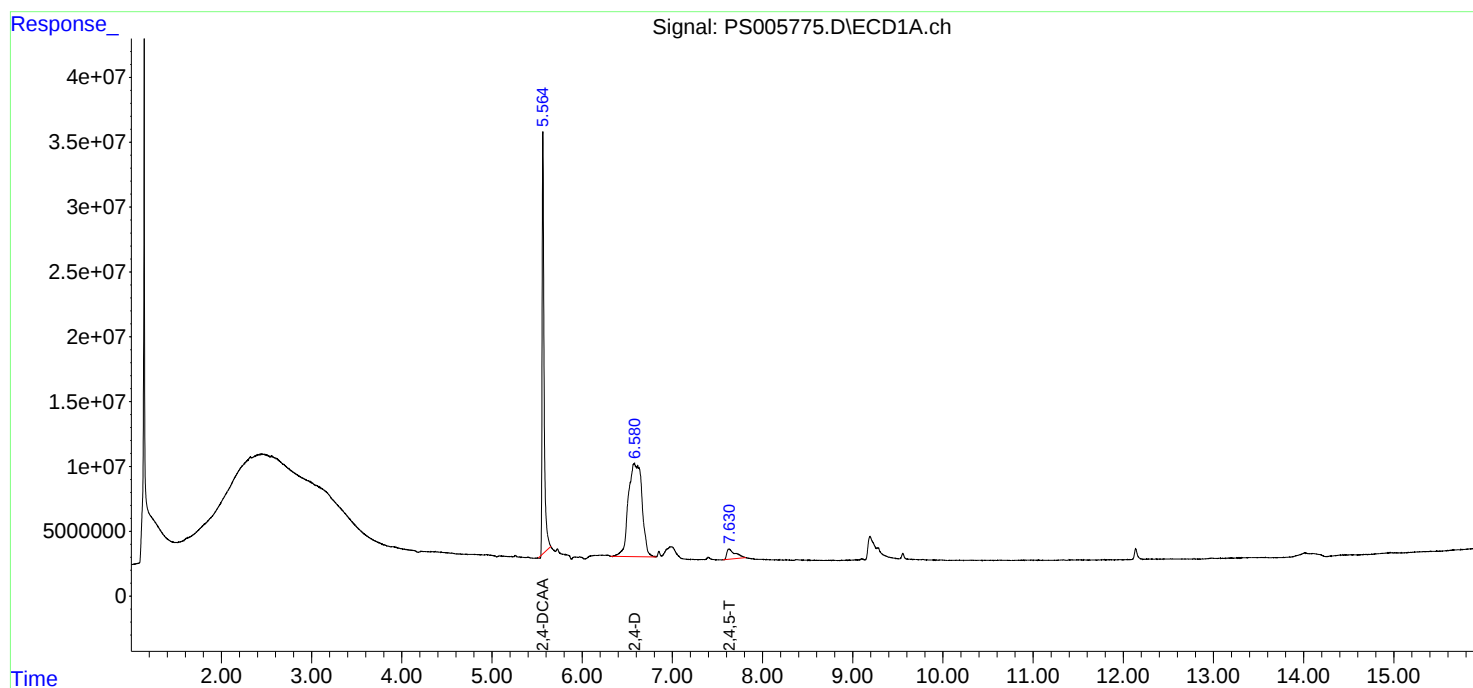


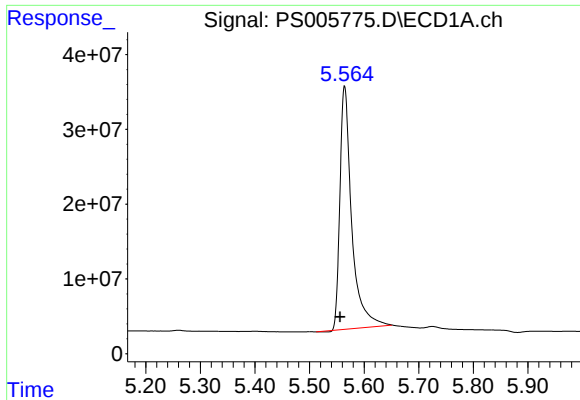

#4 2,4-DCAA


R.T.: 5.565 min
Delta R.T.: 0.009 min
Response: 489036334
Conc: 337.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

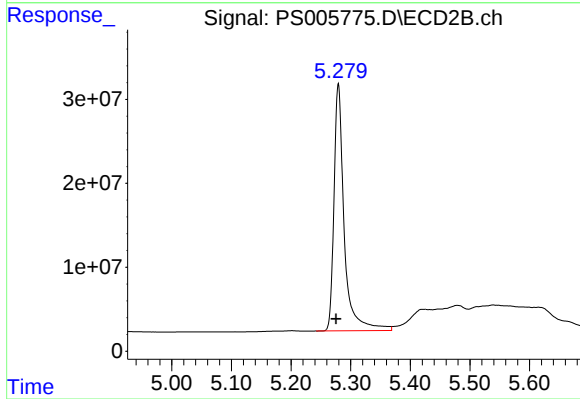


#4 2,4-DCAA

R.T.: 5.280 min
Delta R.T.: 0.004 min
Response: 351667159
Conc: 353.55 ng/ml

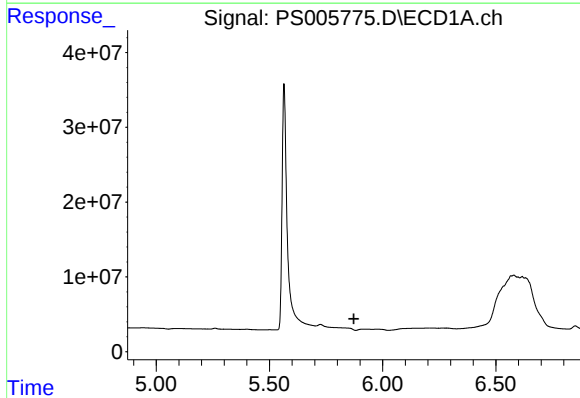


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.873 min
Response: 0
Conc: N.D.

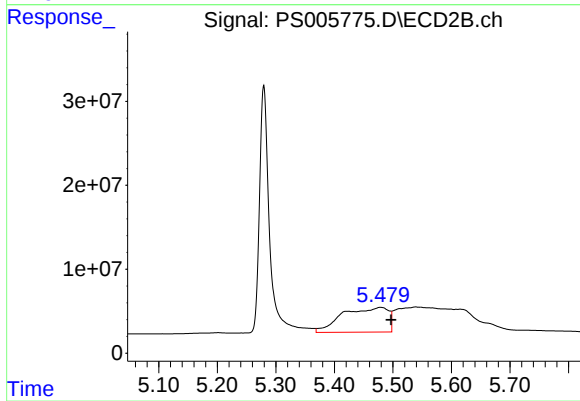

#6 MCP


R.T.: 5.478 min
Delta R.T.: -0.018 min
Response: 160705988
Conc: 56.42 ug/ml

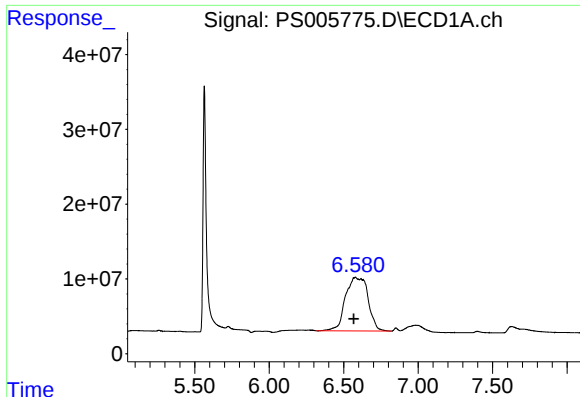

#9 2,4-D


R.T.: 6.577 min
Delta R.T.: 0.008 min
Response: 756795690
Conc: 504.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

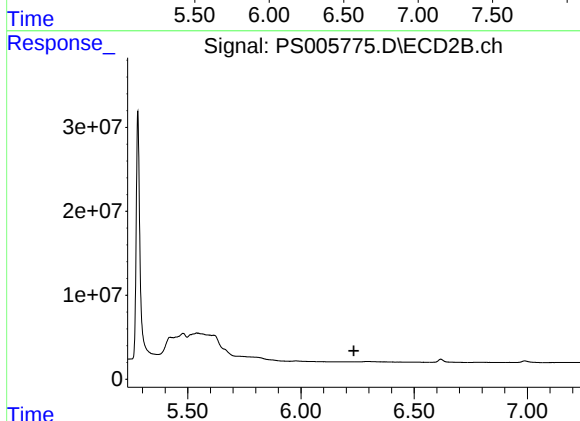


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

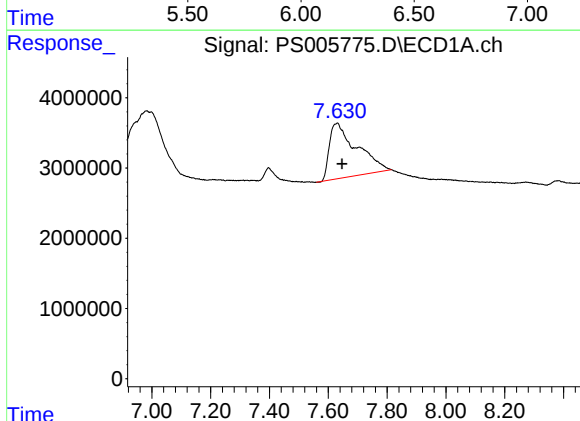


#12 2,4,5-T

R.T.: 7.628 min
Delta R.T.: -0.018 min
Response: 50672206
Conc: 6.07 ng/ml

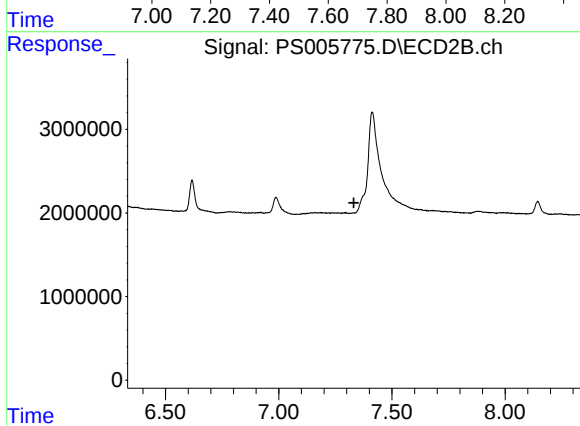

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 7.332 min
Response: 0
Conc: N.D.

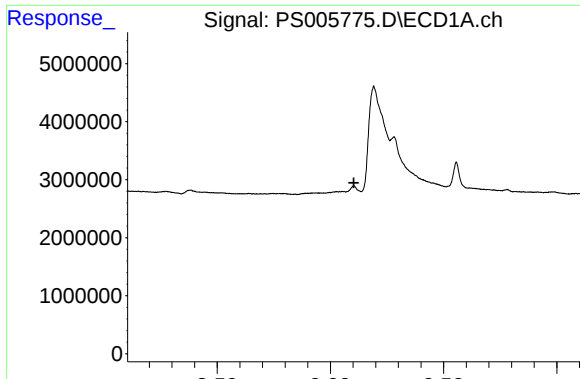

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 9.104 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

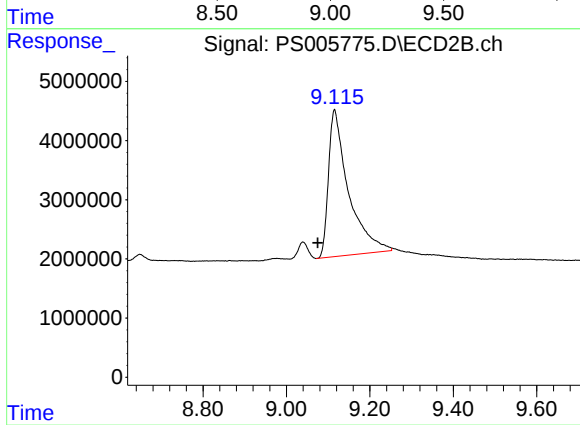

#15 Picloram

R.T.: 9.116 min
Delta R.T.: 0.041 min
Response: 82684846
Conc: 11.01 ng/ml