

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073119\
 Data File : PS005777.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2019 11:54
 Operator : SM\AJ
 Sample : PB121839BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 14:25:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.584	5.298	701.0E6	512.9E6	483.176	515.642
Target Compounds							
2) T	3,5-DICHL...	0.000	4.617	0	31274214	N.D.	24.107
7) T	MCPA	5.991	0.000	37992210	0	5.822	N.D. #
9) T	2,4-D	6.522	6.192	1034.4E6	18151783	690.181	16.896 #
10) T	Pentachlo...	6.872	6.559	21559688	28751213	1.031	2.215 #
12) T	2,4,5-T	7.594	0.000	109.2E6	0	13.088	N.D. #
15) T	Picloram	9.169	9.114	455.2E6	342.5E6	38.889	45.591



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073119\
Data File : PS005777.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2019 11:54
Operator : SM\AJ
Sample : PB121839BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 14:25:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

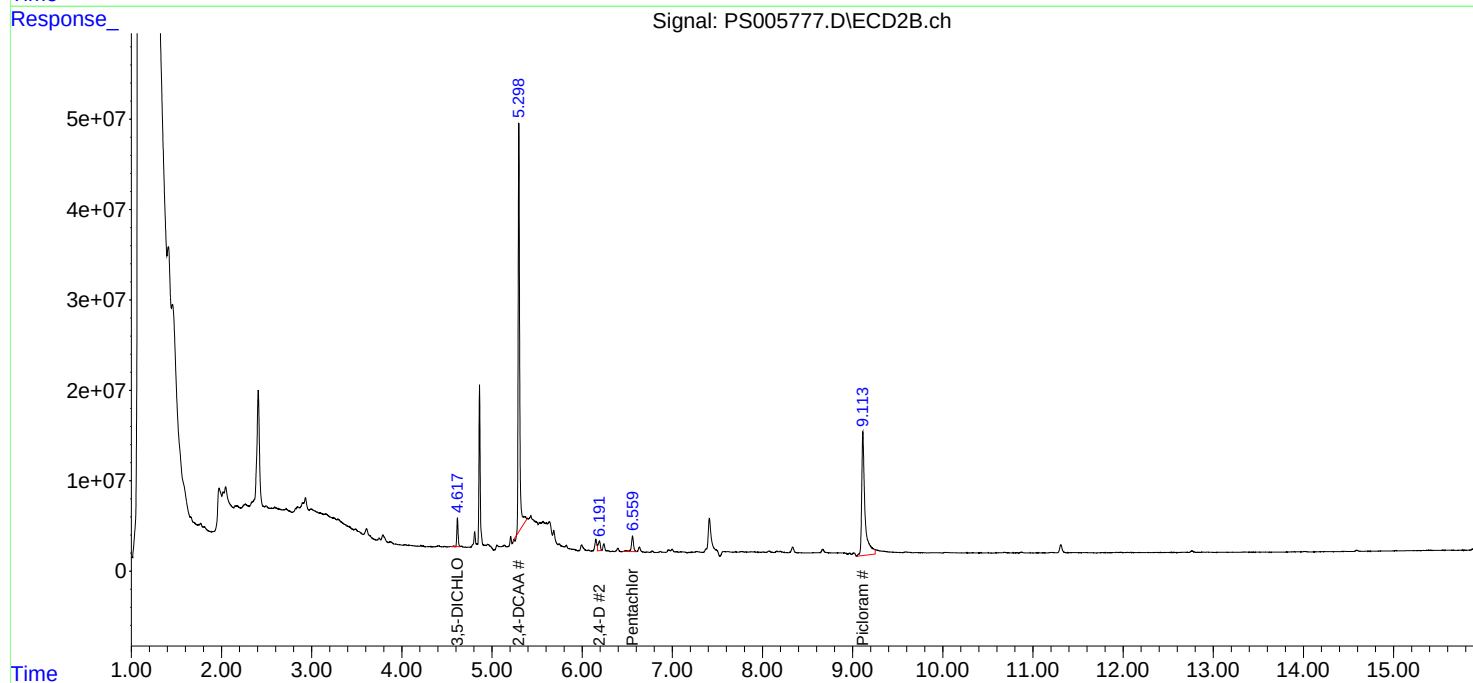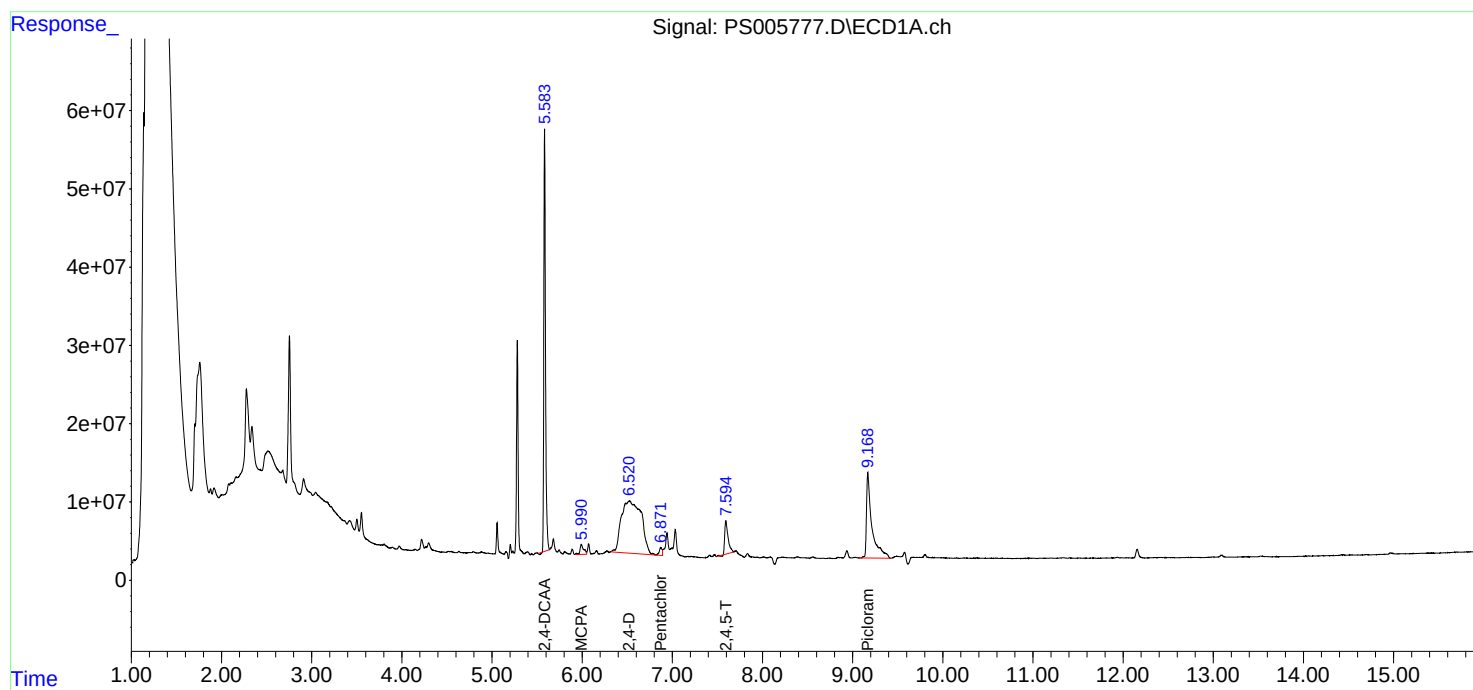


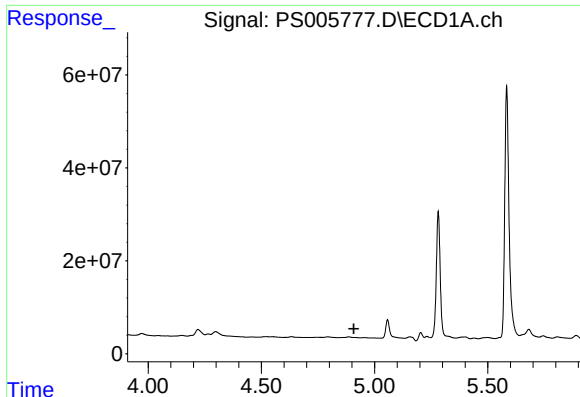

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

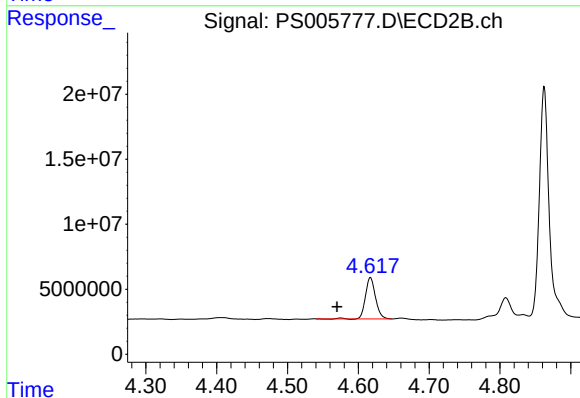


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.617 min
Delta R.T.: 0.047 min
Response: 31274214
Conc: 24.11 ng/ml

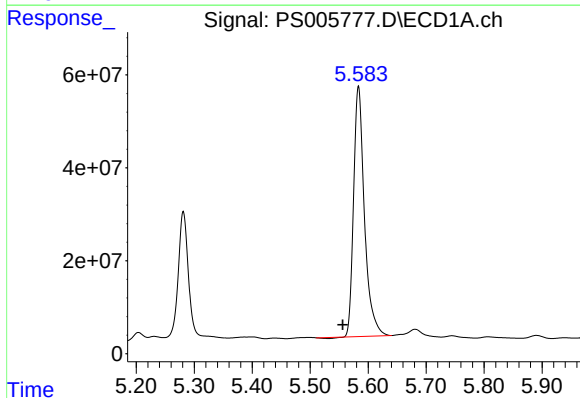


#4 2,4-DCAA

R.T.: 5.584 min
Delta R.T.: 0.027 min
Response: 701000144
Conc: 483.18 ng/ml

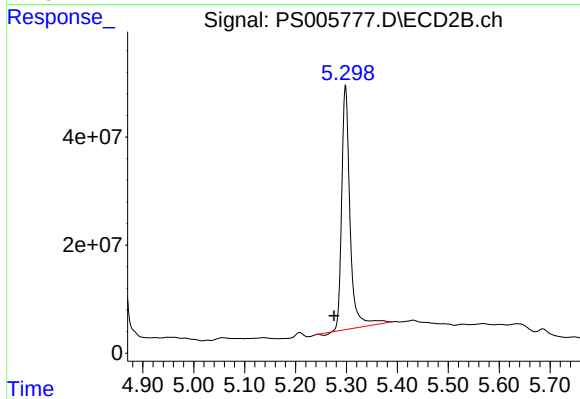

#4 2,4-DCAA


R.T.: 5.298 min
Delta R.T.: 0.022 min
Response: 512897749
Conc: 515.64 ng/ml

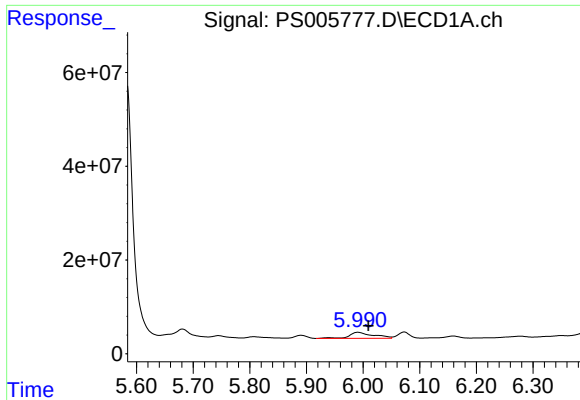

#7 MCPA


R.T.: 5.991 min
Delta R.T.: -0.019 min
Response: 37992210
Conc: 5.82 ug/ml

Instrument :
ECD_S
ClientSampleId :

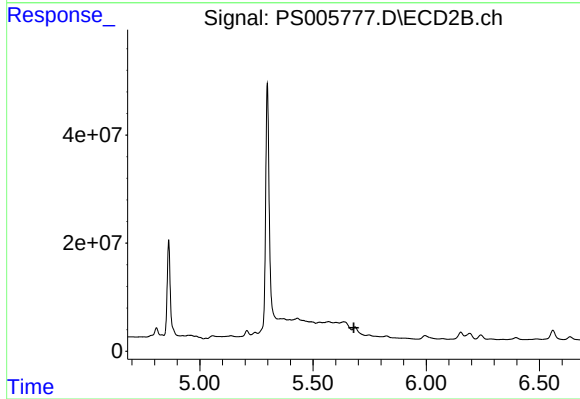


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.681 min
Response: 0
Conc: N.D.

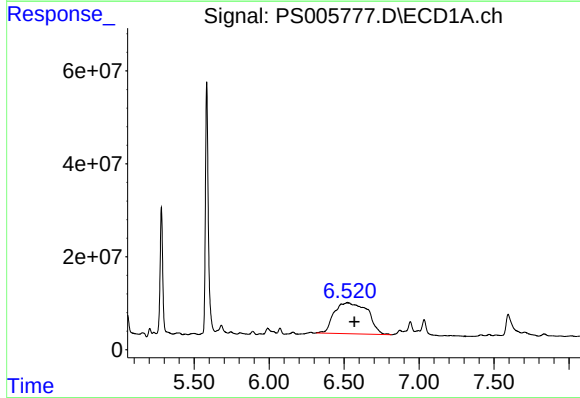


#9 2,4-D

R.T.: 6.522 min
Delta R.T.: -0.047 min
Response: 1034352828
Conc: 690.18 ng/ml

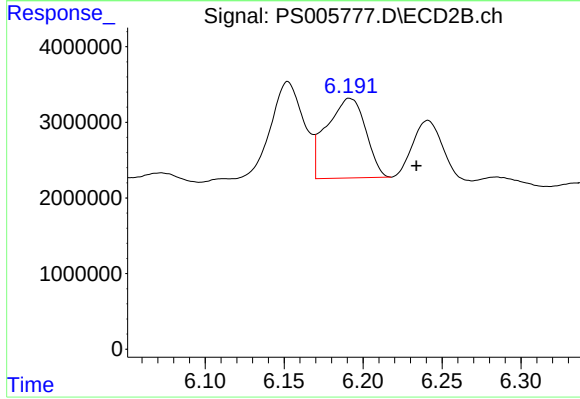

#9 2,4-D


R.T.: 6.192 min
Delta R.T.: -0.042 min
Response: 18151783
Conc: 16.90 ng/ml

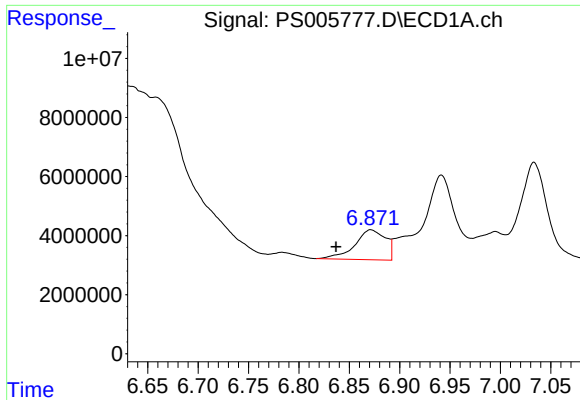

#10 Pentachlorophenol


R.T.: 6.872 min
Delta R.T.: 0.035 min
Response: 21559688
Conc: 1.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

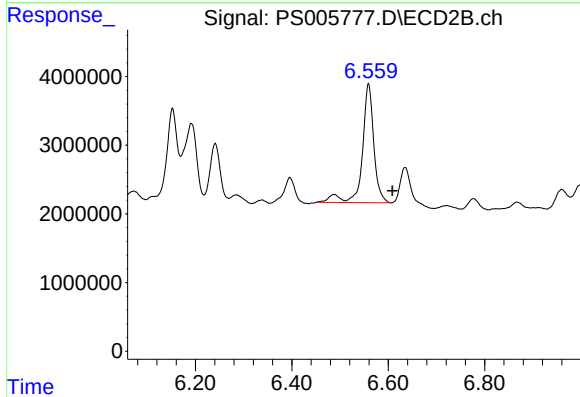


#10 Pentachlorophenol

R.T.: 6.559 min
Delta R.T.: -0.049 min
Response: 28751213
Conc: 2.21 ng/ml

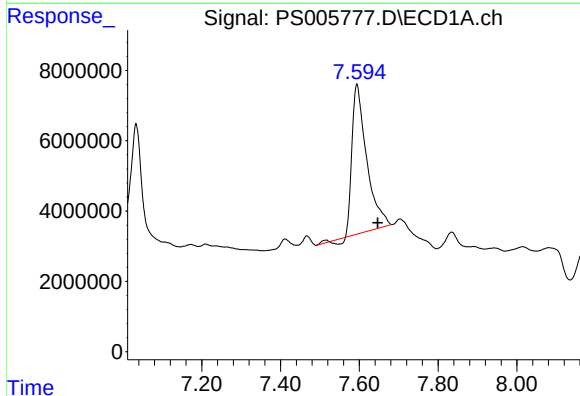


#12 2,4,5-T

R.T.: 7.594 min
Delta R.T.: -0.053 min
Response: 109245857
Conc: 13.09 ng/ml

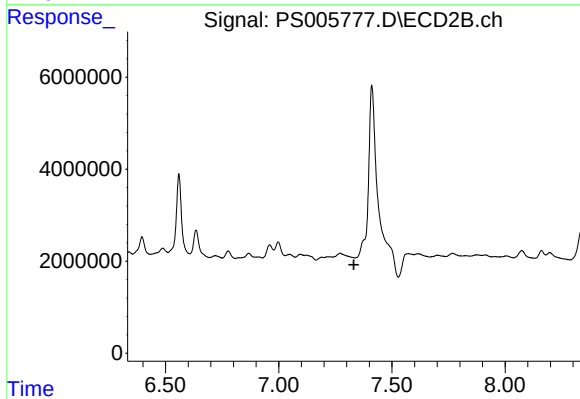

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.332 min
Response: 0
Conc: N.D.

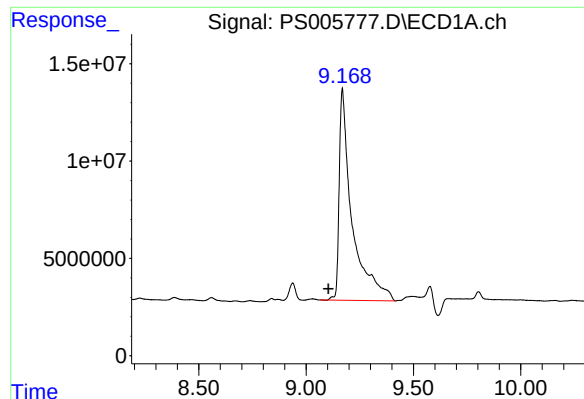

#15 Picloram

R.T.: 9.169 min
Delta R.T.: 0.065 min
Response: 455198746
Conc: 38.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

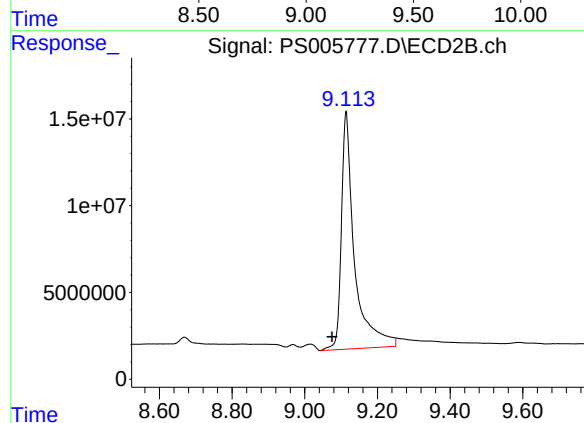

#15 Picloram

R.T.: 9.114 min
Delta R.T.: 0.039 min
Response: 342491004
Conc: 45.59 ng/ml