

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073119\
 Data File : PS005779.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2019 12:38
 Operator : SM\AJ
 Sample : PB121839TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 14:26:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.577	5.296	153.5E6	114.5E6	105.773	115.069
Target Compounds							
2) T	3,5-DICHL...	0.000	4.614	0 45586517		N.D.	35.139
5) T	DICAMBA	0.000	5.427	0 28774191		N.D.	7.708
6) T	MCP	0.000	5.427	0 28774191		N.D.	10.102
7) T	MCPA	5.976	5.678	21328888 55017818		3.268	13.071 #
8) T	DICHLORPROP	0.000	5.985	0 16419101		N.D.	17.779
10) T	Pentachlo...	0.000	6.555	0 23812155		N.D.	1.834
12) T	2,4,5-T	7.578	0.000	49620378	0	5.945	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073119\
Data File : PS005779.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2019 12:38
Operator : SM\AJ
Sample : PB121839TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 14:26:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

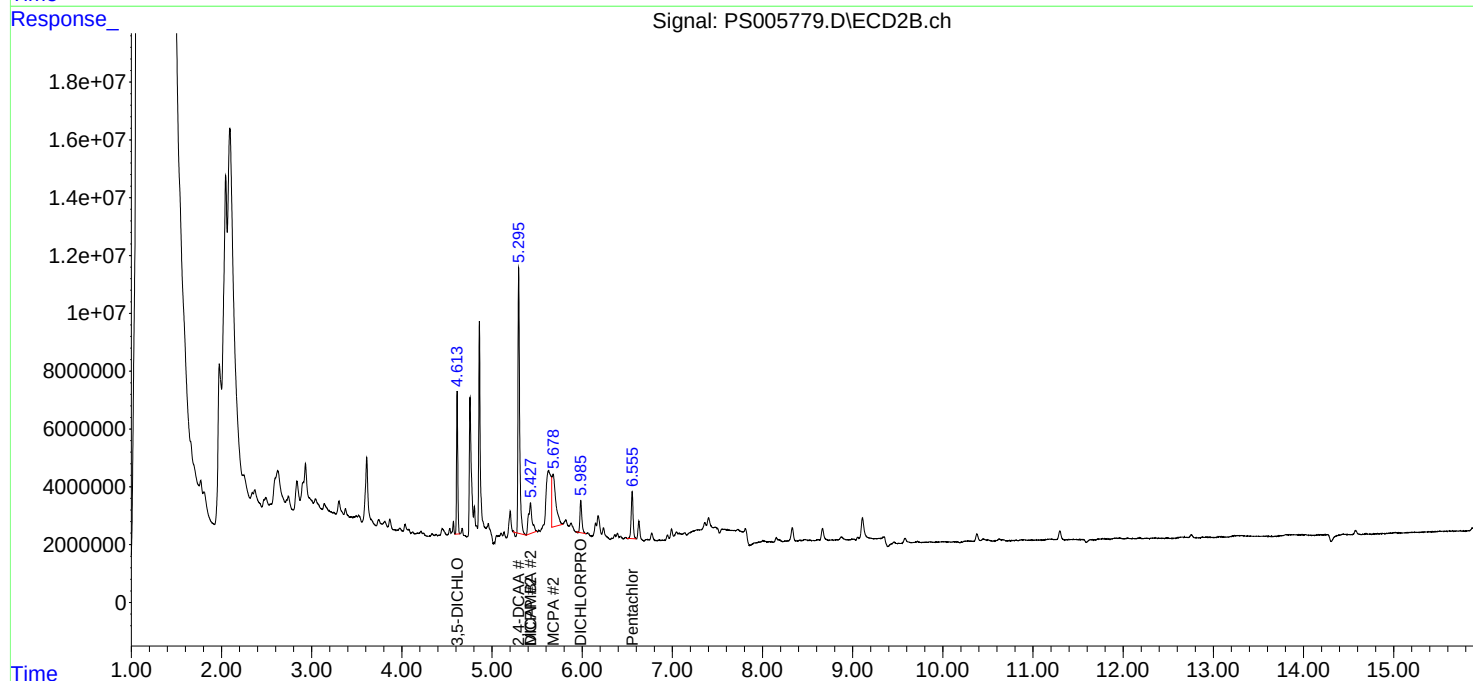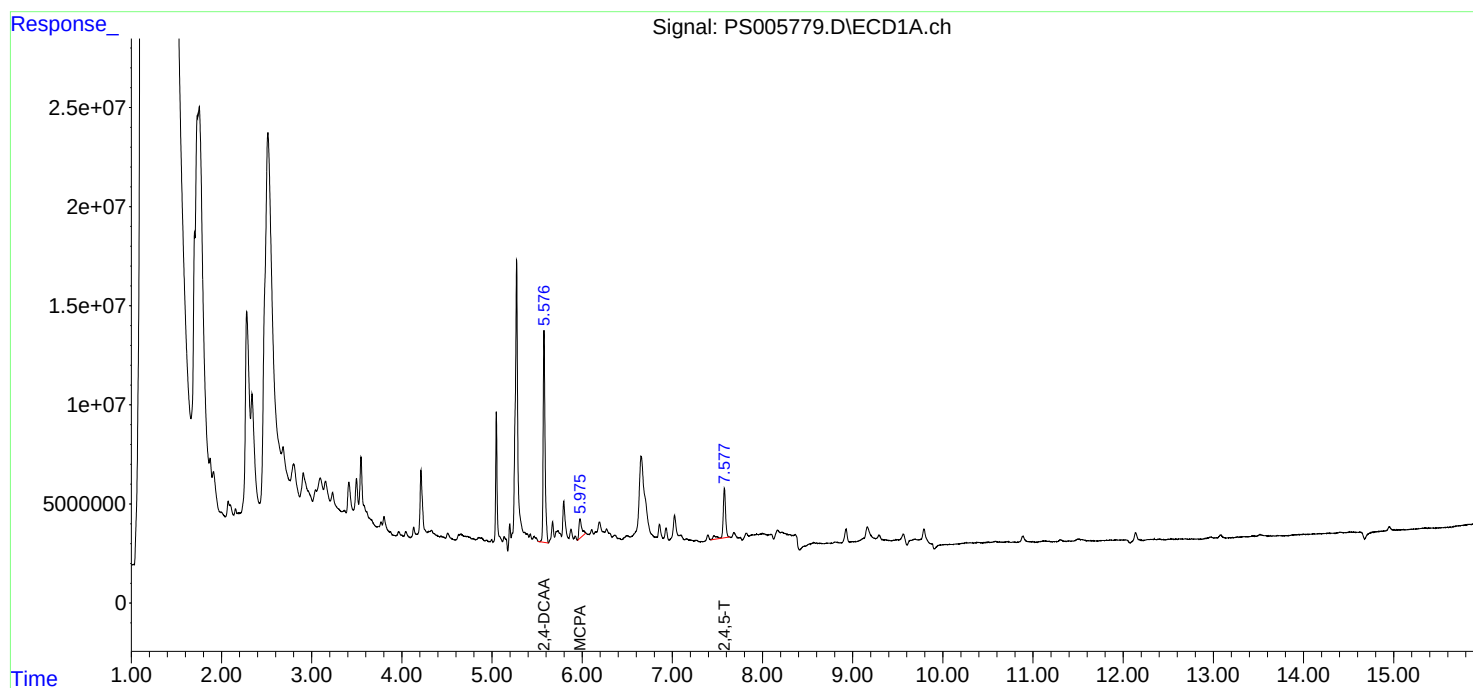


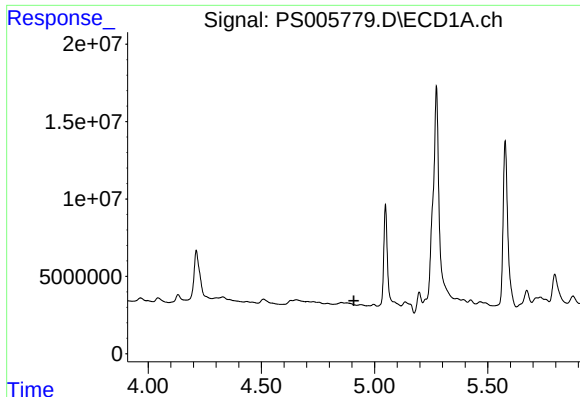

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

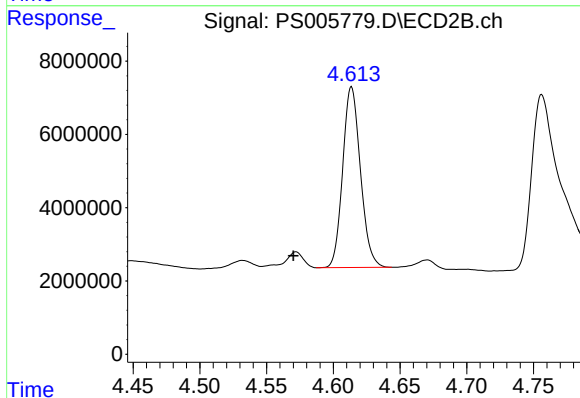


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.614 min
Delta R.T.: 0.044 min
Response: 45586517
Conc: 35.14 ng/ml

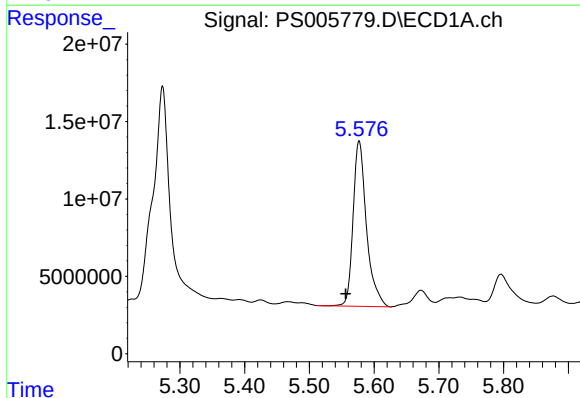


#4 2,4-DCAA

R.T.: 5.577 min
Delta R.T.: 0.021 min
Response: 153456797
Conc: 105.77 ng/ml

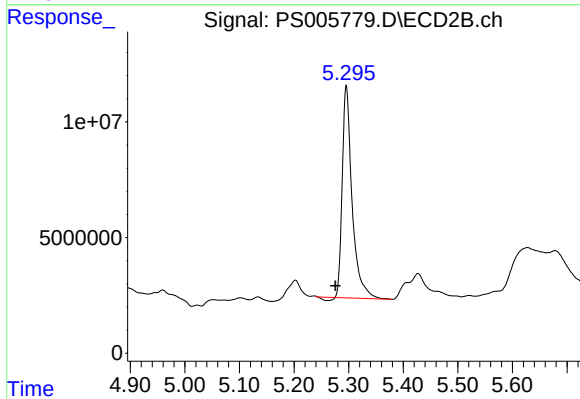

#4 2,4-DCAA


R.T.: 5.296 min
Delta R.T.: 0.020 min
Response: 114456681
Conc: 115.07 ng/ml

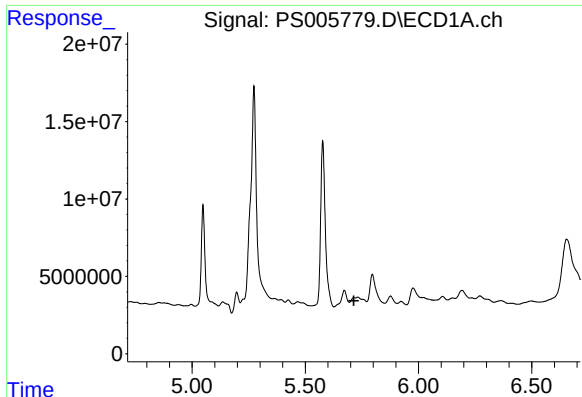

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.714 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

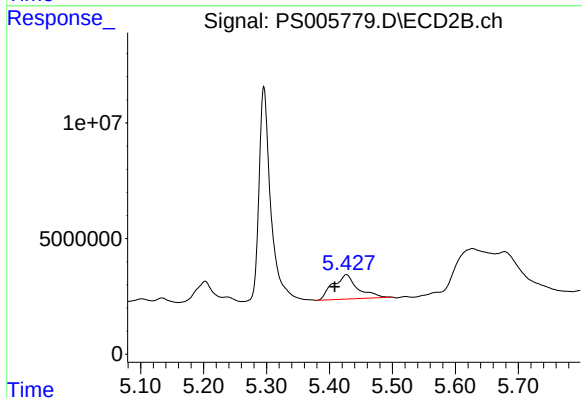


#5 DICAMBA

R.T.: 5.427 min
Delta R.T.: 0.019 min
Response: 28774191
Conc: 7.71 ng/ml

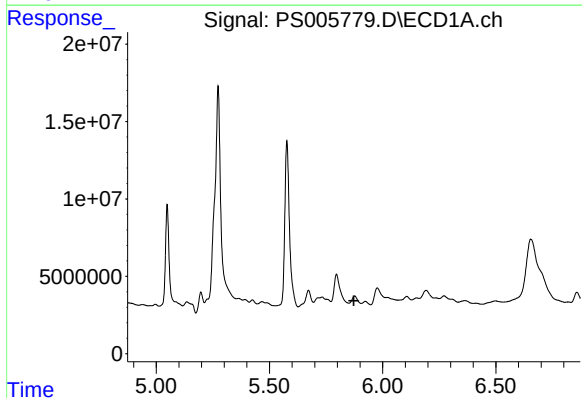


#6 MCP

R.T.: 0.000 min
Exp R.T.: 5.873 min
Response: 0
Conc: N.D.

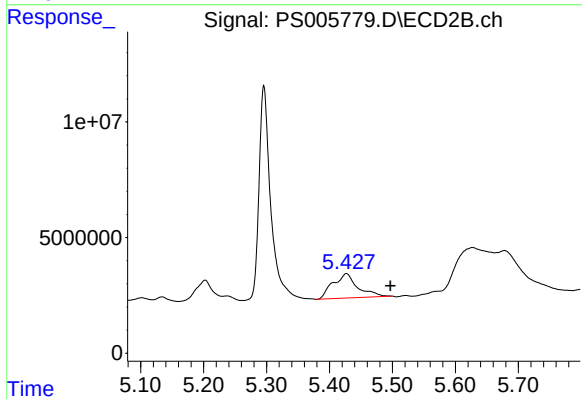

#6 MCP


R.T.: 5.427 min
Delta R.T.: -0.070 min
Response: 28774191
Conc: 10.10 ug/ml

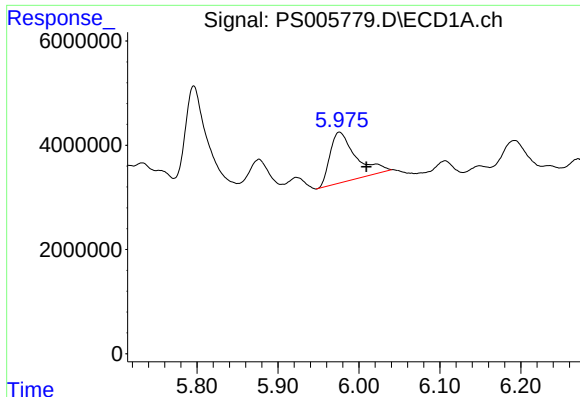

#7 MCPA


R.T.: 5.976 min
Delta R.T.: -0.033 min
Response: 21328888
Conc: 3.27 ug/ml

Instrument :
ECD_S
ClientSampleId :

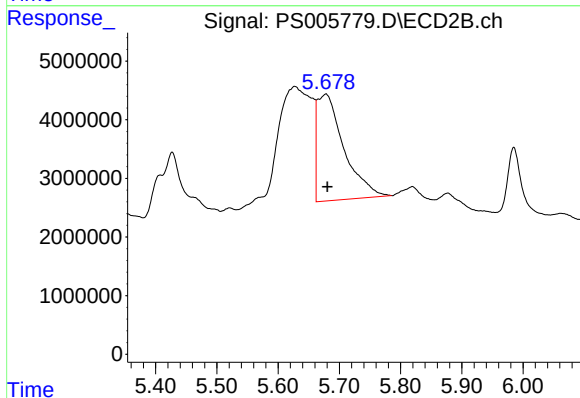


#7 MCPA

R.T.: 5.678 min
Delta R.T.: -0.003 min
Response: 55017818
Conc: 13.07 ug/ml

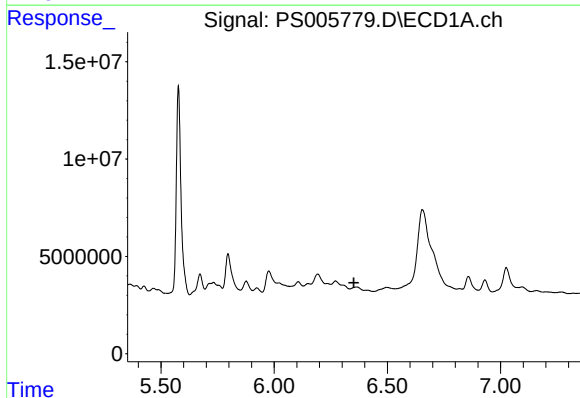


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.352 min
Response: 0
Conc: N.D.

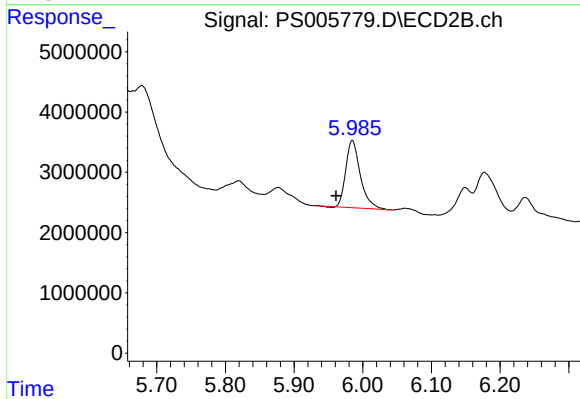

#8 DICHLORPROP


R.T.: 5.985 min
Delta R.T.: 0.024 min
Response: 16419101
Conc: 17.78 ng/ml

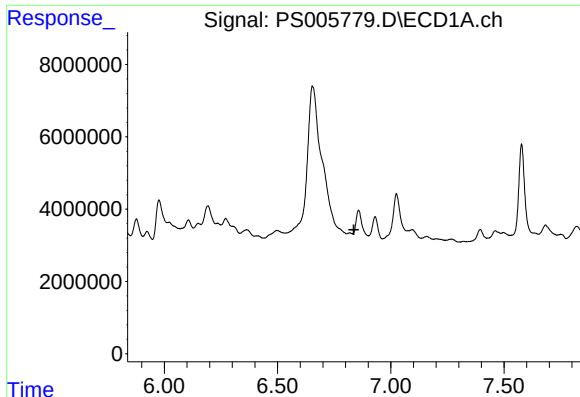

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

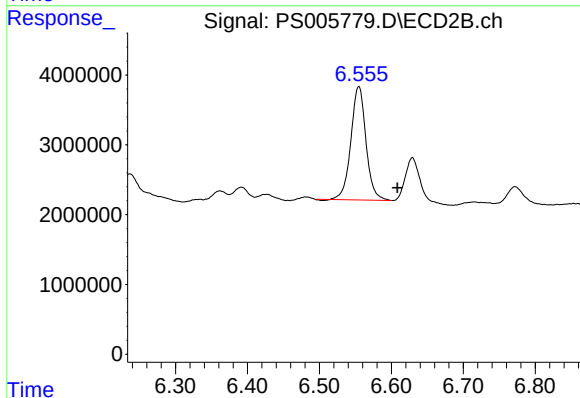


#10 Pentachlorophenol

R.T.: 6.555 min
Delta R.T.: -0.054 min
Response: 23812155
Conc: 1.83 ng/ml

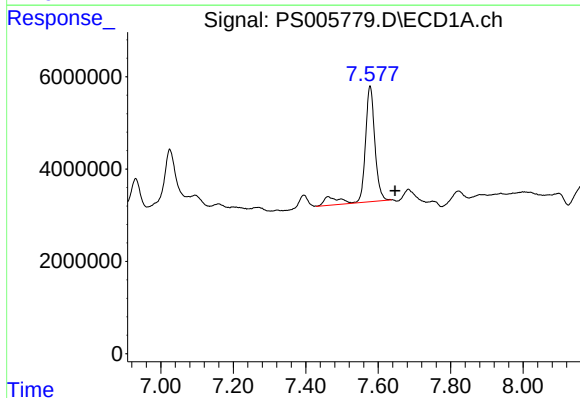

#12 2,4,5-T

R.T.: 7.578 min
Delta R.T.: -0.069 min
Response: 49620378
Conc: 5.94 ng/ml

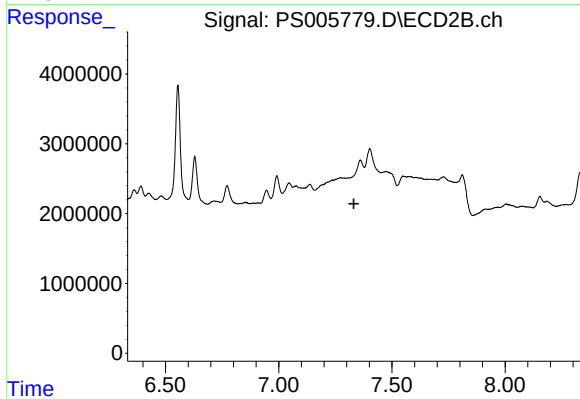

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.332 min
Response: 0
Conc: N.D.