

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073119\
 Data File : PS005785.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2019 14:51
 Operator : SM\AJ
 Sample : K4045-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 GW8-20190726

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 17:24:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.576	5.295	769.2E6	506.7E6	530.204	509.416
Target Compounds							
2) T	3,5-DICHL...	0.000	4.616	0	29177046	N.D.	22.490
6) T	MCP	5.883	0.000	14293381	0	3.085	N.D. #
7) T	MCPA	5.981	5.683	16485877	38628438	2.526	9.178 #
9) T	2,4-D	0.000	6.237	0	16476073	N.D.	15.337
10) T	Pentachlo...	0.000	6.556	0	22275420	N.D.	1.716
12) T	2,4,5-T	7.579	0.000	29618100	0	3.548	N.D. #
15) T	Picloram	0.000	9.097	0	17793761	N.D.	2.369
16) T	DCPA	0.000	9.097	0	17793761	N.D.	2.698



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073119\
Data File : PS005785.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2019 14:51
Operator : SM\AJ
Sample : K4045-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
GW8-20190726

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 17:24:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

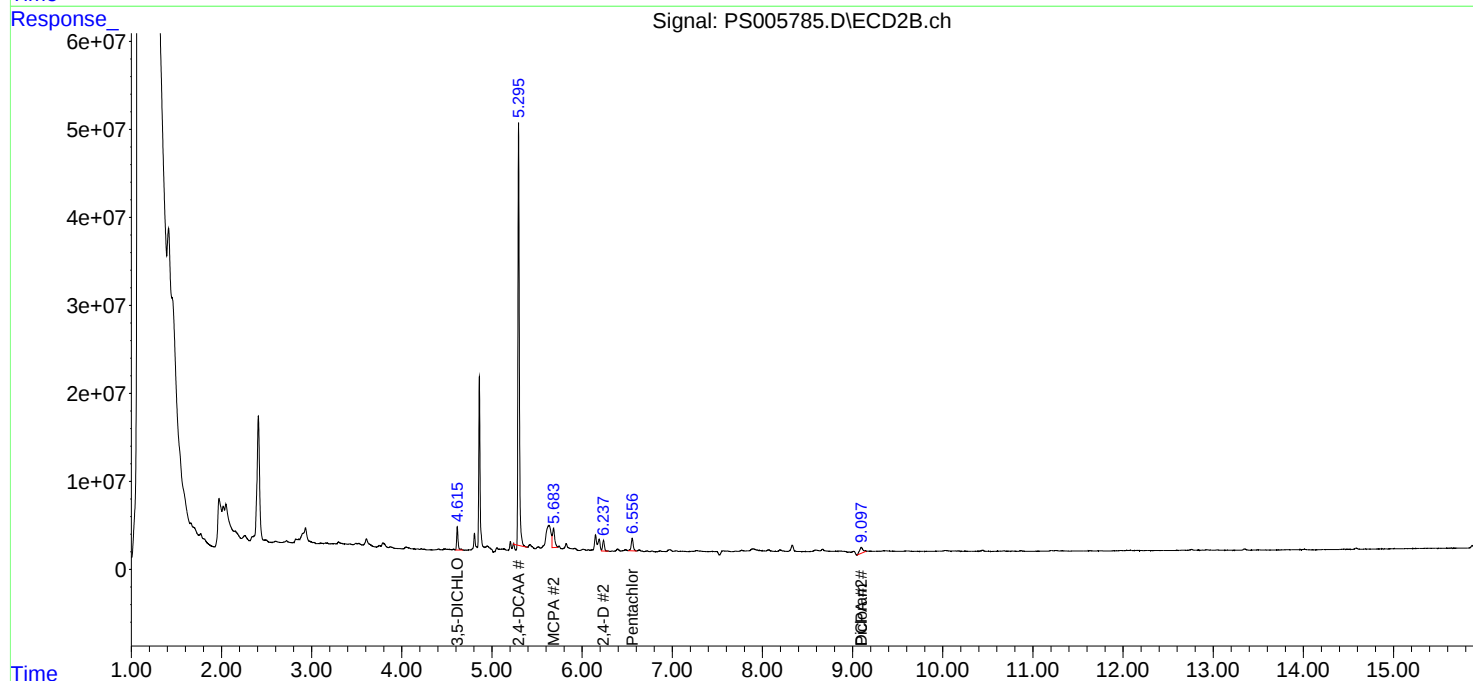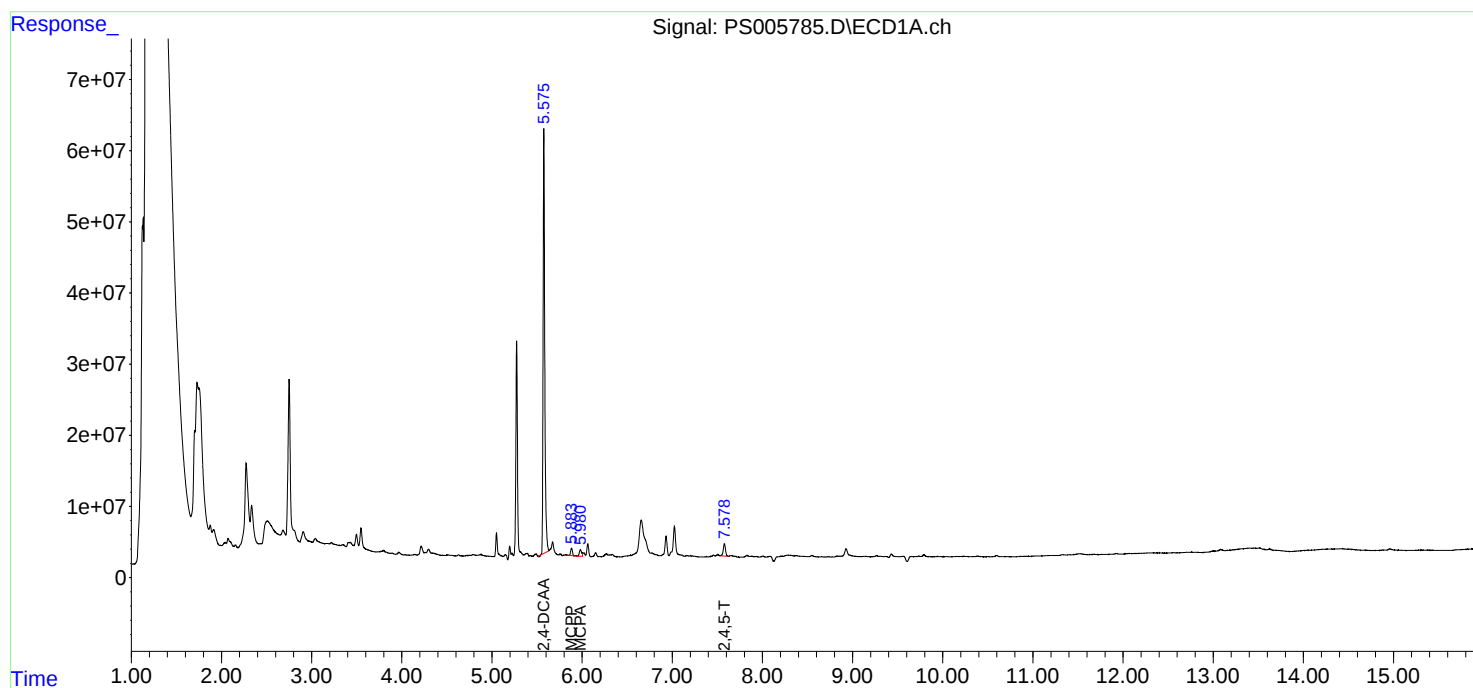


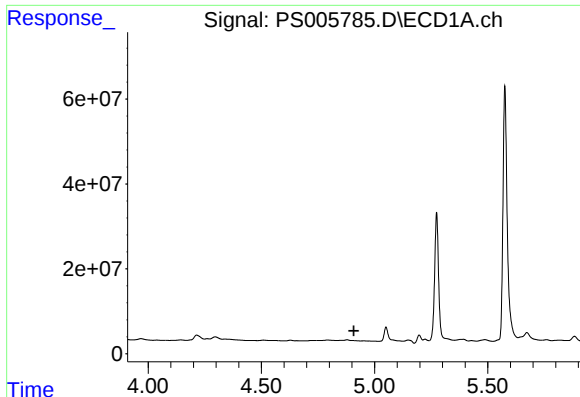

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
GW8-20190726

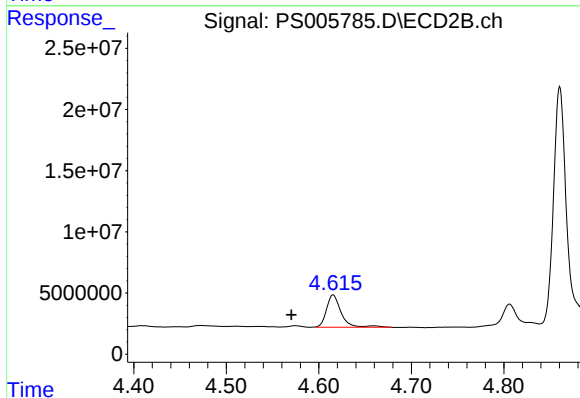


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.616 min
Delta R.T.: 0.045 min
Response: 29177046
Conc: 22.49 ng/ml

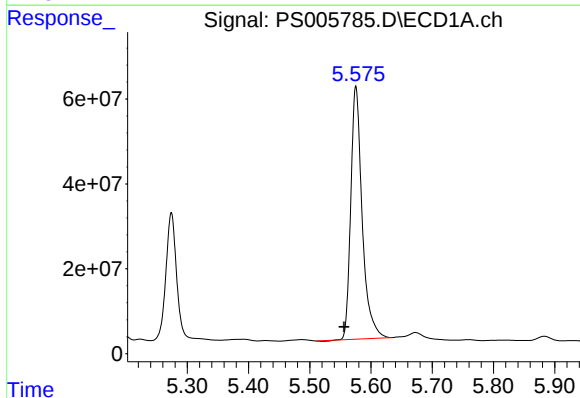


#4 2,4-DCAA

R.T.: 5.576 min
Delta R.T.: 0.019 min
Response: 769229133
Conc: 530.20 ng/ml

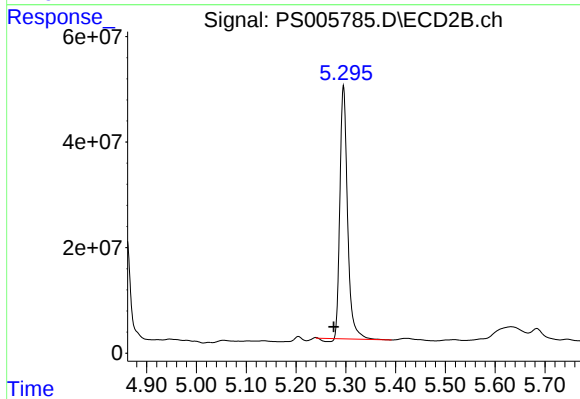

#4 2,4-DCAA


R.T.: 5.295 min
Delta R.T.: 0.020 min
Response: 506705331
Conc: 509.42 ng/ml

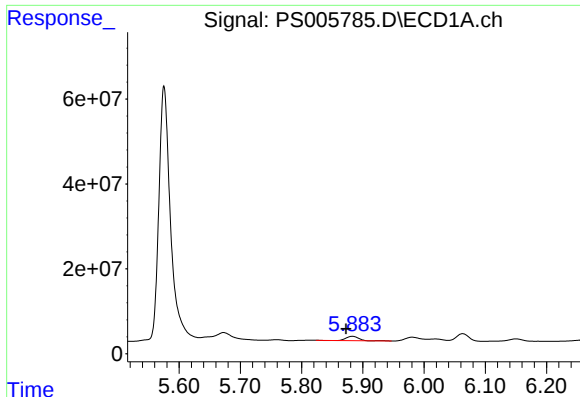

#6 MCPP


R.T.: 5.883 min
Delta R.T.: 0.010 min
Response: 14293381
Conc: 3.08 ug/ml

Instrument :
ECD_S
ClientSampleId :
GW8-20190726

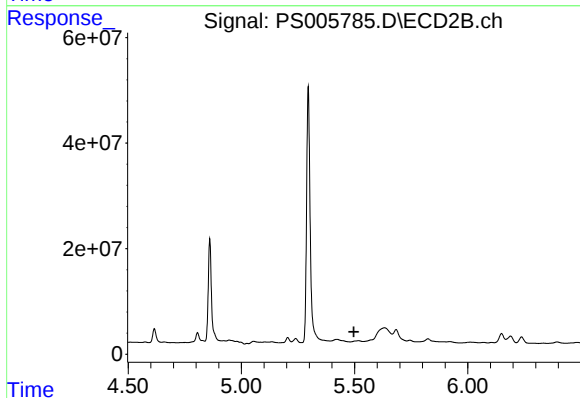


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

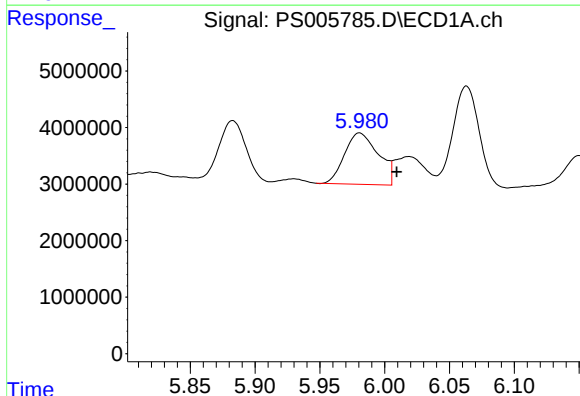


#7 MCPA

R.T.: 5.981 min
Delta R.T.: -0.029 min
Response: 16485877
Conc: 2.53 ug/ml

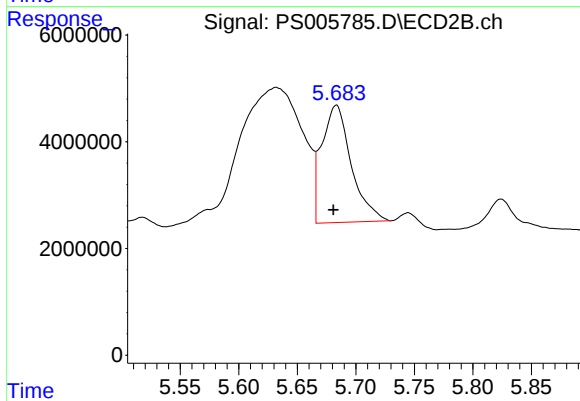

#7 MCPA


R.T.: 5.683 min
Delta R.T.: 0.002 min
Response: 38628438
Conc: 9.18 ug/ml

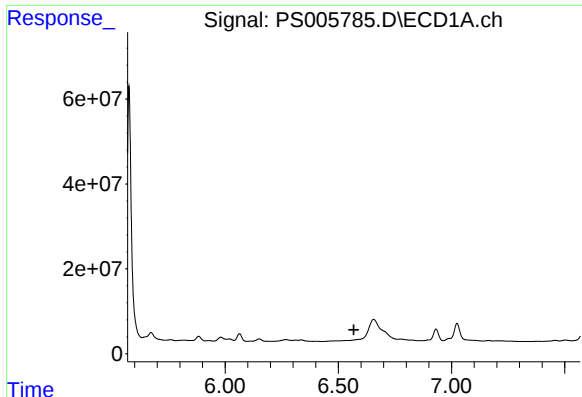

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
GW8-20190726

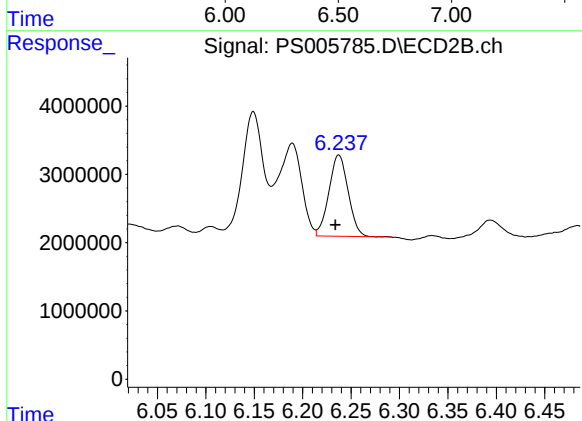


#9 2,4-D

R.T.: 6.237 min
Delta R.T.: 0.004 min
Response: 16476073
Conc: 15.34 ng/ml

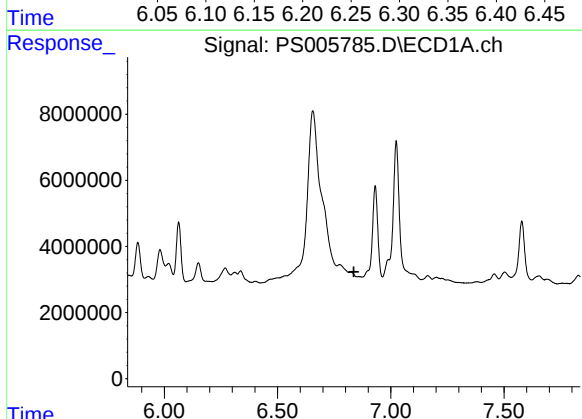


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

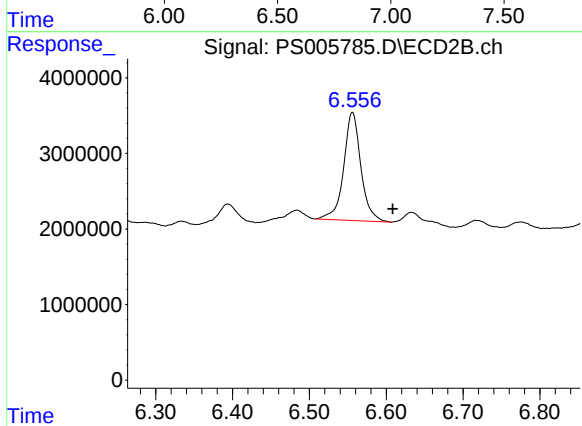

#10 Pentachlorophenol


R.T.: 6.556 min
Delta R.T.: -0.052 min
Response: 22275420
Conc: 1.72 ng/ml

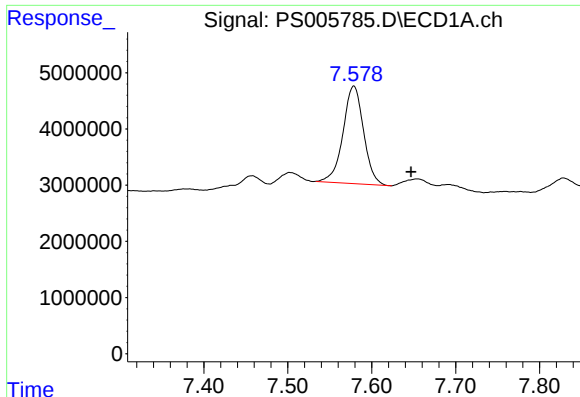

#12 2,4,5-T


R.T.: 7.579 min
Delta R.T.: -0.068 min
Response: 29618100
Conc: 3.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
GW8-20190726

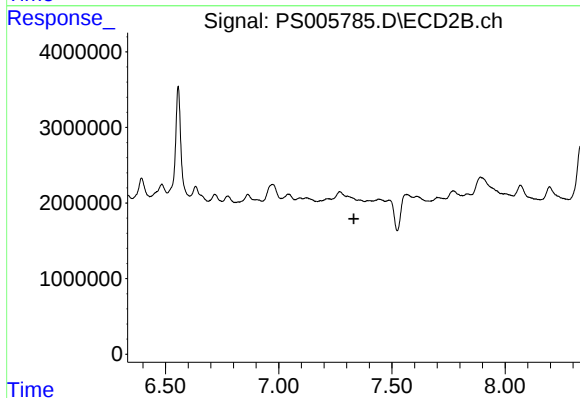


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.332 min
Response: 0
Conc: N.D.

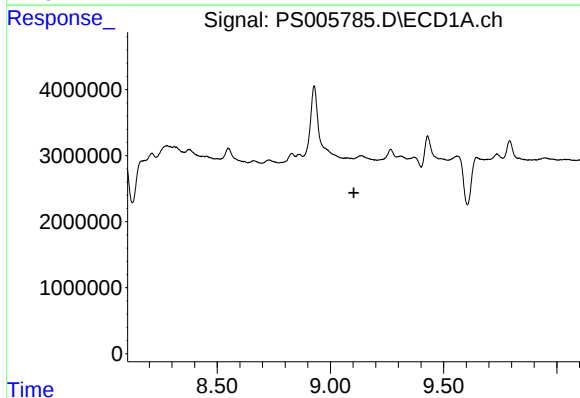


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.104 min
Response: 0
Conc: N.D.

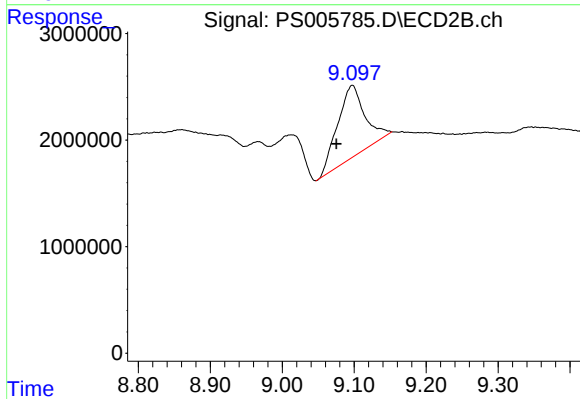

#15 Picloram


R.T.: 9.097 min
Delta R.T.: 0.022 min
Response: 17793761
Conc: 2.37 ng/ml

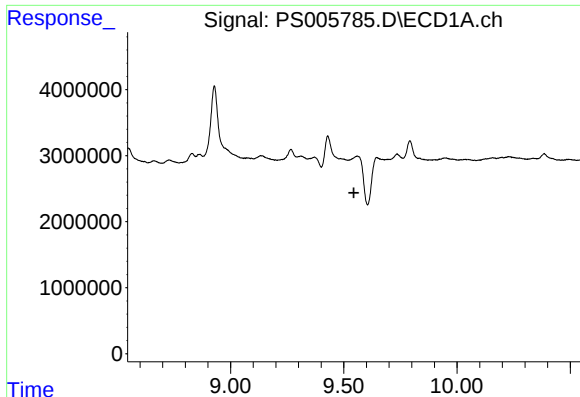

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
GW8-20190726

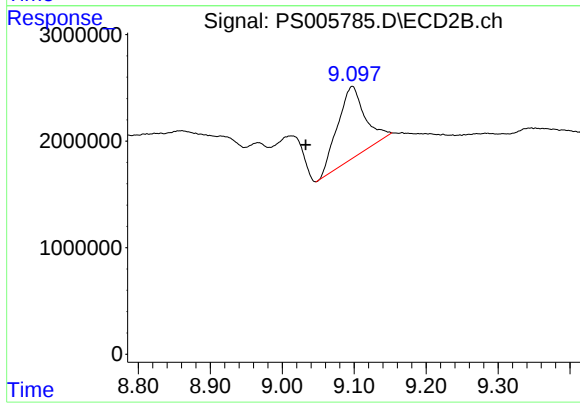

#16 DCPA

R.T.: 9.097 min
Delta R.T.: 0.064 min
Response: 17793761
Conc: 2.70 ng/ml