

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073119\
 Data File : PS005788.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2019 15:57
 Operator : SM\AJ
 Sample : K4021-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 17:25:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.557	5.276	184.4E6	142.7E6	127.100	143.475
Target Compounds							
1) T	Dalapon	2.054	0.000	22143349	0	11.948	N.D. #
2) T	3,5-DICHL...	0.000	4.594	0	54639181	N.D.	42.117
5) T	DICAMBA	5.777	5.410	26481124	29249158	4.434	7.835 #
9) T	2,4-D	6.634	0.000	255.3E6	0	170.358	N.D. #
10) T	Pentachlo...	6.836	0.000	22036373	0	1.054	N.D. #
12) T	2,4,5-T	0.000	7.379	0	72024767	N.D.	15.151
15) T	Picloram	9.124	9.083	312.1E6	238.8E6	26.666	31.786
16) T	DCPA	0.000	9.083	0	238.8E6	N.D.	36.212



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073119\
Data File : PS005788.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2019 15:57
Operator : SM\AJ
Sample : K4021-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
TP-10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 17:25:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

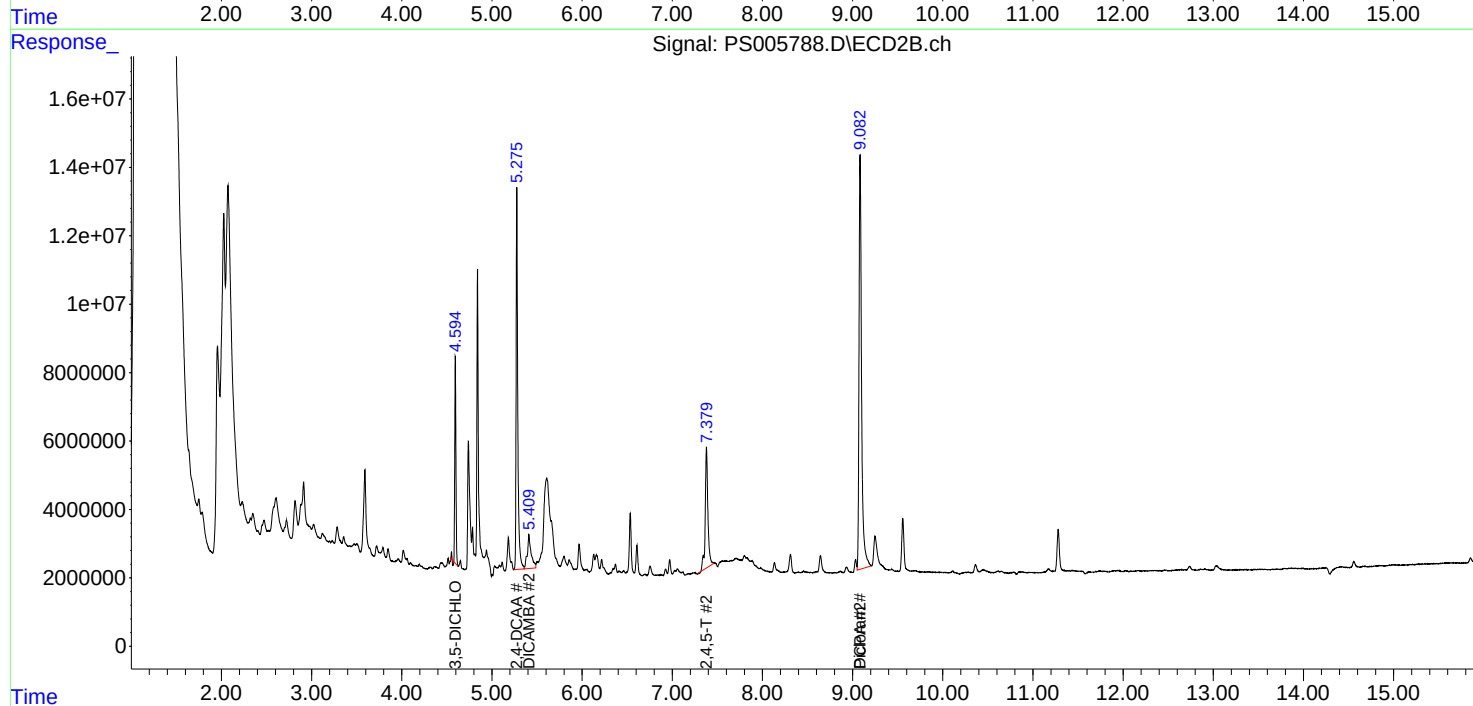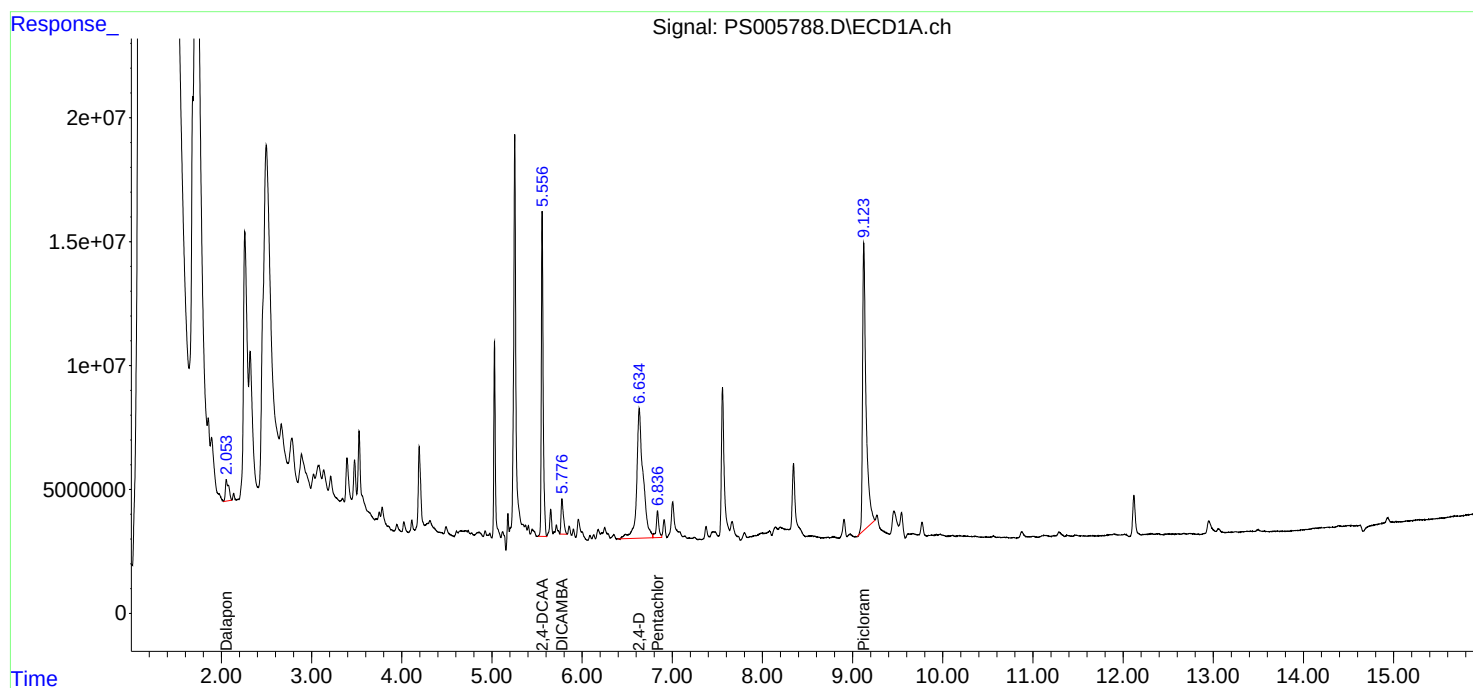


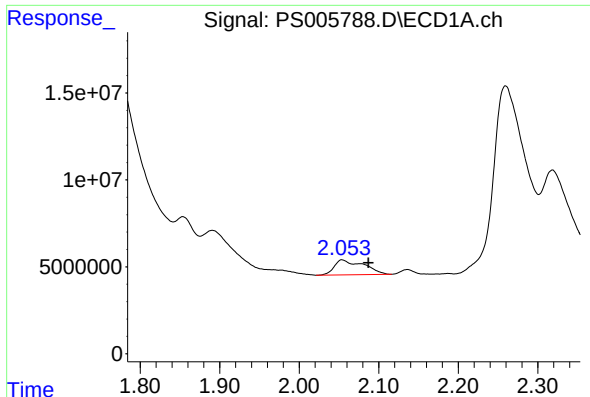

#1 Dalapon


R.T.: 2.054 min
Delta R.T.: -0.033 min
Response: 22143349
Conc: 11.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-10

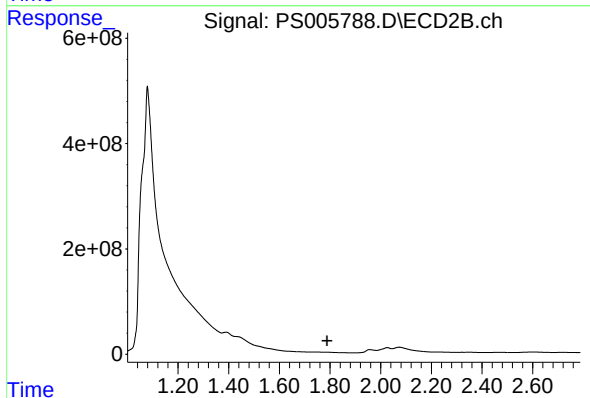


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

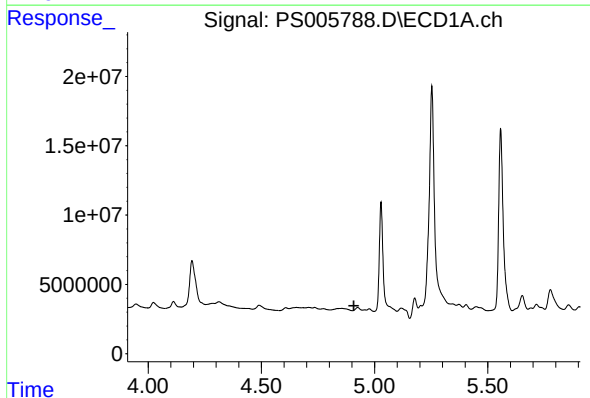


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

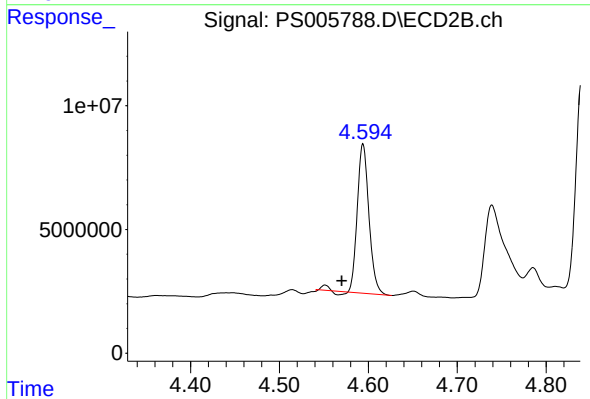

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.594 min
Delta R.T.: 0.024 min
Response: 54639181
Conc: 42.12 ng/ml

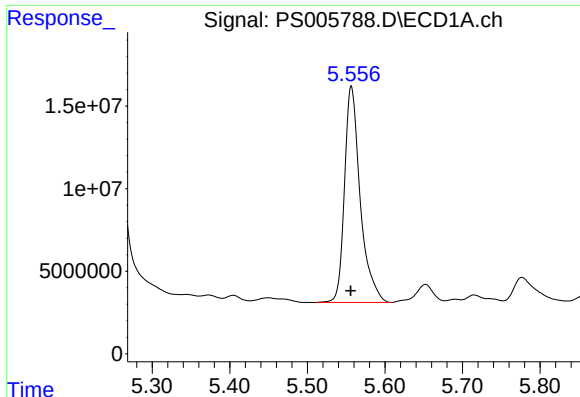

#4 2,4-DCAA


R.T.: 5.557 min
Delta R.T.: 0.000 min
Response: 184398540
Conc: 127.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-10

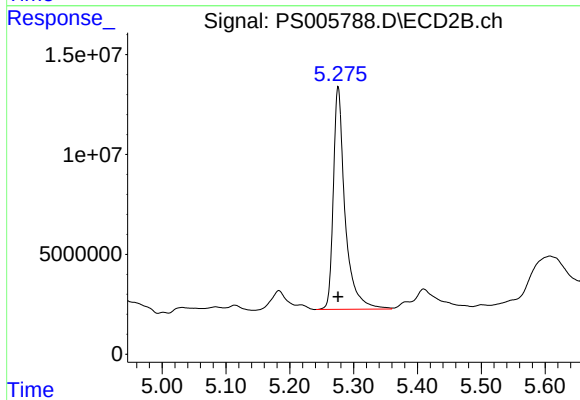


#4 2,4-DCAA

R.T.: 5.276 min
Delta R.T.: 0.000 min
Response: 142711400
Conc: 143.47 ng/ml

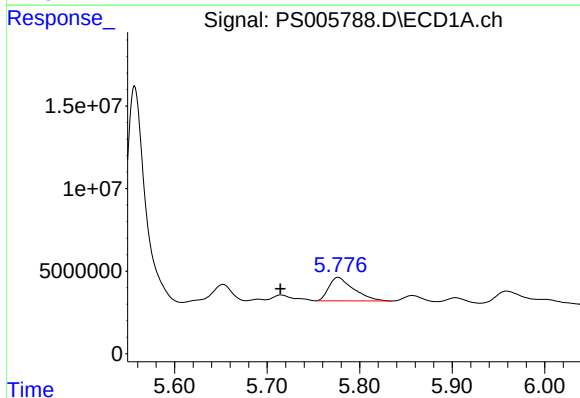


#5 DICAMBA

R.T.: 5.777 min
Delta R.T.: 0.063 min
Response: 26481124
Conc: 4.43 ng/ml

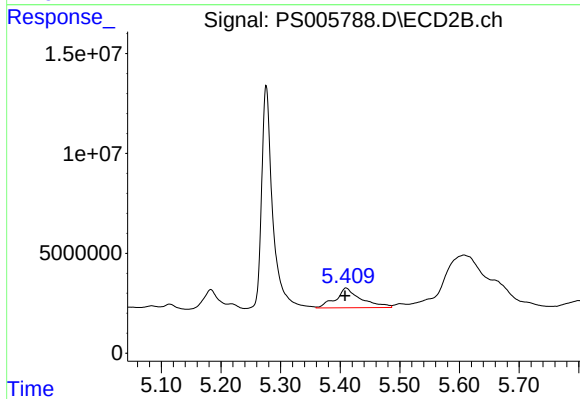

#5 DICAMBA


R.T.: 5.410 min
Delta R.T.: 0.002 min
Response: 29249158
Conc: 7.84 ng/ml

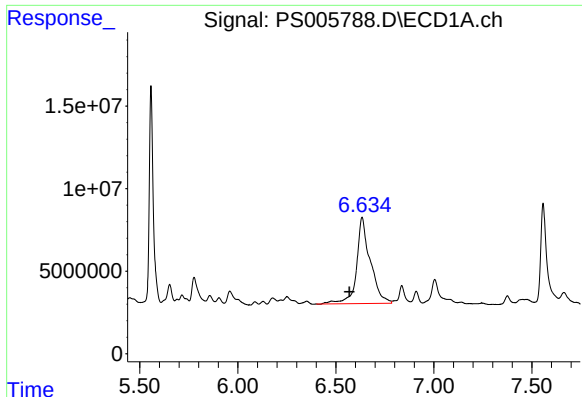

#9 2,4-D


R.T.: 6.634 min
Delta R.T.: 0.065 min
Response: 255310746
Conc: 170.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-10

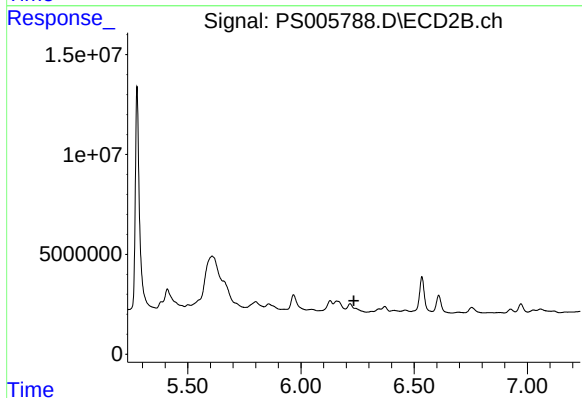


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

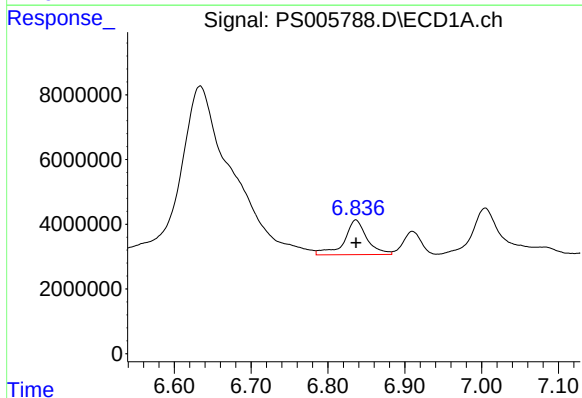


#10 Pentachlorophenol

R.T.: 6.836 min
Delta R.T.: 0.000 min
Response: 22036373
Conc: 1.05 ng/ml

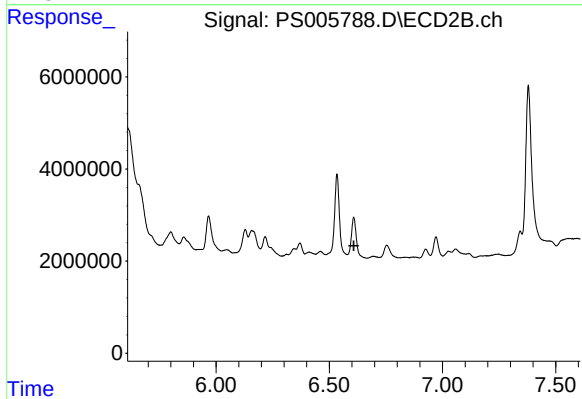

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 6.608 min
Response: 0
Conc: N.D.

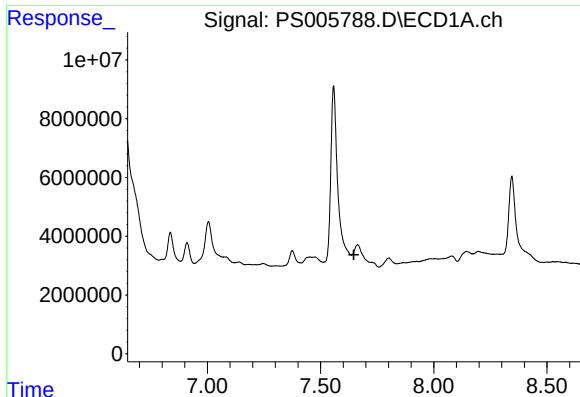

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.647 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-10

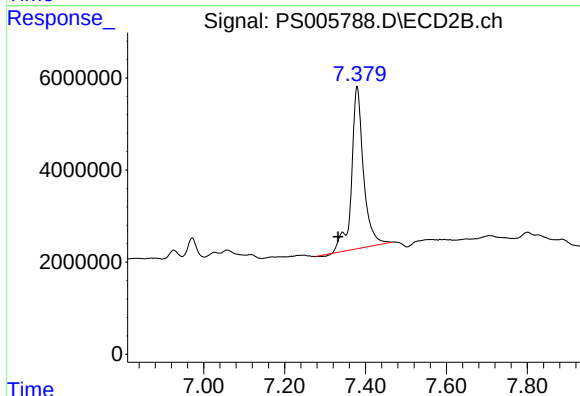


#12 2,4,5-T

R.T.: 7.379 min
Delta R.T.: 0.047 min
Response: 72024767
Conc: 15.15 ng/ml

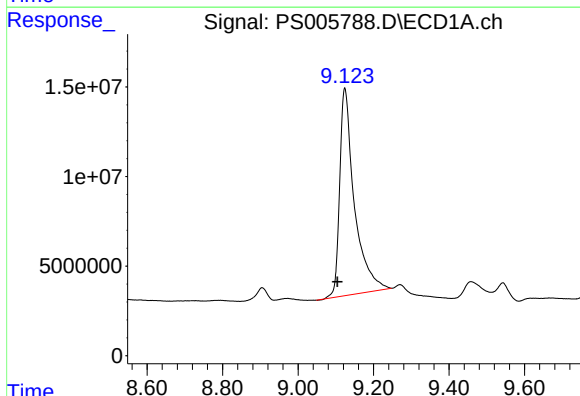


#15 Picloram

R.T.: 9.124 min
Delta R.T.: 0.020 min
Response: 312131266
Conc: 26.67 ng/ml

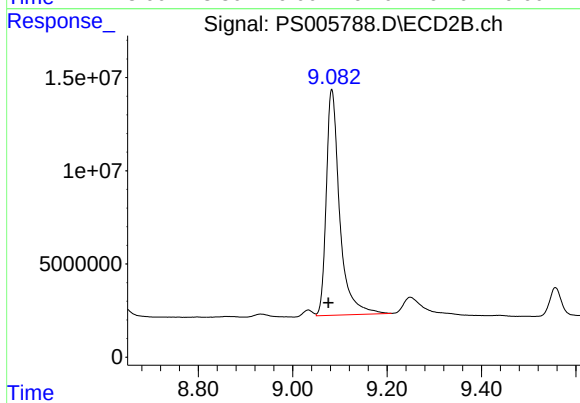

#15 Picloram


R.T.: 9.083 min
Delta R.T.: 0.008 min
Response: 238785602
Conc: 31.79 ng/ml

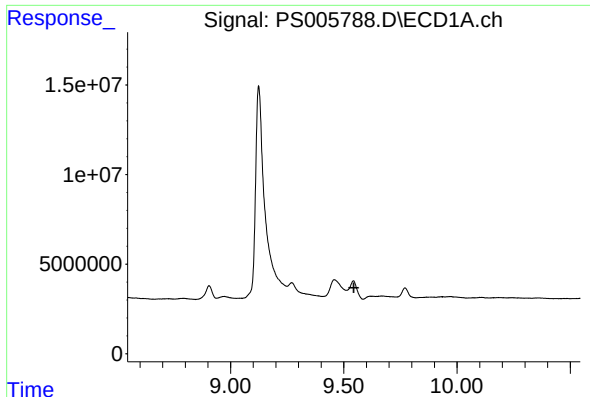

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-10

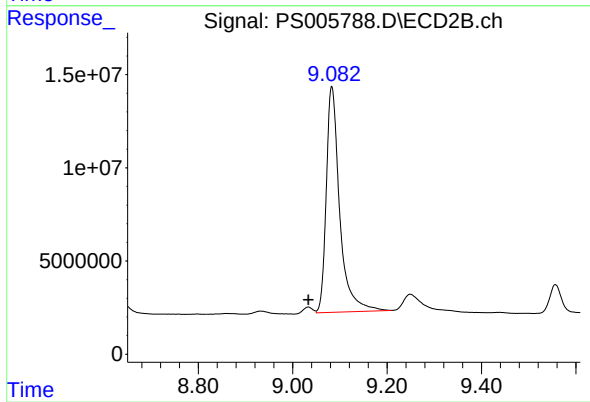

#16 DCPA

R.T.: 9.083 min
Delta R.T.: 0.050 min
Response: 238785602
Conc: 36.21 ng/ml