

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073119\
 Data File : PS005793.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2019 17:48
 Operator : SM\AJ
 Sample : K4044-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 01:52:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.556	5.276	256.6E6	187.3E6	176.892	188.311
Target Compounds							
2) T	3,5-DICHL...	0.000	4.594	0	32765978	N.D.	25.257
5) T	DICAMBA	5.778	0.000	15247696	0	2.553	N.D. #
9) T	2,4-D	6.635	0.000	219.4E6	0	146.415	N.D. #
11) T	2,4,5-TP ...	0.000	7.005	0	21158021	N.D.	4.079



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073119\
Data File : PS005793.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2019 17:48
Operator : SM\AJ
Sample : K4044-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 01:52:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

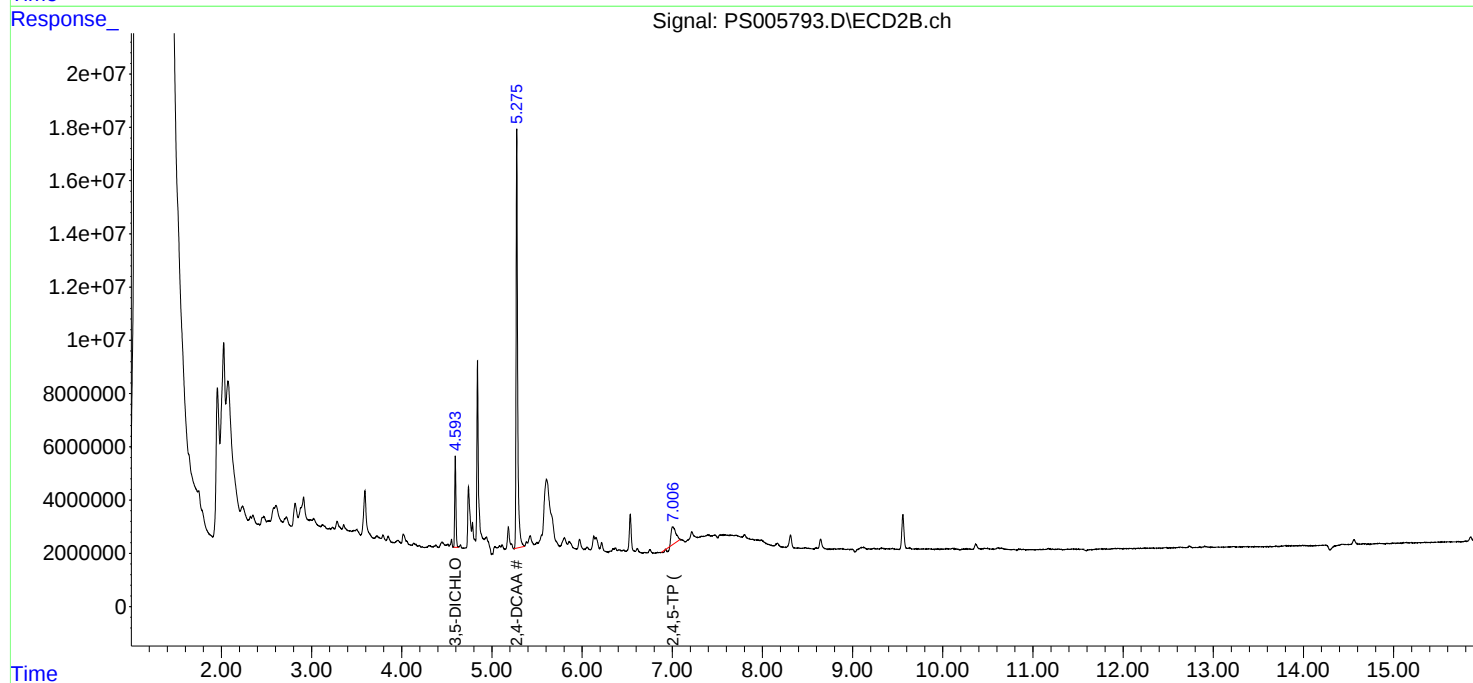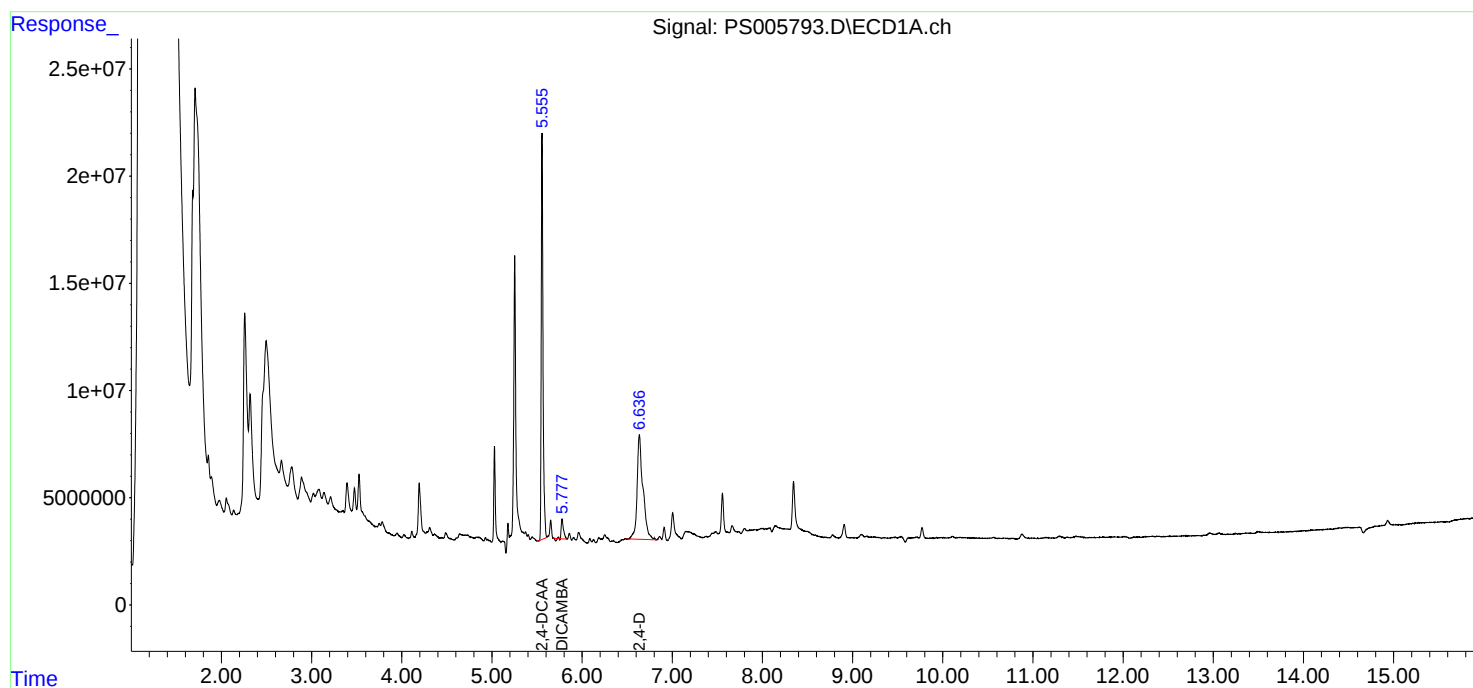


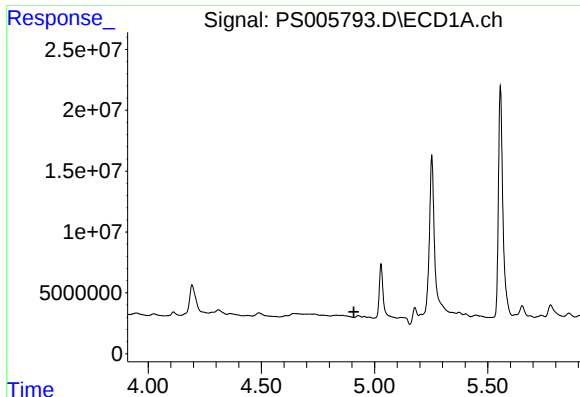

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-1

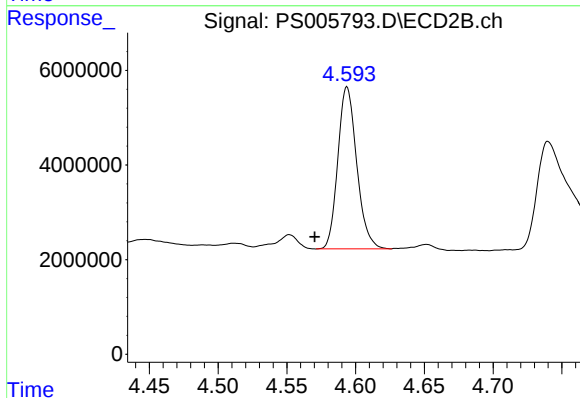


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.594 min
Delta R.T.: 0.024 min
Response: 32765978
Conc: 25.26 ng/ml

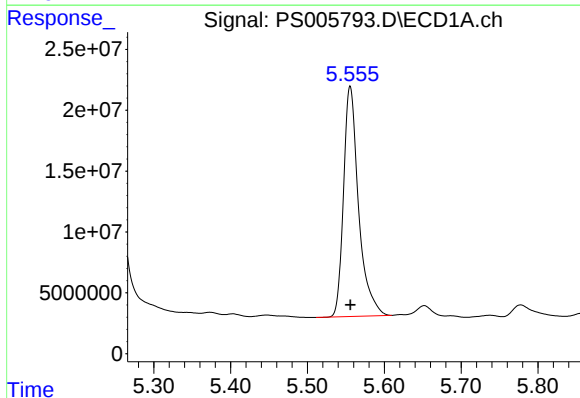


#4 2,4-DCAA

R.T.: 5.556 min
Delta R.T.: 0.000 min
Response: 256638356
Conc: 176.89 ng/ml

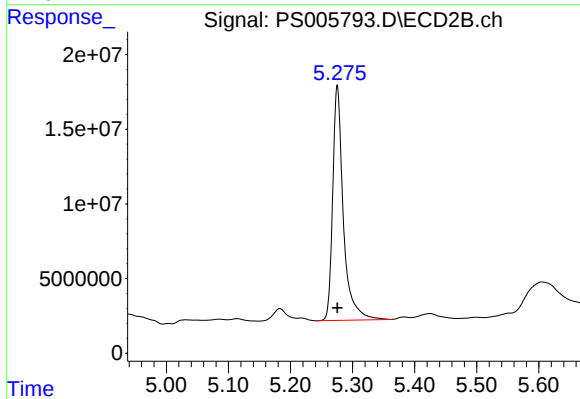

#4 2,4-DCAA


R.T.: 5.276 min
Delta R.T.: 0.000 min
Response: 187309103
Conc: 188.31 ng/ml

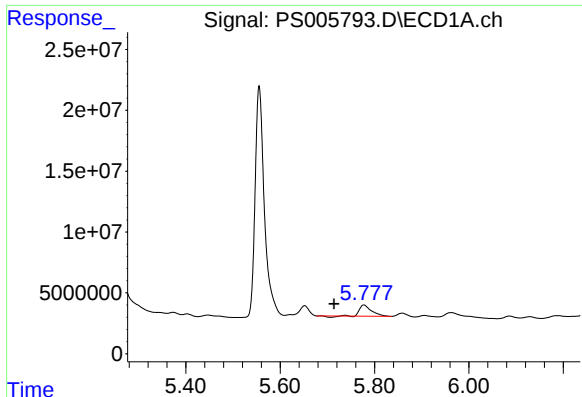

#5 DICAMBA


R.T.: 5.778 min
Delta R.T.: 0.063 min
Response: 15247696
Conc: 2.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-1

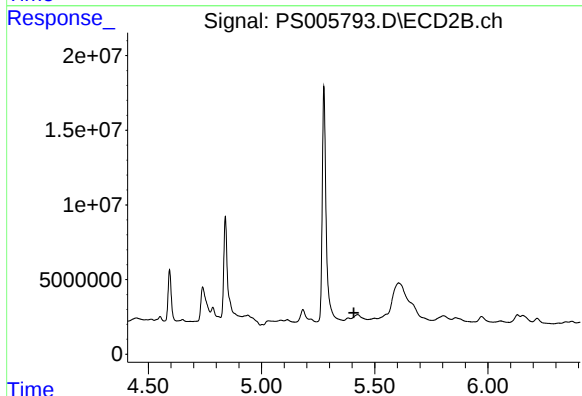


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.408 min
Response: 0
Conc: N.D.

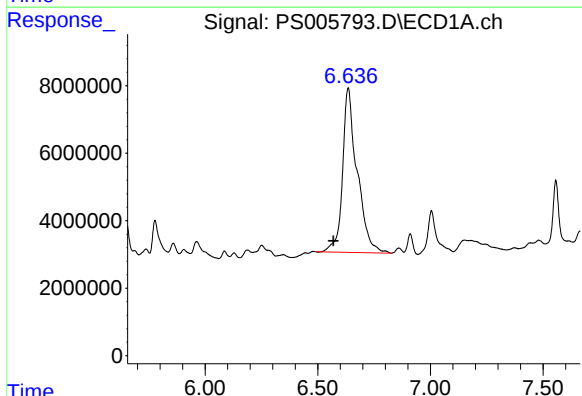


#9 2,4-D

R.T.: 6.635 min
Delta R.T.: 0.066 min
Response: 219426975
Conc: 146.41 ng/ml

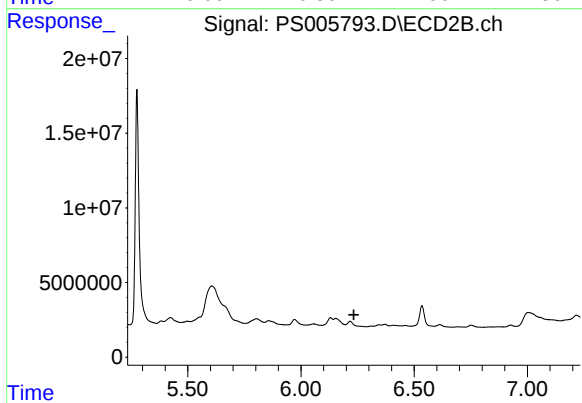

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

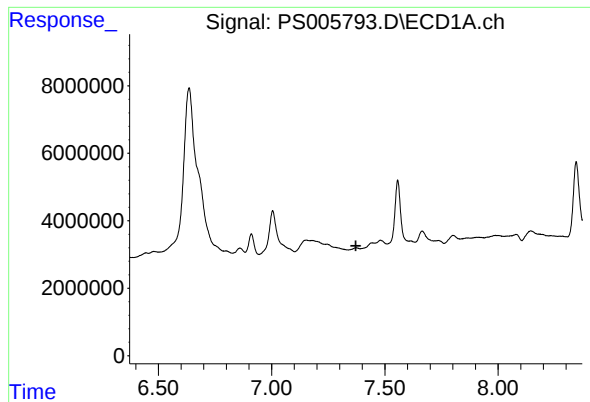

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-1

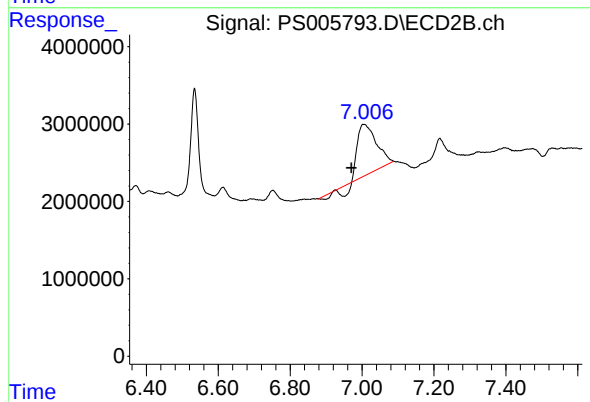

#11 2,4,5-TP (SILVEX)

R.T.: 7.005 min
Delta R.T.: 0.035 min
Response: 21158021
Conc: 4.08 ng/ml